

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012425\
 Data File : BN036024.D
 Acq On : 24 Jan 2025 14:20
 Operator : RC/JU
 Sample : Q1088-10
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0B09

Quant Time: Jan 24 23:18:48 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 21 23:52:22 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.812	152	2495	0.400	ng/ul	0.00
4) Naphthalene-d8	10.604	136	5228	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.450	164	3036	0.400	ng/ul	0.00
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-17.19
17) Chrysene-d12	21.372	240	6349	0.400	ng/ul	0.00
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.67
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.276	96	12535	4.589	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.193	152	2502	0.379	ng/ul	0.00
18) Fluoranthene-d10	19.215	212	7279	0.417	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.322	88	95	0.033	ng/ul#	36
20) Pyrene	19.582	202	1329	0.053	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012425\
Data File : BN036024.D
Acq On : 24 Jan 2025 14:20
Operator : RC/JU
Sample : Q1088-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0B09

Quant Time: Jan 24 23:18:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 21 23:52:22 2025
Response via : Initial Calibration




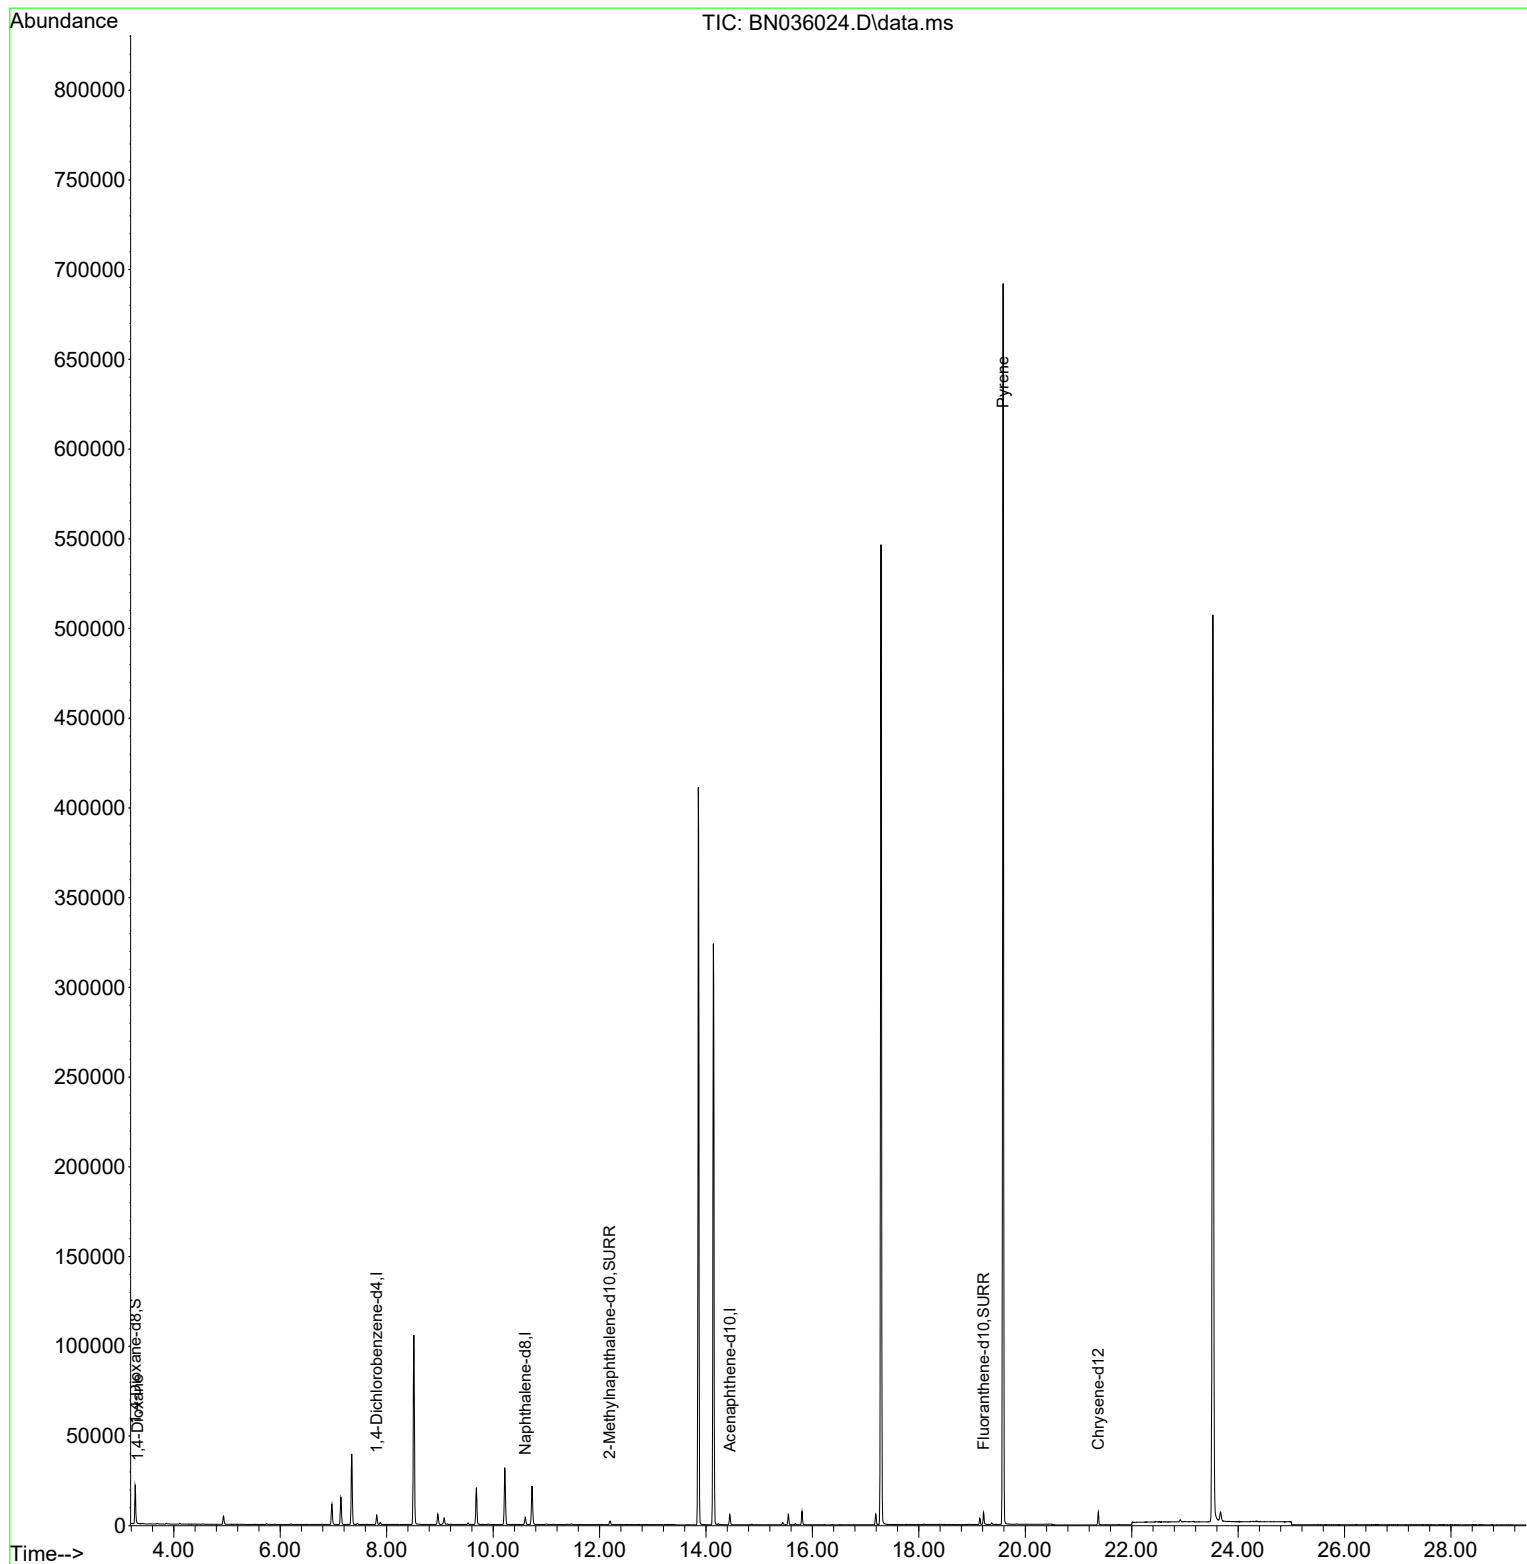


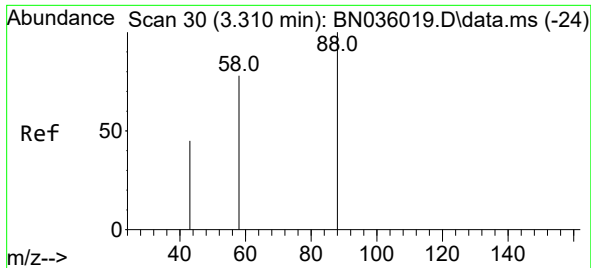

#2
 1,4-Dioxane
 Concen: 0.033 ng/ul
 RT: 3.322 min Scan# 31
 Delta R.T. 0.009 min
 Lab File: BN036024.D
 Acq: 24 Jan 2025 14:20

Instrument :
 BNA_N
 ClientSampleId :
 C0B09

Tgt Ion: 88 Resp: 95
 Ion Ratio Lower Upper
 88 100
 43 124.0 40.7 61.1#
 58 42.3 55.2 82.8#

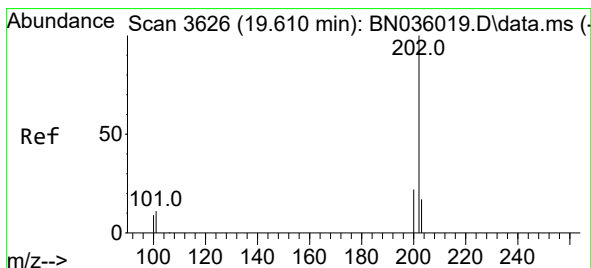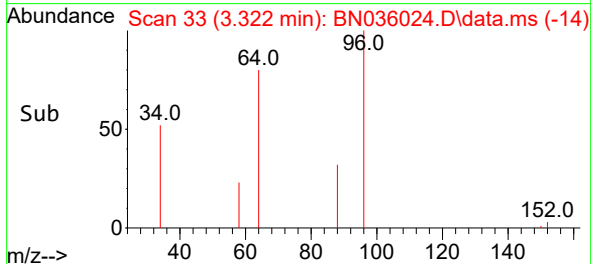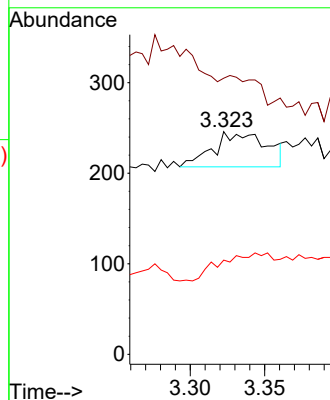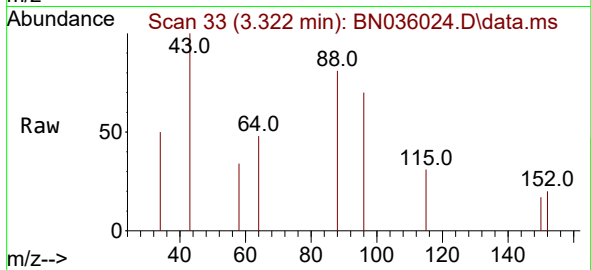

#20
 Pyrene
 Concen: 0.053 ng/ul
 RT: 19.582 min Scan# 3620
 Delta R.T. -0.027 min
 Lab File: BN036024.D
 Acq: 24 Jan 2025 14:20

Tgt Ion: 202 Resp: 1329
 Ion Ratio Lower Upper
 202 100
 101 208.4 9.3 13.9#
 100 1556.1 7.5 11.3#

