
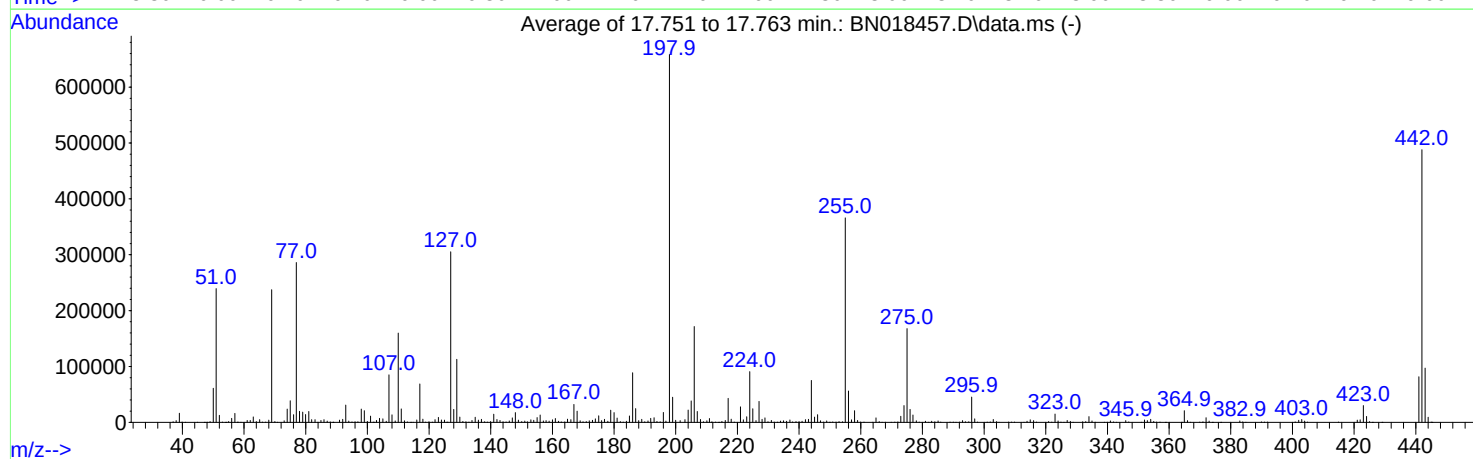


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012522\
 Data File : BN018457.D
 Acq On : 25 Jan 2022 13:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN012422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 24 18:25:49 2022

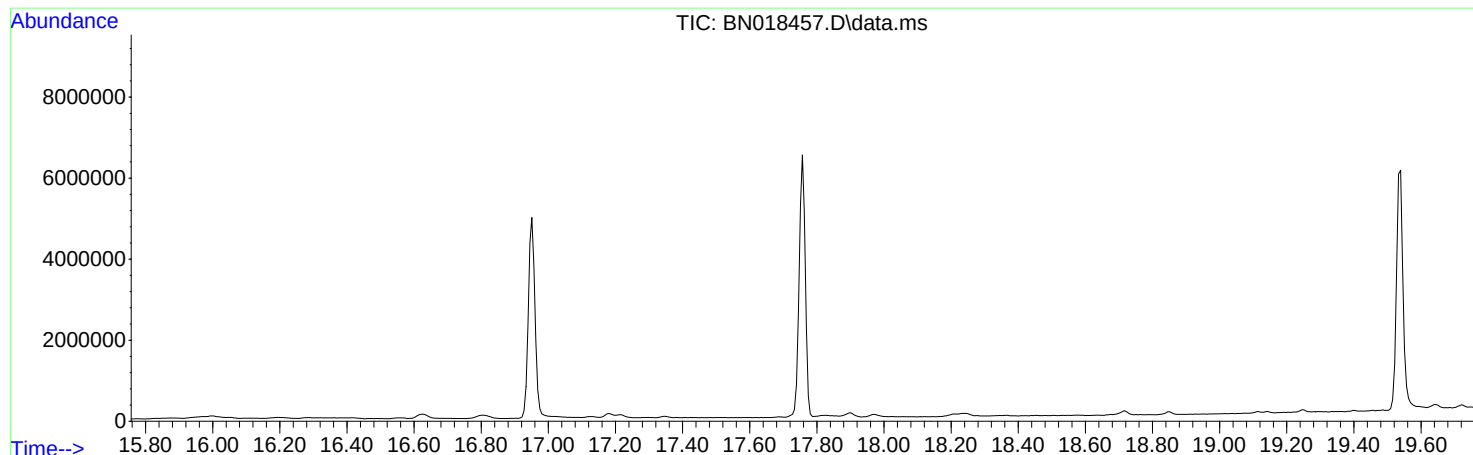




AutoFind: Scans 2510, 2511, 2512; Background Corrected with Scan 2503

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.4	239548	PASS
68	69	0.00	2	1.7	4083	PASS
69	198	0.00	100	36.1	237523	PASS
70	69	0.00	2	0.6	1435	PASS
127	198	10	80	46.4	305365	PASS
197	198	0.00	2	0.4	2436	PASS
198	198	100	100	100.0	658389	PASS
199	198	5	9	6.8	45067	PASS
275	198	10	60	25.5	167851	PASS
365	198	1	100	3.2	20941	PASS
441	198	0.01	100	12.4	81787	PASS
442	442	50	100	100.0	487979	PASS
443	442	15	24	19.9	97075	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012522\
 Data File : BN018457.D
 Acq On : 25 Jan 2022 13:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jan 26 05:36:55 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 26 05:36:49 2022
 Response via : Initial Calibration

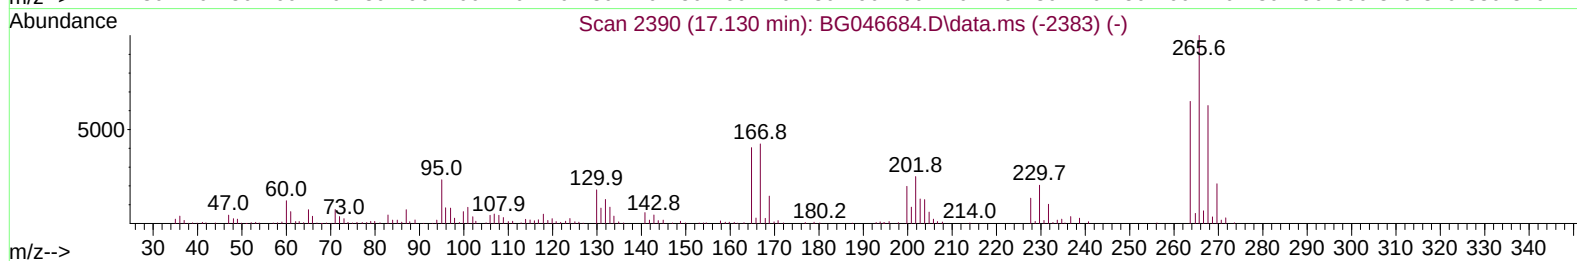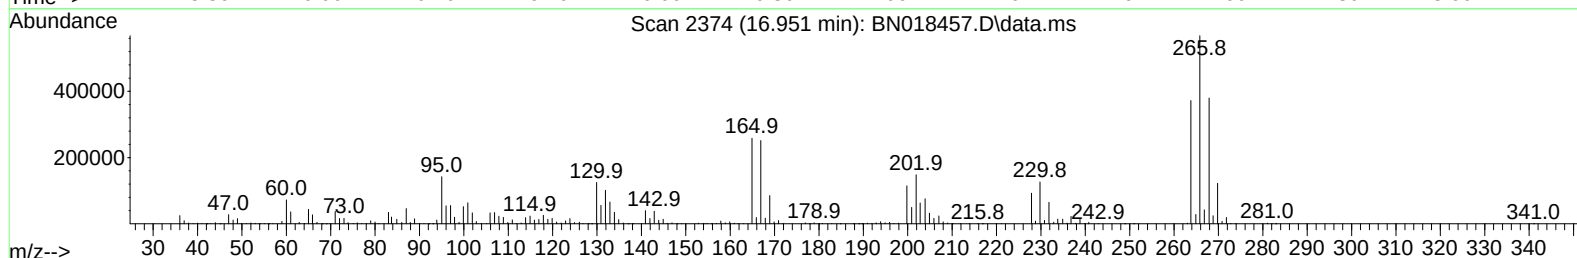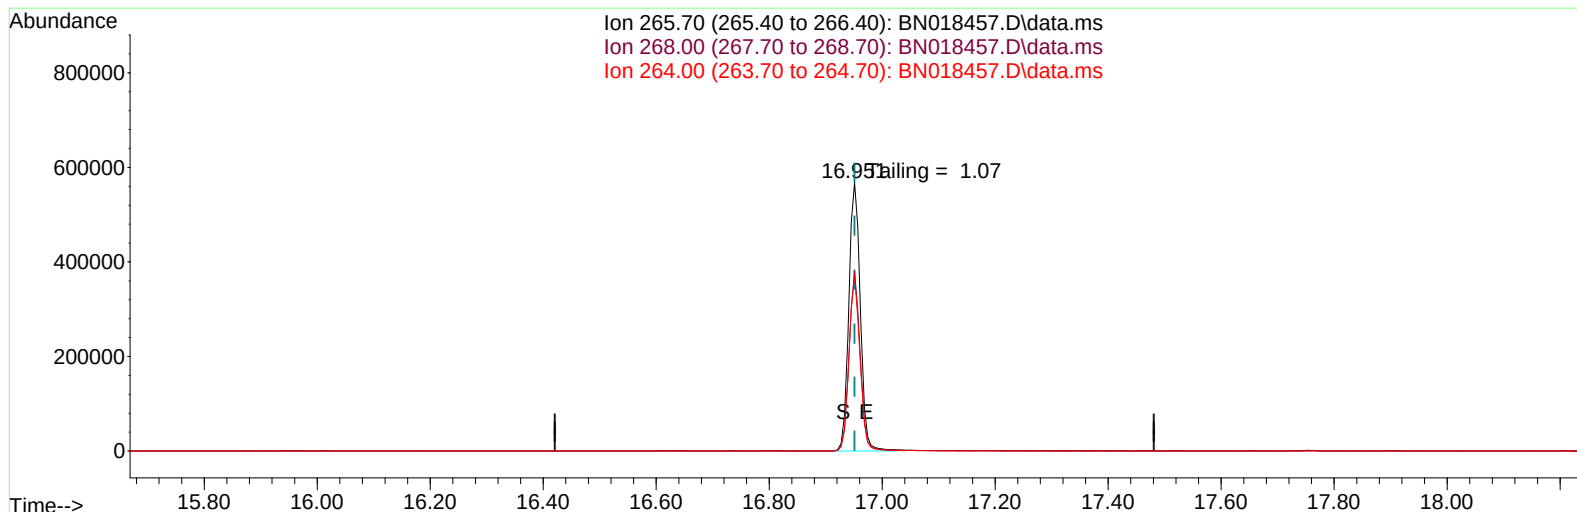

TIC: BN018457.D\data.ms

(70) Pentachlorophenol (C)

16.951min (0.000) 22416.99 ng




response 808014

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.94
264.00	61.60	65.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012522\
 Data File : BN018457.D
 Acq On : 25 Jan 2022 13:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jan 26 05:36:55 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 26 05:36:49 2022
 Response via : Initial Calibration

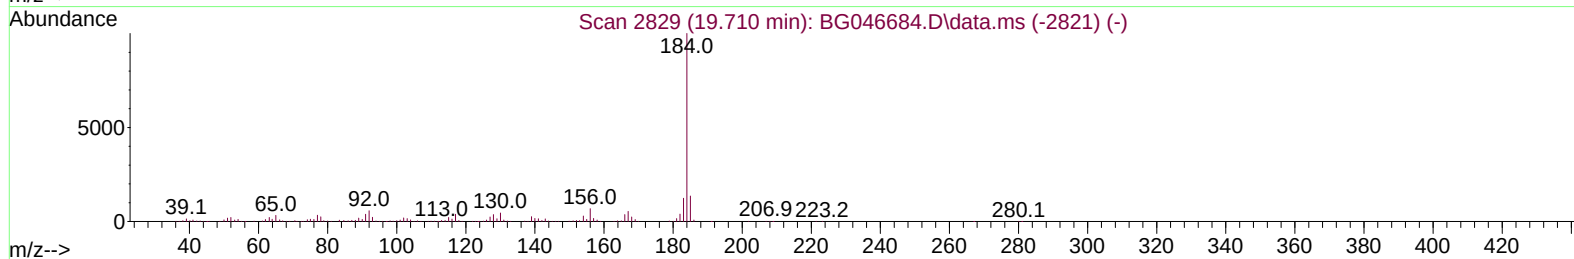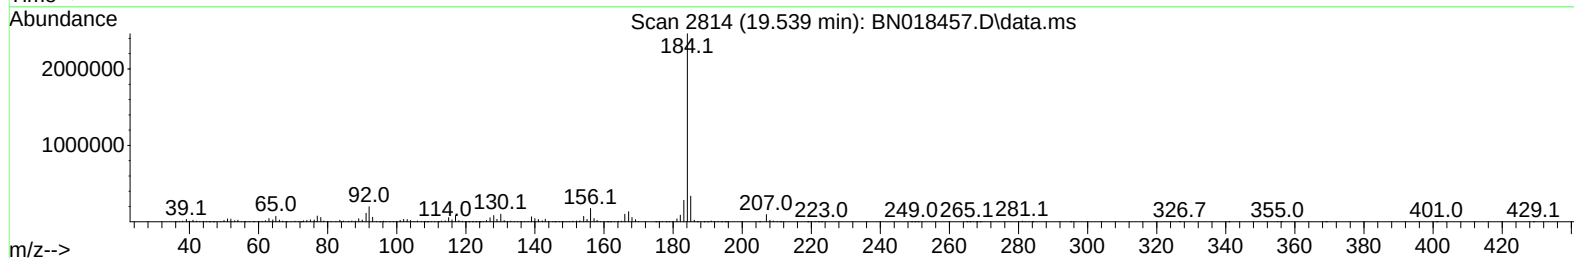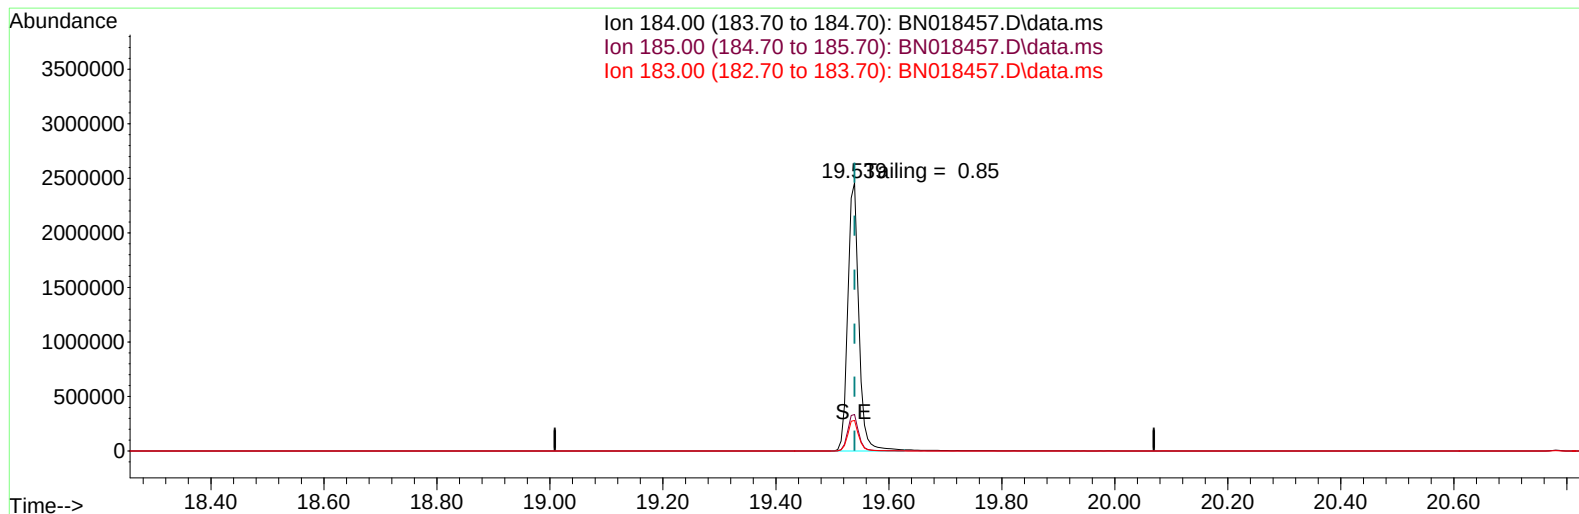

TIC: BN018457.D\data.ms

(77) Benzidine

19.539min (0.000) 0.00 ng

response 3381380

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.63
183.00	13.20	11.38
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/25/2022	BNA_N	<u>BN018457.D</u>
Compound Name	Response	Retention Time
DDT	1930645	20.78
DDD	24996	20.339
DDE	2211	19.833
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
27207	1957852	1.39

Instrument :
BNA_N
ClientSampleId :
DFTPP