
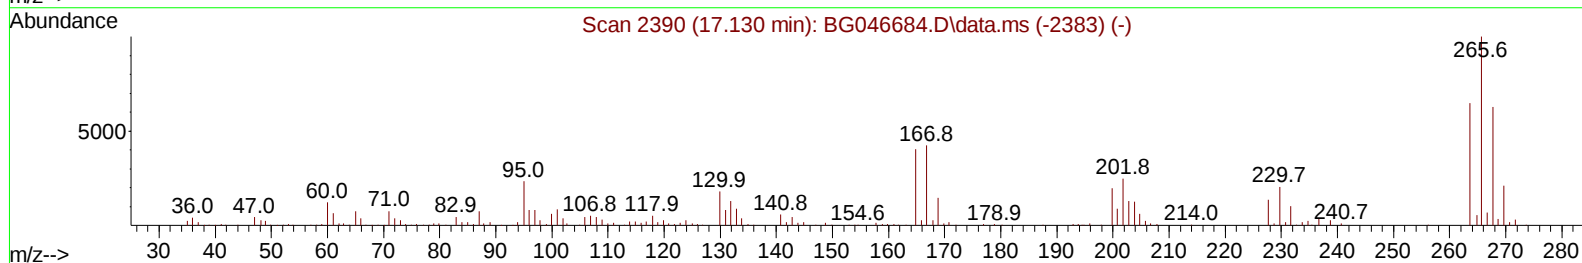
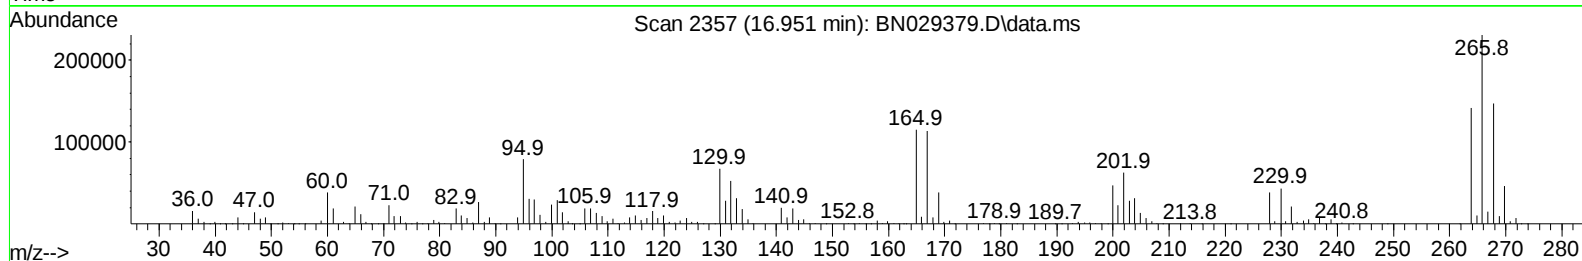


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012524\
Data File : BN029379.D
Acq On : 25 Jan 2024 10:13
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 26 04:05:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 26 04:05:50 2024
Response via : Initial Calibration

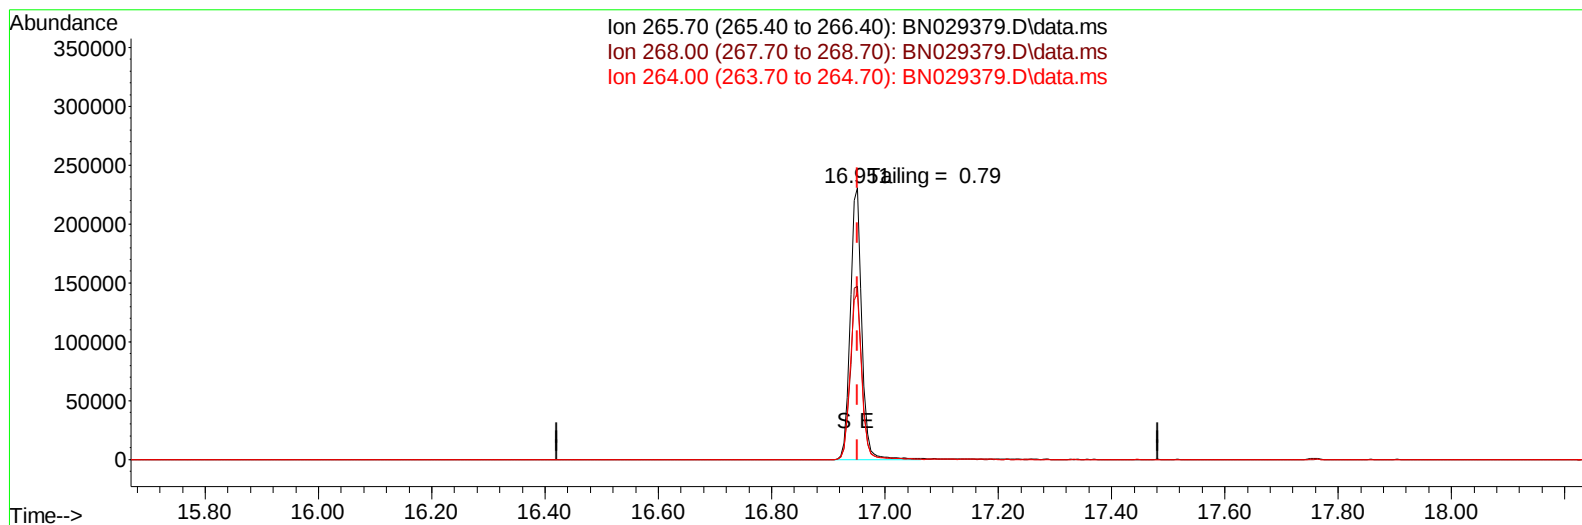

TIC: BN029379.D\data.ms

(70) Pentachlorophenol (C)




16.951min (0.000) 17439.07 ng

response 326405

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.86
264.00	61.60	61.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012524\
Data File : BN029379.D
Acq On : 25 Jan 2024 10:13
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 26 04:05:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 26 04:05:50 2024
Response via : Initial Calibration

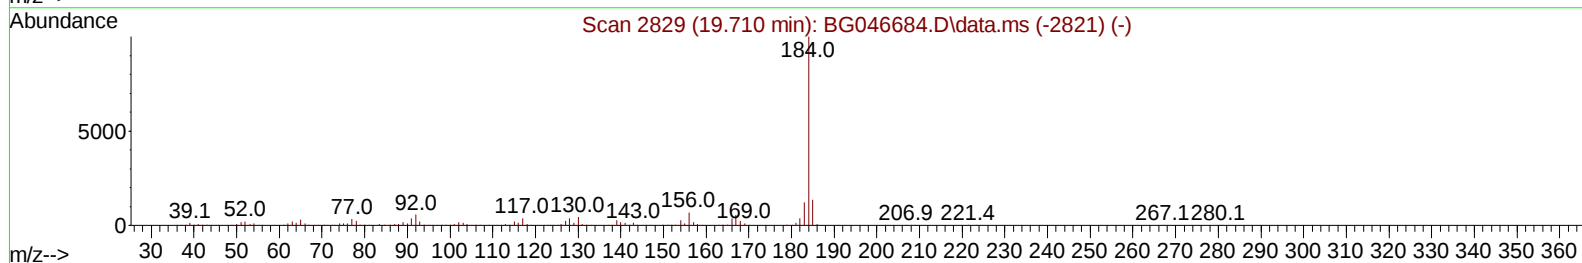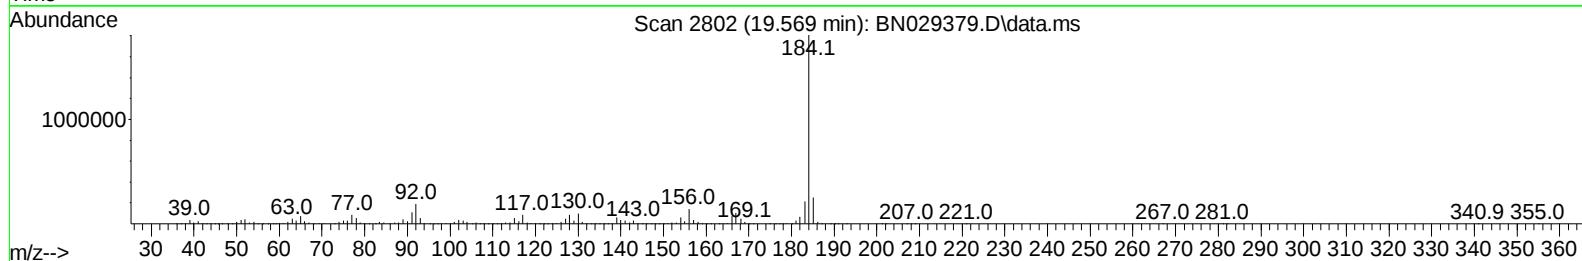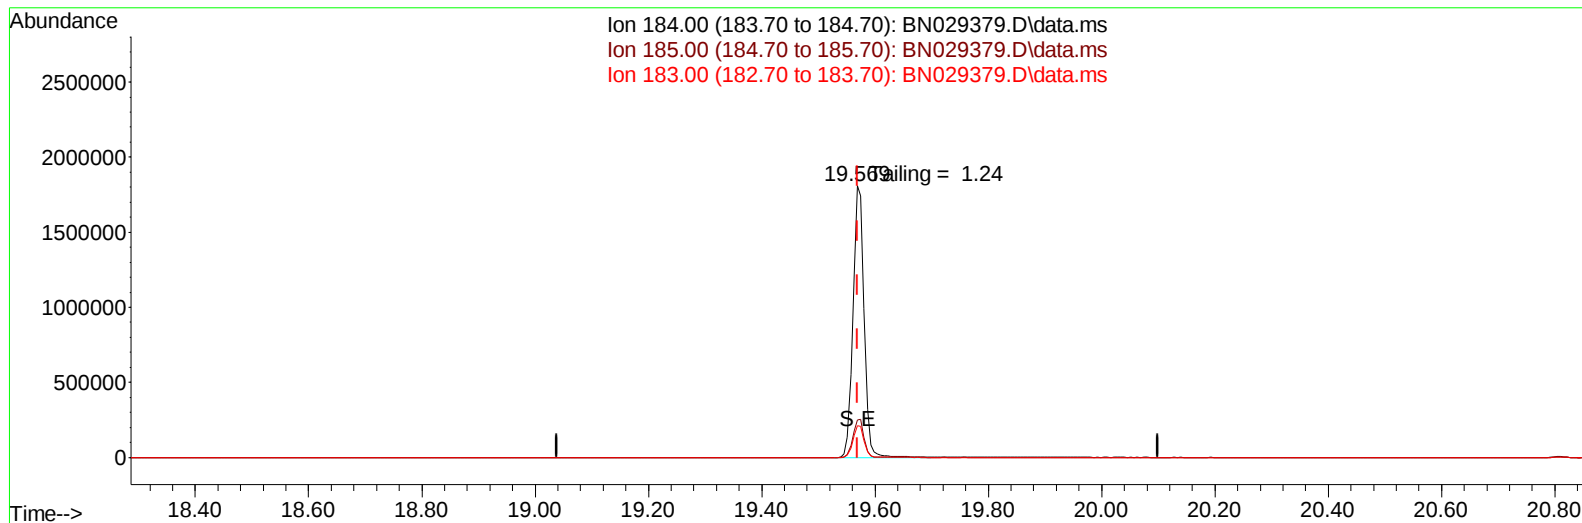

TIC: BN029379.D\data.ms

(77) Benzidine**19.569min (0.000) 0.00 ng****response 2493890**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.85
183.00	13.20	11.74
0.00	0.00	0.00