


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012524\
Data File : BN029379.D
Acq On : 25 Jan 2024 10:13
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN012524.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jan 26 01:42:55 2024

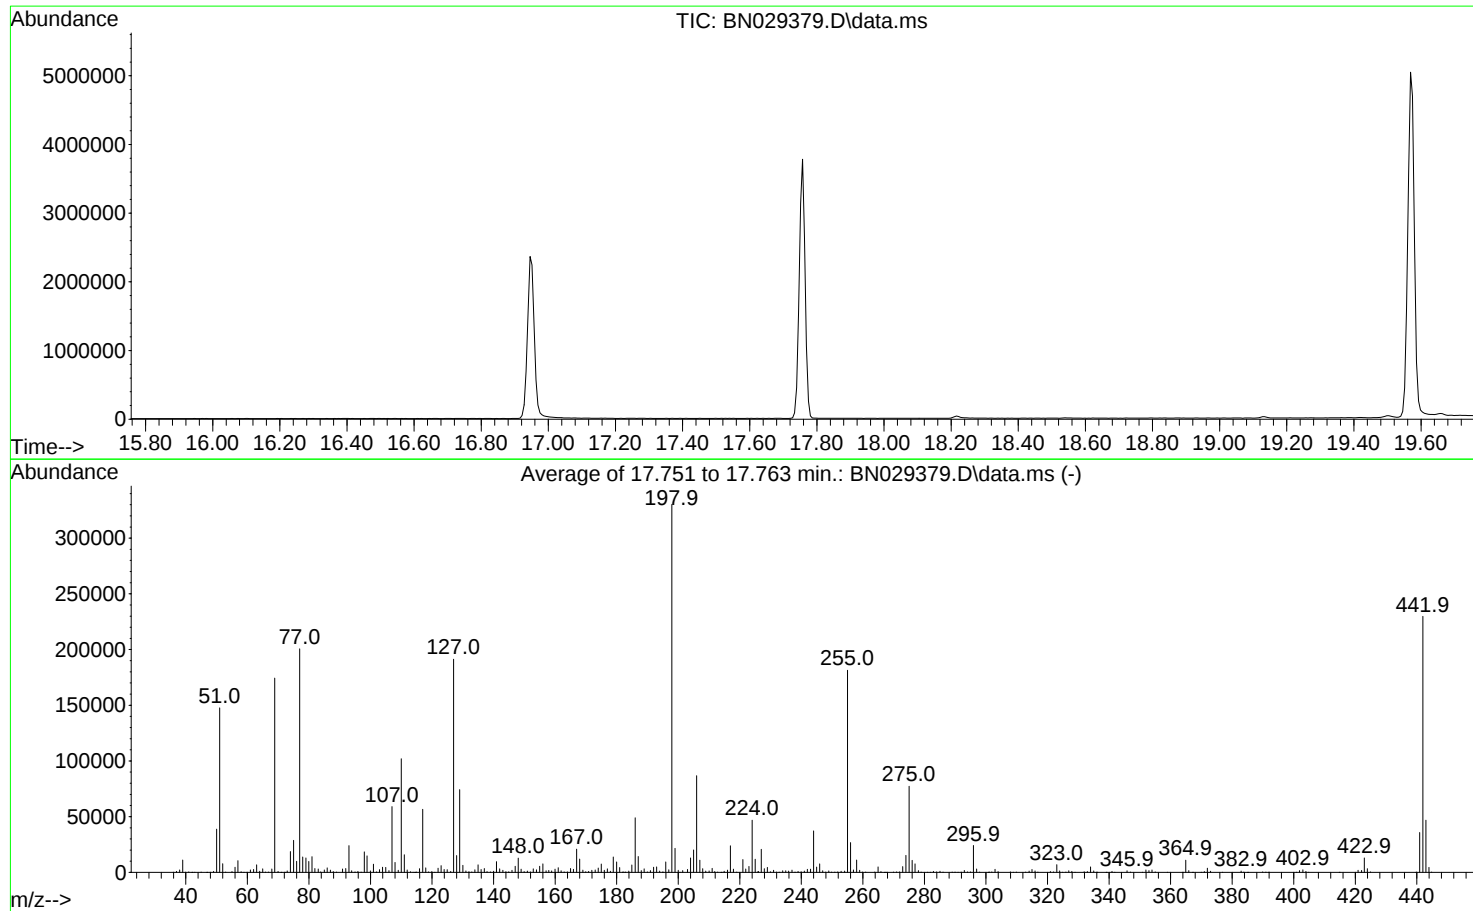




AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.7	147701	PASS
68	69	0.00	2	1.8	3061	PASS
69	198	0.00	100	52.8	174323	PASS
70	69	0.00	2	0.5	913	PASS
127	198	10	80	57.9	191275	PASS
197	198	0.00	2	0.7	2293	PASS
198	198	100	100	100.0	330197	PASS
199	198	5	9	6.5	21600	PASS
275	198	10	60	23.4	77245	PASS
365	198	1	100	3.3	10918	PASS
441	198	0.01	100	10.8	35736	PASS
442	442	50	100	100.0	229781	PASS
443	442	15	24	20.4	46821	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012524\
Data File : BN029379.D
Acq On : 25 Jan 2024 10:13
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 26 04:05:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 26 04:05:50 2024
Response via : Initial Calibration

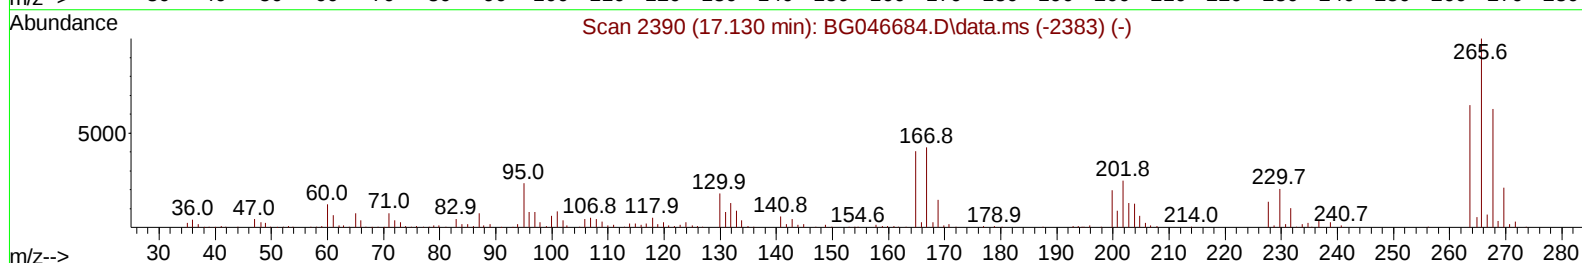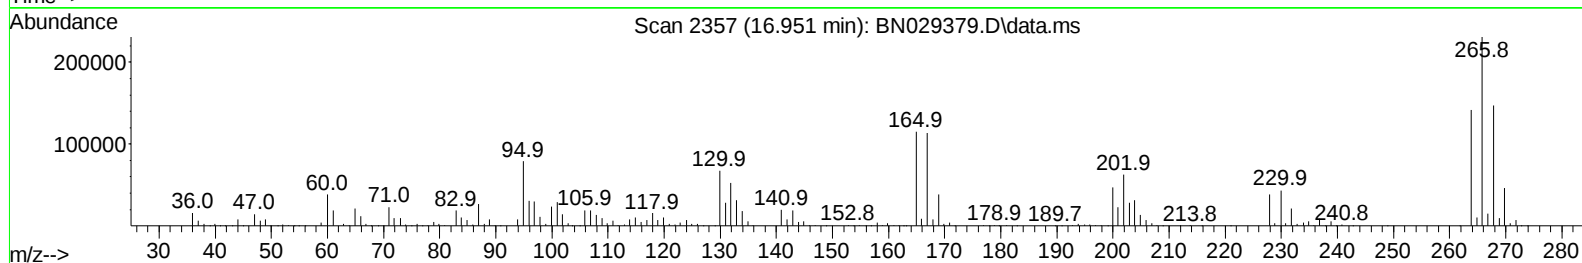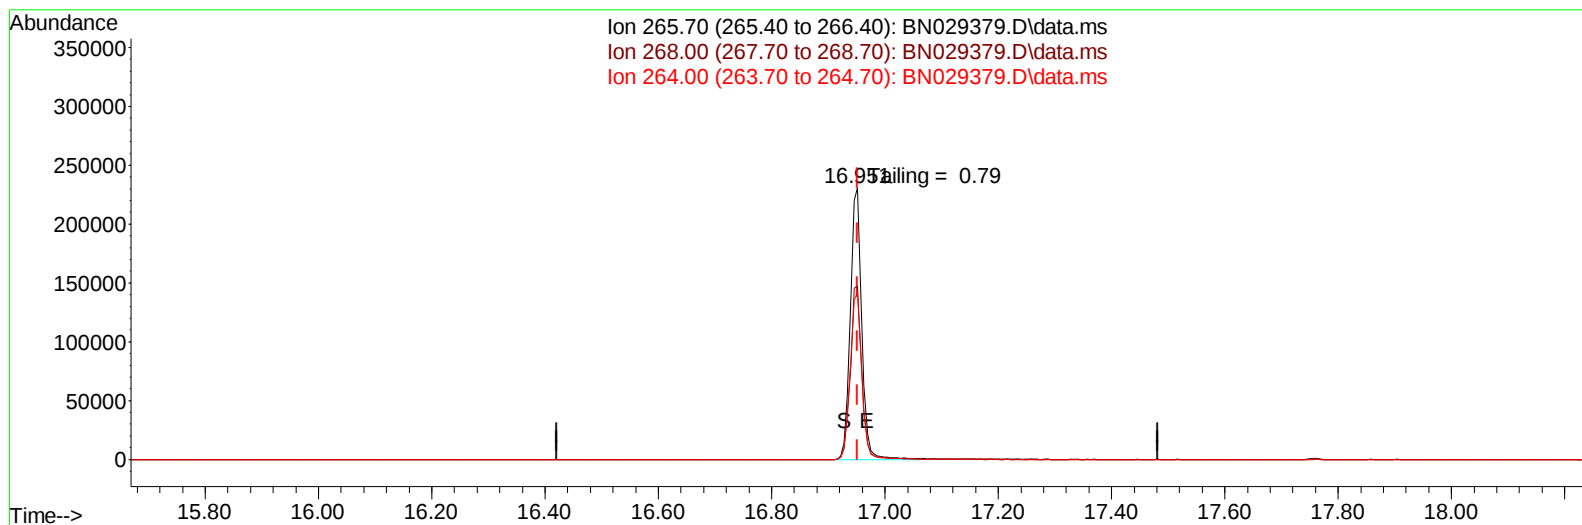

TIC: BN029379.D\data.ms

(70) Pentachlorophenol (C)

16.951min (0.000) 17439.07 ng




response 326405

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.86
264.00	61.60	61.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012524\
Data File : BN029379.D
Acq On : 25 Jan 2024 10:13
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 26 04:05:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 26 04:05:50 2024
Response via : Initial Calibration

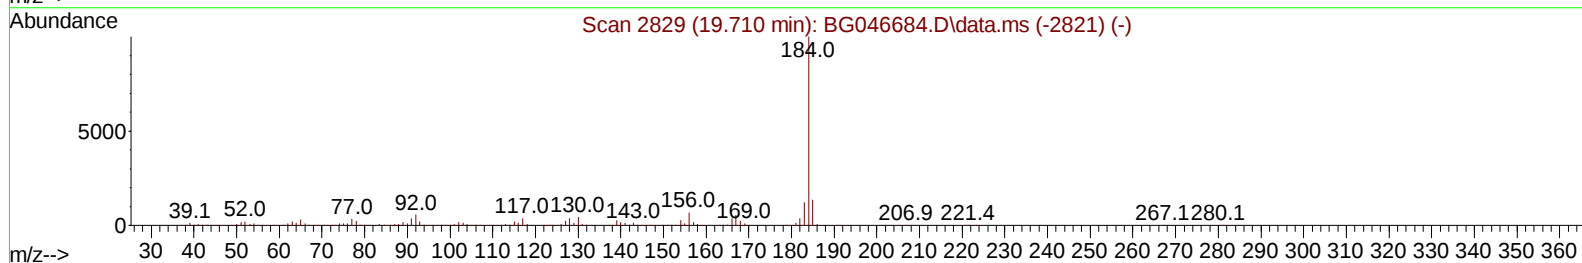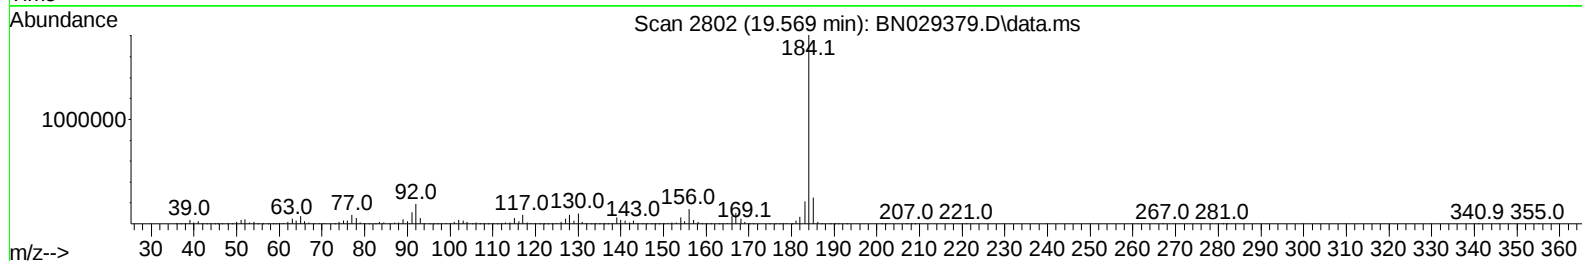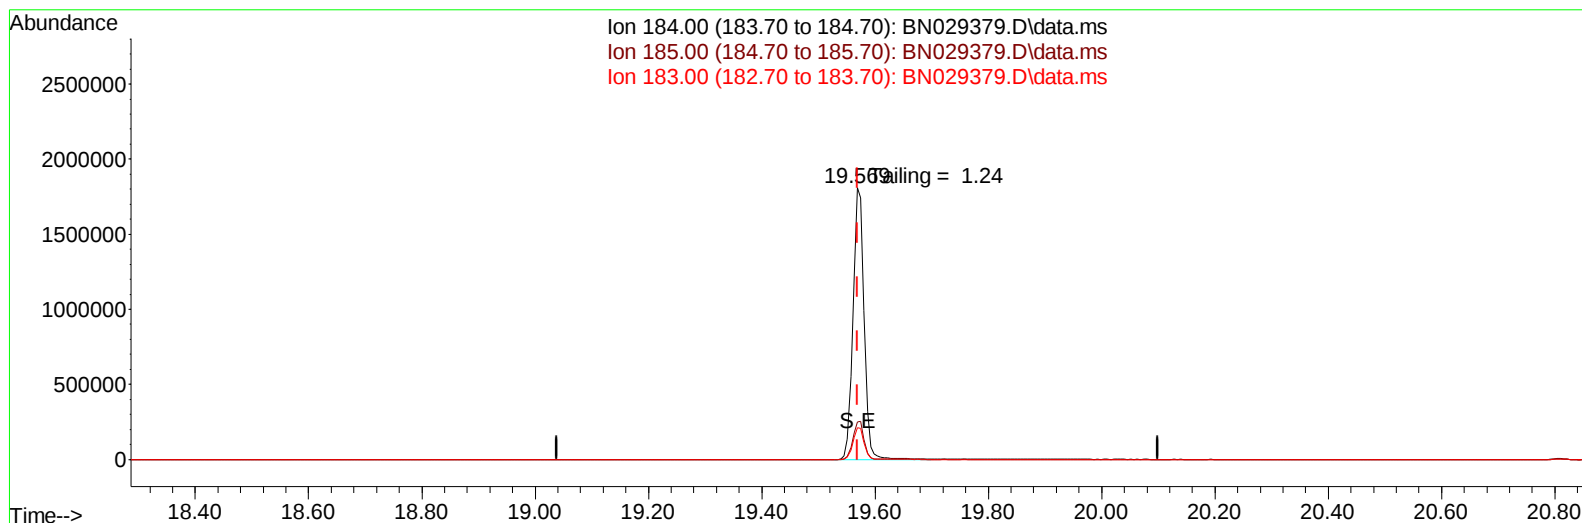

TIC: BN029379.D\data.ms

(77) Benzidine

19.569min (0.000) 0.00 ng

response 2493890

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.85
183.00	13.20	11.74
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/25/2024	BNA_N	<u>BN029379.D</u>
Compound Name	Response	Retention Time
DDT	1098188	20.81
DDD	15854	20.363
DDE	367	19.857
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16221	1114409	1.46

Instrument :
BNA_N
ClientSampleId :
DFTPP