
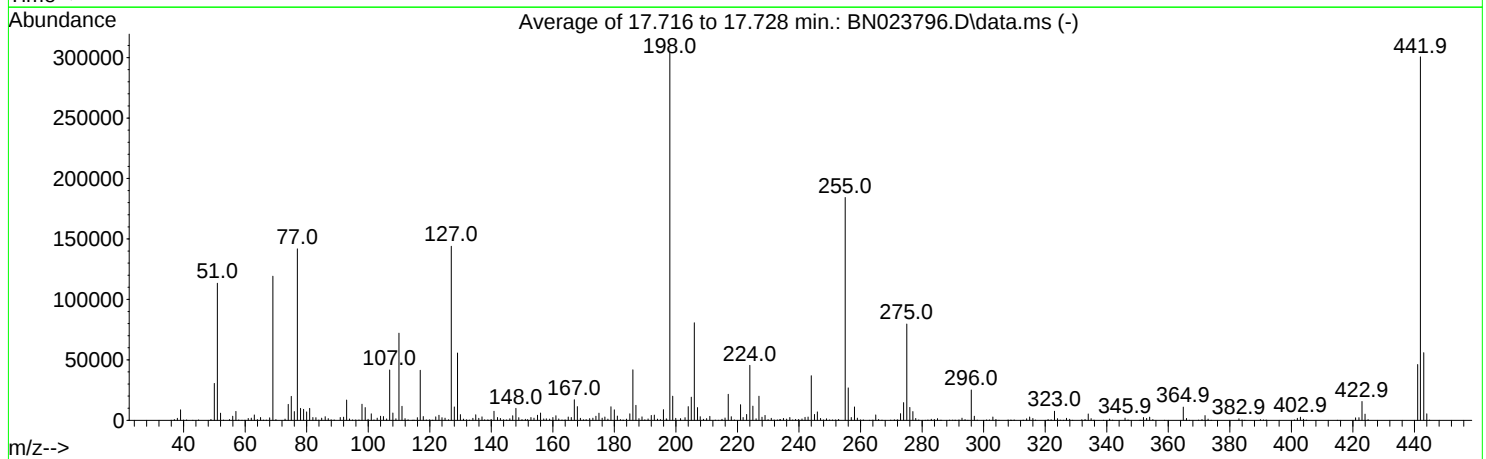


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012623\
Data File : BN023796.D
Acq On : 25 Jan 2023 16:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN011823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jan 26 00:40:21 2023

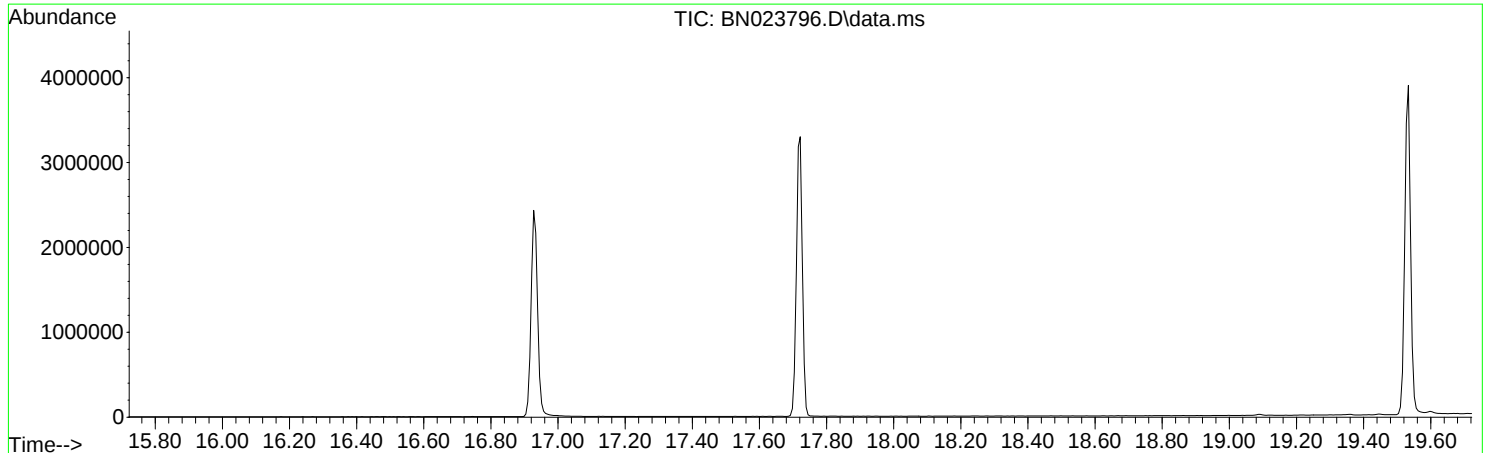




AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.3	113376	PASS
68	69	0.00	2	1.8	2085	PASS
69	198	0.00	100	39.2	119136	PASS
70	69	0.00	2	0.5	635	PASS
127	198	10	80	47.3	143971	PASS
197	198	0.00	2	0.4	1325	PASS
198	198	100	100	100.0	304277	PASS
199	198	5	9	6.6	19999	PASS
275	198	10	60	26.2	79595	PASS
365	198	1	100	3.6	10947	PASS
441	198	0.01	100	15.2	46176	PASS
442	442	50	100	100.0	300608	PASS
443	442	15	24	18.6	55904	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012623\
Data File : BN023796.D
Acq On : 25 Jan 2023 16:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 26 03:20:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 26 03:20:25 2023
Response via : Initial Calibration

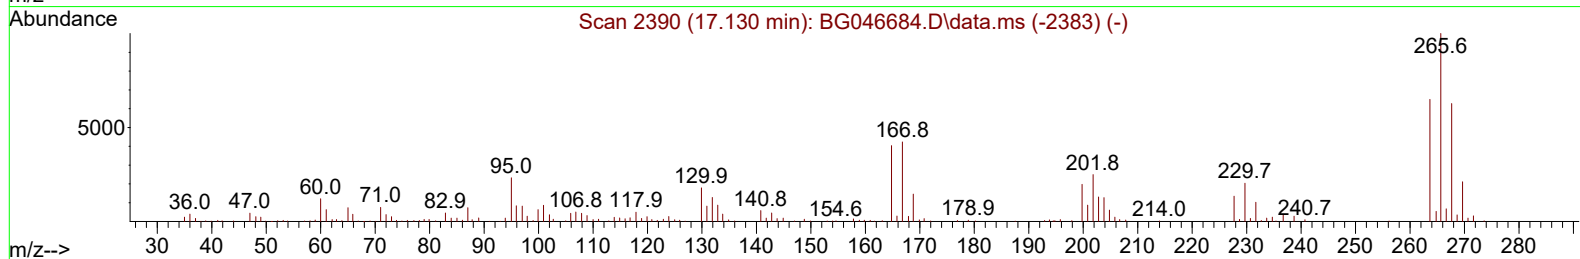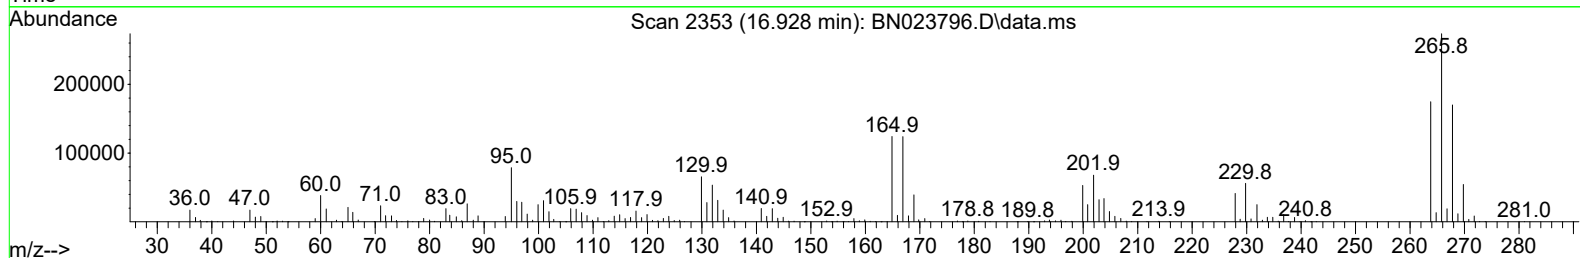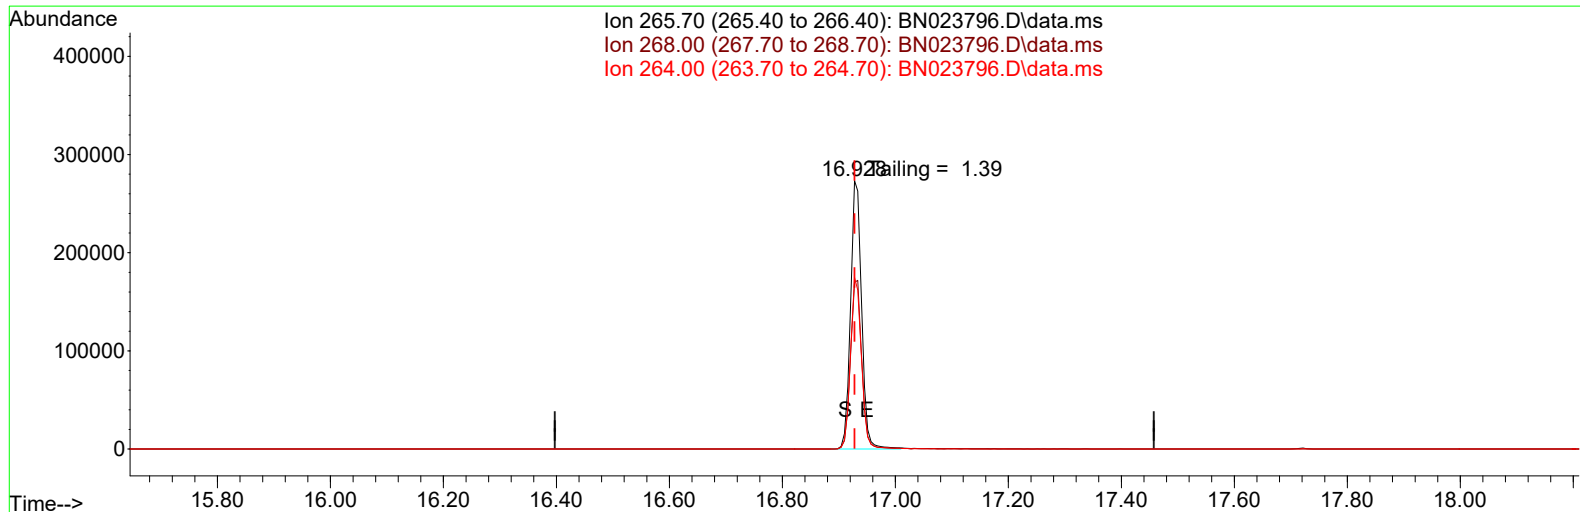

TIC: BN023796.D\data.ms

(70) Pentachlorophenol (C)

16.928min (0.000) 21575.66 ng




response 374198

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.15
264.00	61.60	63.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012623\
Data File : BN023796.D
Acq On : 25 Jan 2023 16:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 26 03:20:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 26 03:20:25 2023
Response via : Initial Calibration

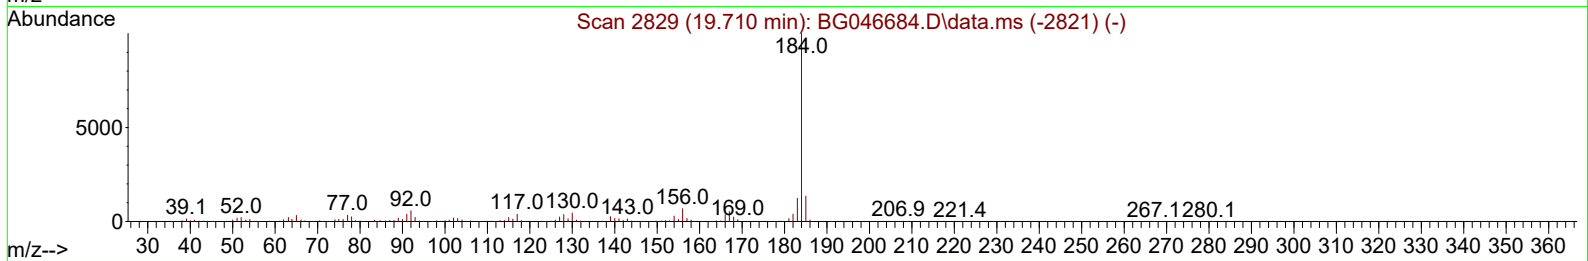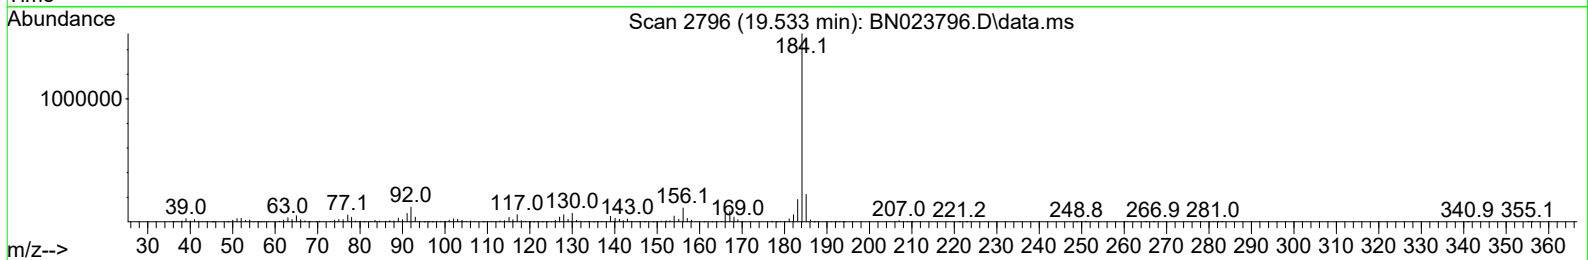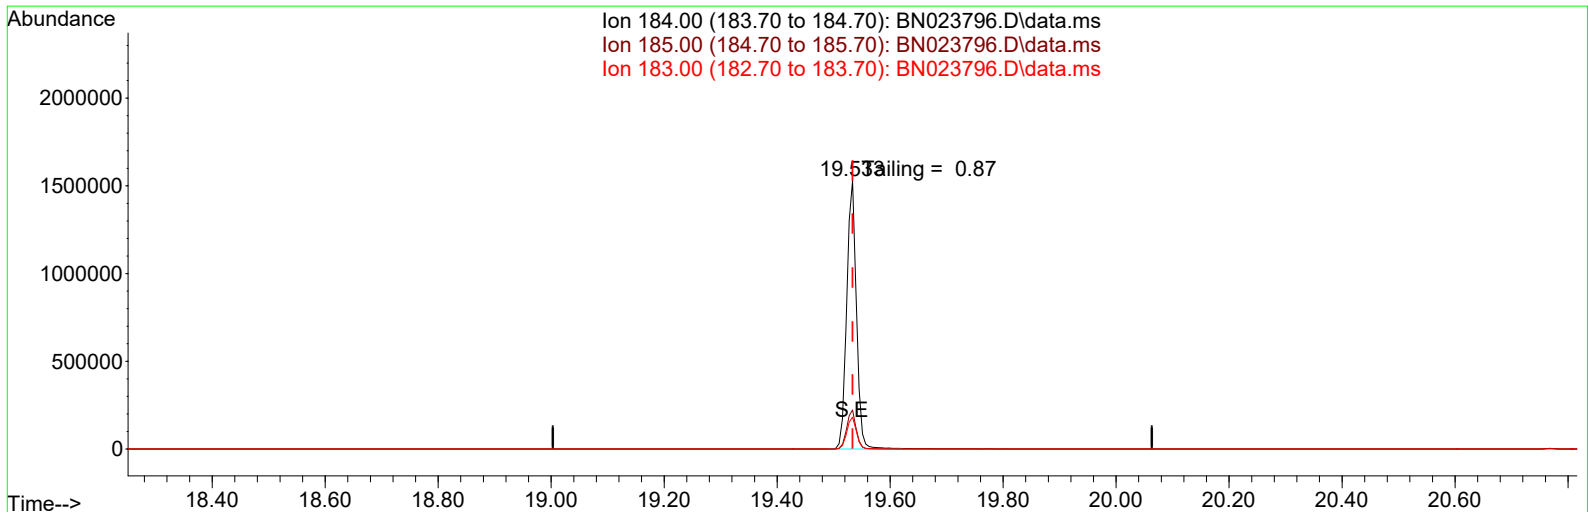

TIC: BN023796.D\data.ms

(77) Benzidine

19.533min (0.000) 0.00 ng

response 1829857

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.58
183.00	13.20	11.86
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/26/2023	BNA_N	<u>BN023796.D</u>
Compound Name	Response	Retention Time
DDT	918711	20.769
DDD	20807	20.322
DDE	1245	19.816
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
22052	940763	2.34

Instrument :
BNA_N
ClientSampleId :
DFTPP