
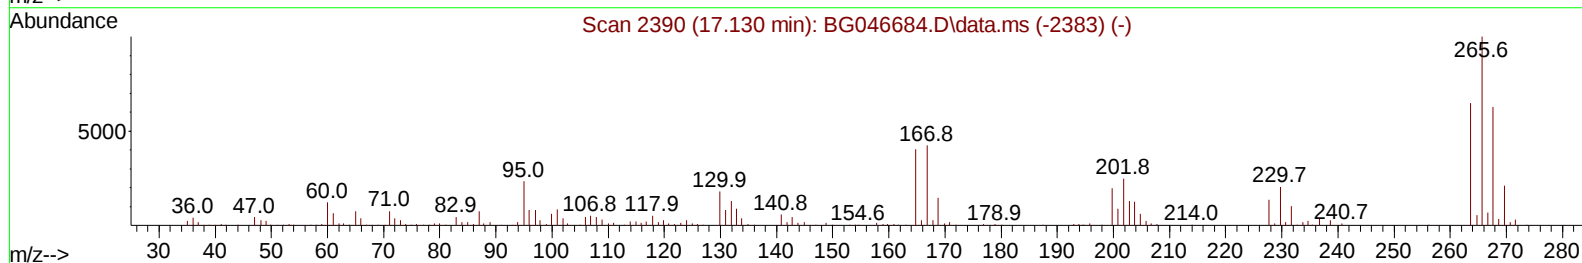
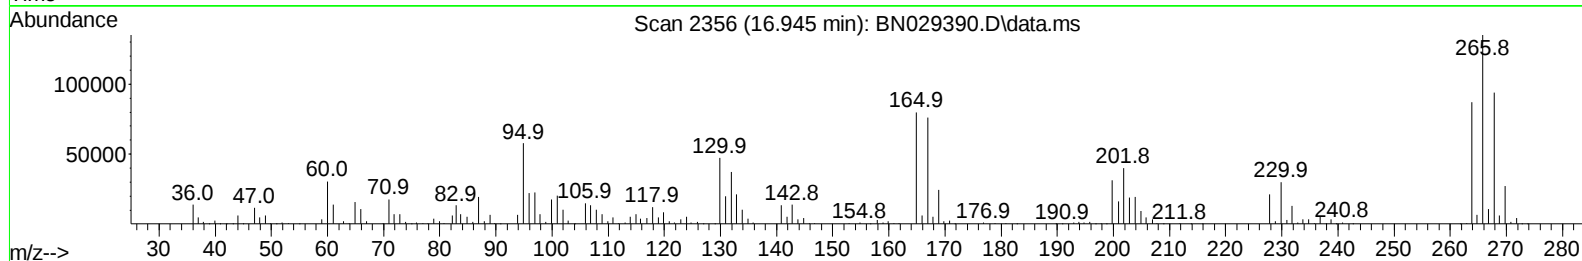


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012624\
Data File : BN029390.D
Acq On : 26 Jan 2024 09:55
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 27 06:30:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 06:30:17 2024
Response via : Initial Calibration

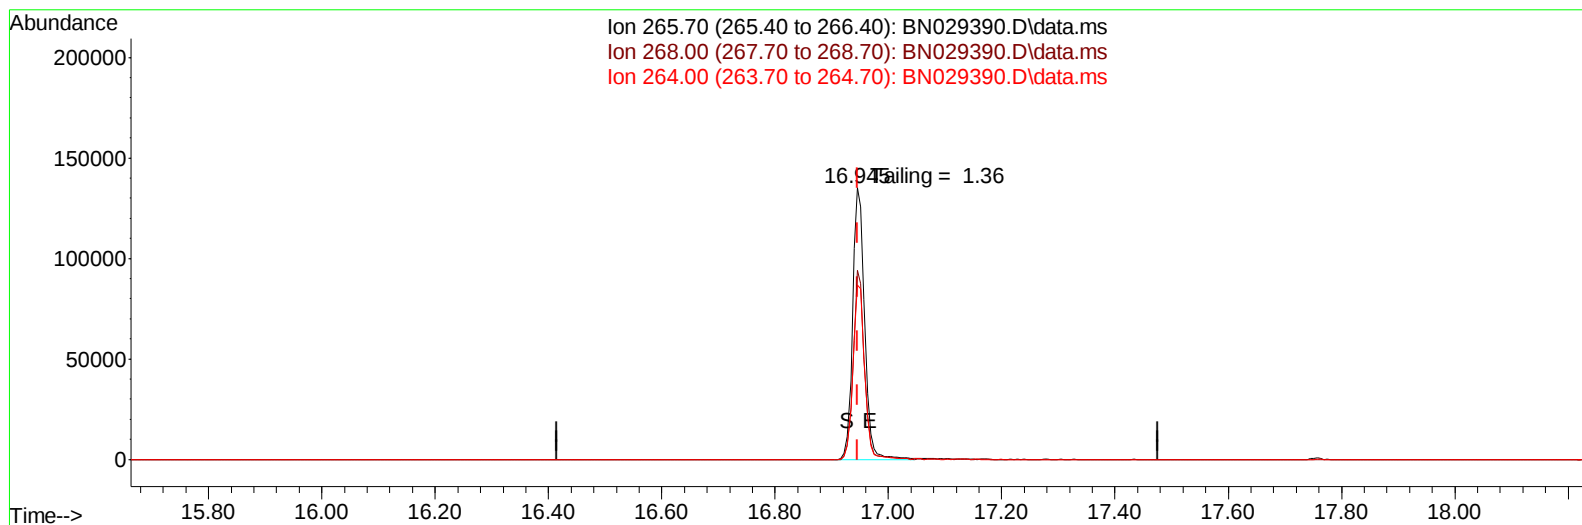




TIC: BN029390.D\data.ms

(70) Pentachlorophenol (C)**16.945min (0.000) 17638.07 ng****response 199462**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	69.62
264.00	61.60	64.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012624\
Data File : BN029390.D
Acq On : 26 Jan 2024 09:55
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 27 06:30:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 06:30:17 2024
Response via : Initial Calibration

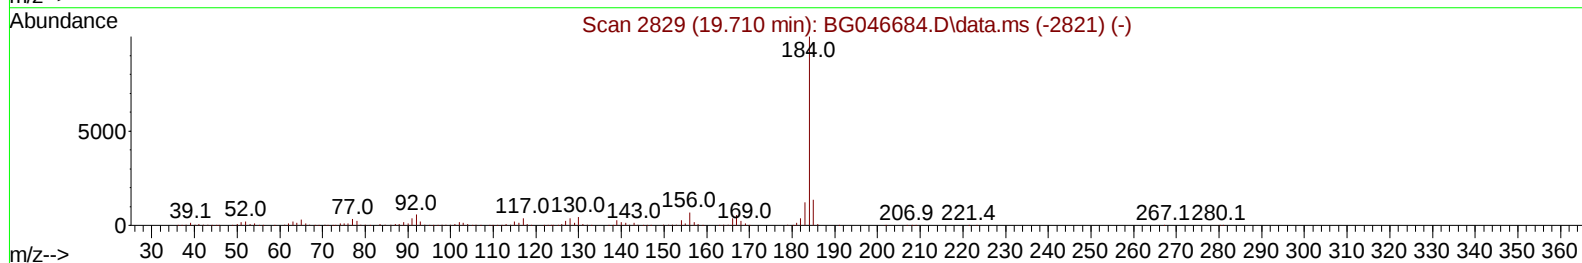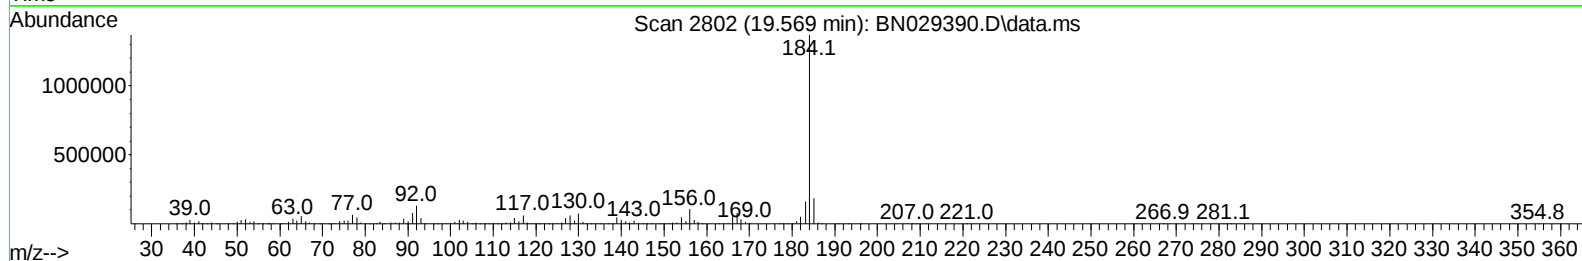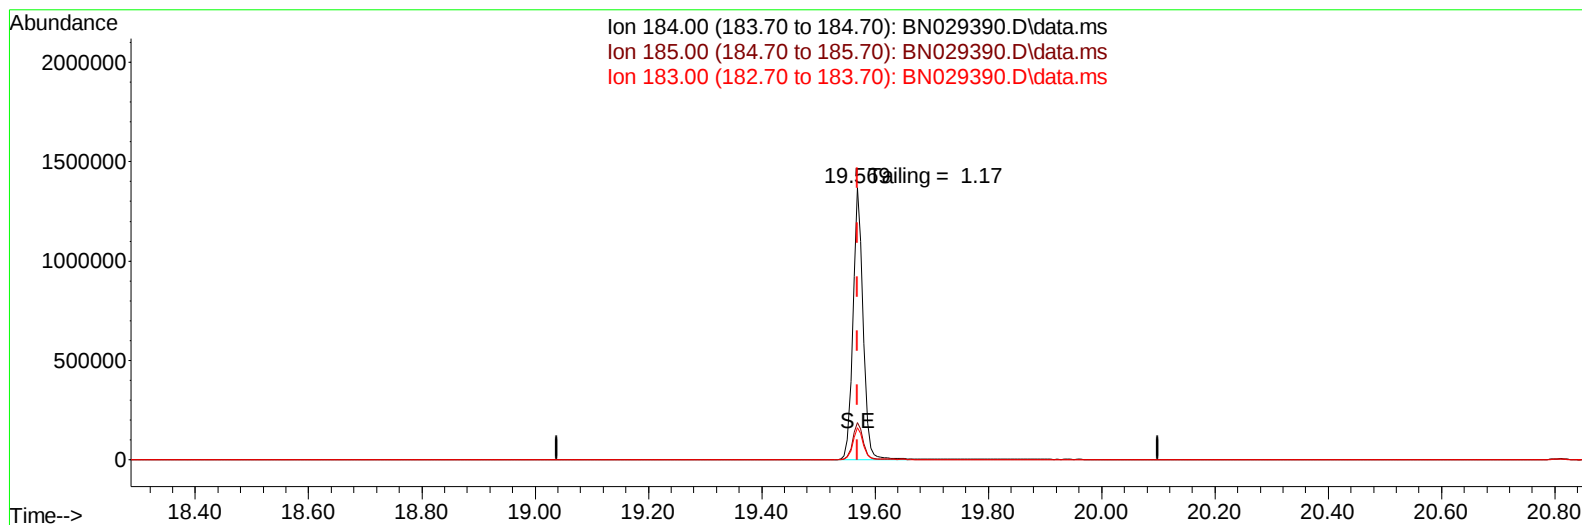

TIC: BN029390.D\data.ms

(77) Benzidine

19.569min (0.000) 0.00 ng

response 1714499

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.63
183.00	13.20	11.82
0.00	0.00	0.00