


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012624\
Data File : BN029390.D
Acq On : 26 Jan 2024 09:55
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN012524.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jan 26 01:42:55 2024

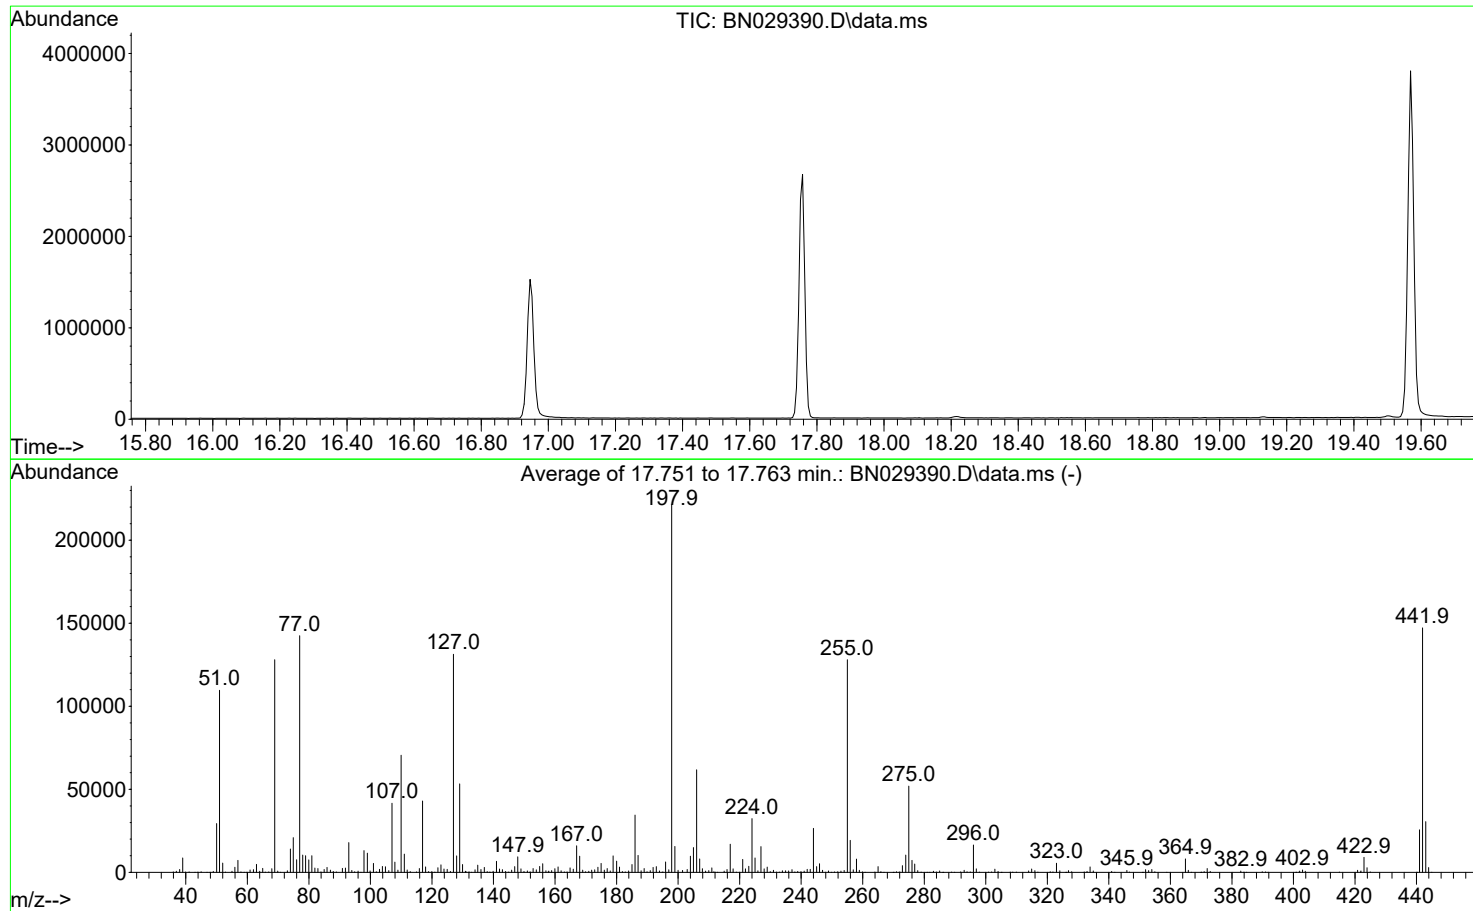

AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.5	109655	PASS
68	69	0.00	2	1.7	2226	PASS
69	198	0.00	100	57.8	128075	PASS
70	69	0.00	2	0.6	780	PASS
127	198	10	80	59.3	131333	PASS
197	198	0.00	2	0.7	1599	PASS
198	198	100	100	100.0	221525	PASS
199	198	5	9	7.0	15598	PASS
275	198	10	60	23.4	51896	PASS
365	198	1	100	3.7	8094	PASS
441	198	0.01	100	11.6	25640	PASS
442	442	50	100	100.0	147285	PASS
443	442	15	24	20.7	30507	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/26/2024	BNA_N	<u>BN029390.D</u>
Compound Name	Response	Retention Time
DDT	777767	20.81
DDD	14350	20.363
DDE	299	19.857
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14649	792416	1.85

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012624\
Data File : BN029390.D
Acq On : 26 Jan 2024 09:55
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 27 06:30:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 06:30:17 2024
Response via : Initial Calibration

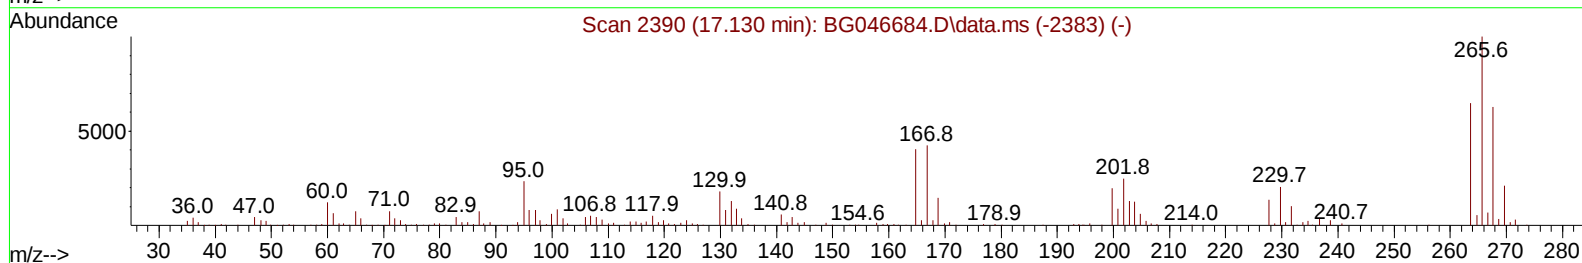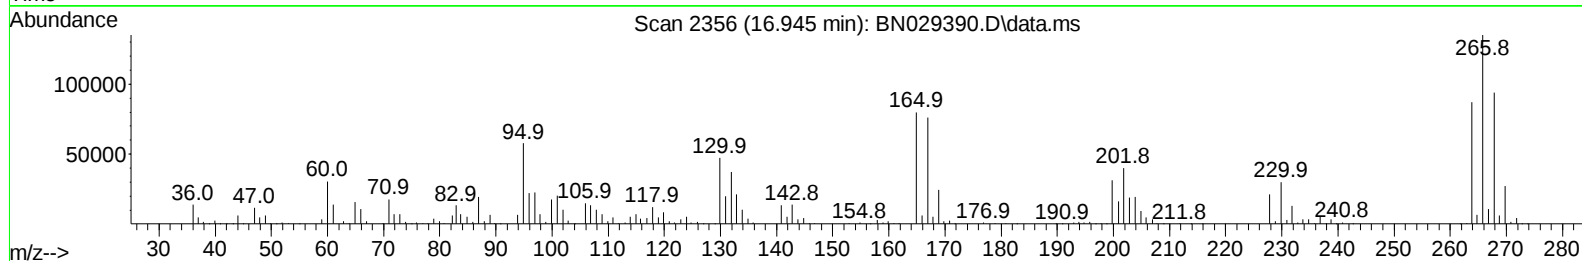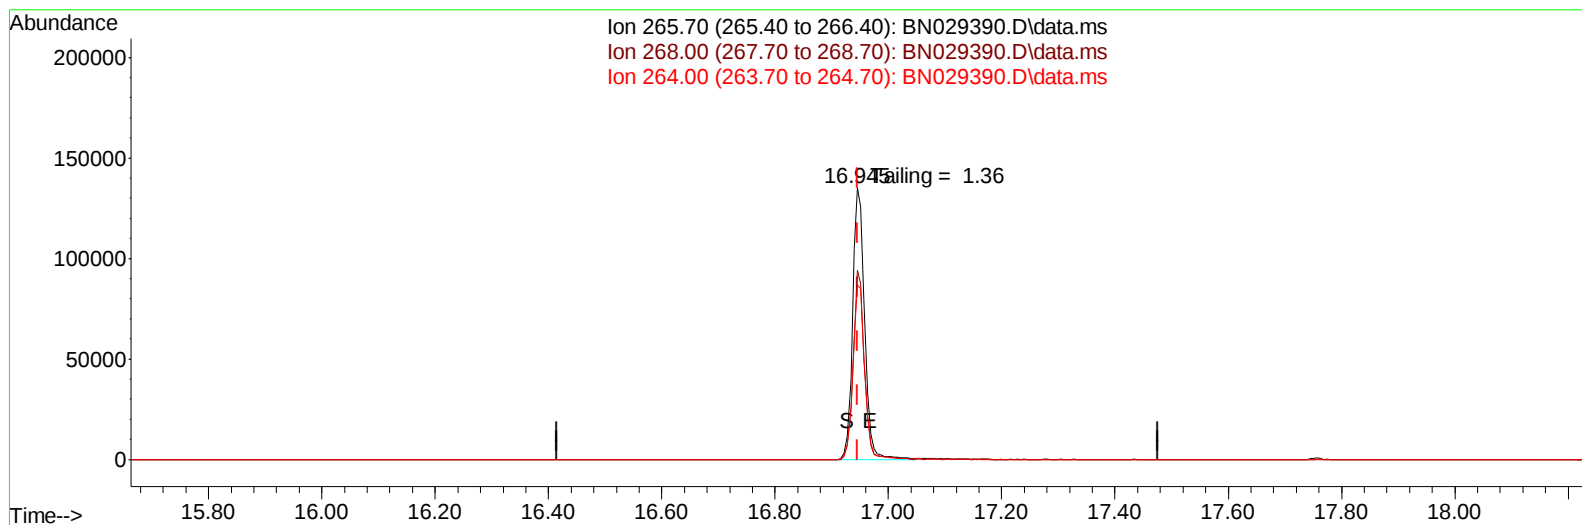

TIC: BN029390.D\data.ms

(70) Pentachlorophenol (C)

16.945min (0.000) 17638.07 ng




response 199462

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	69.62
264.00	61.60	64.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012624\
Data File : BN029390.D
Acq On : 26 Jan 2024 09:55
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 27 06:30:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 27 06:30:17 2024
Response via : Initial Calibration

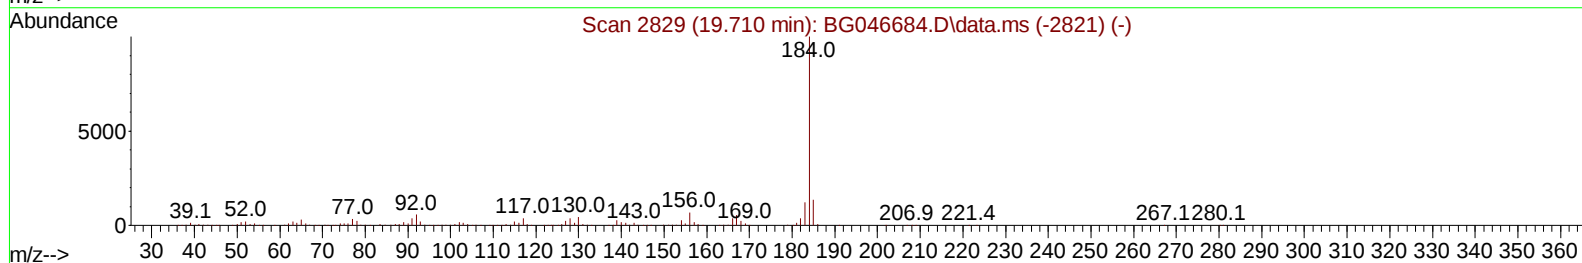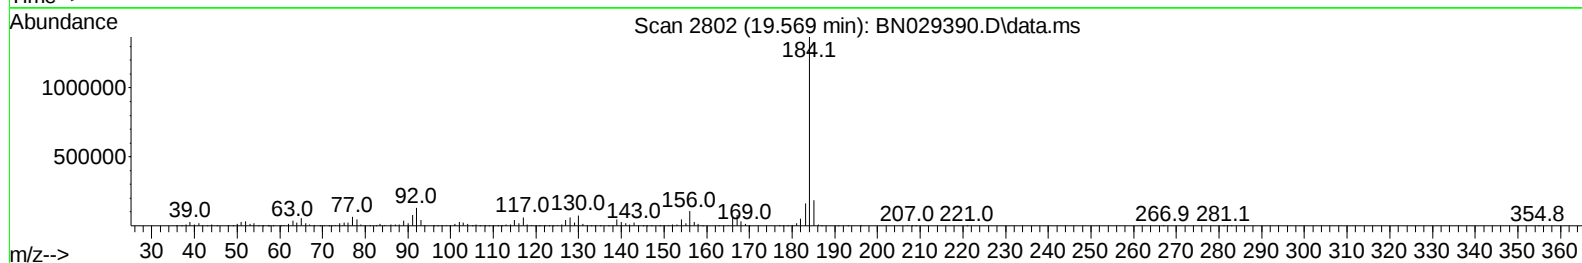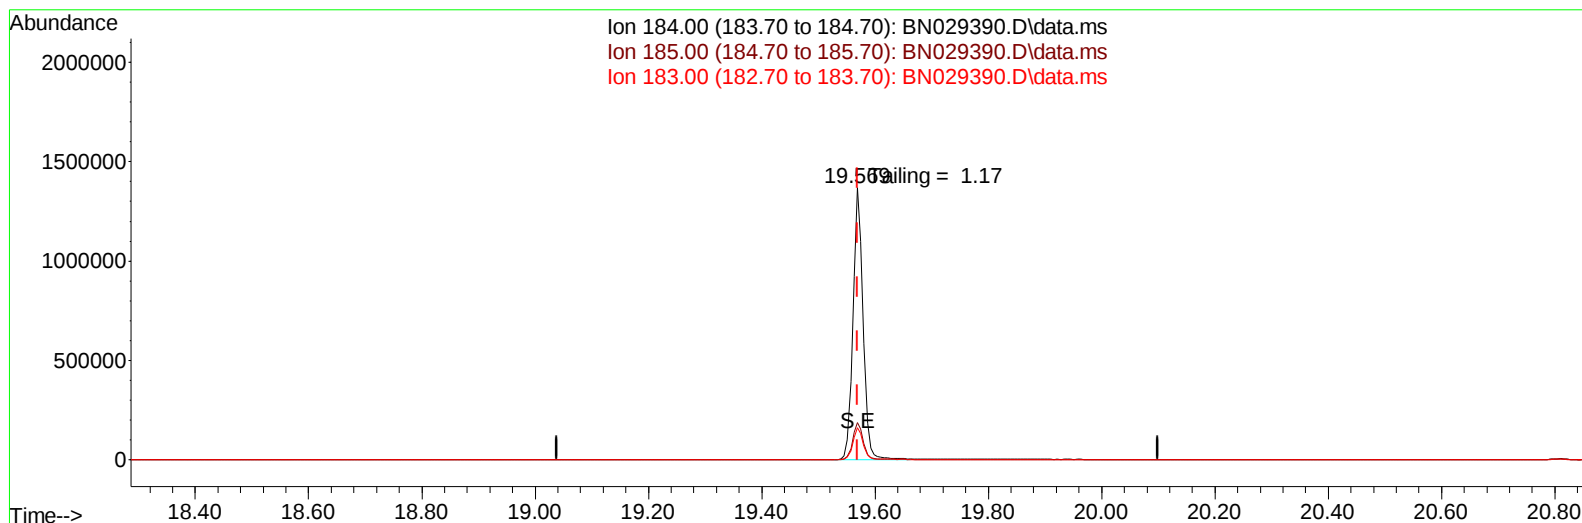

TIC: BN029390.D\data.ms

(77) Benzidine

19.569min (0.000) 0.00 ng

response 1714499

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.63
183.00	13.20	11.82
0.00	0.00	0.00