

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN012721\
 Data File : BN013513.D
 Acq On : 27 Jan 2021 19:32
 Operator : CG/JU
 Sample : M1099-17DL 5X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F1C13DL

Quant Time: Jan 27 23:45:02 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN012721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 27 23:35:53 2021
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	5108	0.40	ng/ul	0.00
2) Naphthalene-d8	10.33	136	19507	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.20	164	10728	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.95	188	22677	0.40	ng/ul	0.00
16) Chrysene-d12	21.15	240	20410	0.40	ng/ul	0.00
20) Perylene-d12	23.32	264	19463	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.92	152	2296	0.08	ng/ul	0.00
14) Fluoranthene-d10	18.99	212	4582	0.08	ng/ul	0.00
Target Compounds				Ovalue		
3) Naphthalene	10.38	128	5864	0.104	ng/ul#	93
5) 2-Methylnaphthalene	12.00	142	2054	0.057	ng/ul	97
7) Acenaphthylene	13.92	152	17311	0.392	ng/ul	99
8) Acenaphthene	14.26	153	6847	0.174	ng/ul	99
9) Fluorene	15.25	166	7011	0.161	ng/ul	99
12) Phenanthrene	16.99	178	33840	0.456	ng/ul	99
13) Anthracene	17.08	178	6160	0.101	ng/ul	96
15) Fluoranthene	19.01	202	26090	0.322	ng/ul	98
17) Pyrene	19.38	202	55190	0.661	ng/ul	98
18) Benzo(a)anthracene	21.14	228	2305	0.034	ng/ul#	1
19) Chrysene	21.19	228	3786	0.045	ng/ul#	89
21) Benzo(b)fluoranthene	22.68	252	4041	0.049	ng/ul#	35
22) Benzo(k)fluoranthene	22.68	252	4041	0.046	ng/ul#	37
23) Benzo(a)pyrene	23.23	252	3126	0.045	ng/ul#	52
24) Indeno(1,2,3-cd)pyrene	25.47	276	2687	0.029	ng/ul#	100
26) Benzo(a,h,i)perylene	26.13	276	6852	0.084	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN012721\
Data File : BN013513.D
Acq On : 27 Jan 2021 19:32
Operator : CG/JU
Sample : M1099-17DL 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F1C13DL

Quant Time: Jan 27 23:45:02 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 27 23:35:53 2021
Response via : Initial Calibration

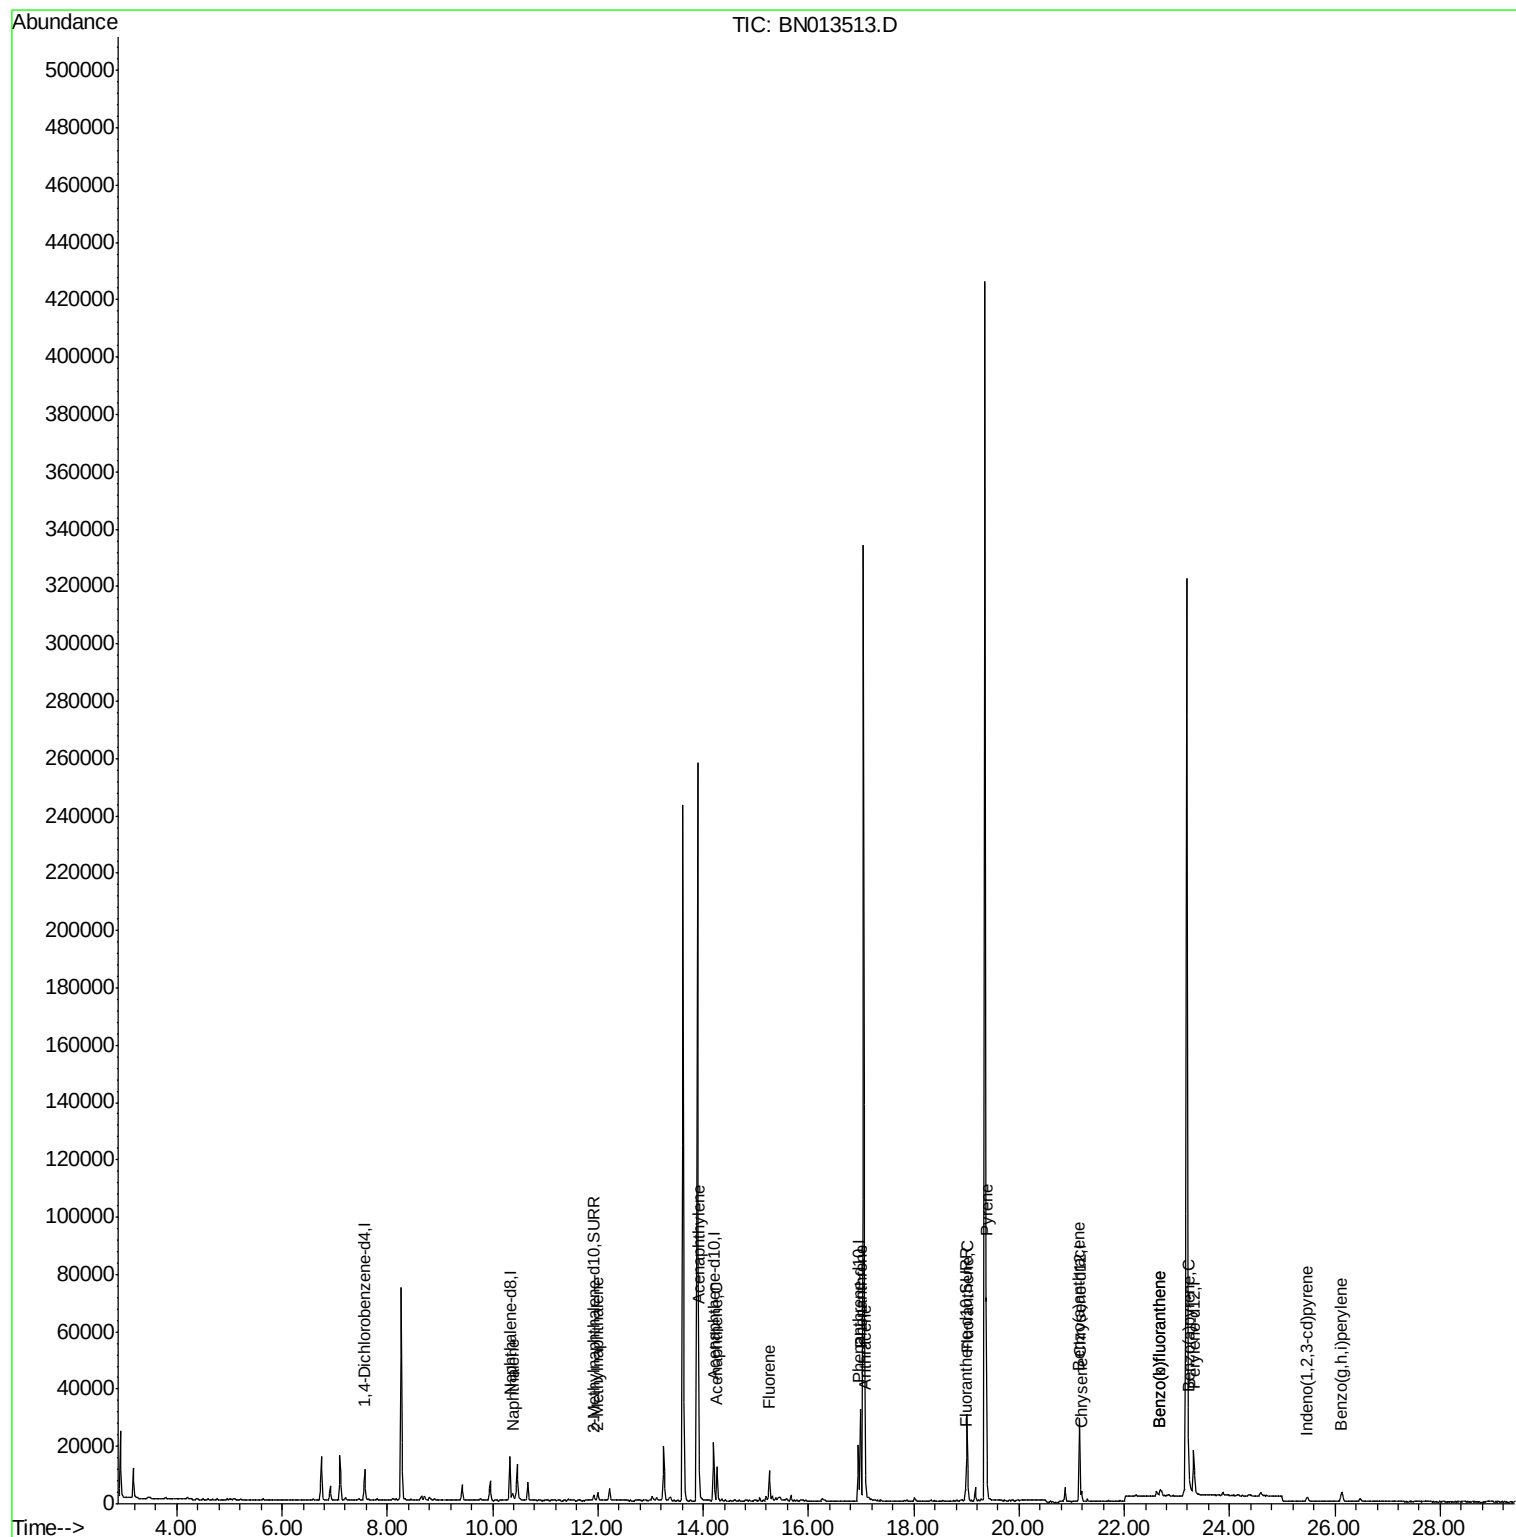

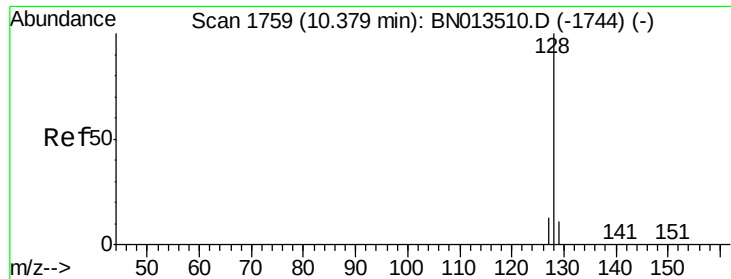

#3

Naphthalene

Concen: 0.104 ng/ul

RT: 10.38 min Scan# 1759

Delta R.T. -0.00 min

Lab File: BN013513.D

Acq: 27 Jan 2021 19:32

Instrument :

BNA_N

ClientSampleId :

F1C13DL


Tot Ion:128 Resp: 5864

Ion Ratio Lower Upper

128 100

129 15.0 9.0 13.6#




127 15.4 10.6 15.8



Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

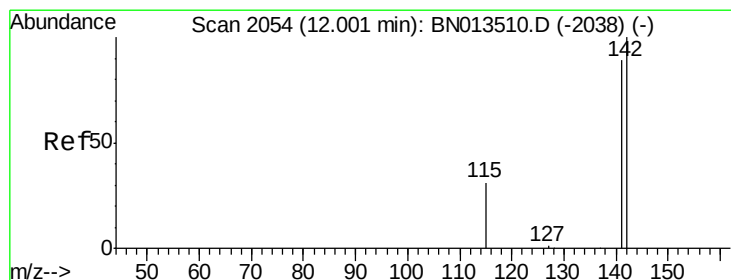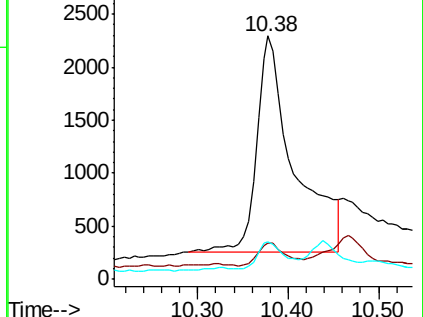

#5

2-Methylnaphthalene

Concen: 0.057 ng/ul

RT: 12.00 min Scan# 2054

Delta R.T. -0.00 min

Lab File: BN013513.D


Acq: 27 Jan 2021 19:32

Tgt Ion:142 Resp: 2054

Ion Ratio Lower Upper



142 100


141 85.2 70.6 106.0



Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

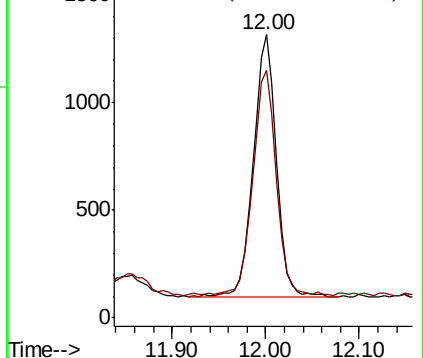



#7

Acenaphthylene

Concen: 0.392 ng/ul

RT: 13.92 min Scan# 2420

Delta R.T. -0.00 min

Lab File: BN013513.D

Acq: 27 Jan 2021 19:32

Instrument :

BNA_N

ClientSampleId :

F1C13DL


Tot Ion:152 Resp: 17311

Ion Ratio Lower Upper




152 100

151 19.8 16.1 24.1

153 14.4 10.7 16.1



Abundance Ion 152.00 (151.70 to 152.70): E
Ion 151.00 (150.70 to 151.70): E
Ion 153.00 (152.70 to 153.70): E

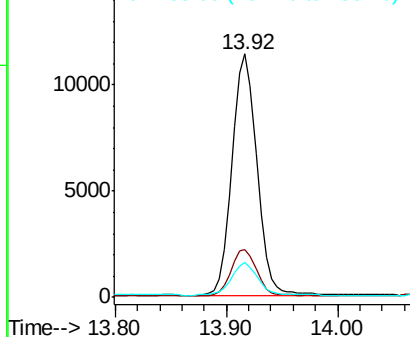

#8

Acenaphthene

Concen: 0.174 ng/ul

RT: 14.26 min Scan# 2495

Delta R.T. -0.00 min

Lab File: BN013513.D

Acq: 27 Jan 2021 19:32


Tgt Ion:153 Resp: 6847

Ion Ratio Lower Upper



153 100


152 48.2 39.5 59.3

154 87.3 70.6 105.8



Abundance Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E
Ion 154.00 (153.70 to 154.70): E

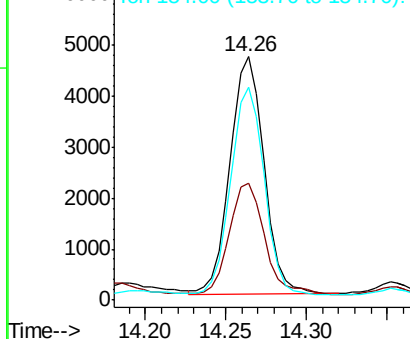



#9

Fluorene

Concen: 0.161 ng/ul

RT: 15.25 min Scan# 2709

Delta R.T. -0.00 min

Lab File: BN013513.D

Acq: 27 Jan 2021 19:32

Instrument :

BNA_N

ClientSampleId :

F1C13DL


Tot Ion:166 Resp: 7011

Ion Ratio Lower Upper

166 100

165 99.2 78.7 118.1




167 16.6 11.3 16.9



Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

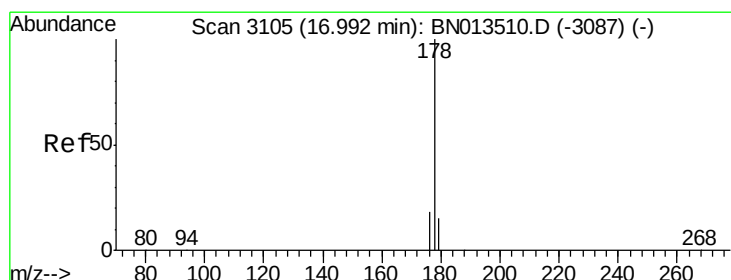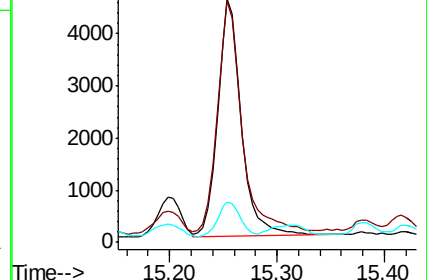

#12

Phenanthrene

Concen: 0.456 ng/ul

RT: 16.99 min Scan# 3105

Delta R.T. -0.00 min

Lab File: BN013513.D

Acq: 27 Jan 2021 19:32


Tgt Ion:178 Resp: 33840

Ion Ratio Lower Upper

178 100

179 15.5 12.5 18.7



176 19.0 15.6 23.4




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

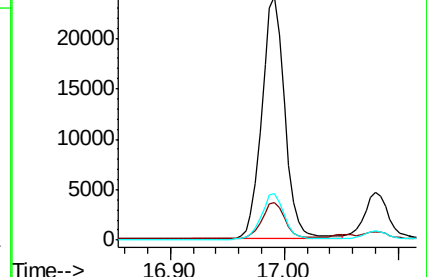

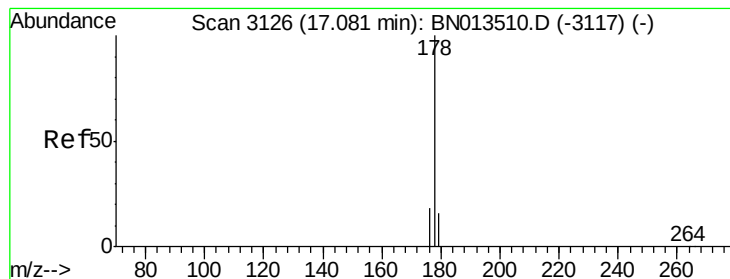

#13

Anthracene

Concen: 0.101 ng/ul

RT: 17.08 min Scan# 3126

Delta R.T. -0.00 min

Lab File: BN013513.D

Acq: 27 Jan 2021 19:32

Instrument :

BNA_N

ClientSampleId :

F1C13DL


Tot Ion:178 Resp: 6160

Ion Ratio Lower Upper

178 100

179 18.1 12.6 19.0




176 19.6 15.0 22.4

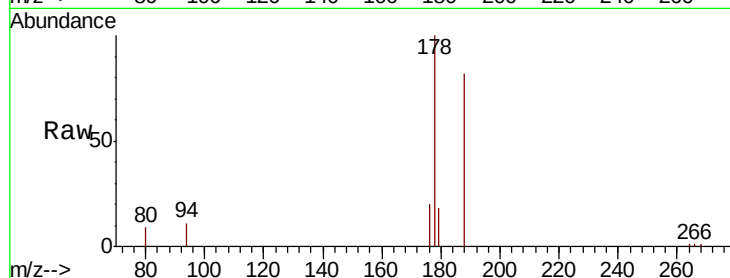

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

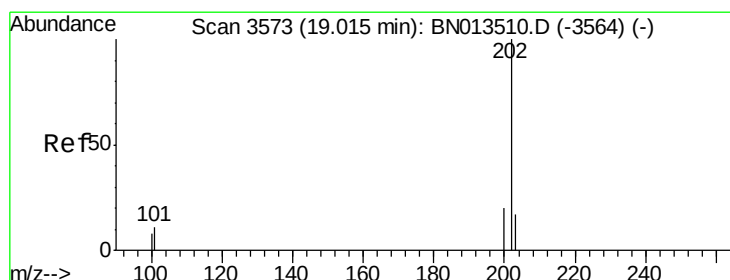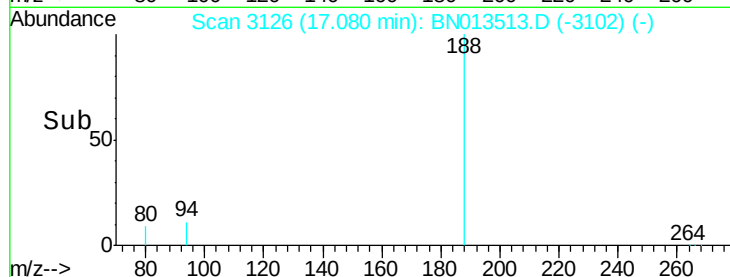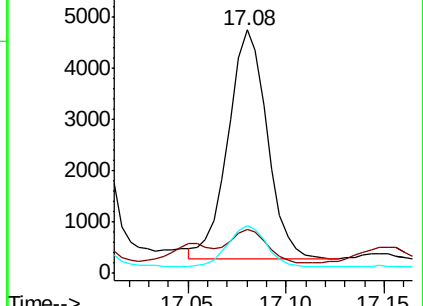

#15

Fluoranthene

Concen: 0.322 ng/ul

RT: 19.01 min Scan# 3573

Delta R.T. -0.00 min

Lab File: BN013513.D

Acq: 27 Jan 2021 19:32


Tgt Ion:202 Resp: 26090

Ion Ratio Lower Upper

202 100

101 12.2 0.0 31.6



100 9.2 0.0 28.5

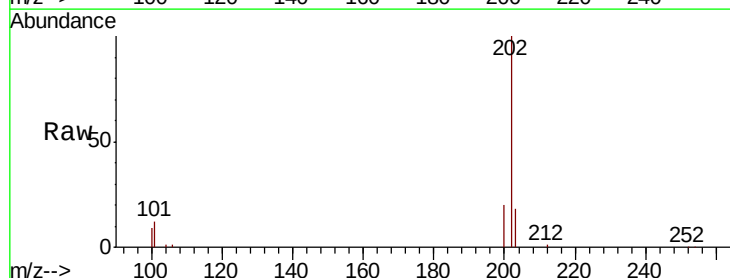


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

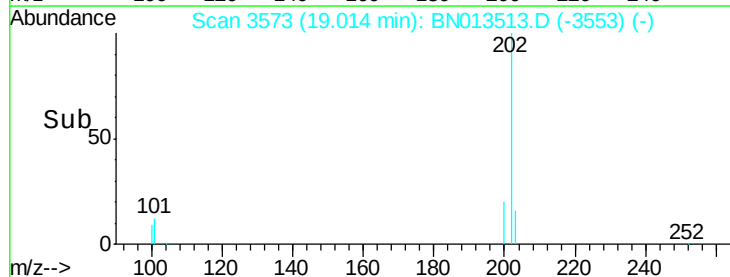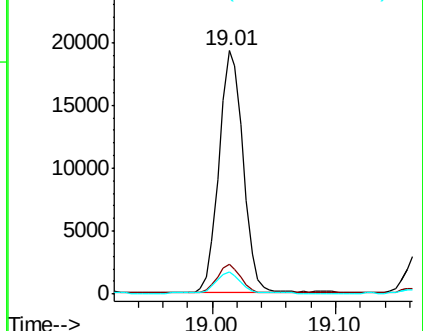

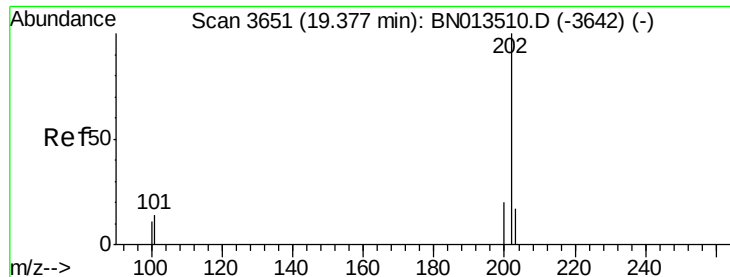

#17

Pvrene

Concen: 0.661 ng/ul

RT: 19.38 min Scan# 3652

Delta R.T. -0.00 min

Lab File: BN013513.D

Acq: 27 Jan 2021 19:32

Instrument :

BNA_N

ClientSampleId :

F1C13DL


Tot Ion:202 Resp: 55190

Ion Ratio Lower Upper

202 100

101 13.0 11.2 16.8




100 10.4 9.0 13.4

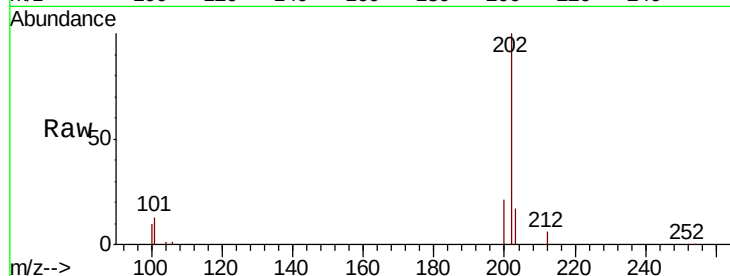

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

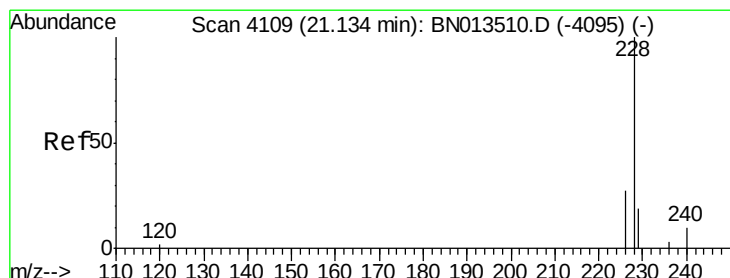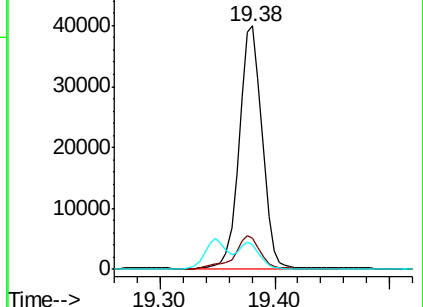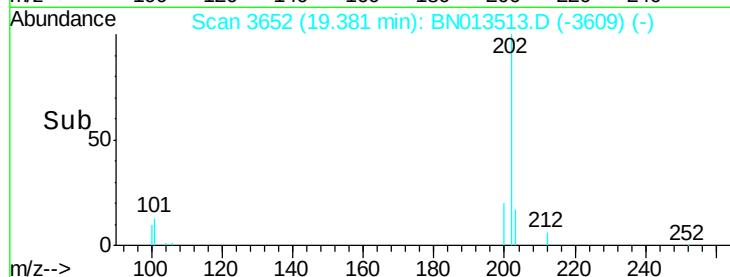

#18

Benzo(a)anthracene

Concen: 0.034 ng/ul

RT: 21.14 min Scan# 4110

Delta R.T. -0.00 min

Lab File: BN013513.D

Acq: 27 Jan 2021 19:32


Tgt Ion:228 Resp: 2305

Ion Ratio Lower Upper

228 100

229 26.2 15.6 23.4#



226 165.7 21.9 32.9#

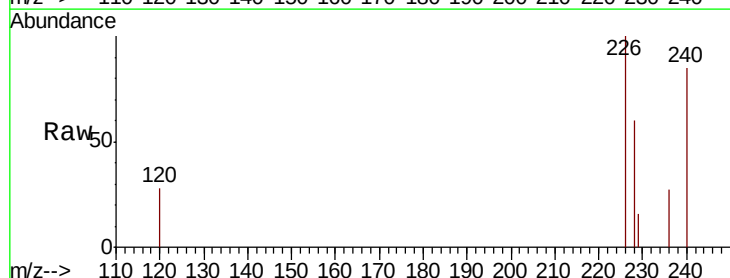


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

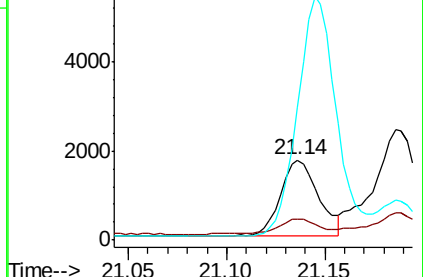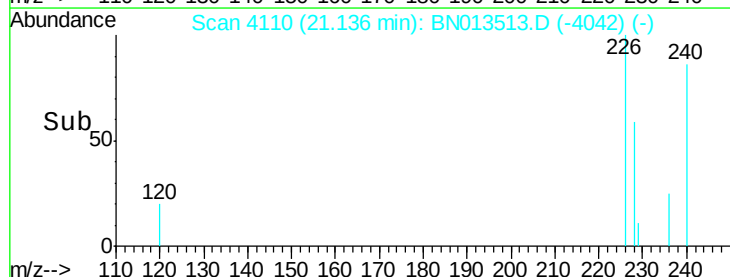

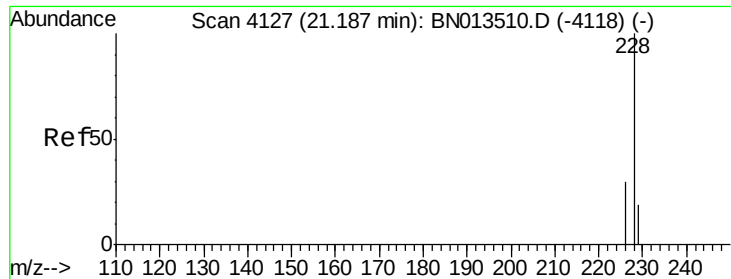

#19

Chrysene

Concen: 0.045 ng/ul

RT: 21.19 min Scan# 4127

Delta R.T. -0.00 min

Lab File: BN013513.D

Acq: 27 Jan 2021 19:32

Instrument :

BNA_N

ClientSampleId :

F1C13DL


Tot Ion:228 Resp: 3786

Ion Ratio Lower Upper

228 100

226 36.2 24.0 36.0#




229 24.9 15.8 23.8#

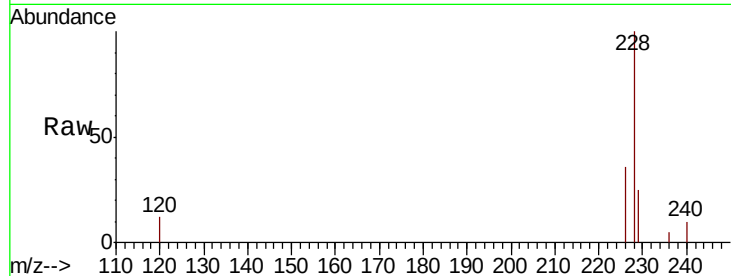

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

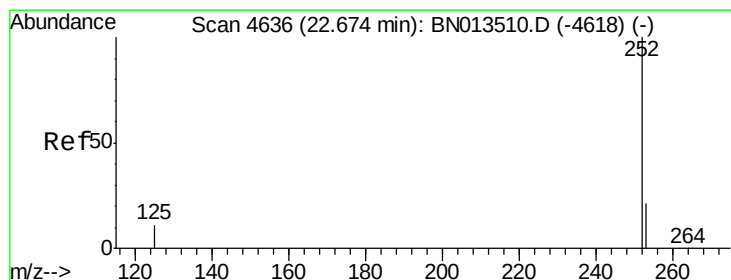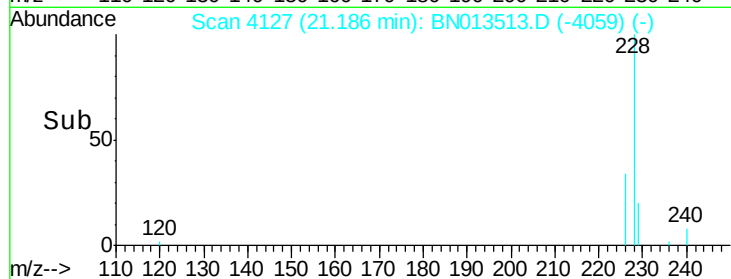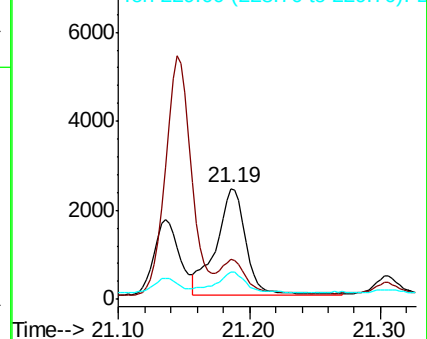

#21

Benzo(b)fluoranthene

Concen: 0.049 ng/ul

RT: 22.68 min Scan# 4637

Delta R.T. 0.00 min

Lab File: BN013513.D

Acq: 27 Jan 2021 19:32


Tgt Ion:252 Resp: 4041

Ion Ratio Lower Upper

252 100

253 50.7 0.0 47.4#



125 46.1 0.0 26.8#




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

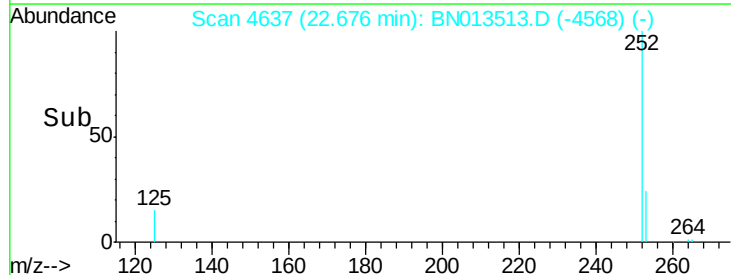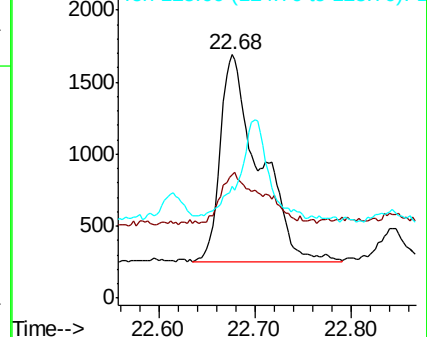

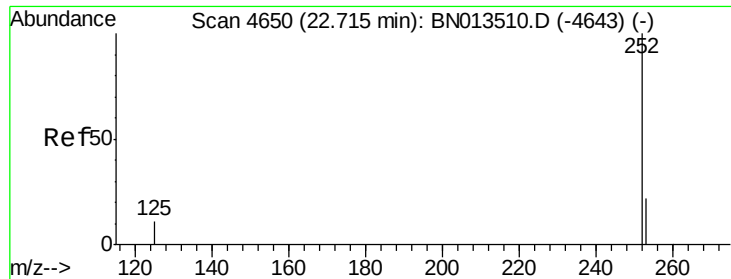

#22

Benzo(k)fluoranthene

Concen: 0.046 ng/ul

RT: 22.68 min Scan# 4637

Delta R.T. -0.04 min

Lab File: BN013513.D

Acq: 27 Jan 2021 19:32

Instrument :

BNA_N

ClientSampleId :

F1C13DL


Tot Ion:252 Resp: 4041

Ion Ratio Lower Upper

252 100

253 50.7 19.2 28.8#




125 46.1 11.4 17.2#

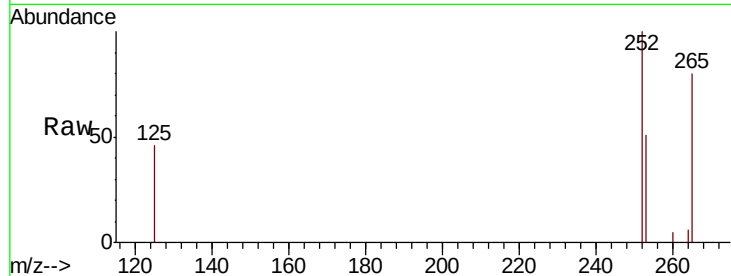

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

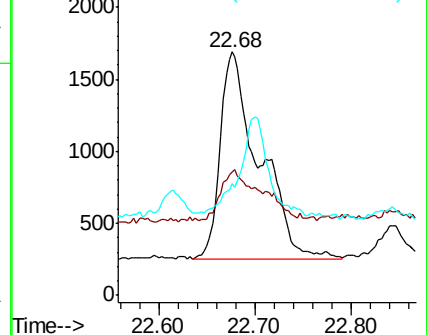

#23

Benzo(a)pyrene

Concen: 0.045 ng/ul

RT: 23.23 min Scan# 4825

Delta R.T. -0.00 min

Lab File: BN013513.D

Acq: 27 Jan 2021 19:32


Tgt Ion:252 Resp: 3126

Ion Ratio Lower Upper

252 100

253 46.0 20.1 30.1#



125 40.9 13.1 19.7#




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

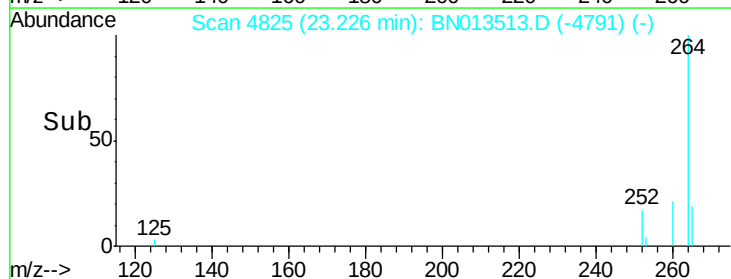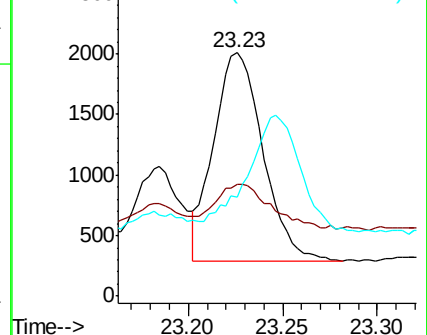




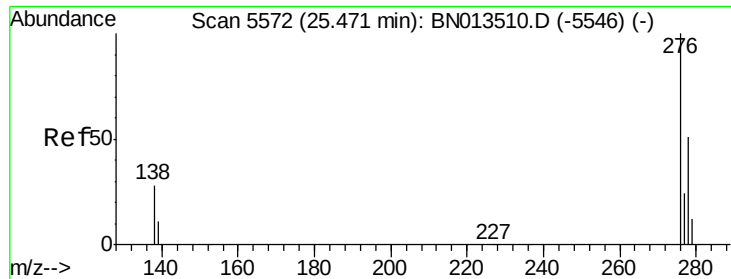


#24

Indeno(1,2,3-cd)pyrene
Concen: 0.029 ng/ul
RT: 25.47 min Scan# 5572
Delta R.T. -0.01 min
Lab File: BN013513.D
Acq: 27 Jan 2021 19:32

Instrument :
BNA_N
ClientSampleId :
F1C13DL

Tot Ion:276 Resp: 2687
Ion Ratio Lower Upper
276 100
138 23.3 0.0 0.0#
227 0.0 0.0 0.0

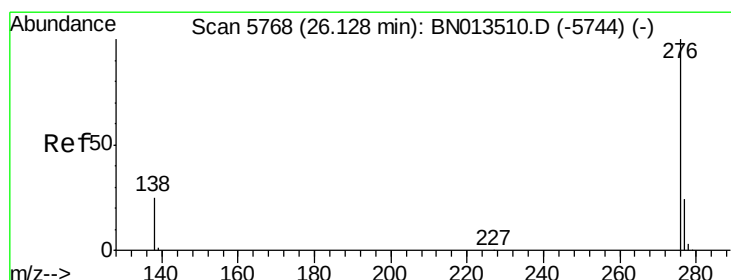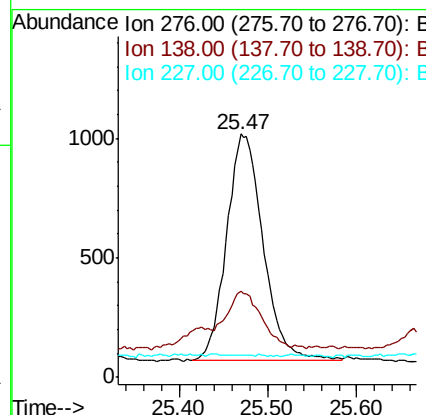

#26

Benzo(g,h,i)perylene
Concen: 0.084 ng/ul
RT: 26.13 min Scan# 5770
Delta R.T. 0.00 min
Lab File: BN013513.D
Acq: 27 Jan 2021 19:32

Tgt Ion:276 Resp: 6852
Ion Ratio Lower Upper
276 100
138 28.4 21.0 31.4
277 25.9 19.5 29.3

