


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN012721\
Data File : BN013500.D
Acq On : 27 Jan 2021 10:35
Operator : CG/JU
Sample : PB134140BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK40

Manual Integrations
APPROVED

mohammad
1/28/2021 11:43:52 AM

Quant Time: Jan 27 12:06:19 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 27 11:55:49 2021
Response via : Initial Calibration

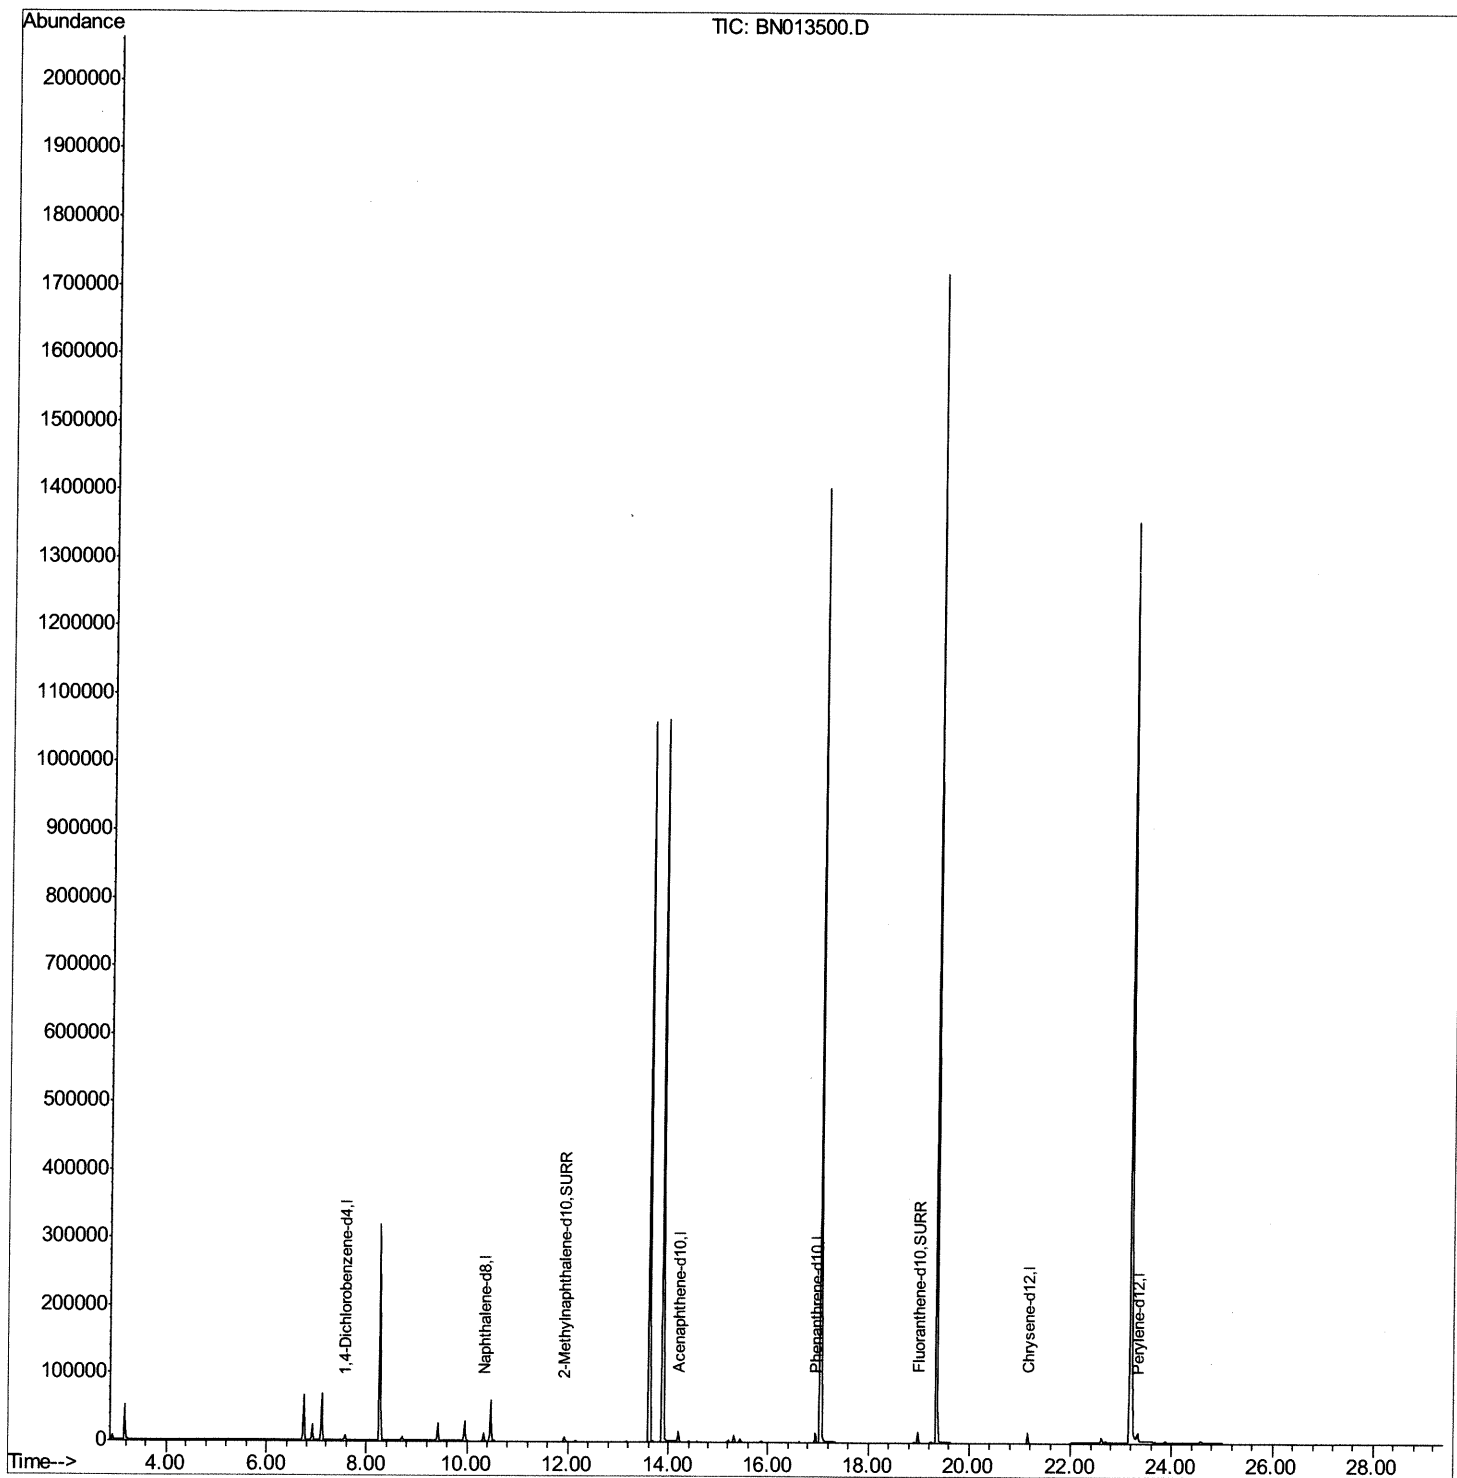


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN012721\
Data File : BN013500.D
Acq On : 27 Jan 2021 10:35
Operator : CG/JU
Sample : PB134140BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK40

Manual Integrations
APPROVED

mohammad
1/28/2021 11:43:52 AM

Quant Time: Jan 27 11:56:54 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 27 11:55:49 2021
Response via : Initial Calibration

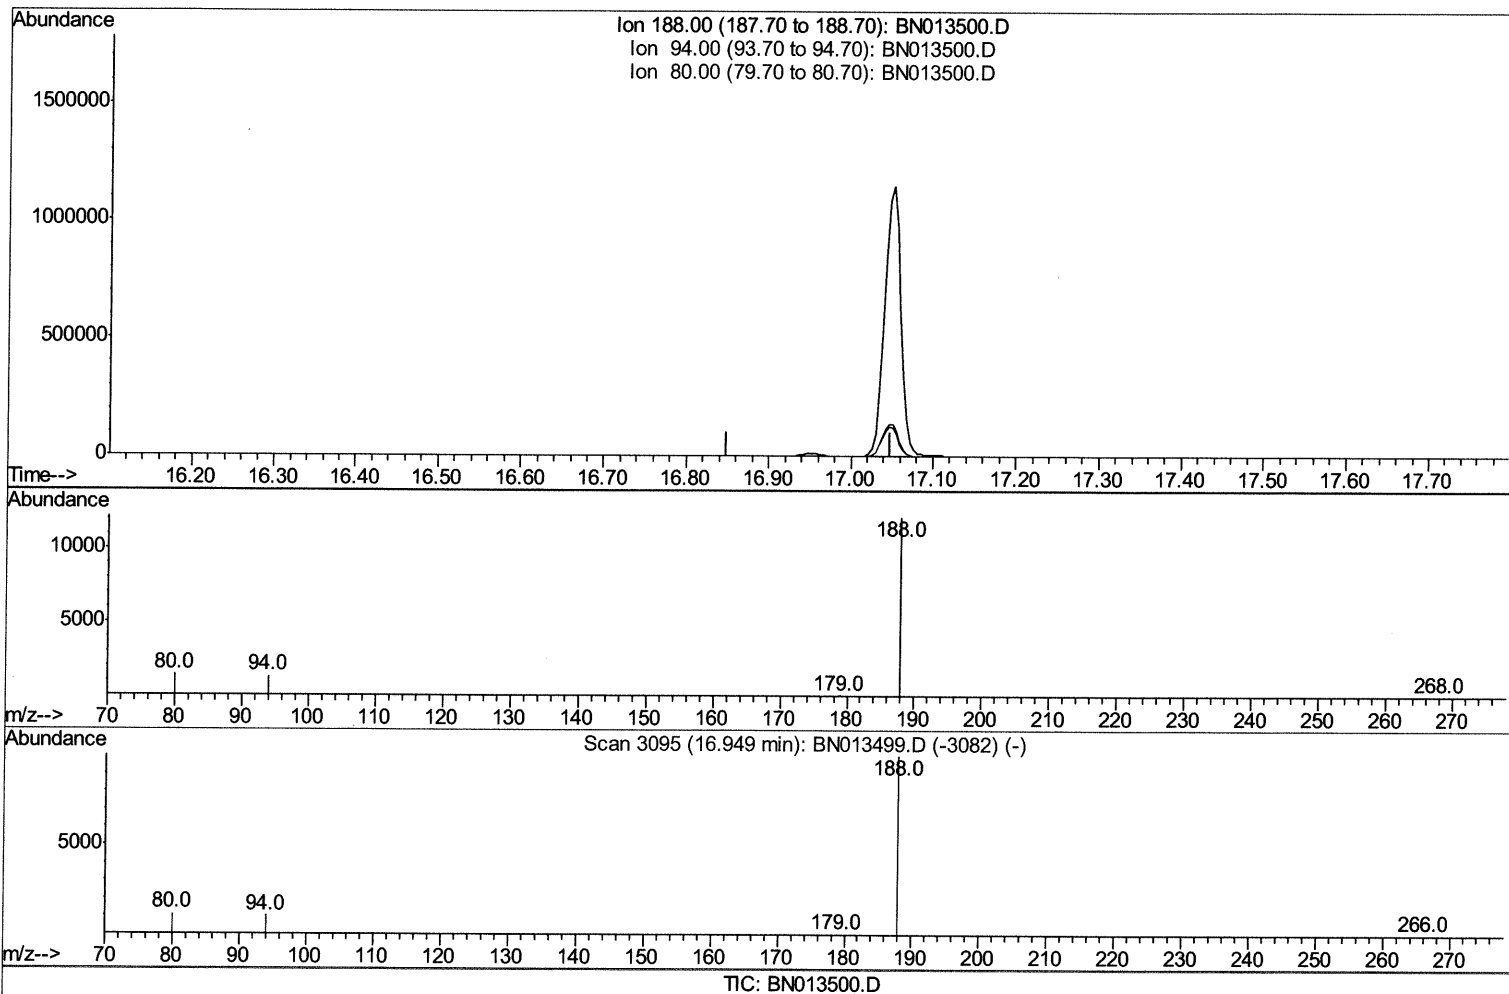

(10) Phenanthrene-d10 (I)

16.949min (-16.949) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	10.80	0.00#
80.00	11.50	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN012721\
Data File : BN013500.D
Acq On : 27 Jan 2021 10:35
Operator : CG/JU
Sample : PB134140BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK40

Manual Integrations
APPROVED

mohammad
1/28/2021 11:43:52 AM

Quant Time: Jan 27 11:56:54 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 27 11:55:49 2021
Response via : Initial Calibration

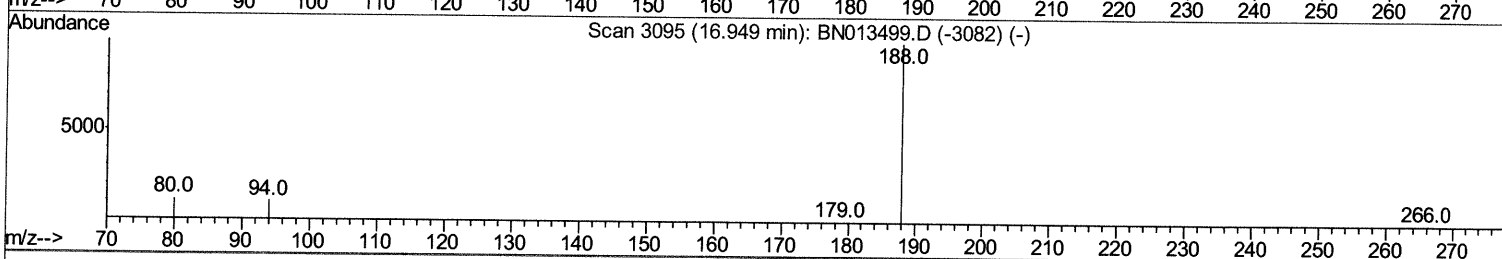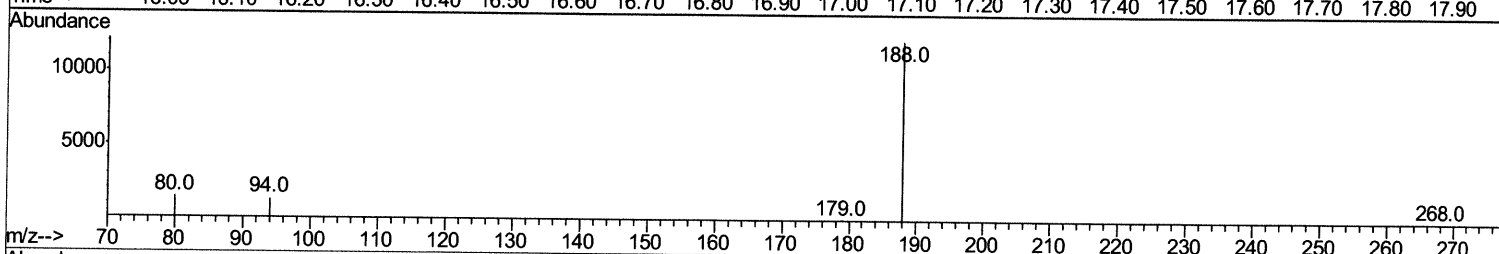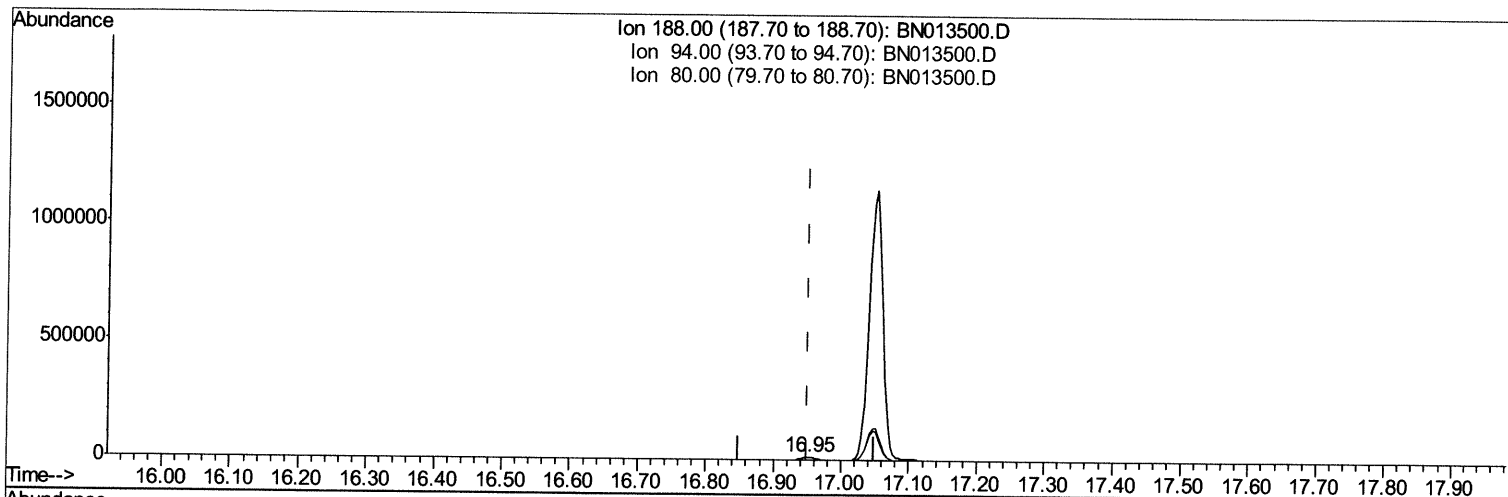

TIC: BN013500.D

(10) Phenanthrene-d10 (I)

16.949min (-0.000) 0.40ng/ul m 01/28/21JU

response 17037

Ion	Exp%	Act%
188.00	100	100
94.00	10.80	10.86
80.00	11.50	11.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN012721\
Data File : BN013500.D
Acq On : 27 Jan 2021 10:35
Operator : CG/JU
Sample : PB134140BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK40

Manual Integrations
APPROVED

mohammad
1/28/2021 11:43:52 AM

Quant Time: Jan 27 12:06:19 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 27 11:55:49 2021
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	4149	0.40	ng/ul	0.00
2) Naphthalene-d8	10.33	136	15202	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.20	164	8556	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.95	188	17037m >	0.40	ng/ul >	0.00
16) Chrysene-d12	21.15	240	14414	0.40	ng/ul	0.00
20) Perylene-d12	23.32	264	16474	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.92	152	8957	0.39	ng/ul	0.00
14) Fluoranthene-d10	18.99	212	17715	0.39	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed