
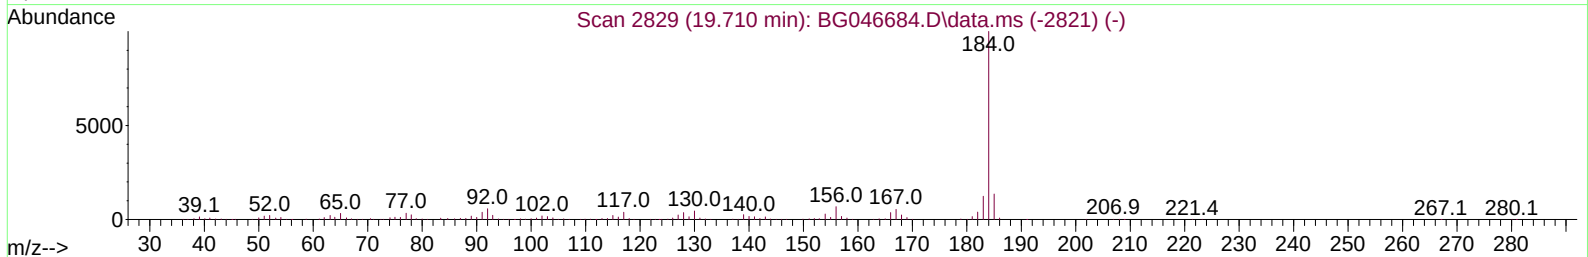
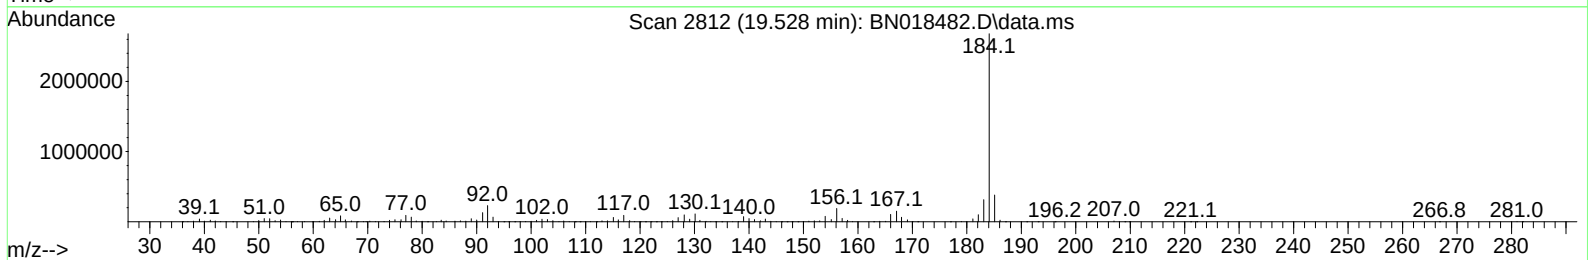


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012722\
 Data File : BN018482.D
 Acq On : 27 Jan 2022 10:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 28 06:36:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 28 06:36:14 2022
 Response via : Initial Calibration

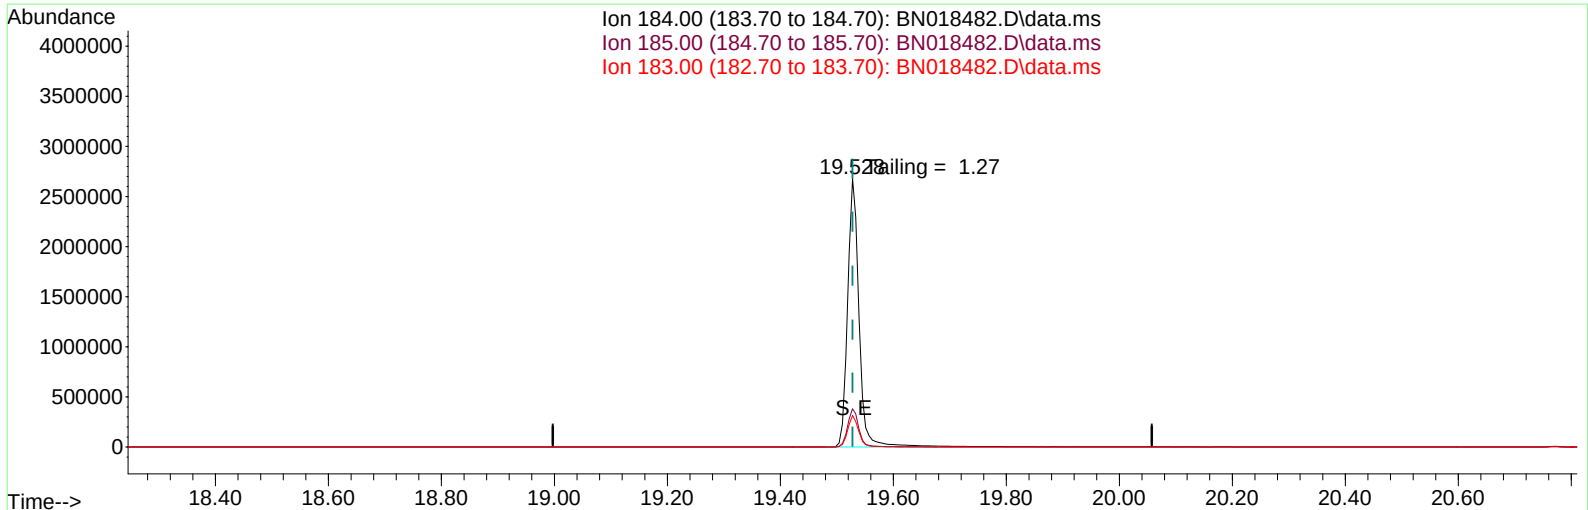

TIC: BN018482.D\data.ms

(77) Benzidine




19.528min (0.000) 0.00 ng

response 3793319

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.24
183.00	13.20	11.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012722\
 Data File : BN018482.D
 Acq On : 27 Jan 2022 10:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 28 06:36:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 28 06:36:14 2022
 Response via : Initial Calibration

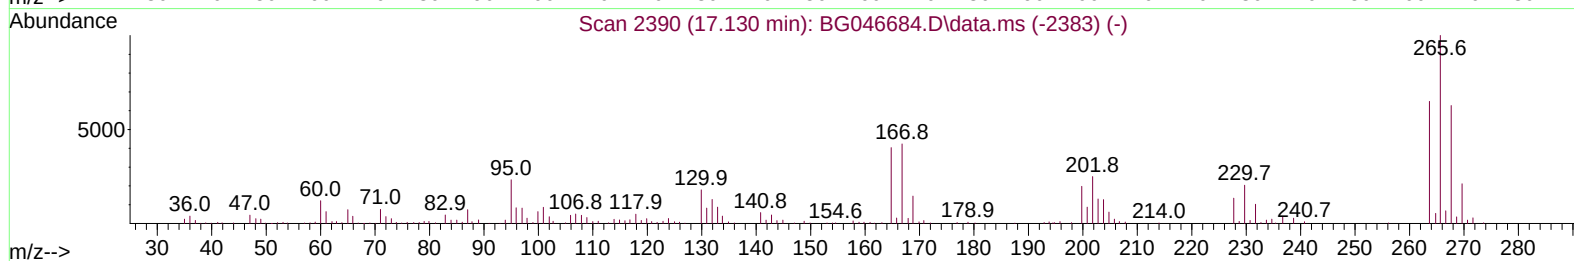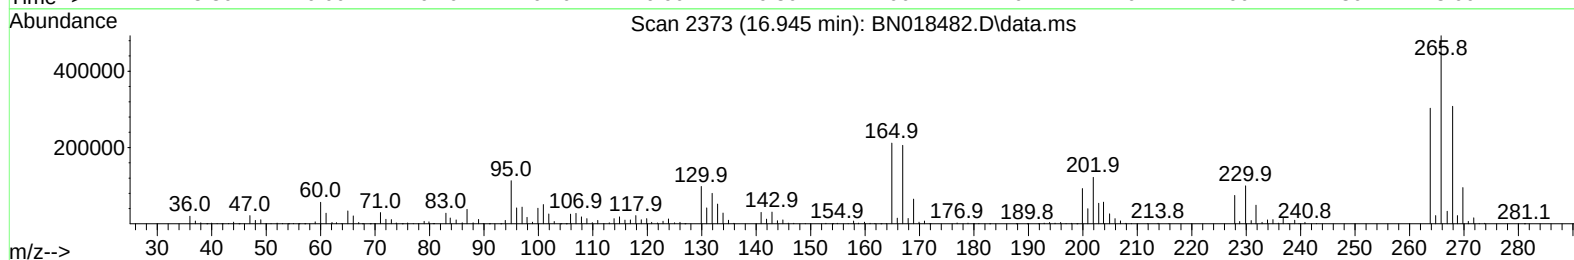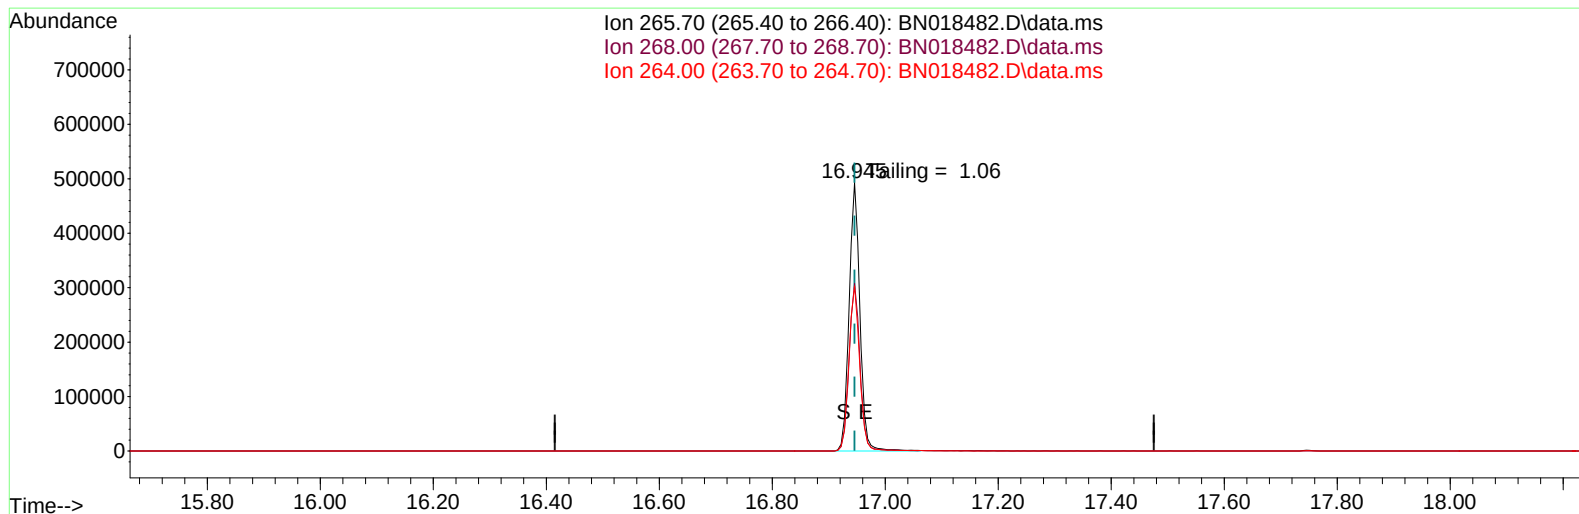

TIC: BN018482.D\data.ms

(70) Pentachlorophenol (C)

16.945min (0.000) 24073.32 ng

response 655557

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.50
264.00	61.60	61.52
0.00	0.00	0.00