


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012722\
 Data File : BN018482.D
 Acq On : 27 Jan 2022 10:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN012722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 28 03:03:43 2022

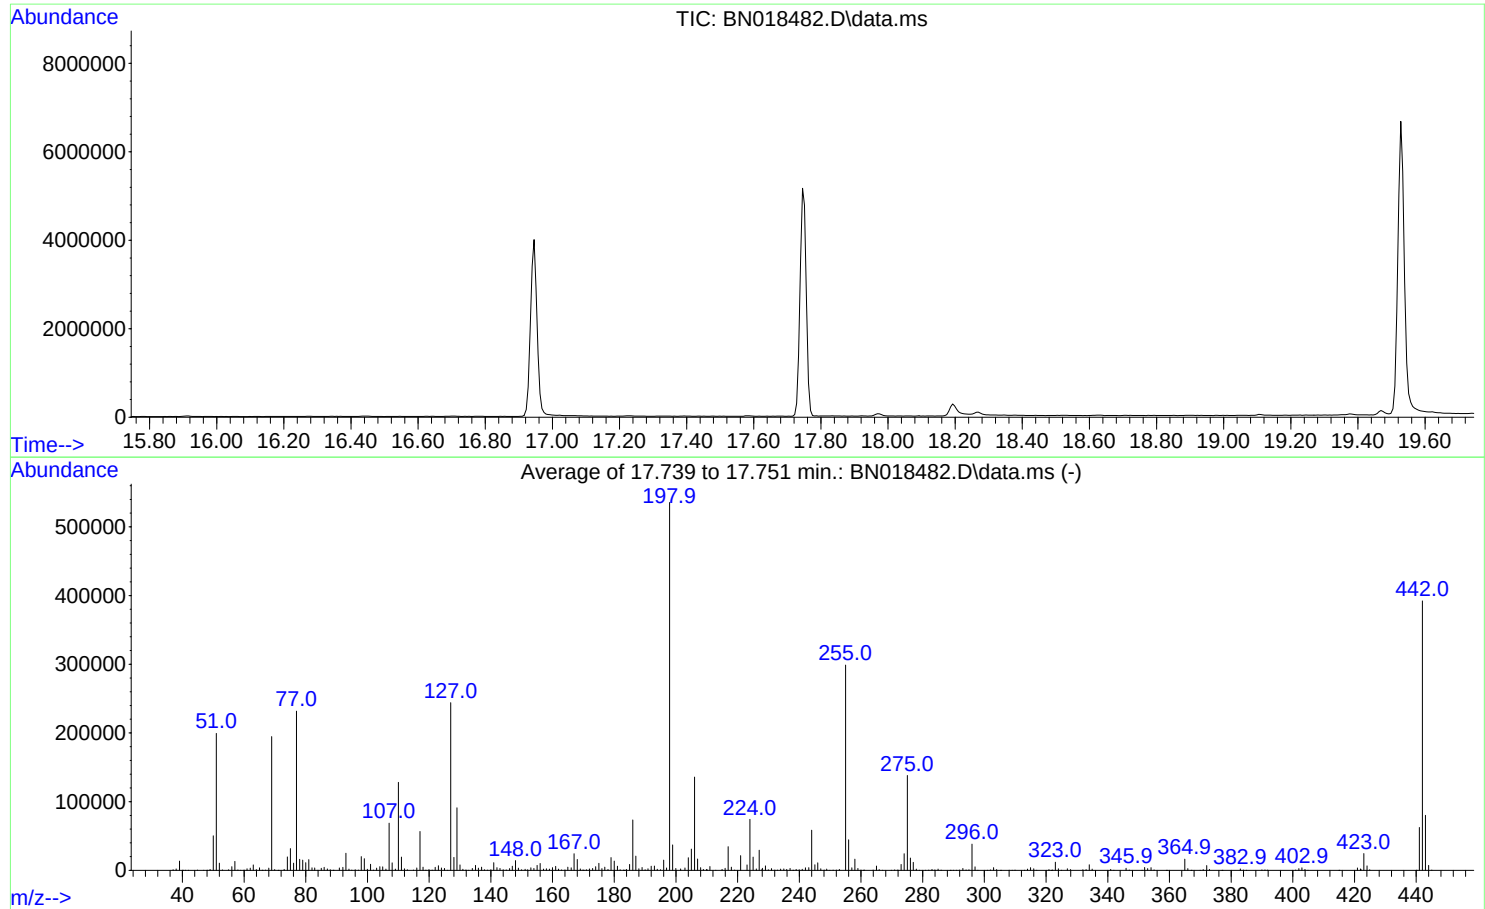




AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2502

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.3	199519	PASS
68	69	0.00	2	1.7	3340	PASS
69	198	0.00	100	36.4	194674	PASS
70	69	0.00	2	0.6	1101	PASS
127	198	10	80	45.6	244053	PASS
197	198	0.00	2	0.6	3401	PASS
198	198	100	100	100.0	535467	PASS
199	198	5	9	6.9	36947	PASS
275	198	10	60	25.8	138067	PASS
365	198	1	100	3.1	16338	PASS
441	198	0.01	100	11.7	62427	PASS
442	442	50	100	100.0	392256	PASS
443	442	15	24	20.5	80248	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012722\
 Data File : BN018482.D
 Acq On : 27 Jan 2022 10:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jan 28 06:36:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 28 06:36:14 2022
 Response via : Initial Calibration

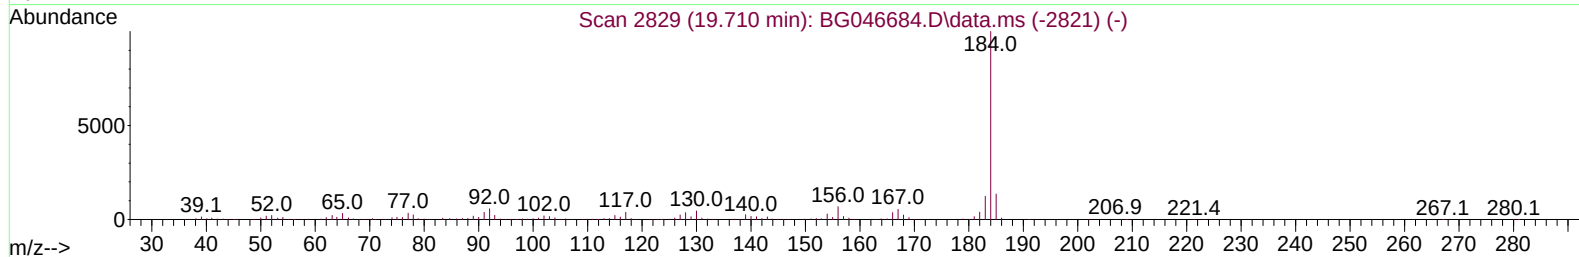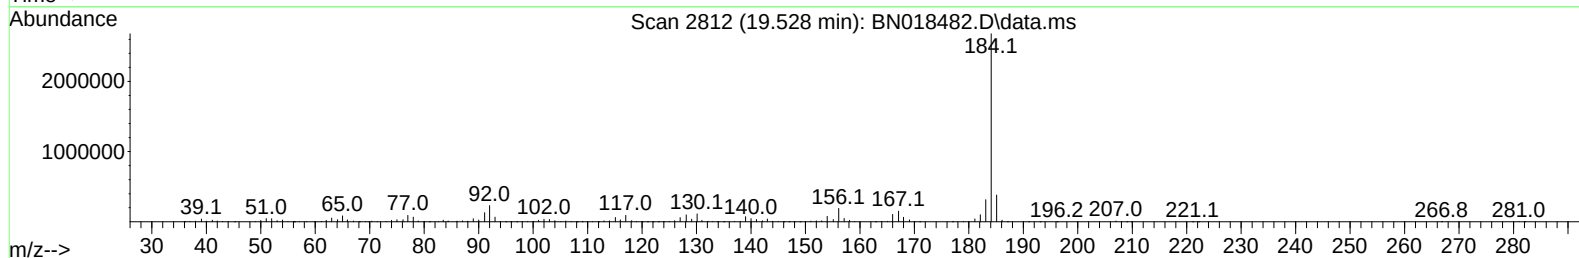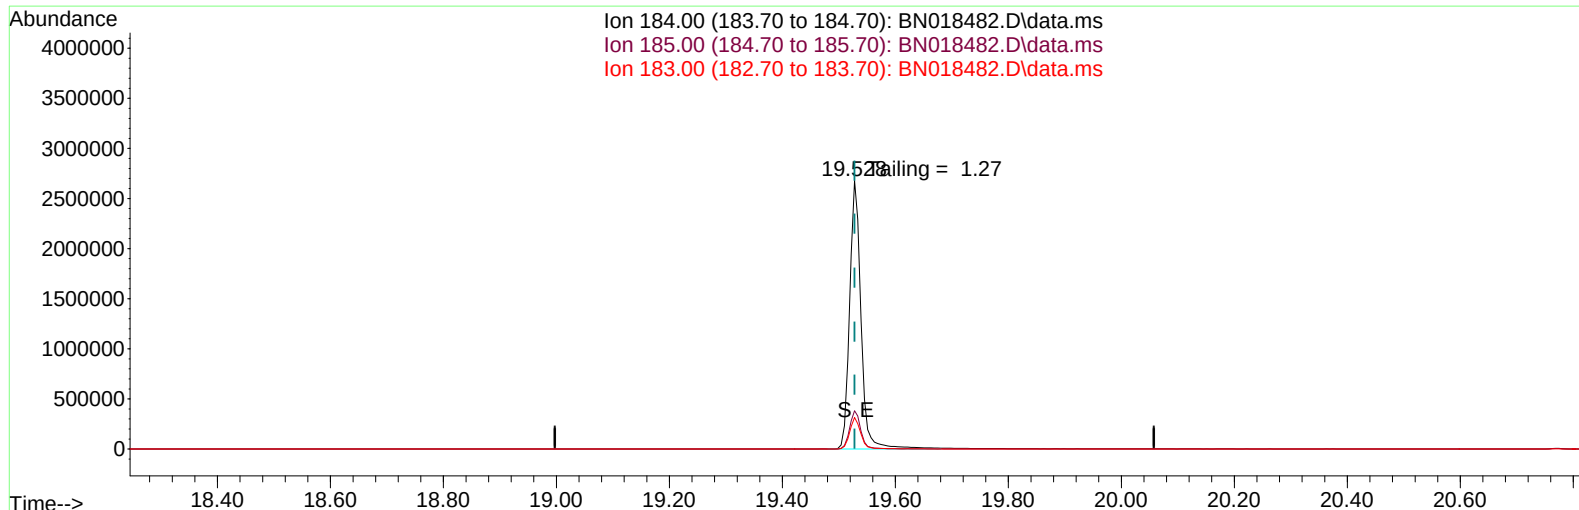

TIC: BN018482.D\data.ms

(77) Benzidine

19.528min (0.000) 0.00 ng




response 3793319

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.24
183.00	13.20	11.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012722\
 Data File : BN018482.D
 Acq On : 27 Jan 2022 10:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jan 28 06:36:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 28 06:36:14 2022
 Response via : Initial Calibration

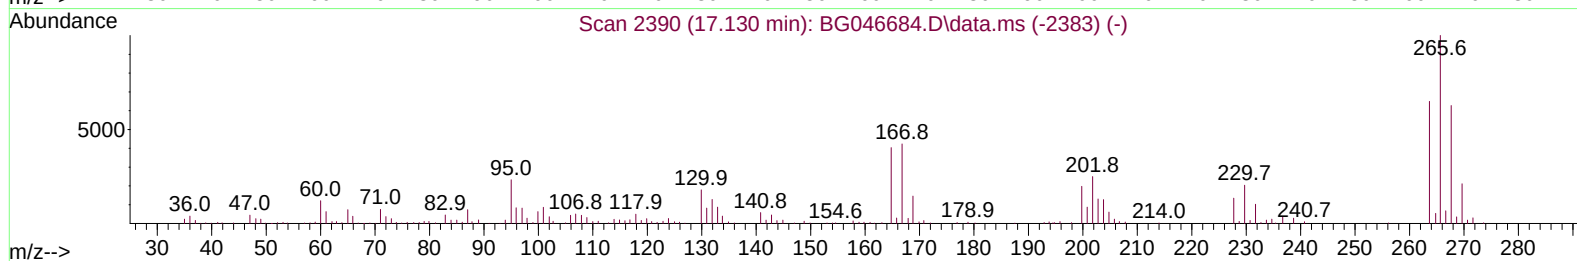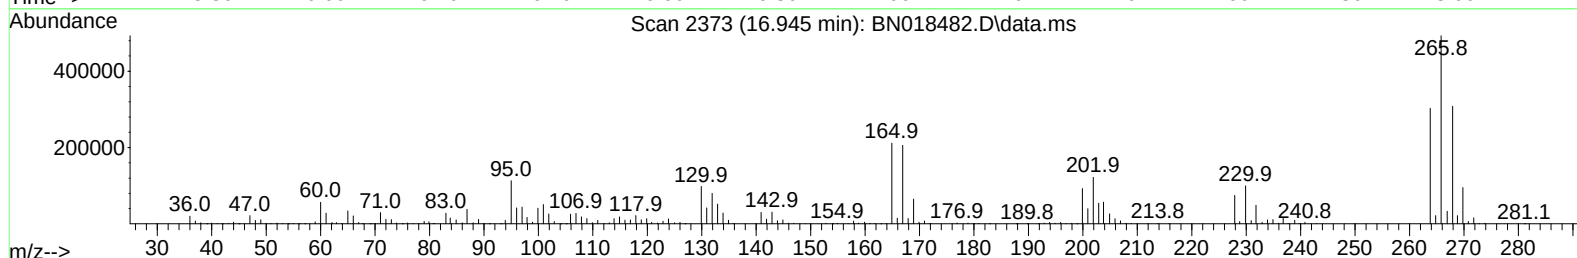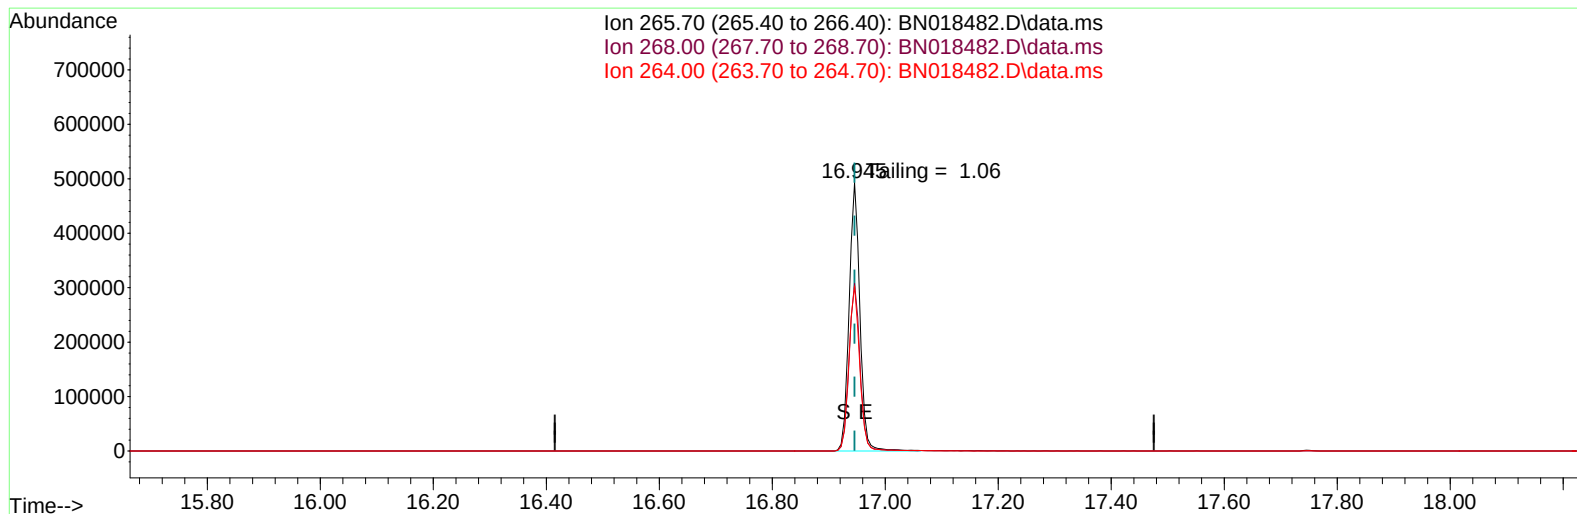

TIC: BN018482.D\data.ms

(70) Pentachlorophenol (C)

16.945min (0.000) 24073.32 ng

response 655557

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.50
264.00	61.60	61.52
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/27/2022	BNA_N	<u>BN018482.D</u>
Compound Name	Response	Retention Time
DDT	1923171	20.769
DDD	13273	20.386
DDE	526	19.828
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13799	1936970	0.71

Instrument :
BNA_N
ClientSampleId :
DFTPP