
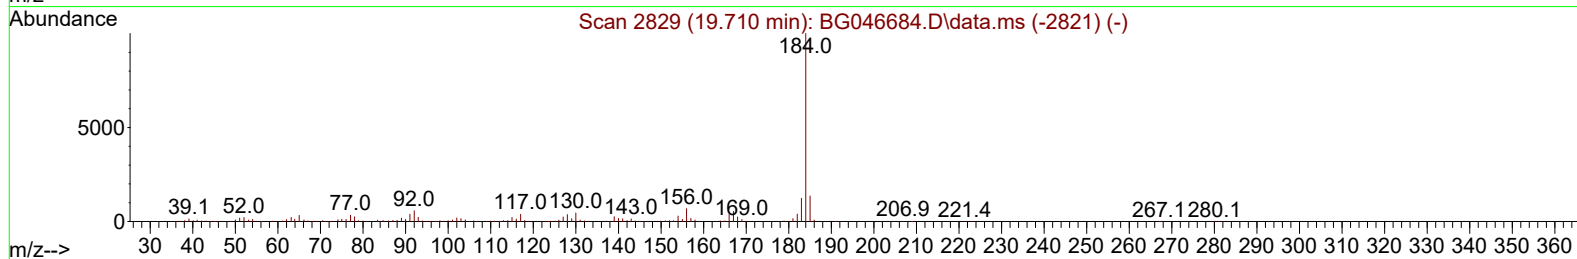
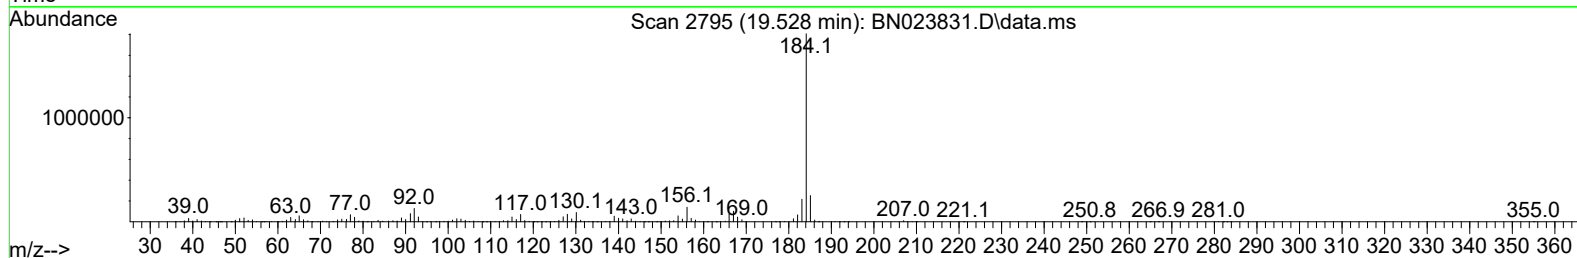


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012723\
Data File : BN023831.D
Acq On : 27 Jan 2023 09:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 28 05:28:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 28 05:28:25 2023
Response via : Initial Calibration

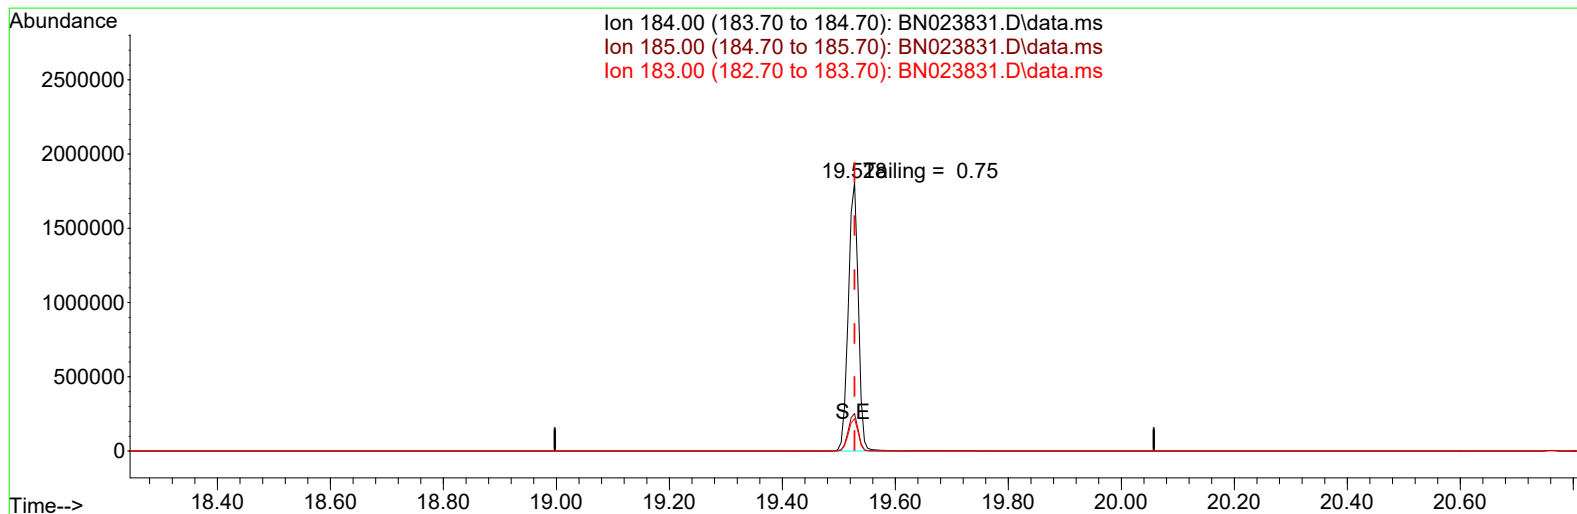

TIC: BN023831.D\data.ms

(77) Benzidine




19.528min (0.000) 0.00 ng

response 2231006

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.96
183.00	13.20	12.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012723\
Data File : BN023831.D
Acq On : 27 Jan 2023 09:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 28 05:28:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 28 05:28:25 2023
Response via : Initial Calibration

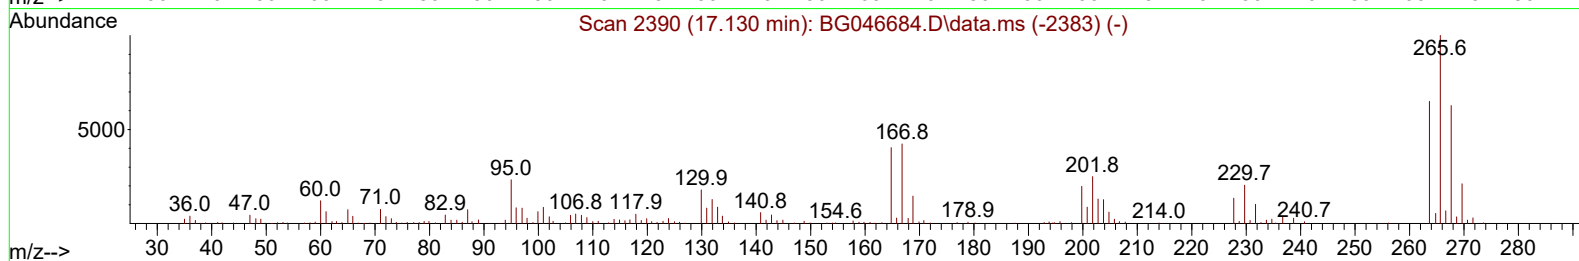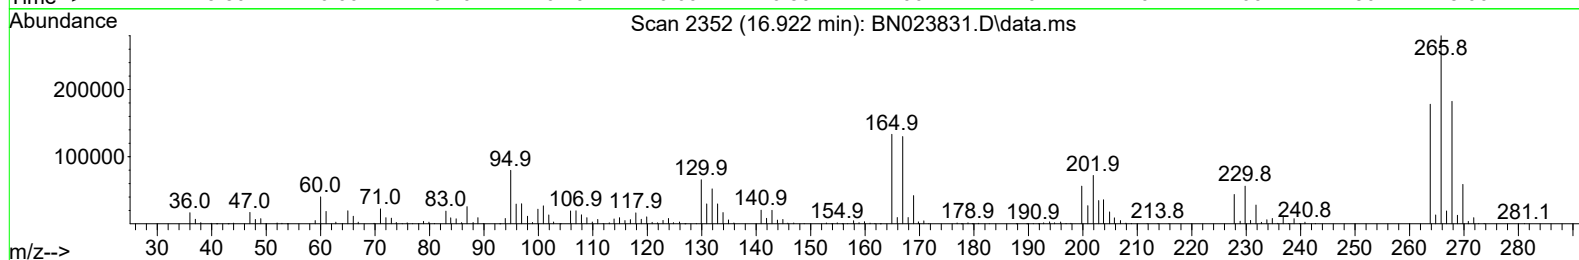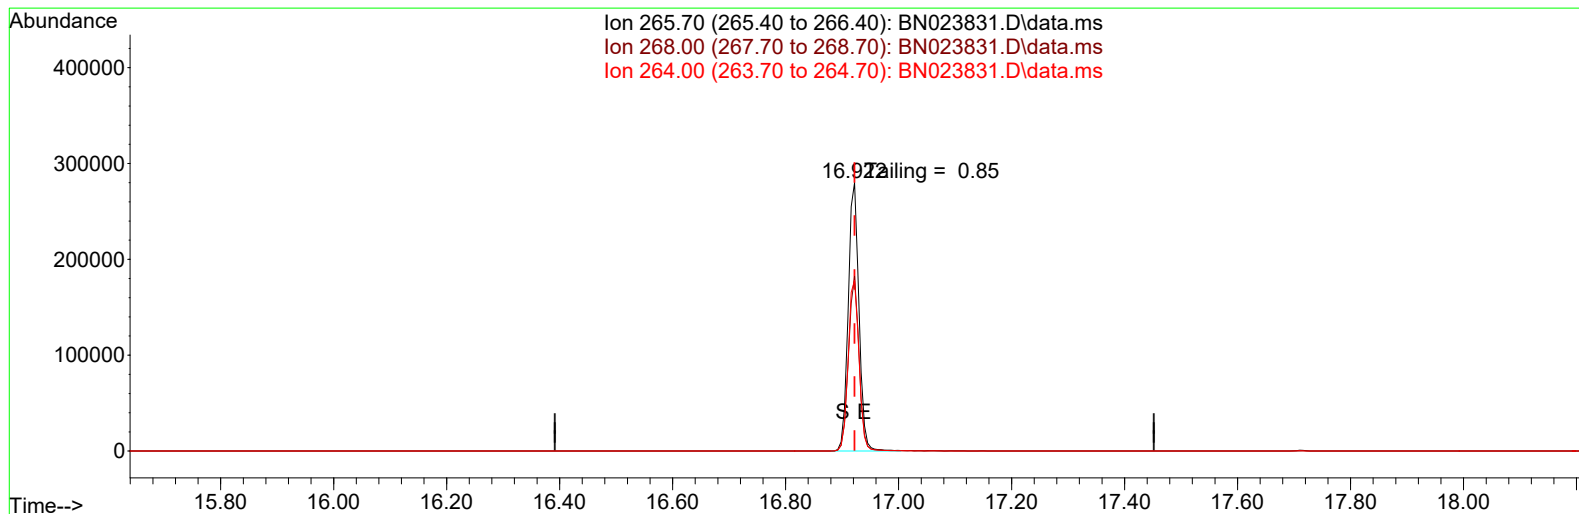

TIC: BN023831.D\data.ms

(70) Pentachlorophenol (C)

16.922min (0.000) 23312.95 ng

response 371214

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.13
264.00	61.60	63.62
0.00	0.00	0.00