


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012723\
Data File : BN023813.D
Acq On : 26 Jan 2023 11:30
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN012723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jan 27 01:06:05 2023

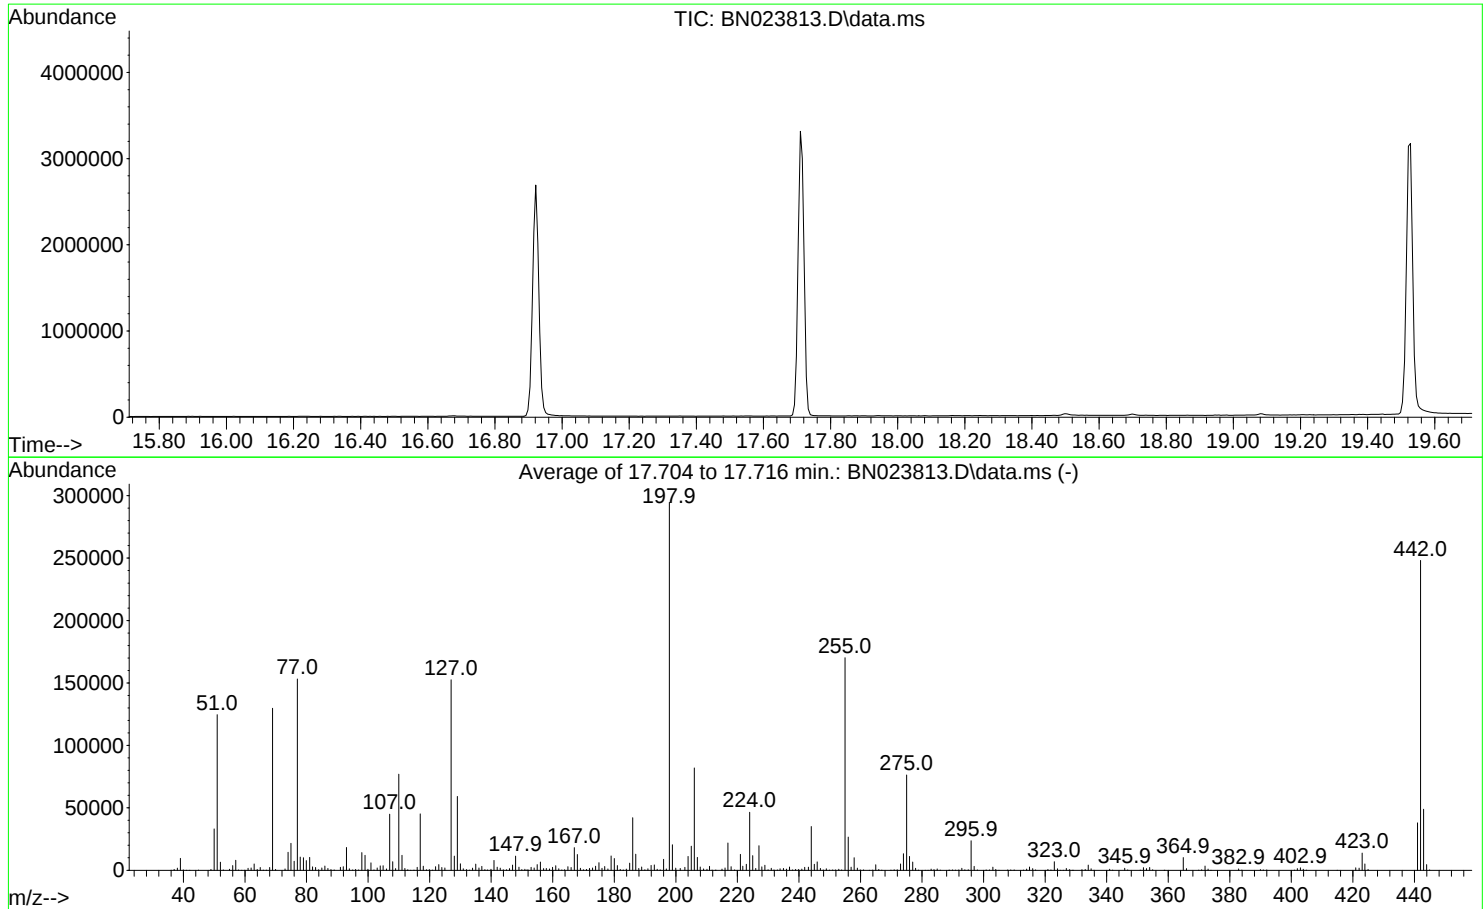




AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.3	124583	PASS
68	69	0.00	2	1.7	2238	PASS
69	198	0.00	100	44.0	129763	PASS
70	69	0.00	2	0.5	688	PASS
127	198	10	80	51.8	152517	PASS
197	198	0.00	2	0.4	1090	PASS
198	198	100	100	100.0	294592	PASS
199	198	5	9	6.9	20437	PASS
275	198	10	60	25.9	76363	PASS
365	198	1	100	3.5	10167	PASS
441	198	0.01	100	12.9	37995	PASS
442	442	50	100	100.0	248200	PASS
443	442	15	24	19.7	48939	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012723\
Data File : BN023813.D
Acq On : 26 Jan 2023 11:30
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 27 05:22:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 27 05:22:50 2023
Response via : Initial Calibration

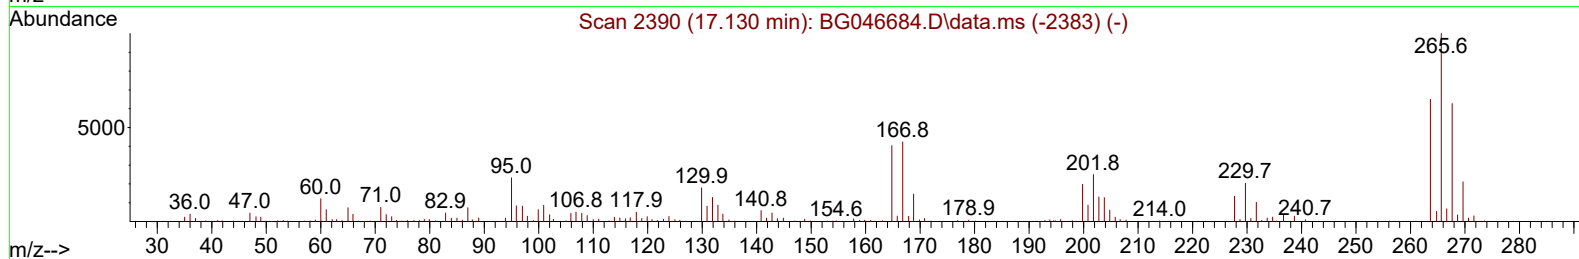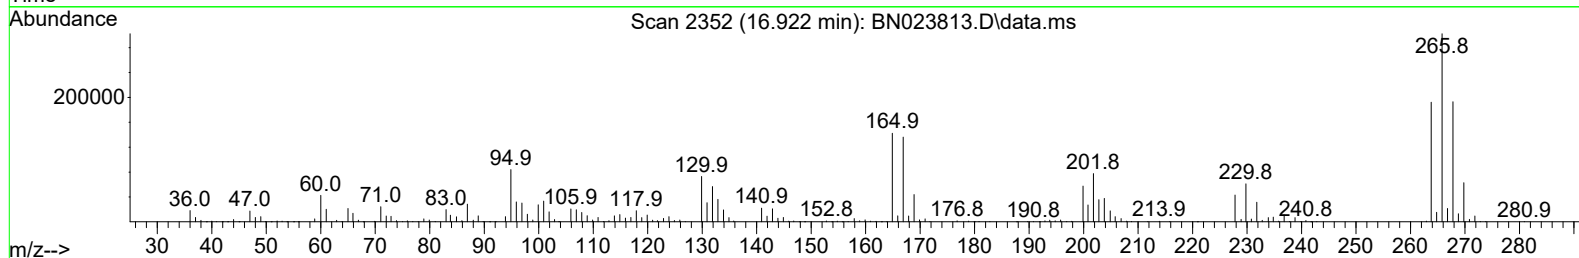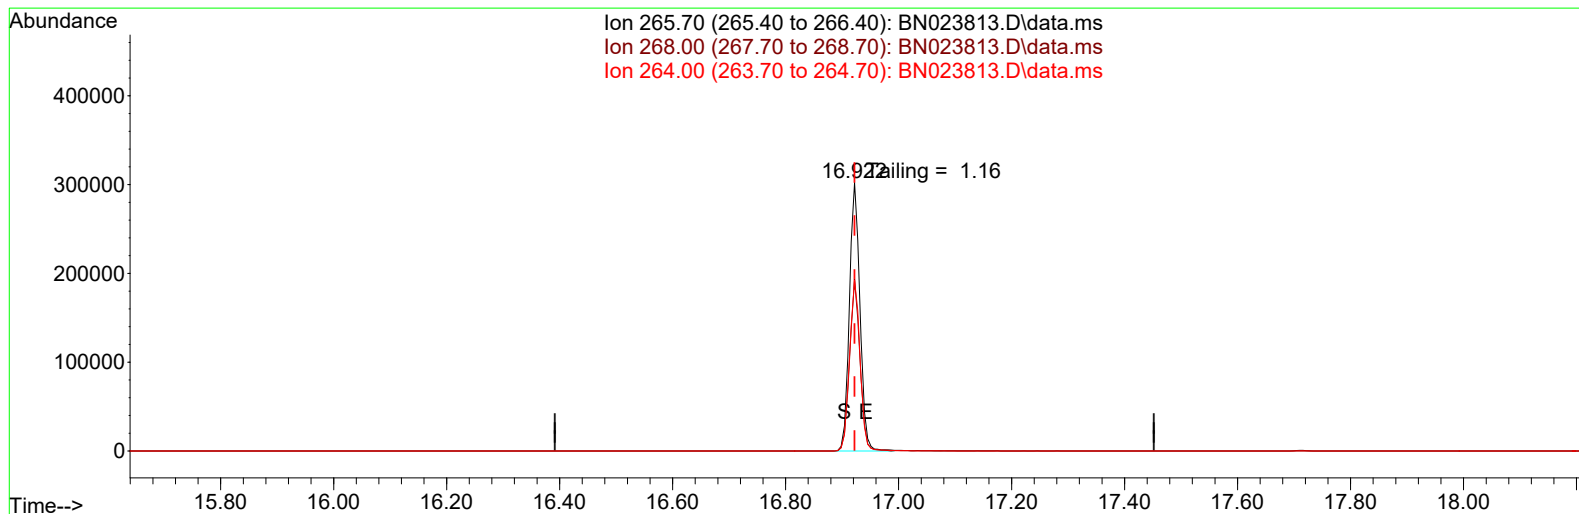

TIC: BN023813.D\data.ms

(70) Pentachlorophenol (C)

16.922min (0.000) 23789.80 ng




response 394116

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.88
264.00	61.60	63.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012723\
Data File : BN023813.D
Acq On : 26 Jan 2023 11:30
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 27 05:22:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 27 05:22:50 2023
Response via : Initial Calibration

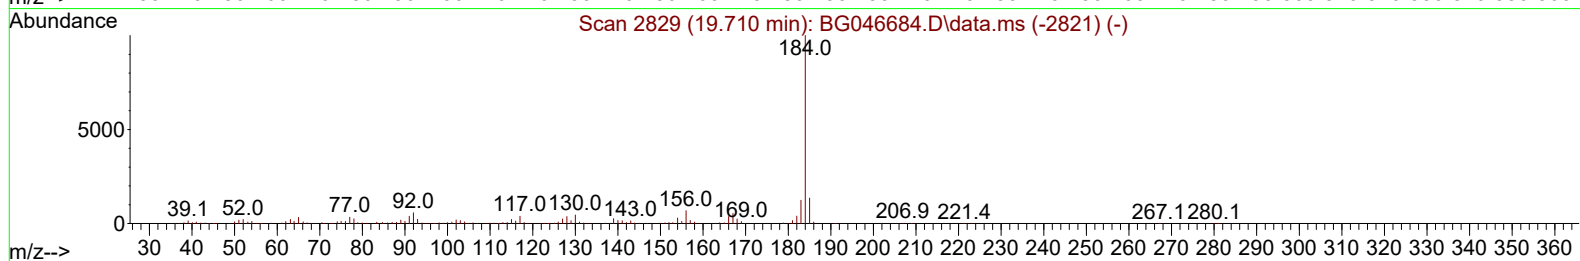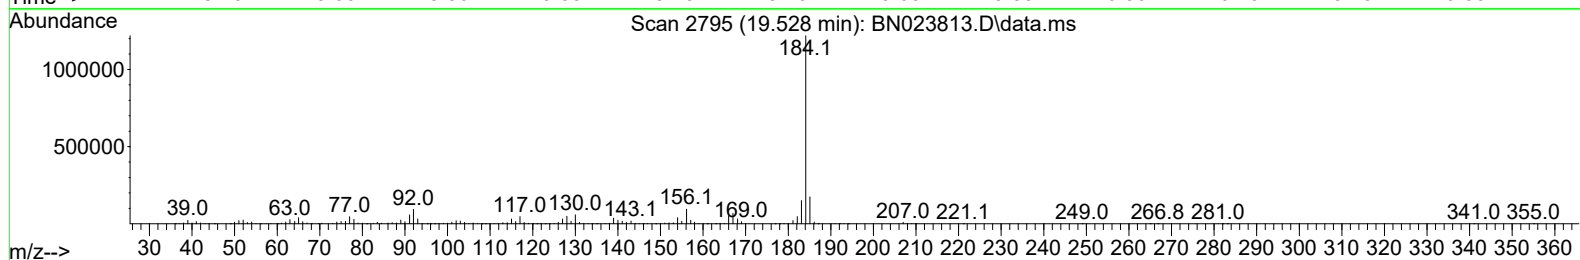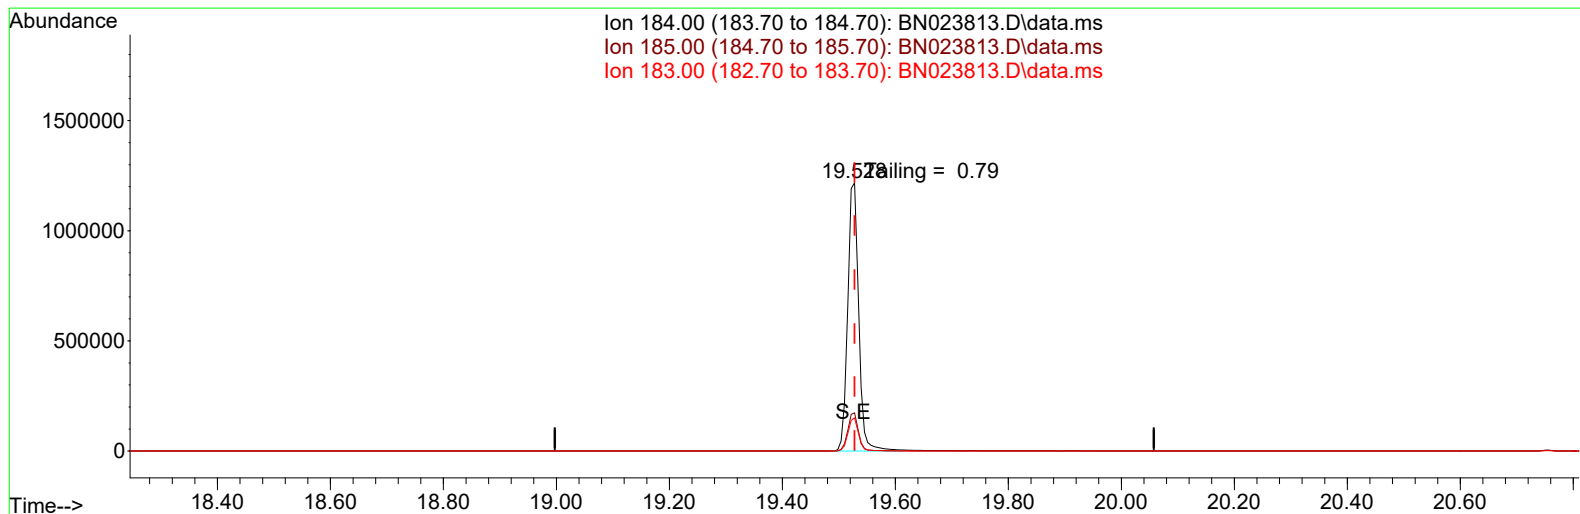

TIC: BN023813.D\data.ms

(77) Benzidine

19.528min (0.000) 0.00 ng

response 1660449

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.29
183.00	13.20	12.35
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/27/2023	BNA_N	<u>BN023813.D</u>
Compound Name	Response	Retention Time
DDT	959376	20.757
DDD	7693	20.363
DDE	0	19.816
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7693	967069	0.80

Instrument :
BNA_N
ClientSampleId :
DFTPP