
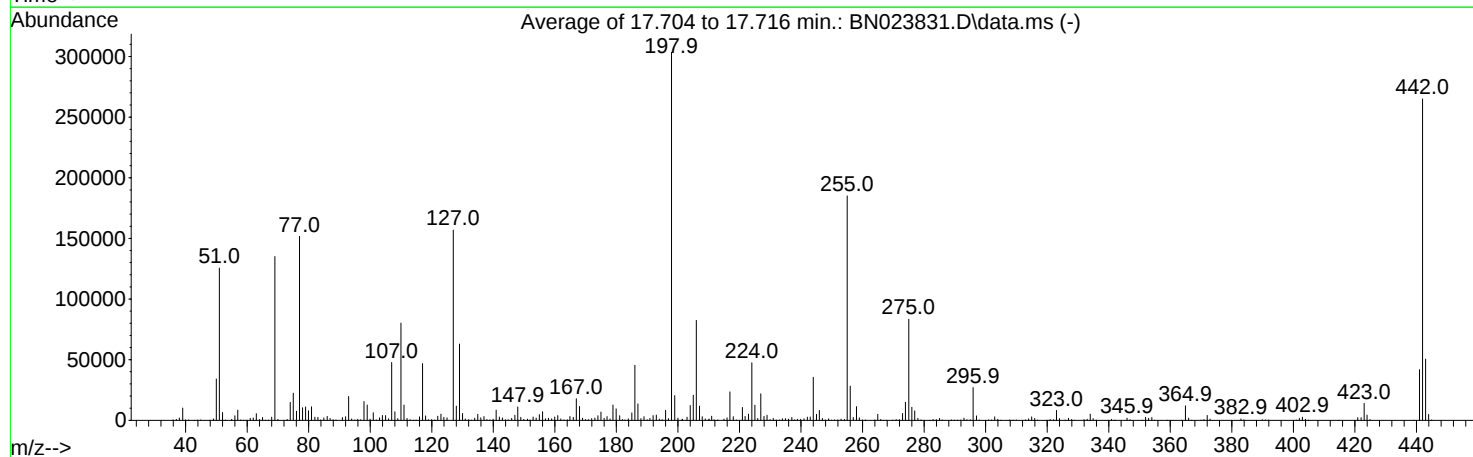


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012723\
 Data File : BN023831.D
 Acq On : 27 Jan 2023 09:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN012723.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 30 02:24:22 2023

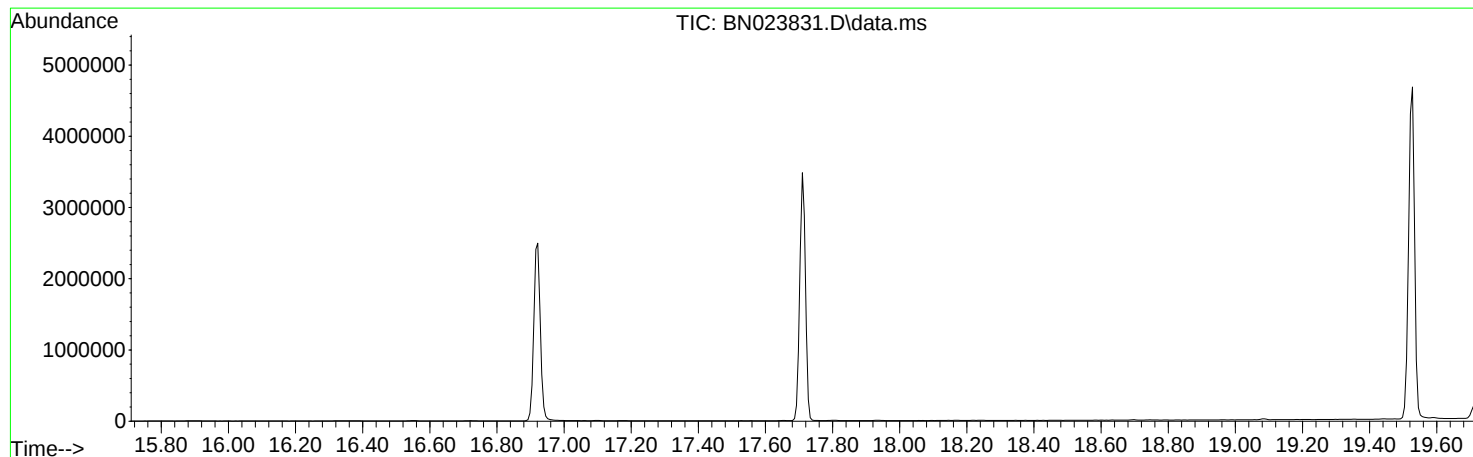




AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.4	125611	PASS
68	69	0.00	2	1.9	2530	PASS
69	198	0.00	100	44.5	135125	PASS
70	69	0.00	2	0.6	765	PASS
127	198	10	80	51.7	156843	PASS
197	198	0.00	2	0.5	1395	PASS
198	198	100	100	100.0	303360	PASS
199	198	5	9	6.7	20427	PASS
275	198	10	60	27.5	83403	PASS
365	198	1	100	4.0	12012	PASS
441	198	0.01	100	13.8	41765	PASS
442	442	50	100	100.0	265024	PASS
443	442	15	24	19.1	50499	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012723\
Data File : BN023831.D
Acq On : 27 Jan 2023 09:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 28 05:28:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 28 05:28:25 2023
Response via : Initial Calibration

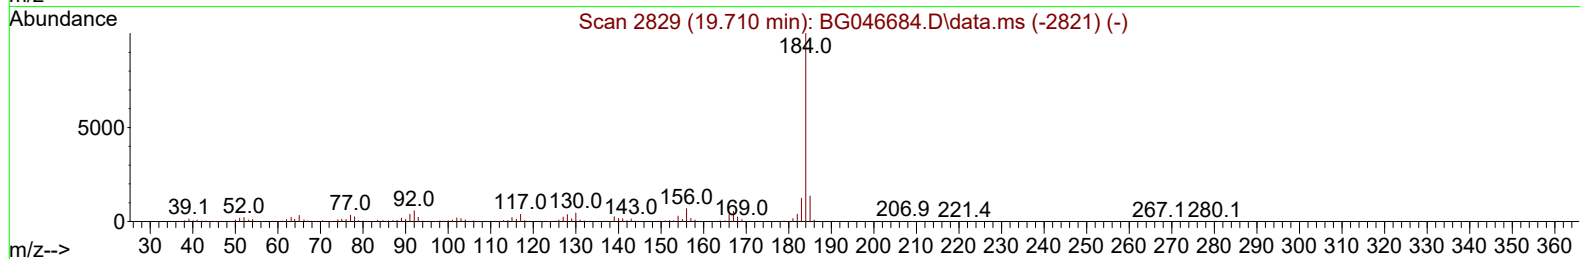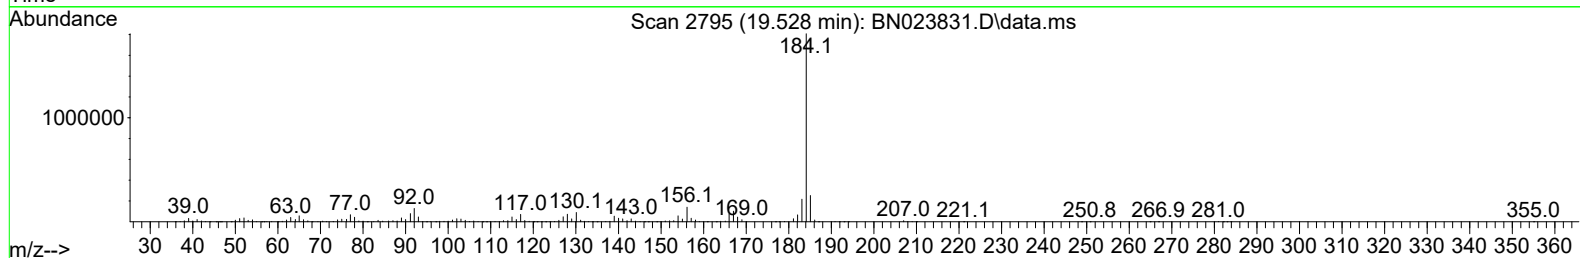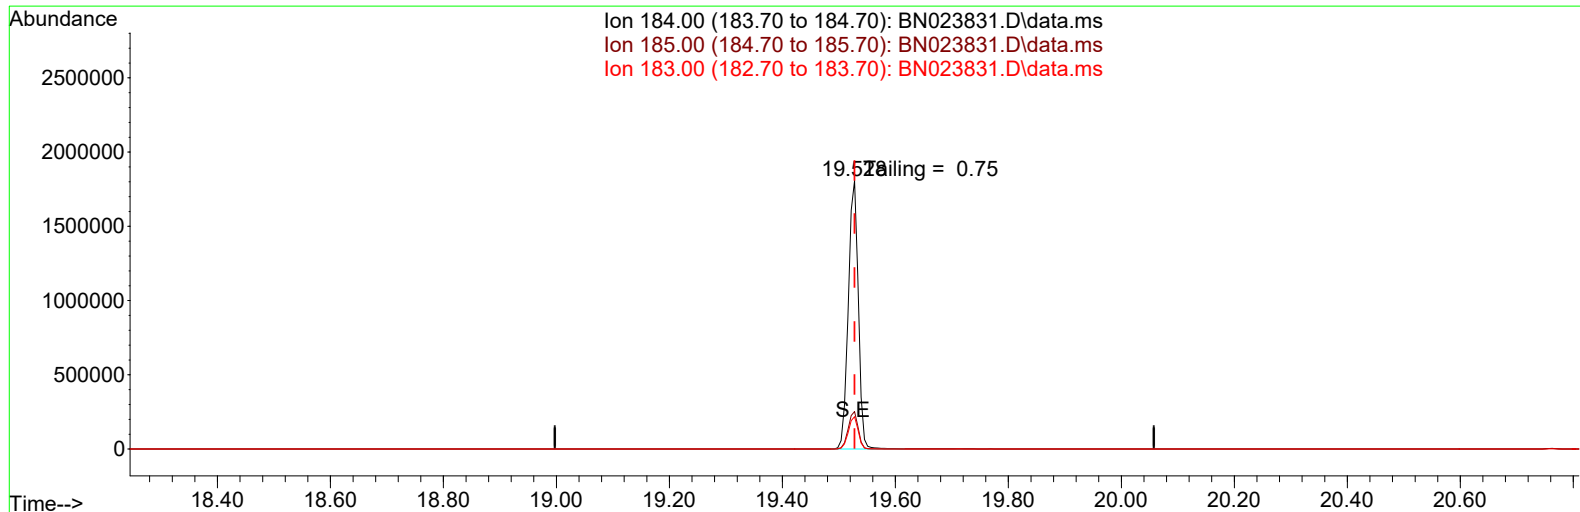

TIC: BN023831.D\data.ms

(77) Benzidine

19.528min (0.000) 0.00 ng




response 2231006

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.96
183.00	13.20	12.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012723\
Data File : BN023831.D
Acq On : 27 Jan 2023 09:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 28 05:28:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 28 05:28:25 2023
Response via : Initial Calibration

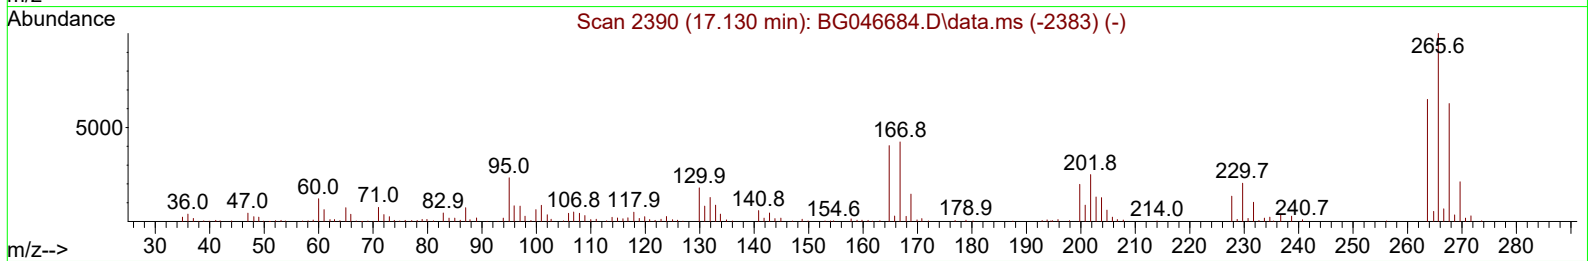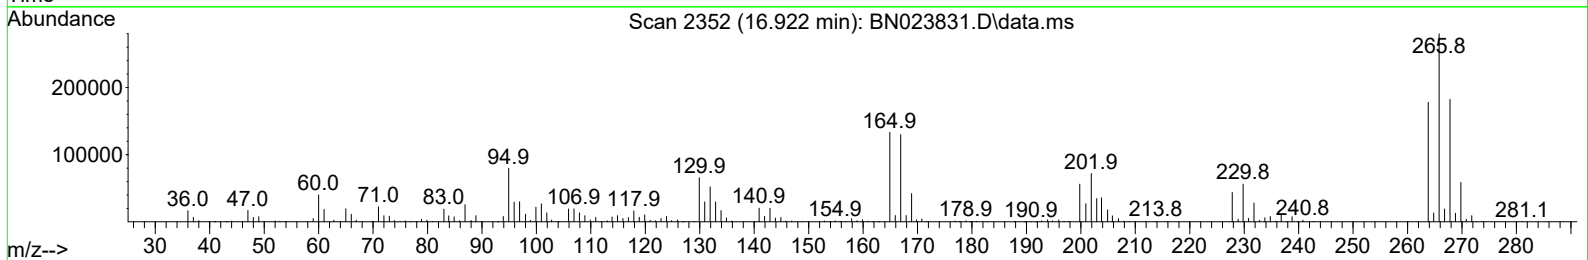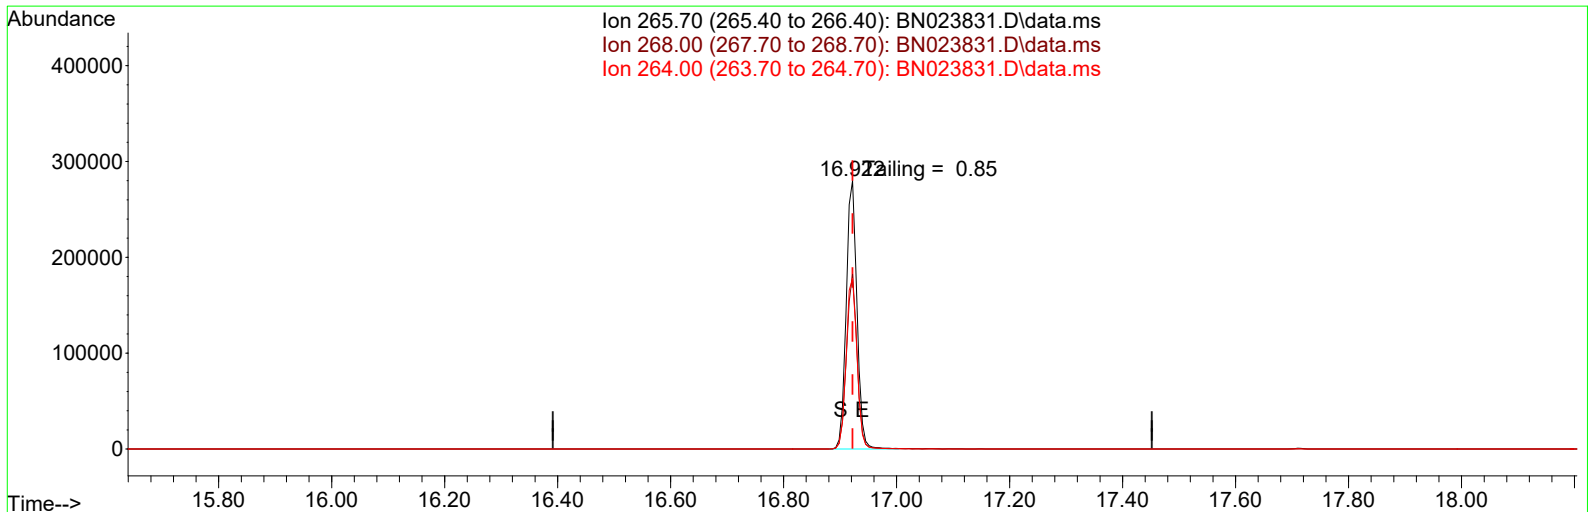

TIC: BN023831.D\data.ms

(70) Pentachlorophenol (C)

16.922min (0.000) 23312.95 ng

response 371214

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.13
264.00	61.60	63.62
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/27/2023	BNA_N	<u>BN023831.D</u>
Compound Name	Response	Retention Time
DDT	1078572	20.763
DDD	9175	20.369
DDE	0	19.816
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9175	1087747	0.84

Instrument :
BNA_N
ClientSampleId :
DFTPP