

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN012820\
 Data File : BN009455.D
 Acq On : 28 Jan 2020 17:37
 Operator : CG/JU
 Sample : L1193-12DL 2X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jan 29 00:11:18 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 22 15:13:20 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	197887	20.00	ng/ul	0.00
18) Naphthalene-d8	10.21	136	813815	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.09	164	475336	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.85	188	947944	20.00	ng/ul	0.00
77) Chrysene-d12	21.06	240	802327	20.00	ng/ul	0.00
85) Perylene-d12	23.19	264	901195	20.00	ng/ul	0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.09	96	7133	1.49	ng/uL	0.00
5) Phenol-d5	6.66	99	162866	9.28	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.81	67	109657	8.80	ng/ul	0.00
9) 2-Chlorophenol-d4	7.00	132	125909	9.83	ng/ul	0.00
13) 4-Methylphenol-d8	8.17	113	130089	9.31	ng/ul	0.00
19) Nitrobenzene-d5	8.60	128	63424	10.71	ng/ul	0.00
22) 2-Nitrophenol-d4	9.31	143	69956	11.27	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.85	165	131535	10.69	ng/ul	0.00
29) 4-Chloroaniline-d4	10.36	131	52900	3.56	ng/ul	0.00
43) Dimethylphthalate-d6	13.52	166	405272	11.52	ng/ul	0.00
46) Acenaphthylene-d8	13.78	160	480723	11.51	ng/ul	0.00
51) 4-Nitrophenol-d4	14.33	143	61866	9.45	ng/ul	0.00
57) Fluorene-d10	15.10	176	342456	11.09	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.24	200	44319	7.72	ng/ul	0.00
70) Anthracene-d10	16.95	188	497468	11.34	ng/ul	0.00
78) Pyrene-d10	19.25	212	518538	12.01	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.05	264	500759	11.01	ng/ul	0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.56	163	82568	2.280	ng/ul	97
47) Acenaphthylene	13.81	152	2092515	46.436	ng/ul	99
54) 2,4-Dinitrotoluene	14.43	165	15600	1.518	ng/ul#	87
58) Fluorene	15.17	166	155083	4.333	ng/ul#	44
69) Phenanthrene	16.98	178	711056	13.294	ng/ul	98
71) Anthracene	16.98	178	711056	13.057	ng/ul	98
76) Fluoranthene	19.07	202	316036	5.154	ng/ul	99
79) Pyrene	19.28	202	717559	12.352	ng/ul	98
82) Benzo(a)anthracene	21.05	228	197432	3.614	ng/ul#	1
84) Chrysene	21.07	228	410569	7.714	ng/ul#	79
87) Benzo(b)fluoranthene	22.56	252	1142727	20.054	ng/ul	94
88) Benzo(k)fluoranthene	22.56	252	1142727	20.395	ng/ul	95
90) Benzo(a)pyrene	23.09	252	1211347	23.683	ng/ul	98
91) Indeno(1,2,3-cd)pyrene	25.26	276	878815	14.178	ng/ul#	95
92) Dibenzo(a,h)anthracene	25.26	278	315240	6.028	ng/ul#	87
93) Benzo(g,h,i)perylene	25.90	276	712049	13.811	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN012820\
Data File : BN009455.D
Acq On : 28 Jan 2020 17:37
Operator : CG/JU
Sample : L1193-12DL 2X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jan 29 00:11:18 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 22 15:13:20 2020
Response via : Initial Calibration




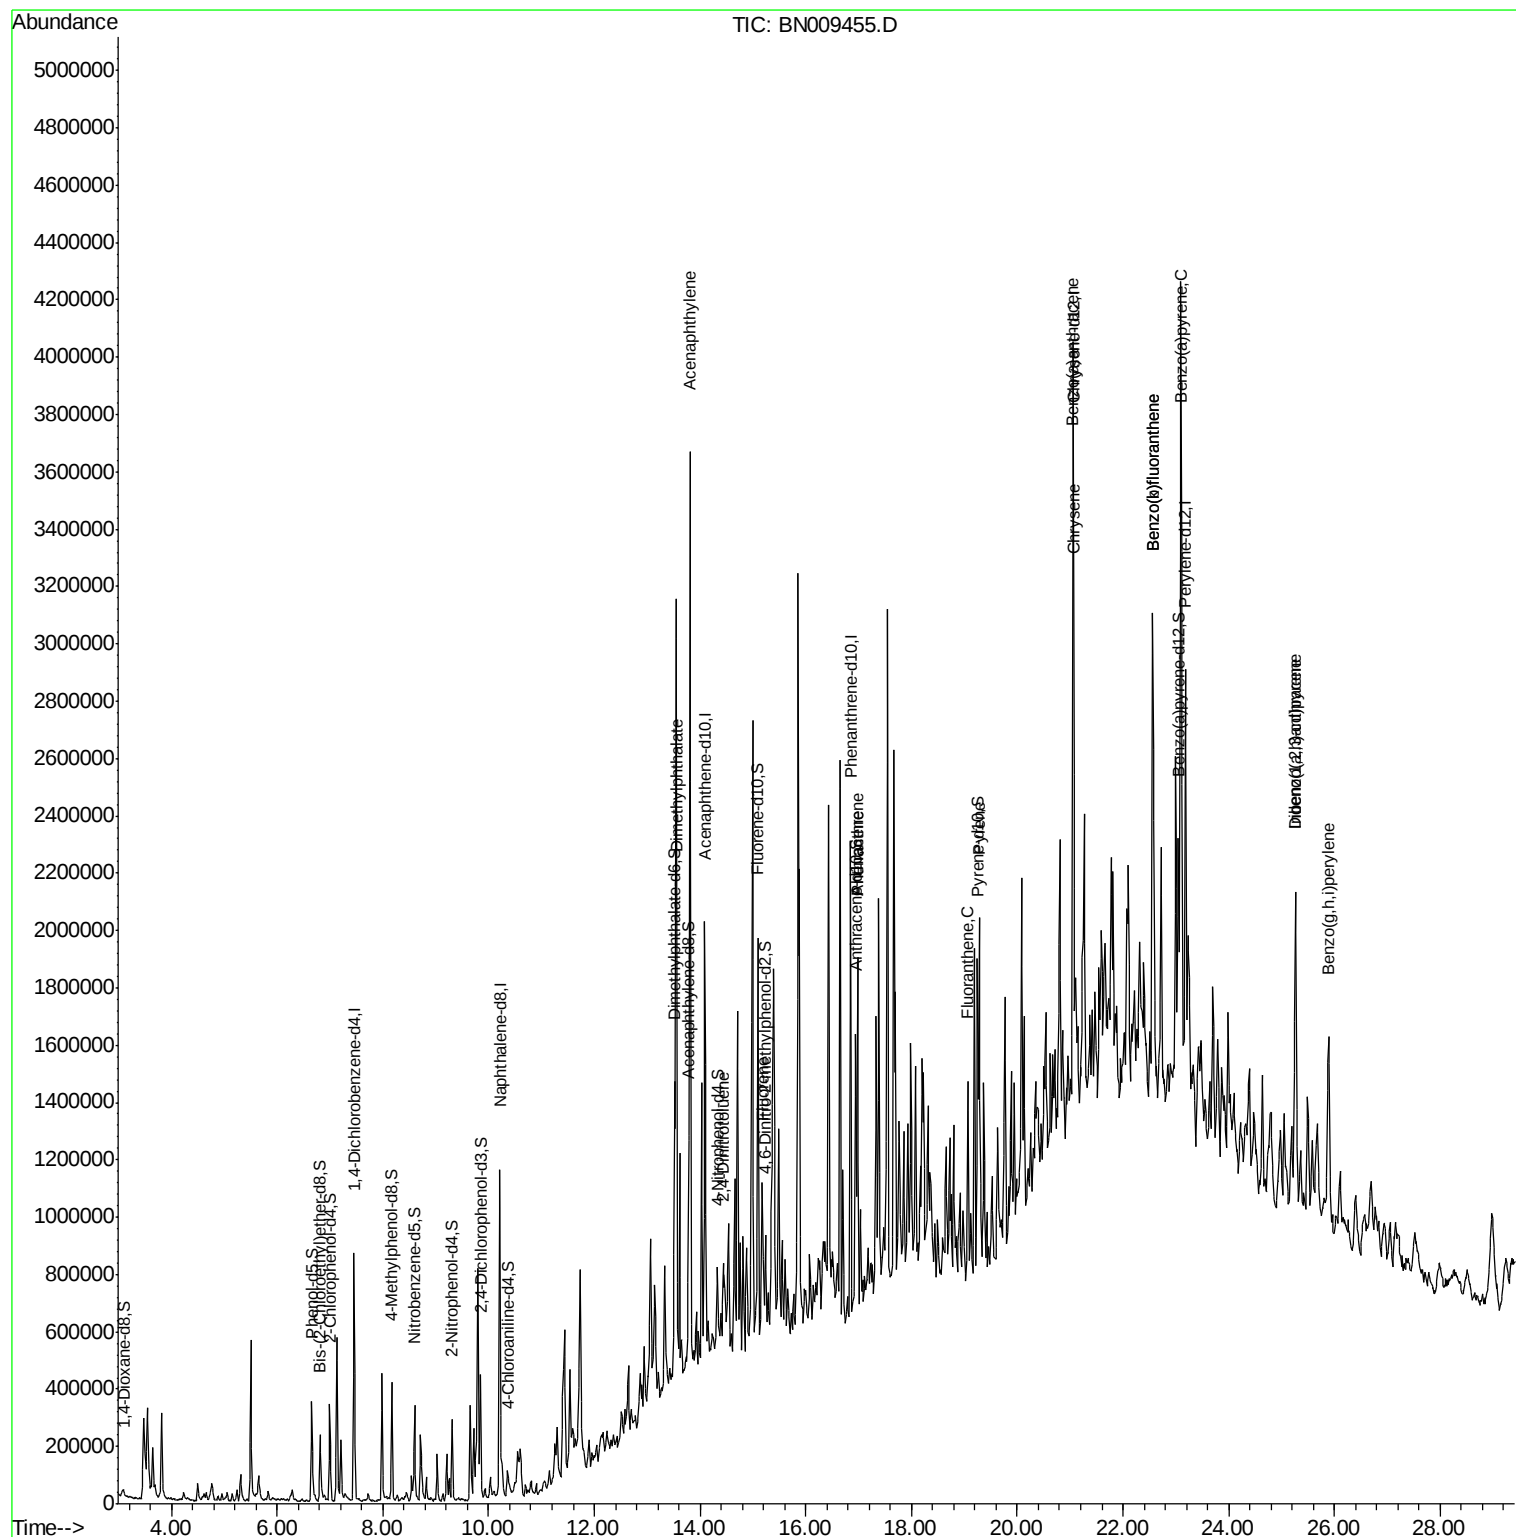




#44
Dimethylphthalate
Concen: 2.280 ng/ul
RT: 13.56 min Scan# 1798
Delta R.T. -0.01 min
Lab File: BN009455.D
Acq: 28 Jan 2020 17:37




Instrument :
BNA_N
ClientSampleId :


Tot Ion:163 Resp: 82568
Ion Ratio Lower Upper
163 100
194 4.1 3.1 4.7
164 12.0 8.3 12.5

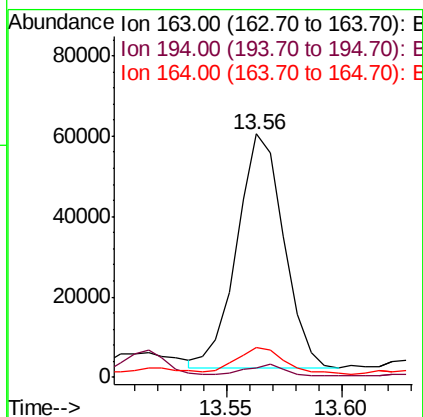

#47
Acenaphthylene
Concen: 46.436 ng/ul
RT: 13.81 min Scan# 1840
Delta R.T. -0.00 min
Lab File: BN009455.D
Acq: 28 Jan 2020 17:37

Tgt Ion:152 Resp: 2092515
Ion Ratio Lower Upper
152 100
151 19.9 16.2 24.4
153 13.1 10.8 16.2

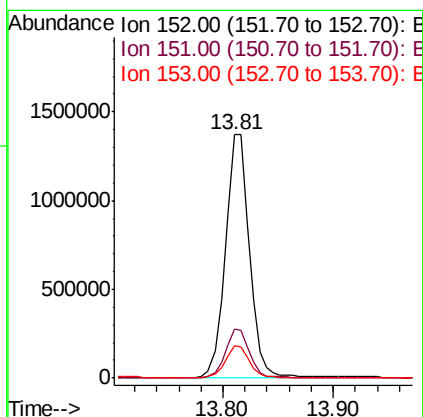

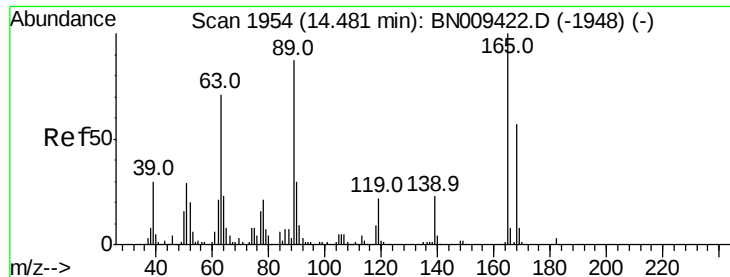

#54

2,4-Dinitrotoluene

Concen: 1.518 ng/ul

RT: 14.43 min Scan# 1946

Delta R.T. -0.05 min

Lab File: BN009455.D

Acq: 28 Jan 2020 17:37

Instrument :

BNA_N

ClientSampleId :


Tot Ion:165 Resp: 15600

Ion Ratio Lower Upper

165 100

63 58.4 55.4 83.0




182 3.8 2.0 3.0#

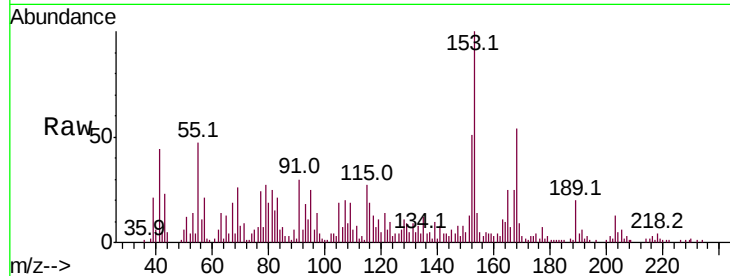

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BNO

Ion 182.00 (181.70 to 182.70): E

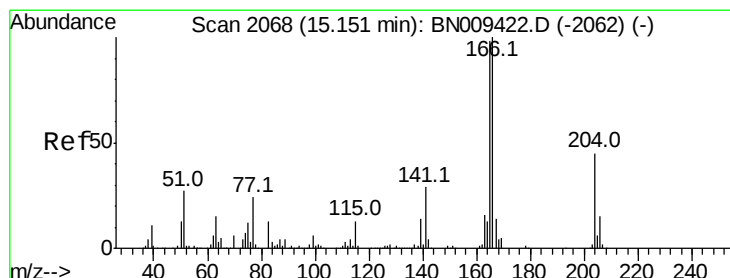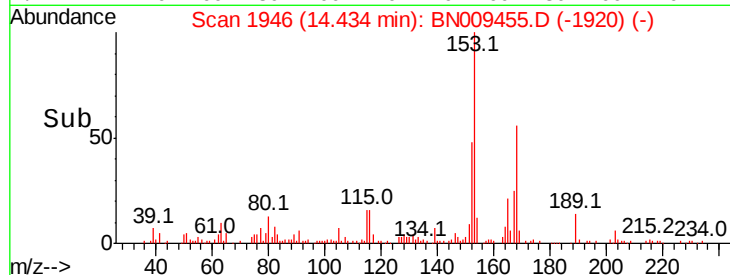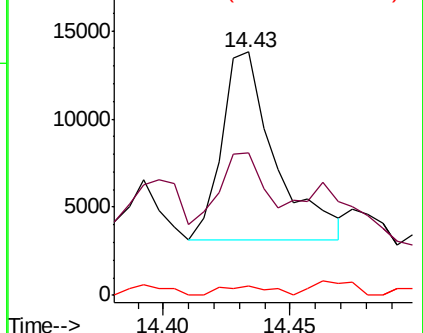

#58

Fluorene

Concen: 4.333 ng/ul

RT: 15.17 min Scan# 2072

Delta R.T. 0.02 min

Lab File: BN009455.D

Acq: 28 Jan 2020 17:37


Tgt Ion:166 Resp: 155083

Ion Ratio Lower Upper

166 100

165 157.4 76.5 114.7#



167 13.4 10.9 16.3

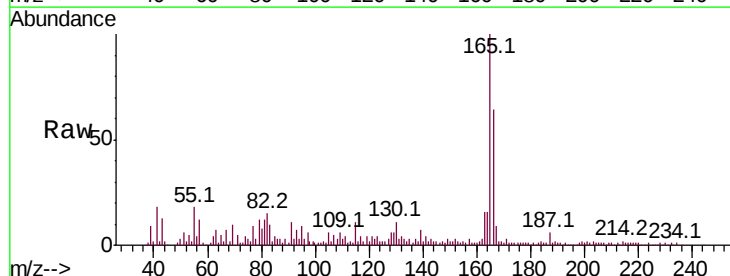


Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

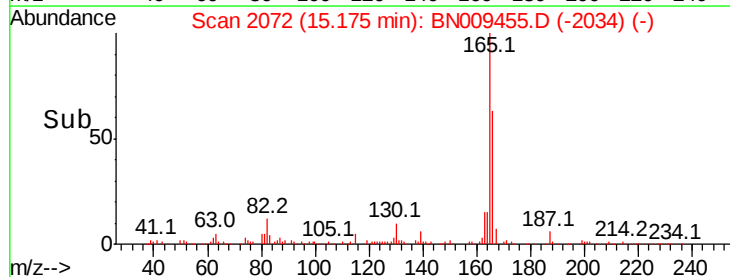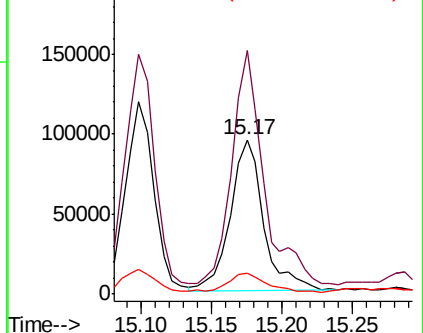



#69

Phenanthrene

Concen: 13.294 ng/ul

RT: 16.98 min Scan# 2379

Delta R.T. 0.09 min

Lab File: BN009455.D

Acq: 28 Jan 2020 17:37

Instrument :

BNA_N

ClientSampleId :


Tot Ion:178 Resp: 711056

Ion Ratio Lower Upper

178 100

179 16.1 13.3 19.9




176 18.1 15.5 23.3

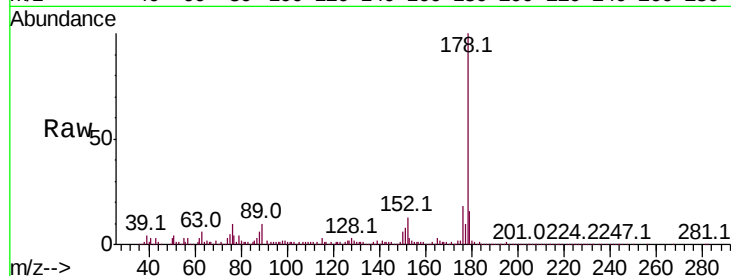

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

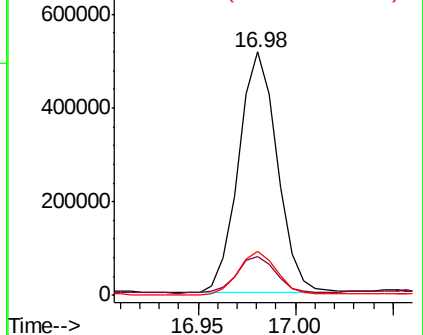

#71

Anthracene

Concen: 13.057 ng/ul

RT: 16.98 min Scan# 2379

Delta R.T. -0.00 min

Lab File: BN009455.D

Acq: 28 Jan 2020 17:37


Tgt Ion:178 Resp: 711056

Ion Ratio Lower Upper

178 100

179 16.1 11.8 17.6



176 18.1 14.6 22.0




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E




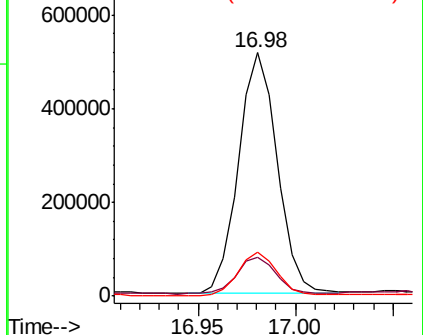




#76
Fluoranthene
Concen: 5.154 ng/ul
RT: 19.07 min Scan# 2734
Delta R.T. 0.15 min
Lab File: BN009455.D
Acq: 28 Jan 2020 17:37




Instrument :
BNA_N
ClientSampleId :


Tot Ion:	202	Resp:	316036
Ion	Ratio	Lower	Upper
202	100		
101	12.6	9.7	14.5
100	8.9	7.1	10.7

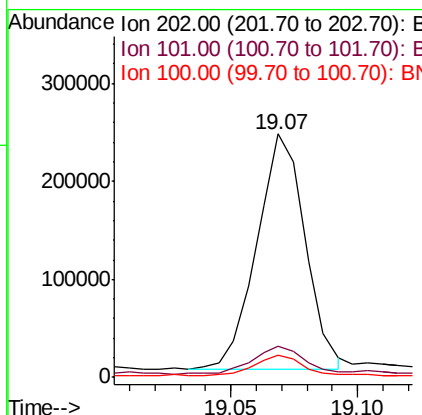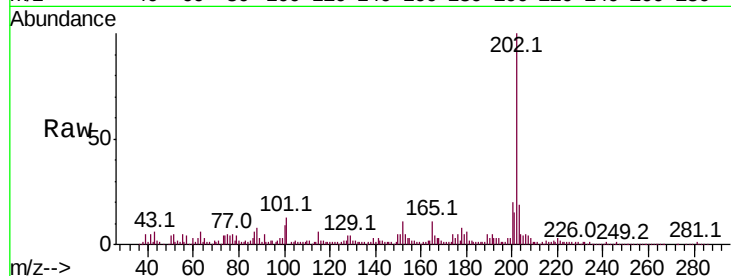

#79
Pyrene
Concen: 12.352 ng/ul
RT: 19.28 min Scan# 2770
Delta R.T. -0.00 min
Lab File: BN009455.D
Acq: 28 Jan 2020 17:37

Tgt Ion:	202	Resp:	717559
Ion	Ratio	Lower	Upper
202	100		
101	14.5	10.9	16.3
100	11.6	8.6	12.8

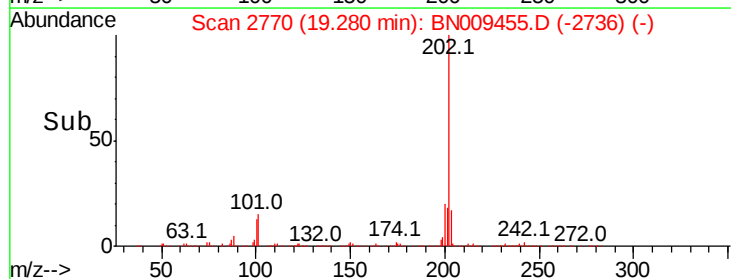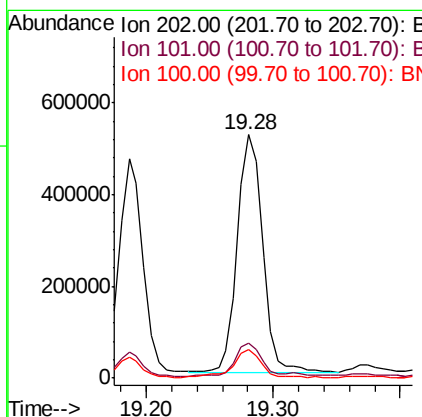

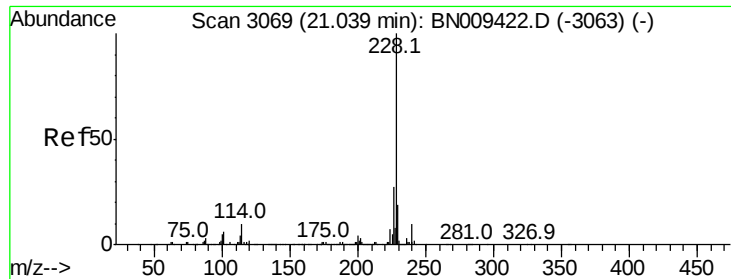

#82

Benzo(a)anthracene

Concen: 3.614 ng/ul

RT: 21.05 min Scan# 3070

Delta R.T. 0.01 min

Lab File: BN009455.D

Acq: 28 Jan 2020 17:37

Instrument :

BNA_N

ClientSampleId :





Tot Ion:228 Resp: 197432

Ion Ratio Lower Upper

228 100

229 33.2 15.9 23.9#

226 120.7 20.9 31.3#

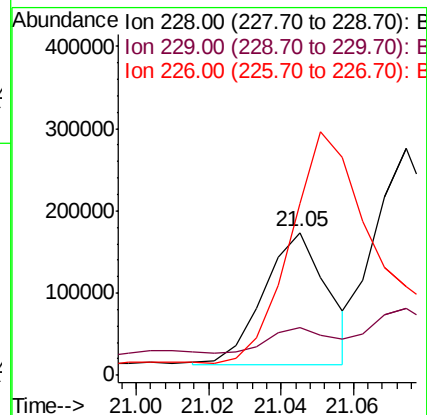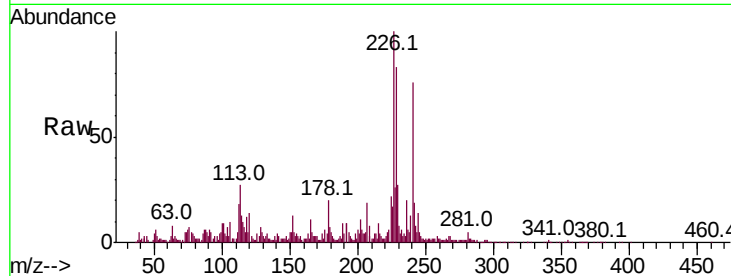

#84

Chrysene

Concen: 7.714 ng/ul

RT: 21.07 min Scan# 3075

Delta R.T. -0.02 min

Lab File: BN009455.D

Acq: 28 Jan 2020 17:37




Tgt Ion:228 Resp: 410569


Ion Ratio Lower Upper

228 100

226 39.1 22.9 34.3#

229 29.7 15.4 23.0#

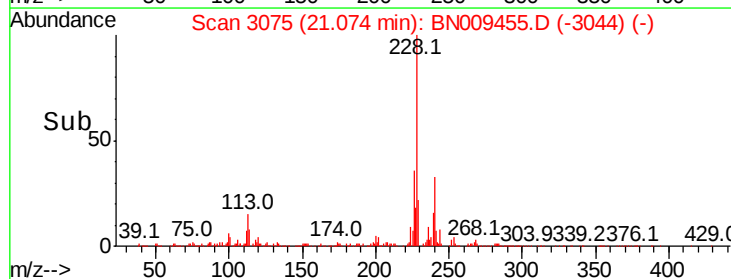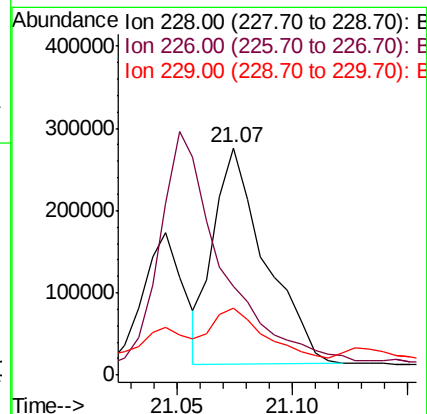



#87

Benzo(b)fluoranthene

Concen: 20.054 ng/ul

RT: 22.56 min Scan# 3328

Delta R.T. 0.01 min

Lab File: BN009455.D

Acq: 28 Jan 2020 17:37


Instrument :

BNA_N

ClientSampleId :

Tot Ion:252 Resp: 1142727




Ion	Ratio	Lower	Upper
252	100		
253	23.9	16.5	24.7
125	11.6	8.2	12.2



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

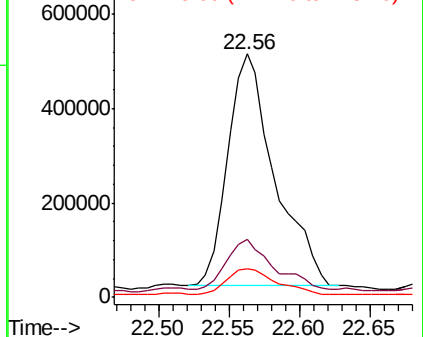

#88

Benzo(k)fluoranthene

Concen: 20.395 ng/ul

RT: 22.56 min Scan# 3328


Delta R.T. -0.03 min

Lab File: BN009455.D

Acq: 28 Jan 2020 17:37

Tgt Ion:252 Resp: 1142727



Ion	Ratio	Lower	Upper
252	100		
253	23.9	17.0	25.4
125	11.6	7.8	11.8




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

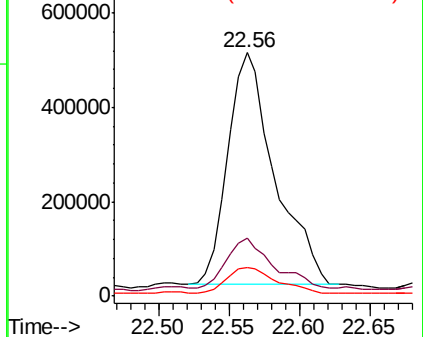



#90

Benzo(a)pyrene

Concen: 23.683 ng/ul

RT: 23.09 min Scan# 3418

Delta R.T. 0.01 min

Lab File: BN009455.D

Acq: 28 Jan 2020 17:37


Instrument :

BNA_N

ClientSampled :

Tot Ion:252 Resp: 1211347

Ion	Ratio	Lower	Upper
252	100		
253	23.5	18.0	27.0
125	12.4	9.8	14.6






Abundance

Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

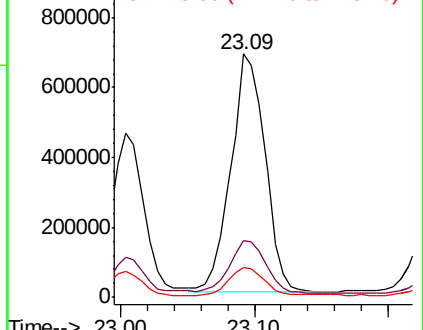

#91

Indeno(1,2,3-cd)pyrene

Concen: 14.178 ng/ul

RT: 25.26 min Scan# 3787


Delta R.T. 0.02 min

Lab File: BN009455.D

Acq: 28 Jan 2020 17:37

Tgt Ion:276 Resp: 878815

Ion	Ratio	Lower	Upper
276	100		
138	32.1	21.4	32.0#
277	25.6	20.4	30.6






Abundance

Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

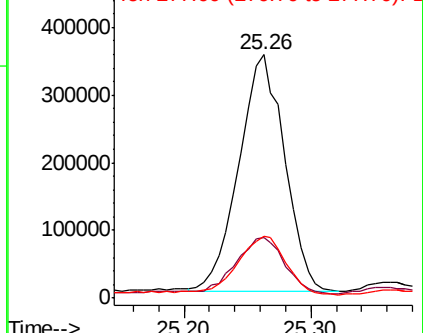




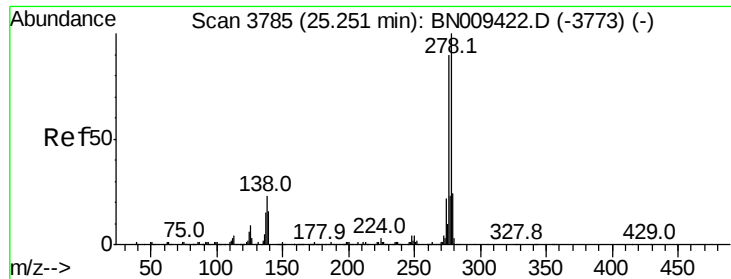


#92

Dibenzo(a,h)anthracene
Concen: 6.028 ng/ul
RT: 25.26 min Scan# 3787
Delta R.T. 0.01 min
Lab File: BN009455.D
Acq: 28 Jan 2020 17:37

Instrument :
BNA_N
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
278	100		
139	22.3	13.9	20.9#
279	31.2	19.3	28.9#

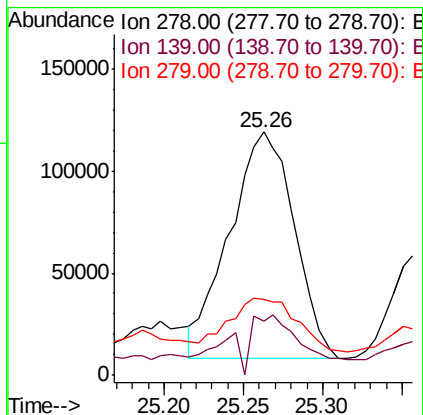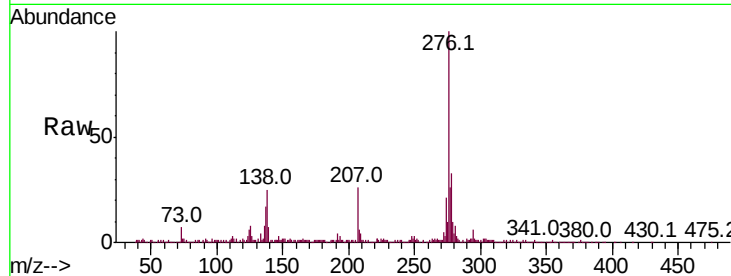

#93

Benzo(g,h,i)perylene
Concen: 13.811 ng/ul
RT: 25.90 min Scan# 3895
Delta R.T. 0.02 min
Lab File: BN009455.D
Acq: 28 Jan 2020 17:37

Tgt Ion	Ratio	Lower	Upper
276	100		
138	23.3	16.6	24.8
277	23.9	18.7	28.1

