

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN012820\
 Data File : BN009454.D
 Acq On : 28 Jan 2020 17:01
 Operator : CG/JU
 Sample : L1193-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GASP2

Quant Time: Jan 28 17:57:25 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 22 15:13:20 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	169475	20.00	ng/ul	0.00
18) Naphthalene-d8	10.21	136	729089	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.09	164	435731	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.85	188	869993	20.00	ng/ul	0.00
77) Chrysene-d12	21.06	240	742938	20.00	ng/ul	0.00
85) Perylene-d12	23.17	264	786363	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.09	96	12978	3.17	ng/uL	0.00
5) Phenol-d5	6.66	99	270085	17.97	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.81	67	210001	19.68	ng/ul	0.00
9) 2-Chlorophenol-d4	7.00	132	219774	20.03	ng/ul	0.00
13) 4-Methylphenol-d8	8.17	113	225621	18.86	ng/ul	0.00
19) Nitrobenzene-d5	8.60	128	117191	22.10	ng/ul	0.00
22) 2-Nitrophenol-d4	9.31	143	131096	23.57	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.85	165	207300	18.80	ng/ul	0.00
29) 4-Chloroaniline-d4	10.36	131	296106	22.24	ng/ul	0.00
43) Dimethylphthalate-d6	13.52	166	796435	24.70	ng/ul	0.00
46) Acenaphthylene-d8	13.78	160	780944	20.40	ng/ul	0.00
51) 4-Nitrophenol-d4	14.32	143	121911	20.31	ng/ul	0.00
57) Fluorene-d10	15.10	176	599471	21.18	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.23	200	106892	20.29	ng/ul	0.00
70) Anthracene-d10	16.95	188	929506	23.09	ng/ul	0.00
78) Pyrene-d10	19.25	212	981653	24.56	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.04	264	913714	23.02	ng/ul	0.00


Target Compounds					Ovalue	
44) Dimethylphthalate	13.56	163	130497	3.931	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN012820\
Data File : BN009454.D
Acq On : 28 Jan 2020 17:01
Operator : CG/JU
Sample : L1193-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GASP2

Quant Time: Jan 28 17:57:25 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 22 15:13:20 2020
Response via : Initial Calibration

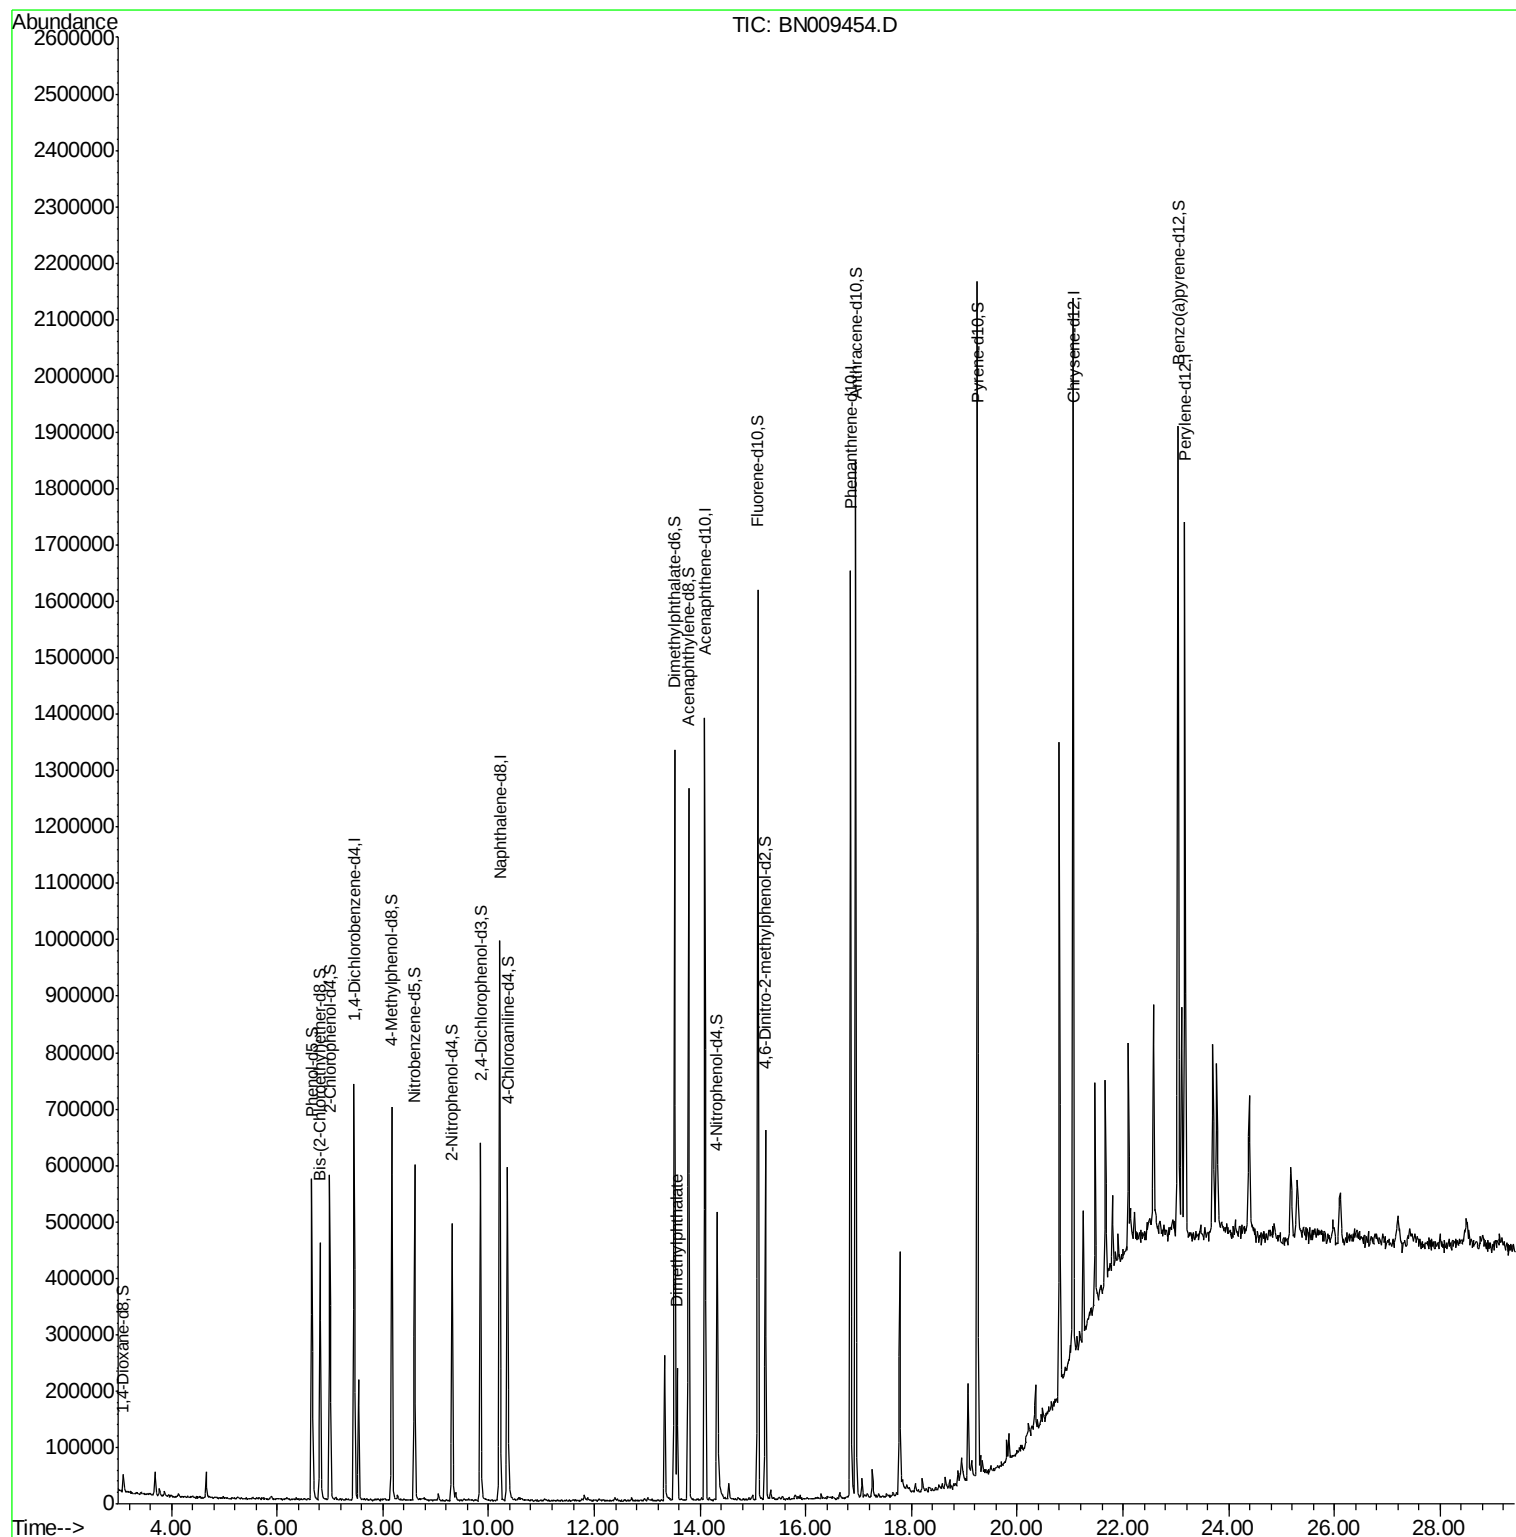

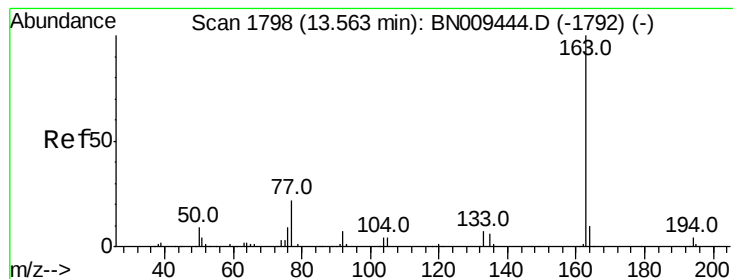

#44

Dimethylphthalate

Concen: 3.931 ng/ul

RT: 13.56 min Scan# 1798

Delta R.T. -0.01 min

Lab File: BN009454.D

Acq: 28 Jan 2020 17:01

Instrument :

BNA_N

ClientSampleId :

GASP2



Tot Ion:163 Resp: 130497

Ion Ratio Lower Upper

163 100

194 4.0 3.1 4.7

164 10.3 8.3 12.5

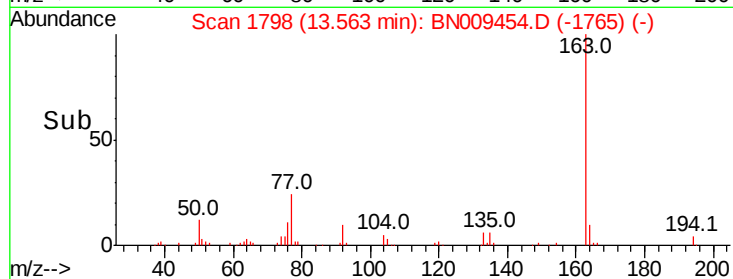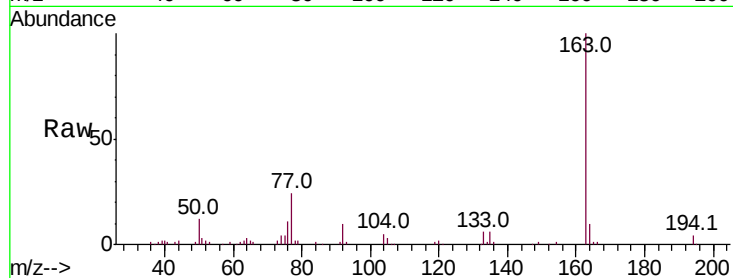

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

