

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN012820\
 Data File : BN009445.D
 Acq On : 28 Jan 2020 11:24
 Operator : CG/JU
 Sample : L1250-05
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012220MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.069	12	14	18	rVB4	4075	3475	0.19%	0.038%
2	3.487	83	85	89	rBV4	2947	2266	0.12%	0.025%
3	3.705	119	122	123	rBV3	1906	2124	0.11%	0.023%
4	3.775	129	134	140	rBV6	9335	12948	0.69%	0.142%
5	3.899	153	155	157	rBV2	3374	3058	0.16%	0.034%
6	4.005	171	173	177	rVB4	2558	2508	0.13%	0.028%
7	4.216	206	209	210	rBV2	4677	3002	0.16%	0.033%
8	4.387	236	238	243	rVB5	3152	4202	0.22%	0.046%
9	4.452	246	249	253	rVB4	1952	2734	0.15%	0.030%
10	4.810	307	310	313	rVB4	2424	2597	0.14%	0.029%
11	5.040	347	349	351	rVB3	2436	2021	0.11%	0.022%
12	5.163	368	370	374	rVB4	2266	2826	0.15%	0.031%
13	5.210	376	378	381	rBV4	1826	2239	0.12%	0.025%
14	5.346	397	401	402	rBV3	1630	2096	0.11%	0.023%
15	5.399	407	410	414	rVB4	1916	2224	0.12%	0.024%
16	5.534	428	433	436	rVB5	1663	2715	0.14%	0.030%
17	5.628	445	449	450	rBV2	2507	3073	0.16%	0.034%
18	5.746	467	469	471	rVB3	2383	2105	0.11%	0.023%
19	5.810	478	480	484	rVV4	2427	2657	0.14%	0.029%
20	5.846	484	486	488	rVB3	2075	1882	0.10%	0.021%
21	5.999	508	512	514	rVB4	2837	3039	0.16%	0.033%
22	6.081	522	526	527	rVV4	2020	2536	0.14%	0.028%
23	6.093	527	528	531	rVB3	3215	2047	0.11%	0.023%
24	6.204	545	547	552	rBV3	1578	2416	0.13%	0.027%
25	7.034	687	688	691	rBV3	2273	2220	0.12%	0.024%
26	7.140	700	706	707	rBV3	1518	2332	0.12%	0.026%
27	7.157	707	709	713	rVB3	1987	2449	0.13%	0.027%
28	7.457	754	760	771	rBV	511085	829494	44.23%	9.125%
29	7.604	782	785	790	rVB3	1938	3382	0.18%	0.037%
30	7.646	790	792	794	rBV3	2386	1890	0.10%	0.021%
31	7.798	815	818	820	rBV2	2314	2550	0.14%	0.028%
32	7.998	851	852	856	rBV3	1944	2697	0.14%	0.030%
33	8.428	921	925	926	rBV3	1626	1882	0.10%	0.021%
34	9.193	1052	1055	1058	rBV2	2033	2273	0.12%	0.025%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN012820\
 Data File : BN009445.D
 Acq On : 28 Jan 2020 11:24
 Operator : CG/JU
 Sample : L1250-05
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012220MA.M
 Title : SVOA CALIBRATION

35	9.522	1107	1111	1116	rVB5	1867	3589	0.19%	0.039%
36	9.640	1128	1131	1134	rBV4	2161	2489	0.13%	0.027%
37	9.845	1162	1166	1171	rBV3	2691	4837	0.26%	0.053%
38	10.022	1193	1196	1199	rBV2	1602	1992	0.11%	0.022%
39	10.210	1219	1228	1243	rBV	652166	1137066	60.63%	12.509%
40	10.740	1315	1318	1321	rBV4	1722	2479	0.13%	0.027%
41	10.998	1359	1362	1364	rBV3	1475	2167	0.12%	0.024%
42	11.092	1375	1378	1382	rBV5	1714	2004	0.11%	0.022%
43	11.445	1435	1438	1440	rBV2	1360	2055	0.11%	0.023%
44	11.545	1453	1455	1458	rVB4	2015	2159	0.12%	0.024%
45	11.581	1458	1461	1464	rBV3	1467	2627	0.14%	0.029%
46	11.645	1470	1472	1475	rBV2	1908	2321	0.12%	0.026%
47	11.669	1475	1476	1479	rBV3	1780	1952	0.10%	0.021%
48	12.939	1688	1692	1695	rVB2	1345	2288	0.12%	0.025%
49	12.975	1695	1698	1702	rBV3	1688	2305	0.12%	0.025%
50	13.039	1706	1709	1712	rVB3	2241	2871	0.15%	0.032%
51	13.081	1712	1716	1718	rBV4	1482	2304	0.12%	0.025%
52	13.769	1831	1833	1837	rVB2	1748	2124	0.11%	0.023%
53	13.886	1850	1853	1854	rVB	2652	2046	0.11%	0.023%
54	13.933	1857	1861	1867	rVB4	2413	5188	0.28%	0.057%
55	13.986	1867	1870	1873	rBV4	2394	3993	0.21%	0.044%
56	14.092	1882	1888	1904	rBV2	949389	1490545	79.48%	16.398%
57	14.439	1944	1947	1950	rVB3	2743	2840	0.15%	0.031%
58	14.475	1950	1953	1954	rBV	2045	2306	0.12%	0.025%
59	14.528	1959	1962	1963	rVV2	2705	2294	0.12%	0.025%
60	14.580	1966	1971	1974	rVV2	2165	3444	0.18%	0.038%
61	15.016	2044	2045	2051	rBV4	1660	2646	0.14%	0.029%
62	15.716	2162	2164	2169	rBV4	1550	2617	0.14%	0.029%
63	15.833	2182	2184	2187	rBV3	2468	2140	0.11%	0.024%
64	15.892	2193	2194	2197	rVB2	2428	2021	0.11%	0.022%
65	16.151	2236	2238	2242	rVB3	3812	4022	0.21%	0.044%
66	16.198	2242	2246	2248	rBV3	2706	4547	0.24%	0.050%
67	16.322	2265	2267	2269	rVB3	2514	2209	0.12%	0.024%
68	16.374	2274	2276	2279	rVB	2702	2847	0.15%	0.031%
69	16.410	2279	2282	2284	rBV3	1756	2000	0.11%	0.022%
70	16.616	2313	2317	2318	rBV4	1817	2631	0.14%	0.029%
71	16.639	2318	2321	2323	rVB2	2697	3184	0.17%	0.035%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN012820\
 Data File : BN009445.D
 Acq On : 28 Jan 2020 11:24
 Operator : CG/JU
 Sample : L1250-05
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012220MA.M
 Title : SVOA CALIBRATION

72	16.845	2350	2356	2373	rBV	1152026	1737958	92.67%	19.120%
73	17.210	2416	2418	2421	rVB3	2773	2618	0.14%	0.029%
74	17.304	2431	2434	2435	rBV2	2237	1893	0.10%	0.021%
75	17.569	2478	2479	2484	rBV3	2064	2792	0.15%	0.031%
76	17.627	2487	2489	2493	rVV3	2062	2092	0.11%	0.023%
77	17.786	2514	2516	2518	rVV2	1975	1944	0.10%	0.021%
78	17.851	2524	2527	2531	rBV3	2893	3627	0.19%	0.040%
79	17.892	2533	2534	2538	rBV3	2515	2343	0.12%	0.026%
80	17.933	2538	2541	2542	rVB3	2661	2425	0.13%	0.027%
81	17.980	2548	2549	2553	rBV4	3666	3344	0.18%	0.037%
82	18.427	2622	2625	2629	rBV4	3757	5305	0.28%	0.058%
83	18.569	2648	2649	2653	rVB4	3619	2034	0.11%	0.022%
84	18.921	2708	2709	2711	rBV2	4060	3180	0.17%	0.035%
85	19.074	2733	2735	2736	rBV3	4073	2936	0.16%	0.032%
86	19.568	2817	2819	2820	rBV2	4611	2446	0.13%	0.027%
87	21.051	3066	3071	3080	rBV	1466534	1875340	100.00%	20.631%
88	23.168	3425	3431	3443	rVB2	996376	1790499	95.48%	19.698%


Sum of corrected areas: 9089884

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN012820\
Data File : BN009445.D
Acq On : 28 Jan 2020 11:24
Operator : CG/JU
Sample : L1250-05
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

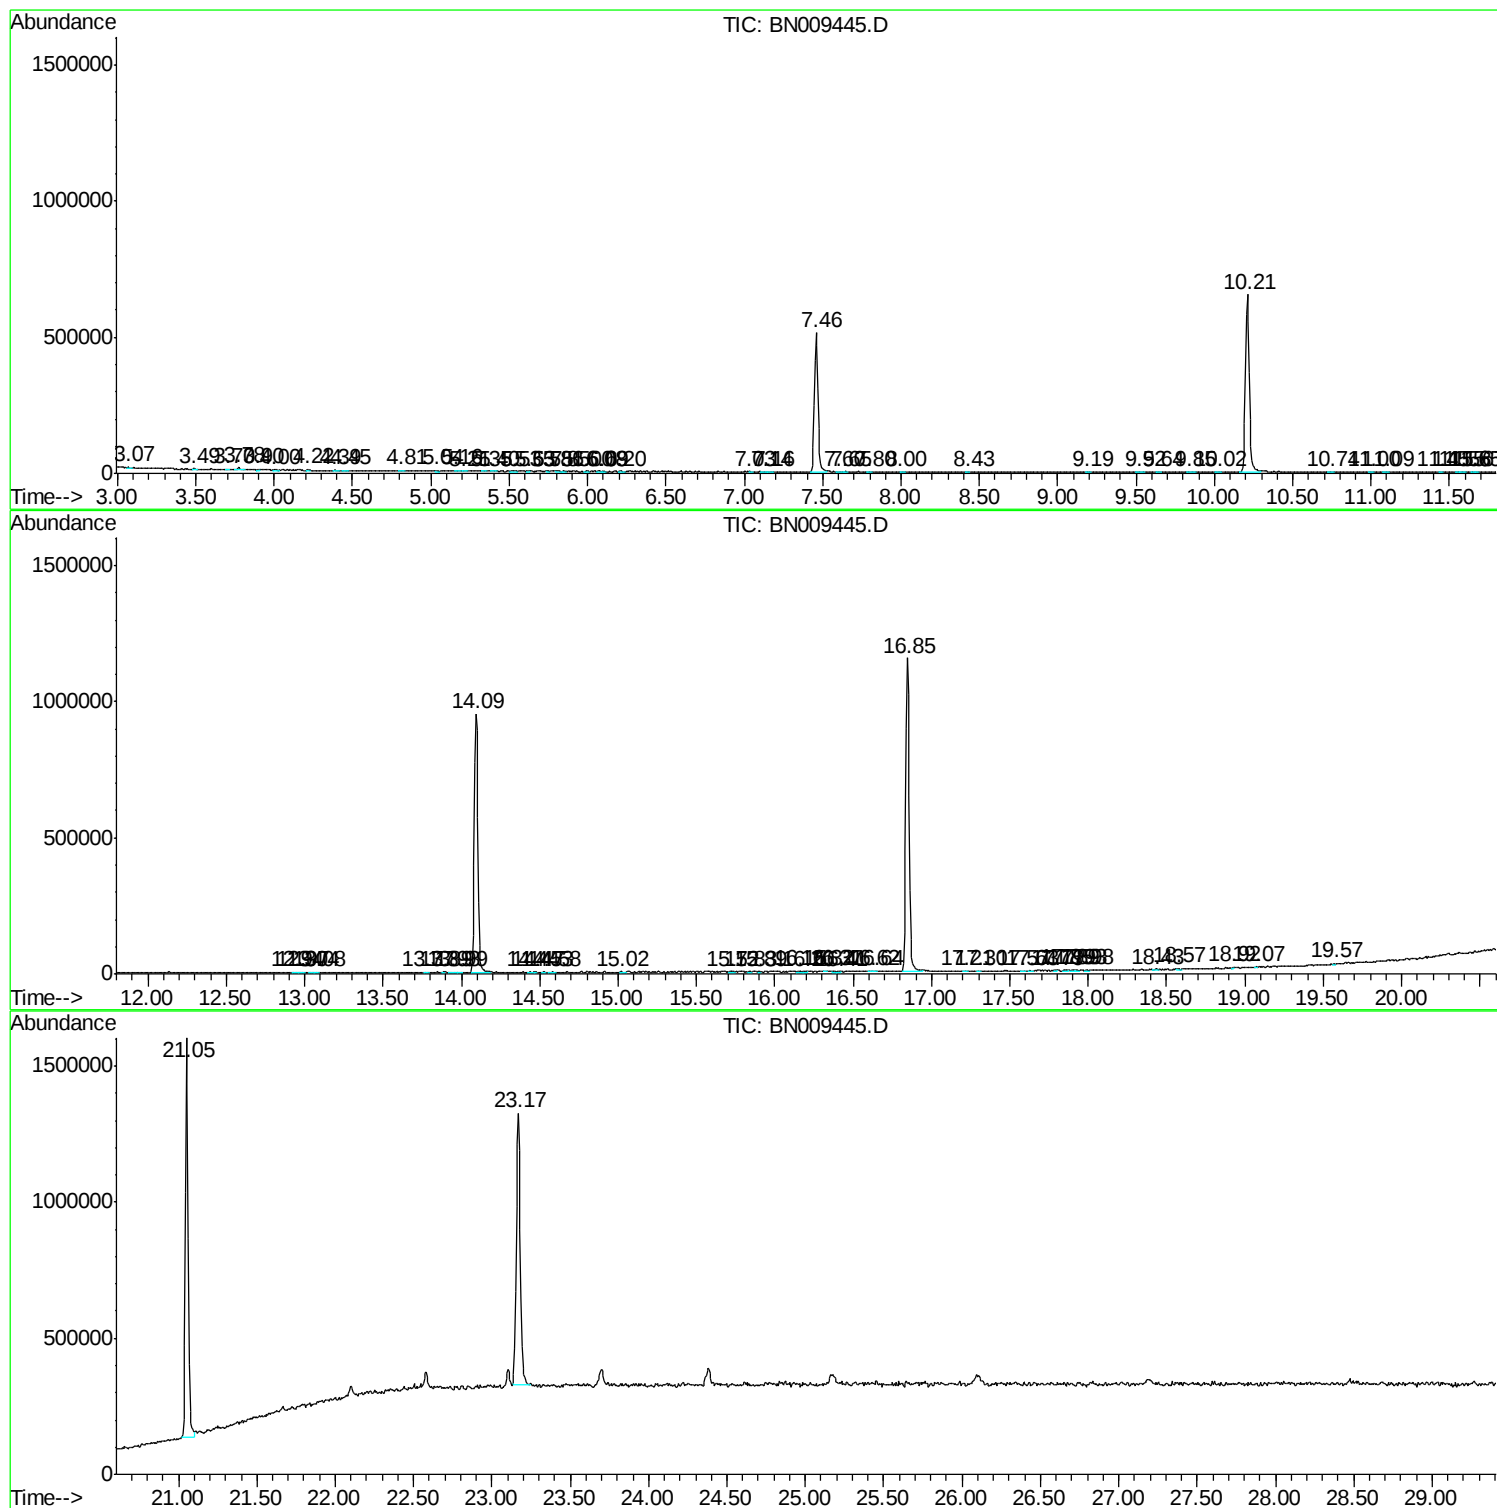

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN012820\
Data_File : BN009445.D
Acq_On : 28-Jan-2020 11:244
Operator : CG/JUU
Sample : L1250-055
Misc :
ALS_Vial : 3 Sample_Multiplier: 11

Instrument :
BNA_N
ClientSampleId :
SVOC-GPC-BLANK

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012220MA.MM
Quant_Title : SVOA_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response		--Internal Standard--	
					#	RT	Resp Conc

No Library Search Compounds Detected
