

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN012820\
 Data File : BN009460.D
 Acq On : 28 Jan 2020 21:13
 Operator : CG/JU
 Sample : TESTBL-2
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 TESTBL-2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012220MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.087	14	17	25	rVB2	28814	40436	1.75%	0.135%
2	3.275	47	49	50	rBV2	3266	2485	0.11%	0.008%
3	3.693	114	120	128	rBV	44407	70922	3.07%	0.236%
4	3.775	131	134	140	rVB2	7259	10581	0.46%	0.035%
5	3.875	147	151	155	rVB5	8178	9988	0.43%	0.033%
6	3.946	160	163	165	rVV3	2295	2797	0.12%	0.009%
7	3.999	169	172	175	rVB5	4884	5234	0.23%	0.017%
8	4.140	193	196	200	rVB4	4478	4699	0.20%	0.016%
9	4.211	206	208	211	rVB3	3427	2958	0.13%	0.010%
10	4.399	236	240	243	rBV5	2743	4041	0.18%	0.013%
11	4.564	266	268	274	rBV6	2248	4136	0.18%	0.014%
12	4.652	279	283	293	rBV	49378	79892	3.46%	0.266%
13	4.905	324	326	329	rBV4	1975	2745	0.12%	0.009%
14	5.052	348	351	352	rBV2	2814	2964	0.13%	0.010%
15	5.246	380	384	386	rBV4	2525	3618	0.16%	0.012%
16	5.893	489	494	498	rBV4	6569	8320	0.36%	0.028%
17	5.952	500	504	507	rBV3	2189	3305	0.14%	0.011%
18	6.111	526	531	535	rVB5	3550	5656	0.24%	0.019%
19	6.652	617	623	634	rBV	466584	765751	33.16%	2.549%
20	6.811	644	650	658	rBV	345975	556490	24.10%	1.852%
21	6.999	676	682	690	rBV	494334	766946	33.22%	2.553%
22	7.105	696	700	703	rBV2	4885	7357	0.32%	0.024%
23	7.458	754	760	771	rVV	650258	1020395	44.19%	3.396%
24	8.169	875	881	892	rBV	556537	900396	39.00%	2.997%
25	8.281	896	900	907	rVB3	15372	24420	1.06%	0.081%
26	8.599	946	954	964	rBV	476637	769235	33.32%	2.560%
27	8.769	980	983	985	rVV3	2452	2654	0.11%	0.009%
28	8.810	989	990	995	rVV4	2190	2468	0.11%	0.008%
29	8.869	995	1000	1002	rVB4	2148	2796	0.12%	0.009%
30	9.057	1030	1032	1036	rVB2	2700	2703	0.12%	0.009%
31	9.310	1068	1075	1085	rBV	382399	635689	27.53%	2.116%
32	9.846	1160	1166	1180	rVV	518108	914777	39.62%	3.045%
33	10.210	1220	1228	1238	rBV	896972	1456346	63.07%	4.847%
34	10.357	1245	1253	1267	rBV	392607	744269	32.23%	2.477%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN012820\
 Data File : BN009460.D
 Acq On : 28 Jan 2020 21:13
 Operator : CG/JU
 Sample : TESTBL-2
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 TESTBL-2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012220MA.M
 Title : SVOA CALIBRATION

35	10.575	1289	1290	1295	rBV4	2407	2719	0.12%	0.009%
36	10.757	1318	1321	1324	rVB3	1982	3059	0.13%	0.010%
37	11.346	1418	1421	1422	rBV2	2563	3052	0.13%	0.010%
38	11.463	1435	1441	1442	rBV3	1985	3614	0.16%	0.012%
39	11.810	1492	1500	1509	rVB6	7153	17030	0.74%	0.057%
40	12.534	1620	1623	1630	rBV4	1413	3282	0.14%	0.011%
41	13.122	1720	1723	1726	rBV3	2167	3527	0.15%	0.012%
42	13.340	1757	1760	1764	rVB3	1634	2761	0.12%	0.009%
43	13.516	1784	1790	1803	rBV	936506	1301826	56.38%	4.333%
44	13.781	1828	1835	1842	rBV	1049623	1515702	65.65%	5.045%
45	14.092	1882	1888	1900	rVB2	1297664	1876282	81.26%	6.245%
46	14.322	1921	1927	1946	rBV	284729	599367	25.96%	1.995%
47	14.545	1961	1965	1969	rBV4	3150	4888	0.21%	0.016%
48	14.616	1975	1977	1979	rBV2	2601	2865	0.12%	0.010%
49	15.098	2052	2059	2066	rBV	1287980	1849848	80.12%	6.157%
50	15.151	2066	2068	2073	rVV3	3648	4638	0.20%	0.015%
51	15.234	2077	2082	2096	rVV	398982	573958	24.86%	1.910%
52	15.339	2096	2100	2108	rVB4	14765	21101	0.91%	0.070%
53	15.545	2132	2135	2139	rBV4	2049	3564	0.15%	0.012%
54	15.816	2180	2181	2185	rBV3	1817	2345	0.10%	0.008%
55	15.851	2185	2187	2189	rVV3	3254	2437	0.11%	0.008%
56	15.887	2189	2193	2195	rVV4	4597	5108	0.22%	0.017%
57	16.422	2281	2284	2287	rBV4	1974	2354	0.10%	0.008%
58	16.639	2317	2321	2327	rBV4	8058	16389	0.71%	0.055%
59	16.845	2350	2356	2363	rBV	1565757	2112406	91.49%	7.030%
60	16.945	2367	2373	2383	rVV2	1462874	2043723	88.51%	6.802%
61	17.063	2392	2393	2397	rVB3	2637	2602	0.11%	0.009%
62	17.122	2400	2403	2405	rBV3	2720	3231	0.14%	0.011%
63	17.357	2439	2443	2444	rBV3	2399	2920	0.13%	0.010%
64	17.386	2444	2448	2451	rVV4	10385	13122	0.57%	0.044%
65	17.557	2474	2477	2481	rBV3	6637	8542	0.37%	0.028%
66	17.639	2488	2491	2494	rBV5	2455	3005	0.13%	0.010%
67	17.681	2496	2498	2500	rBV2	3556	3112	0.13%	0.010%
68	17.728	2505	2506	2509	rVB3	3203	2878	0.12%	0.010%
69	17.775	2511	2514	2518	rVB4	5616	8494	0.37%	0.028%
70	17.839	2522	2525	2527	rVV3	2727	3379	0.15%	0.011%
71	18.075	2560	2565	2569	rBV	16059	20550	0.89%	0.068%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN012820\
 Data File : BN009460.D
 Acq On : 28 Jan 2020 21:13
 Operator : CG/JU
 Sample : TESTBL-2
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 TESTBL-2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012220MA.M
 Title : SVOA CALIBRATION

72	18.157	2577	2579	2581	rBV2	3357	3289	0.14%	0.011%
73	18.333	2606	2609	2610	rBV3	4661	5118	0.22%	0.017%
74	18.545	2643	2645	2647	rBV3	3549	3806	0.16%	0.013%
75	18.645	2659	2662	2665	rBV6	5658	8002	0.35%	0.027%
76	18.710	2668	2673	2675	rBV4	19885	36035	1.56%	0.120%
77	18.769	2681	2683	2684	rBV2	4730	4175	0.18%	0.014%
78	18.786	2684	2686	2687	rVV2	4935	3870	0.17%	0.013%
79	18.822	2690	2692	2695	rVV3	5587	6880	0.30%	0.023%
80	18.880	2698	2702	2706	rBV3	17826	27548	1.19%	0.092%
81	19.069	2732	2734	2736	rBV3	4253	4354	0.19%	0.014%
82	19.139	2743	2746	2750	rVB2	10376	13451	0.58%	0.045%
83	19.180	2750	2753	2754	rBV3	4464	4241	0.18%	0.014%
84	19.251	2757	2765	2772	rBV	1745383	2308932	100.00%	7.685%
85	19.304	2772	2774	2777	rVB3	15162	14753	0.64%	0.049%
86	20.998	3060	3062	3066	rBV3	36099	43729	1.89%	0.146%
87	21.051	3066	3071	3080	rVV	1659752	2189043	94.81%	7.286%
88	22.098	3247	3249	3255	rVB2	91404	111046	4.81%	0.370%
89	22.574	3327	3330	3336	rVB2	114019	170055	7.37%	0.566%
90	23.039	3403	3409	3416	rBV	1235954	2102534	91.06%	6.998%
91	23.174	3425	3432	3438	rBV	1180298	2098437	90.88%	6.984%


Sum of corrected areas: 30046447

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN012820\
Data File : BN009460.D
Acq On : 28 Jan 2020 21:13
Operator : CG/JU
Sample : TESTBL-2
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
TESTBL-2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

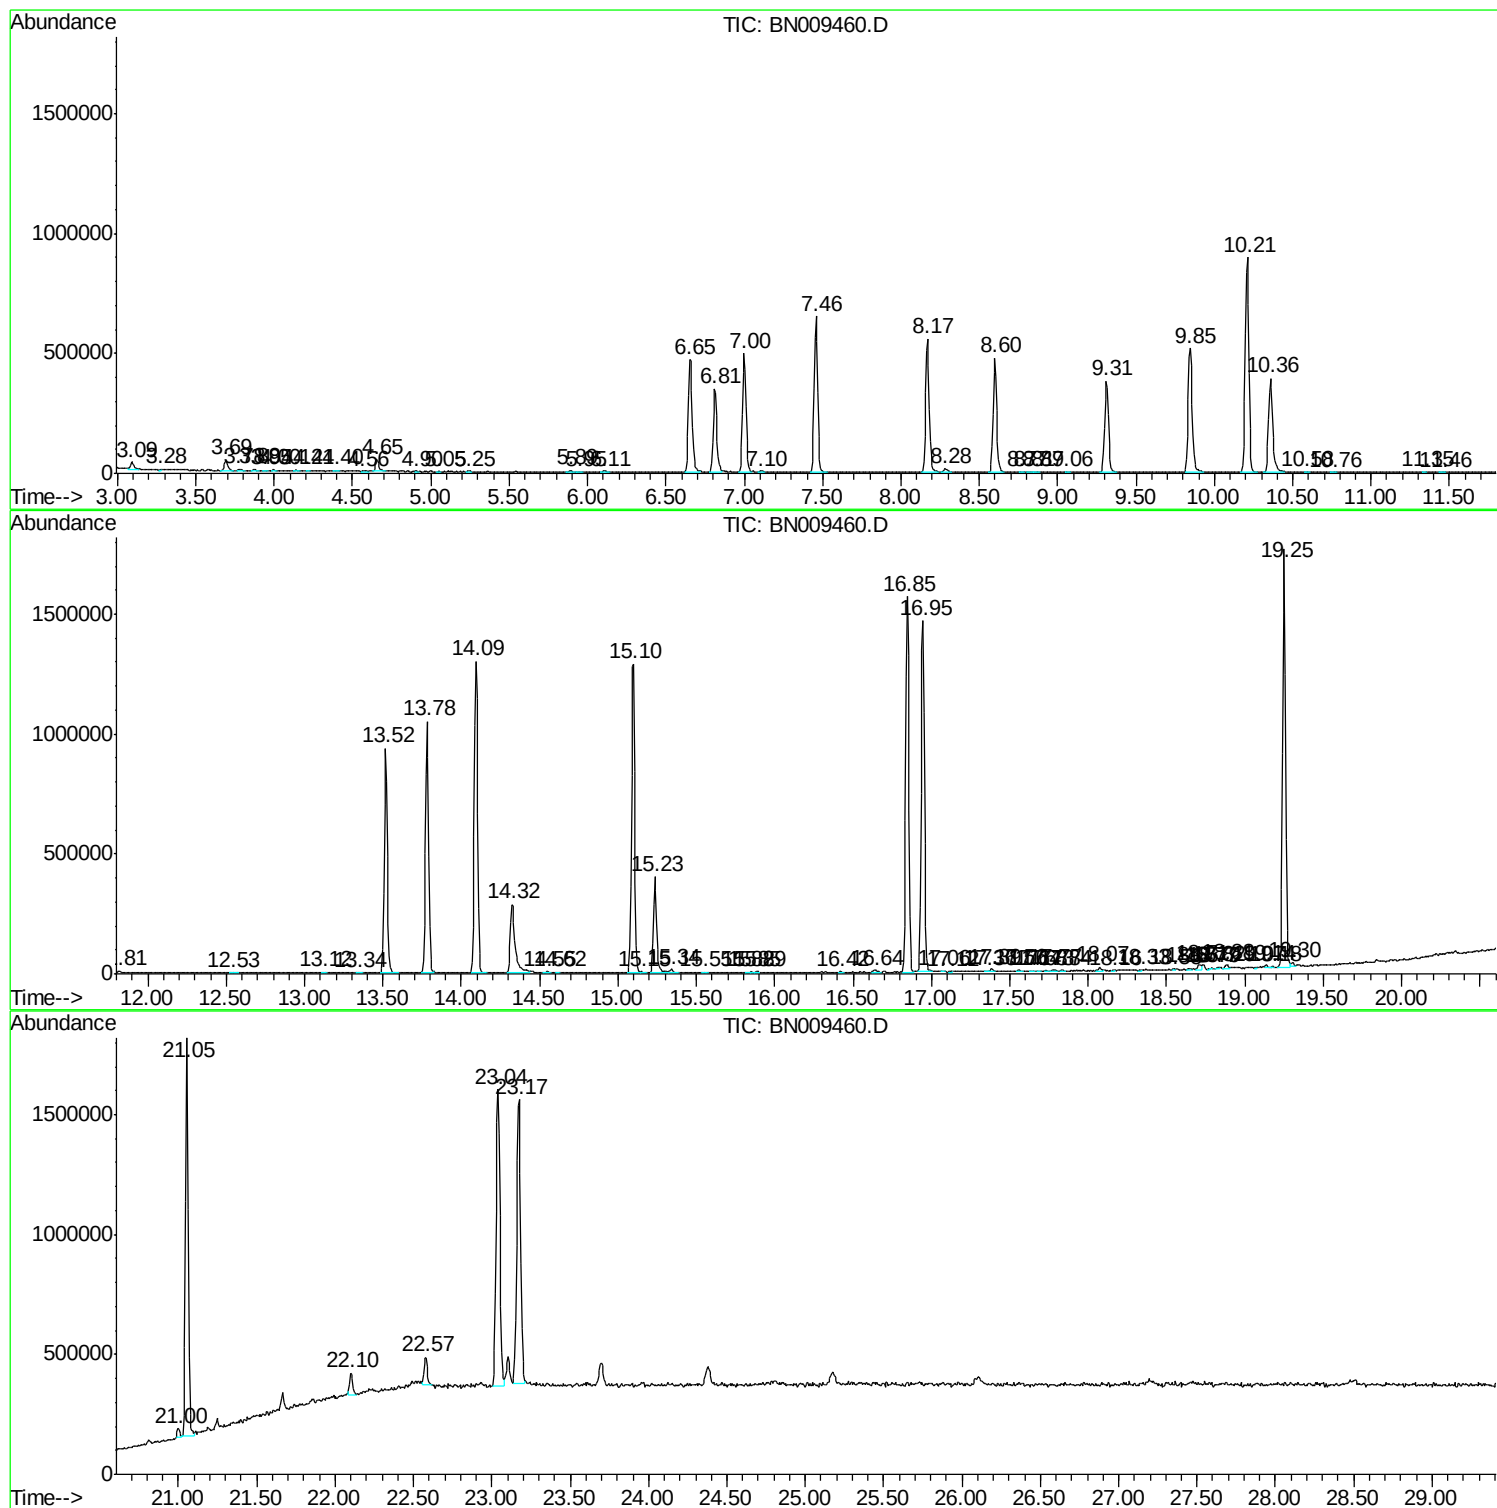

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN012820\
Data_File : BN009460.D
Acq_On : 28-Jan-2020 21:133
Operator : CG/JUU
Sample : TESTBL-22
Misc :
ALS_Vial : 17 Sample_Multiplier: 11

Instrument :
BNA_N
ClientSampleId :
TESTBL-2

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012220MA.MM
Quant_Title : SVOA_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
