

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN012820\
 Data File : BN009462.D
 Acq On : 28 Jan 2020 22:24
 Operator : CG/JU
 Sample : PB126330BL
 Misc : GCMS CONFIRMATION
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK30

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012220MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.323	54	57	61	rVV4	6163	7096	0.37%	0.072%
2	3.770	129	133	137	rVB3	9724	11943	0.63%	0.122%
3	3.846	143	146	149	rBV4	1879	2845	0.15%	0.029%
4	3.975	165	168	172	rBV5	2218	3000	0.16%	0.031%
5	4.393	234	239	241	rBV3	2493	3993	0.21%	0.041%
6	4.499	254	257	259	rVB3	2297	3054	0.16%	0.031%
7	4.522	259	261	262	rBV2	2360	1911	0.10%	0.019%
8	4.681	286	288	294	rBV4	3751	7646	0.40%	0.078%
9	5.264	384	387	389	rBV2	2433	2635	0.14%	0.027%
10	5.387	405	408	410	rBV3	1396	2186	0.11%	0.022%
11	5.605	443	445	449	rVB3	1819	1938	0.10%	0.020%
12	5.769	471	473	475	rBV3	2589	2405	0.13%	0.025%
13	5.875	489	491	494	rBV3	1647	1961	0.10%	0.020%
14	5.969	504	507	509	rBV4	1882	2108	0.11%	0.021%
15	6.399	577	580	584	rVV5	1455	2284	0.12%	0.023%
16	6.599	612	614	617	rBV3	1301	2032	0.11%	0.021%
17	7.452	753	759	772	rBV	707244	1107752	57.98%	11.296%
18	7.534	772	773	777	rVB2	2346	2216	0.12%	0.023%
19	7.687	795	799	803	rBV3	1650	3118	0.16%	0.032%
20	8.887	998	1003	1007	rBV4	1470	2734	0.14%	0.028%
21	10.210	1220	1228	1238	rBV	860263	1445316	75.65%	14.738%
22	10.275	1238	1239	1243	rVB3	2685	2159	0.11%	0.022%
23	10.634	1295	1300	1301	rBV2	1855	2185	0.11%	0.022%
24	10.810	1327	1330	1333	rVB2	1579	2079	0.11%	0.021%
25	10.840	1333	1335	1339	rBV2	1404	2058	0.11%	0.021%
26	11.199	1394	1396	1399	rVB2	1694	2105	0.11%	0.021%
27	11.240	1399	1403	1404	rBV2	1571	1937	0.10%	0.020%
28	11.316	1413	1416	1420	rBV3	1788	2894	0.15%	0.030%
29	11.452	1435	1439	1441	rVB2	1661	2036	0.11%	0.021%
30	14.093	1881	1888	1895	rBV2	1177747	1710269	89.52%	17.440%
31	14.322	1925	1927	1931	rBV2	1827	2055	0.11%	0.021%
32	14.440	1943	1947	1950	rBV3	1588	2066	0.11%	0.021%
33	15.645	2149	2152	2154	rBV3	1391	1955	0.10%	0.020%
34	15.857	2187	2188	2191	rBV2	2507	2435	0.13%	0.025%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN012820\
 Data File : BN009462.D
 Acq On : 28 Jan 2020 22:24
 Operator : CG/JU
 Sample : PB126330BL
 Misc : GCMS CONFIRMATION
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK30

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012220MA.M
 Title : SVOA CALIBRATION

35	15.916	2195	2198	2200	rBV2	1920	2216	0.12%	0.023%
36	16.634	2317	2320	2322	rBV4	6100	6160	0.32%	0.063%
37	16.698	2327	2331	2333	rVV3	1998	3411	0.18%	0.035%
38	16.734	2335	2337	2341	rVB3	1658	2439	0.13%	0.025%
39	16.845	2350	2356	2369	rBV	1354788	1910515	100.00%	19.482%
40	16.945	2370	2373	2378	rVB4	3844	5336	0.28%	0.054%
41	17.028	2385	2387	2389	rVB2	3258	2020	0.11%	0.021%
42	17.092	2396	2398	2401	rBV3	1775	2625	0.14%	0.027%
43	17.210	2413	2418	2420	rVB4	1889	2888	0.15%	0.029%
44	17.228	2420	2421	2423	rBV	2379	2003	0.10%	0.020%
45	17.422	2450	2454	2456	rBV4	2559	2943	0.15%	0.030%
46	17.498	2464	2467	2468	rVB3	2373	2189	0.11%	0.022%
47	17.516	2468	2470	2472	rBV2	2632	2945	0.15%	0.030%
48	17.604	2483	2485	2488	rVB3	2631	2012	0.11%	0.021%
49	17.734	2505	2507	2509	rBV2	2387	1918	0.10%	0.020%
50	17.769	2512	2513	2515	rVV2	2538	2399	0.13%	0.024%
51	18.075	2562	2565	2568	rBV4	2185	2808	0.15%	0.029%
52	18.145	2575	2577	2579	rVB3	2851	1974	0.10%	0.020%
53	18.257	2594	2596	2599	rVB3	2746	2365	0.12%	0.024%
54	18.392	2618	2619	2622	rBV2	2210	2432	0.13%	0.025%
55	18.575	2648	2650	2654	rBV4	2237	2522	0.13%	0.026%
56	18.663	2663	2665	2668	rBV4	2339	3030	0.16%	0.031%
57	18.722	2674	2675	2677	rBV2	3764	3171	0.17%	0.032%
58	18.916	2707	2708	2710	rBV2	4134	3310	0.17%	0.034%
59	18.975	2715	2718	2719	rVB3	3780	3346	0.18%	0.034%
60	19.216	2757	2759	2760	rBV2	3665	2507	0.13%	0.026%
61	19.233	2760	2762	2763	rBV	5861	3651	0.19%	0.037%
62	19.281	2768	2770	2774	rVB5	5839	7393	0.39%	0.075%
63	19.381	2785	2787	2790	rBV4	4423	3166	0.17%	0.032%
64	19.539	2812	2814	2815	rBV2	4694	2677	0.14%	0.027%
65	21.051	3066	3071	3079	rBV	1369523	1783560	93.35%	18.188%
66	23.169	3425	3431	3438	rVB	949688	1668075	87.31%	17.010%


Sum of corrected areas: 9806412

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN012820\
Data File : BN009462.D
Acq On : 28 Jan 2020 22:24
Operator : CG/JU
Sample : PB126330BL
Misc : GCMS CONFIRMATION
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK30

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

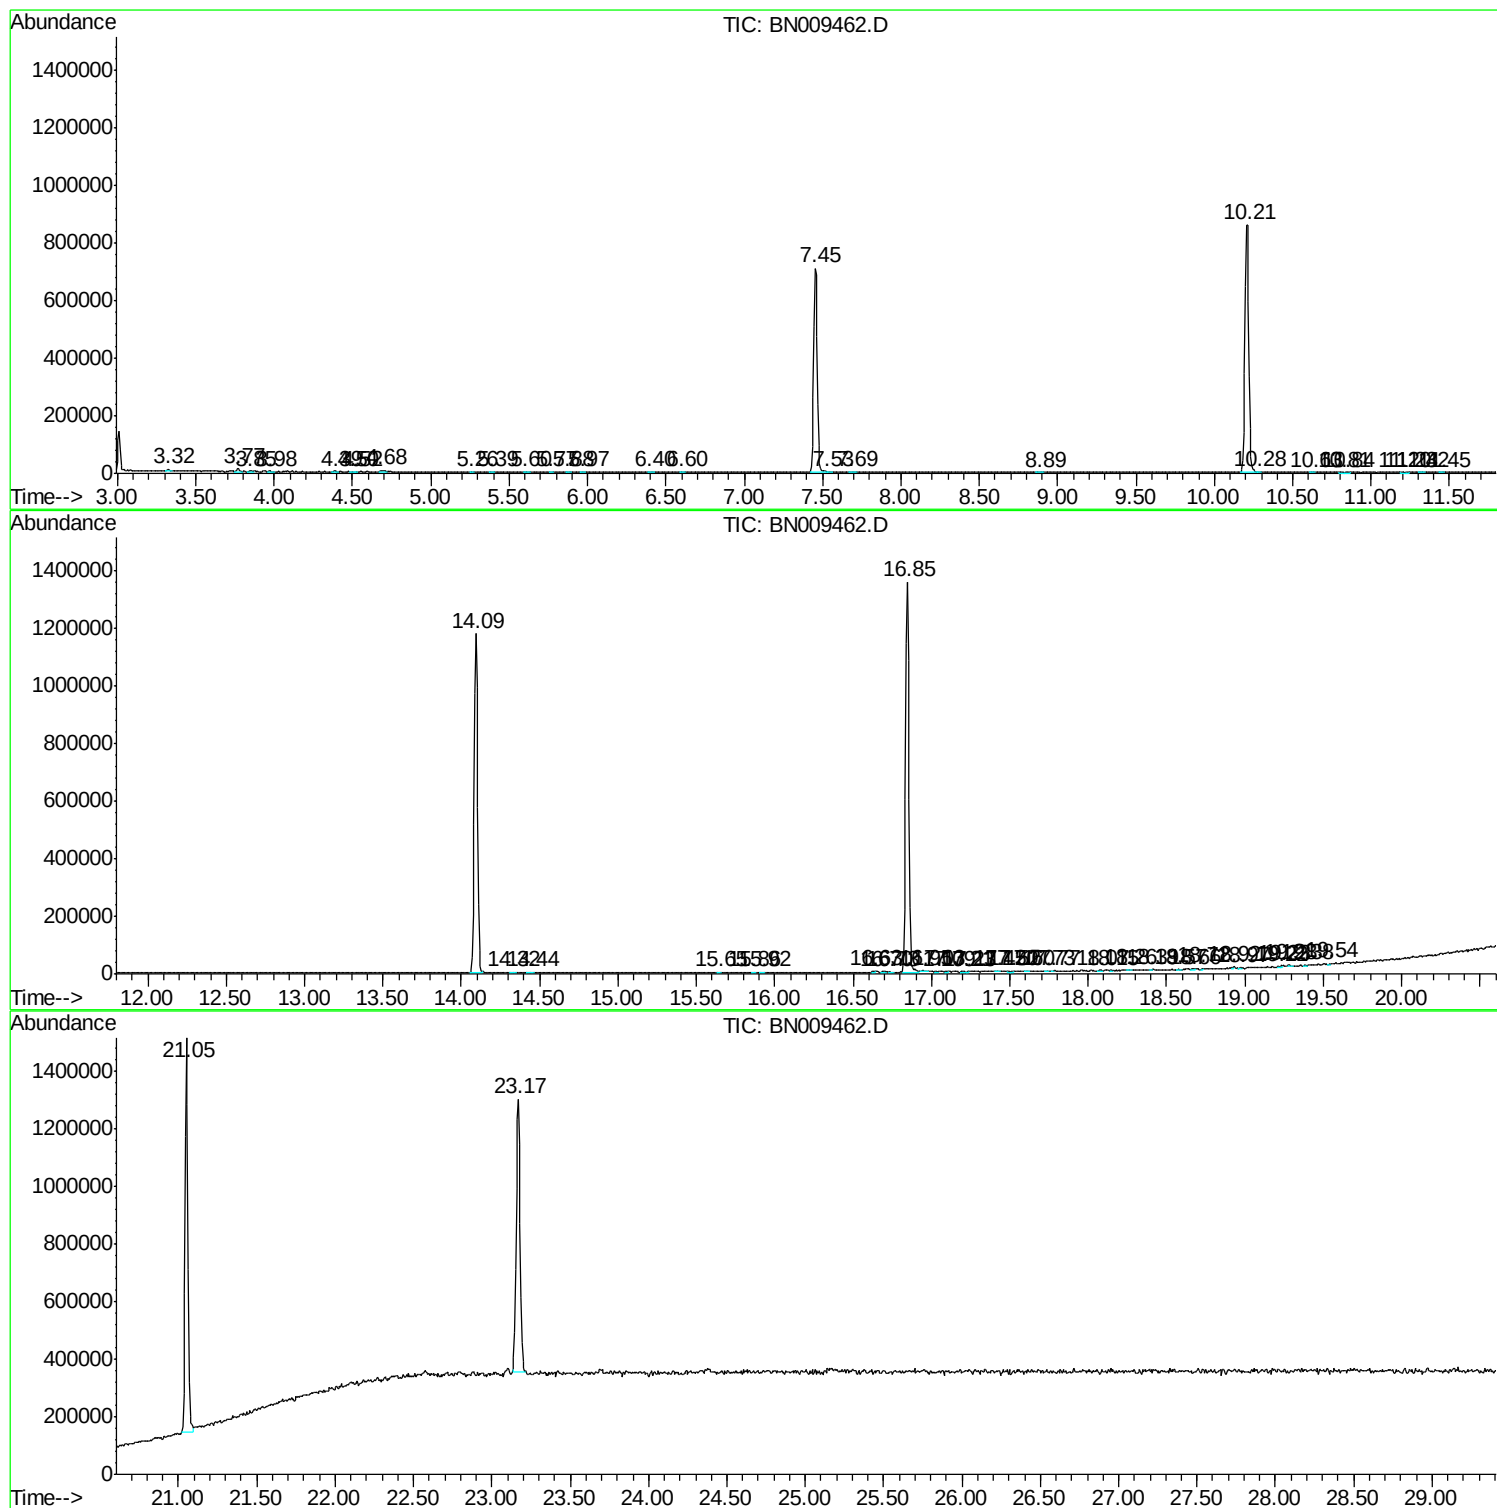

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN012820\
Data File : BN009462.D
Acq On : 28 Jan 2020 22:24
Operator : CG/JU
Sample : PB126330BL
Misc : GCMS CONFIRMATION
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK30

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN012820\
Data File : BN009462.D
Acq On : 28 Jan 2020 22:24
Operator : CG/JU
Sample : PB126330BL
Misc : GCMS CONFIRMATION
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK30

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc