

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012825\
 Data File : BN036090.D
 Acq On : 29 Jan 2025 01:41
 Operator : RC/JU
 Sample : Q1184-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E2948

Quant Time: Jan 29 08:08:06 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 21 23:52:22 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.808	152	3126	0.400	ng/ul	0.00
4) Naphthalene-d8	10.600	136	7470	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.450	164	4812	0.400	ng/ul	0.00
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-17.19
17) Chrysene-d12	21.381	240	10302	0.400	ng/ul	0.00
23) Perylene-d12	23.541	264	640510	0.400	ng/ul	#-0.13
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.272	96	14741	4.307	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.195	152	3483	0.369	ng/ul	0.00
18) Fluoranthene-d10	19.220	212	11277	0.398	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.592	202	1681	0.041	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012825\
Data File : BN036090.D
Acq On : 29 Jan 2025 01:41
Operator : RC/JU
Sample : Q1184-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E2948

Quant Time: Jan 29 08:08:06 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 21 23:52:22 2025
Response via : Initial Calibration

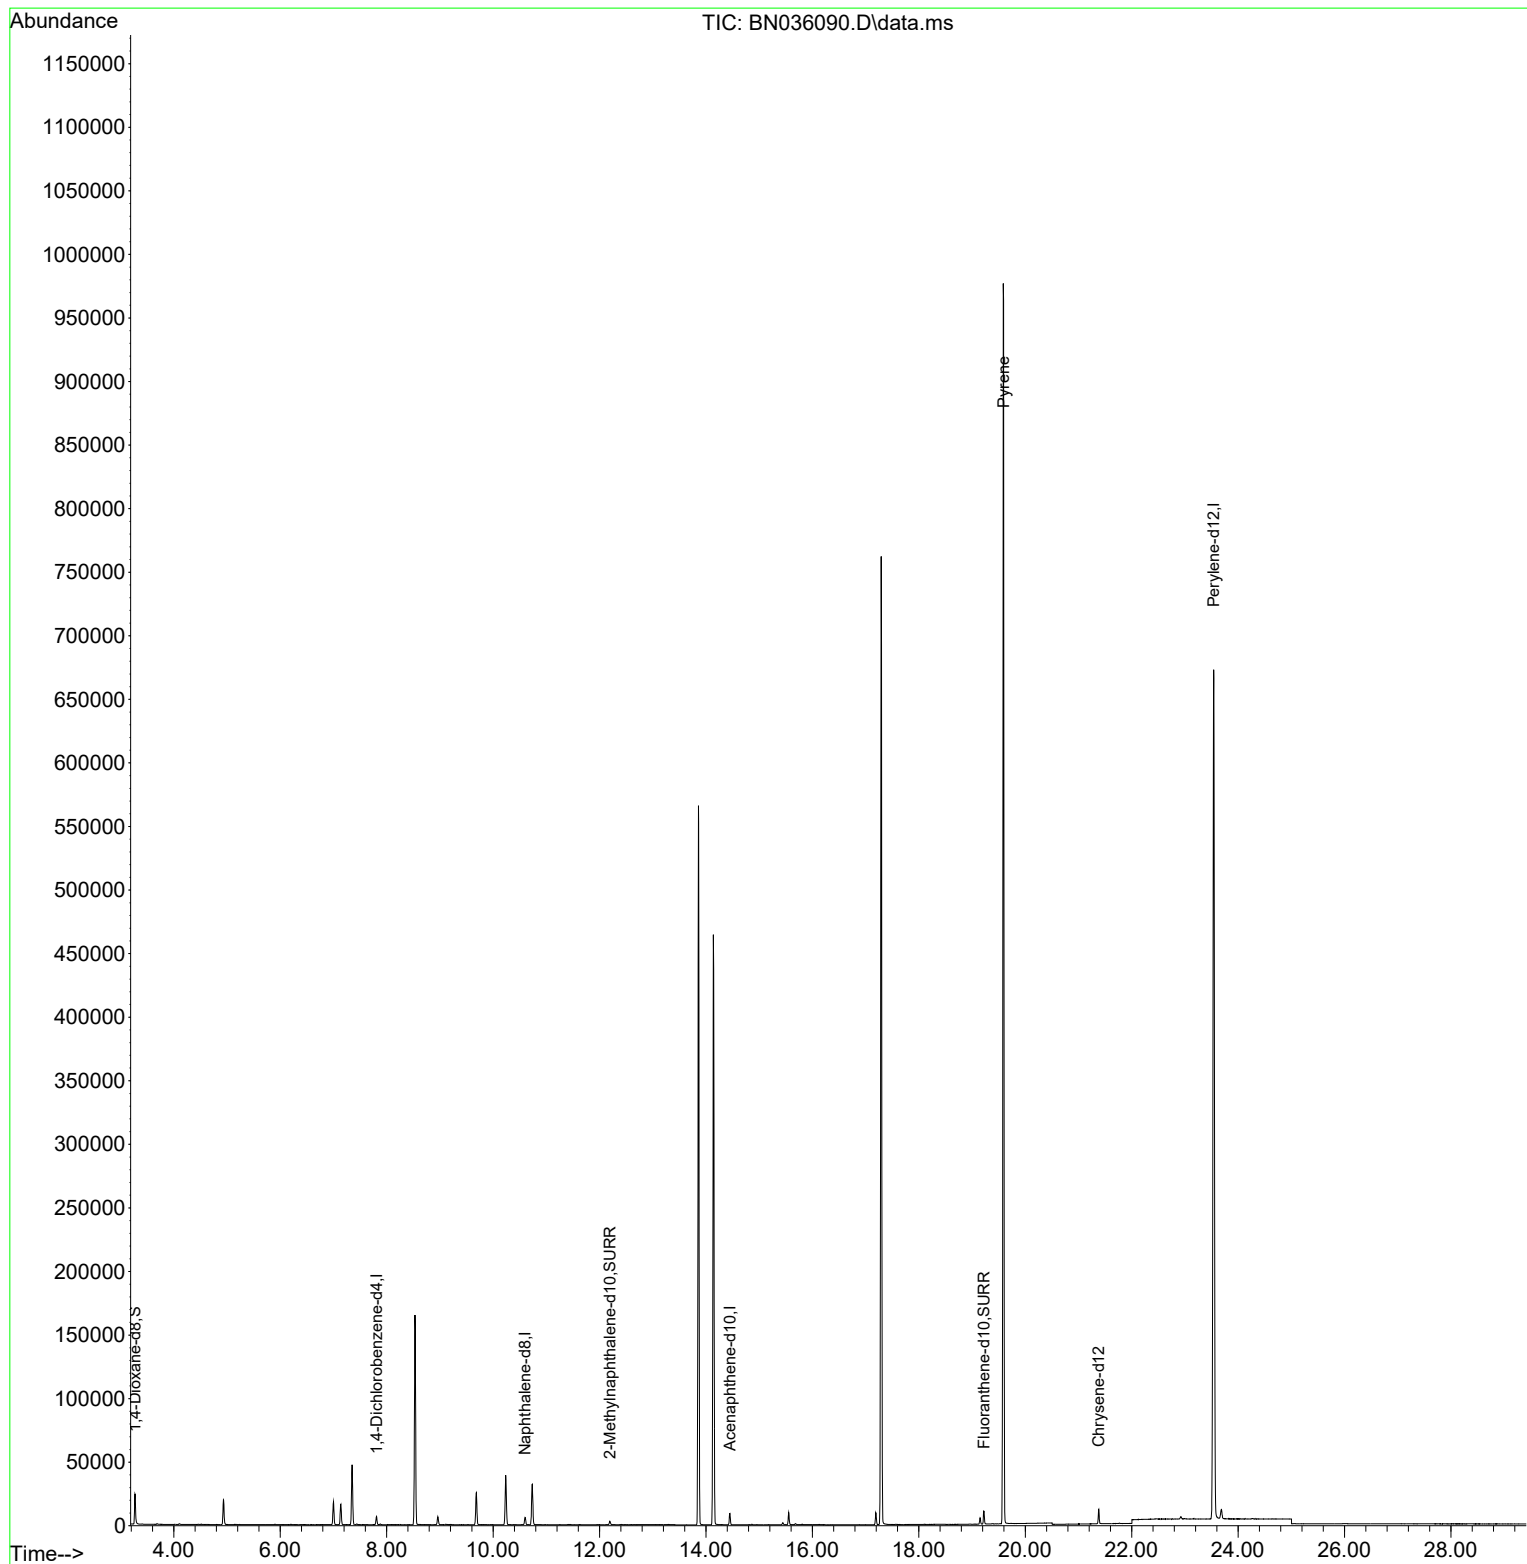

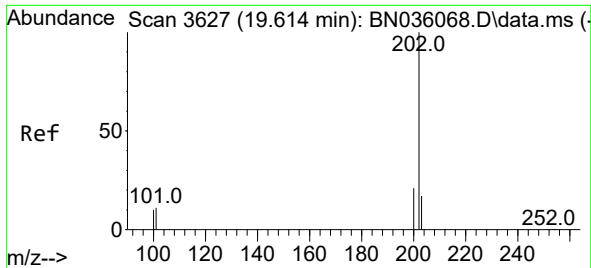

#20
 Pyrene
 Concen: 0.041 ng/ul
 RT: 19.592 min Scan# 30
 Delta R.T. -0.018 min
 Lab File: BN036090.D
 Acq: 29 Jan 2025 01:41

Instrument :
 BNA_N
 ClientSampleId :
 E2948

Tgt Ion:202 Resp: 1681
 Ion Ratio Lower Upper
 202 100
 101 163.0 9.3 13.9#
 100 1101.9 7.5 11.3#

