

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012825\
 Data File : BN036091.D
 Acq On : 29 Jan 2025 02:17
 Operator : RC/JU
 Sample : Q1184-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E2949

Quant Time: Jan 29 08:08:12 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 21 23:52:22 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.807	152	2238	0.400	ng/ul	0.00
4) Naphthalene-d8	10.600	136	5397	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.450	164	3465	0.400	ng/ul	0.00
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-17.19
17) Chrysene-d12	21.380	240	7569	0.400	ng/ul	0.00
23) Perylene-d12	23.540	264	584581	0.400	ng/ul	#-0.13
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.268	96	12399	5.060	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.195	152	2609	0.383	ng/ul	0.00
18) Fluoranthene-d10	19.224	212	9330	0.449	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.445	166	1174	0.088	ng/ul#	19
20) Pyrene	19.587	202	1293	0.043	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012825\
Data File : BN036091.D
Acq On : 29 Jan 2025 02:17
Operator : RC/JU
Sample : Q1184-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E2949

Quant Time: Jan 29 08:08:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 21 23:52:22 2025
Response via : Initial Calibration




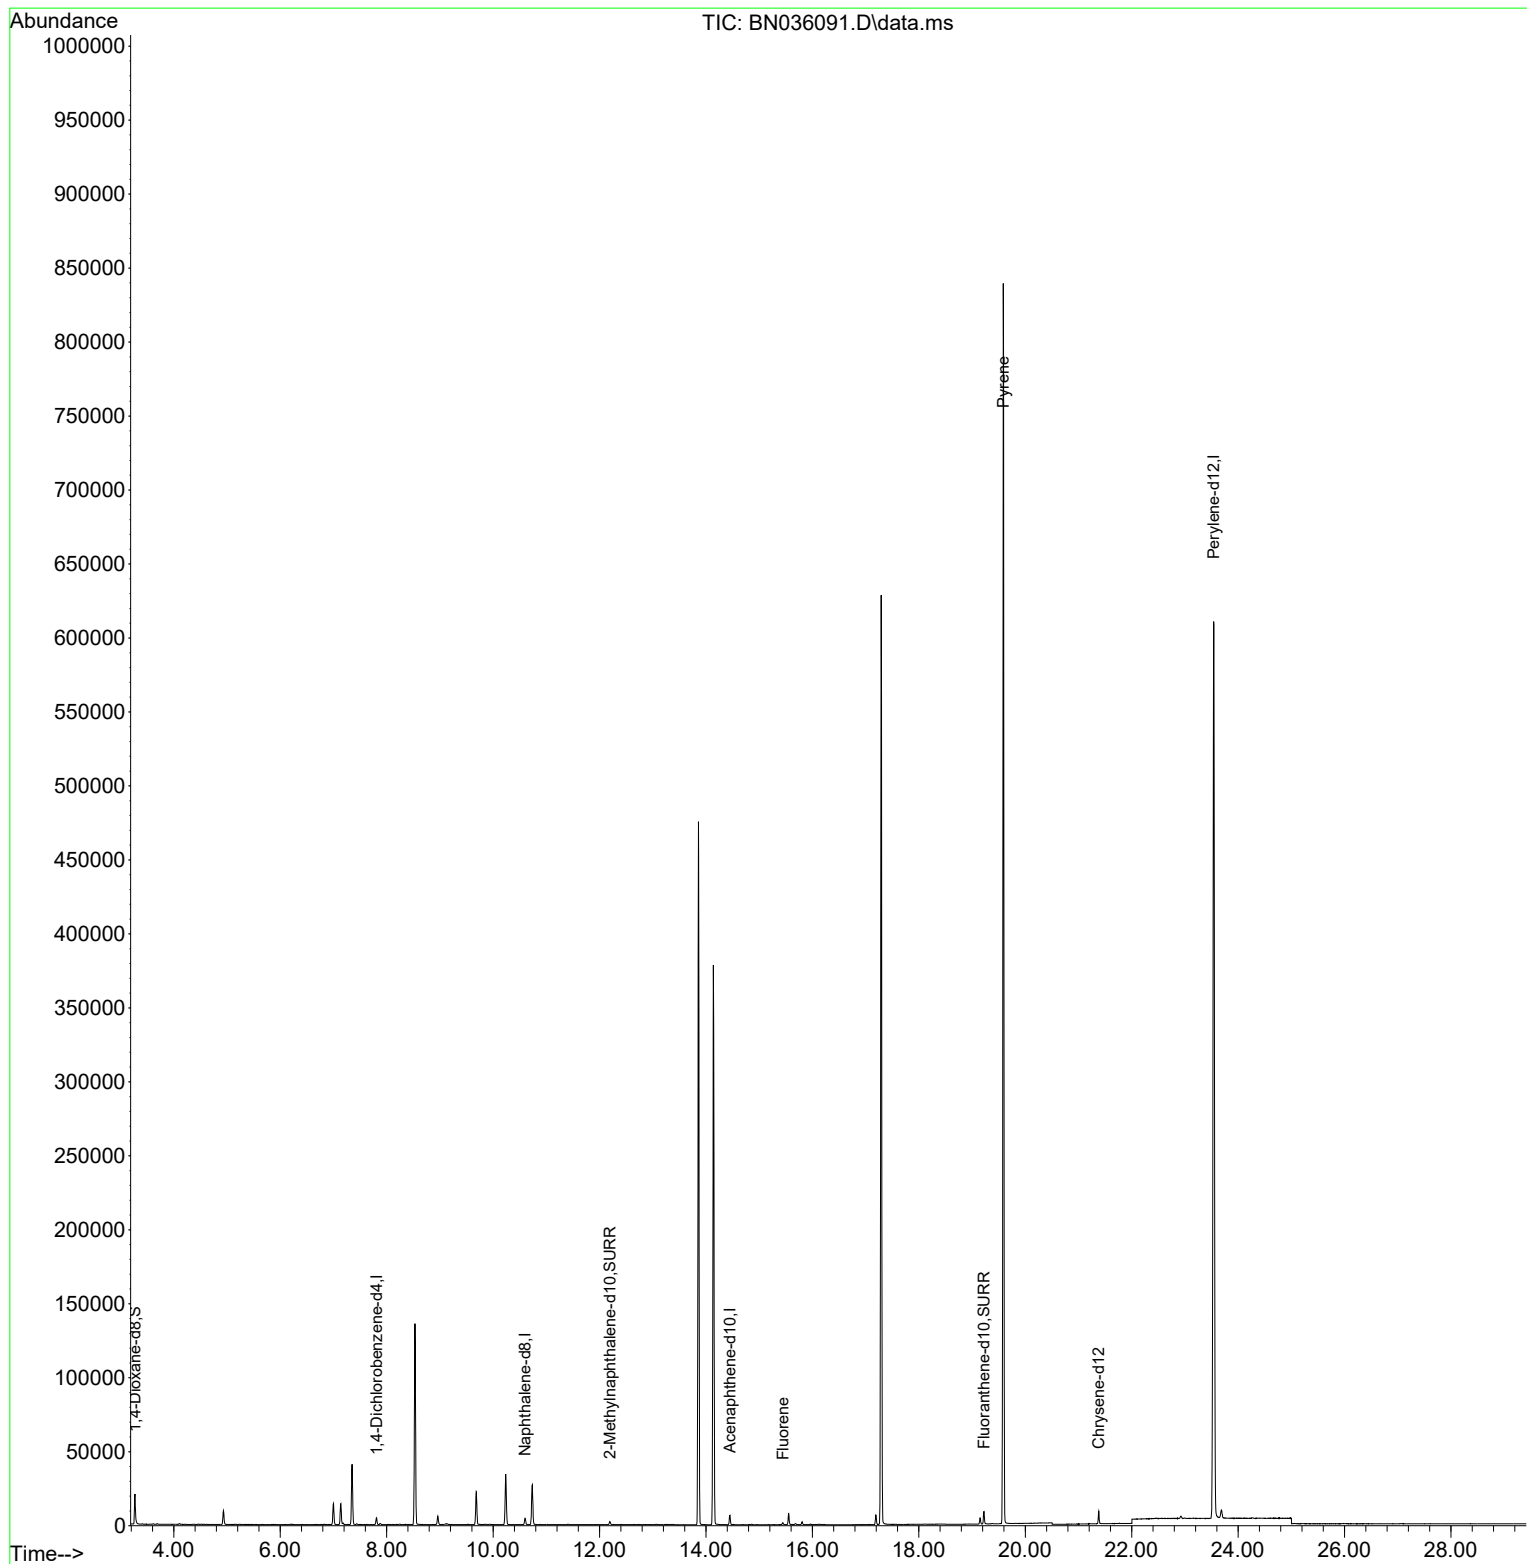


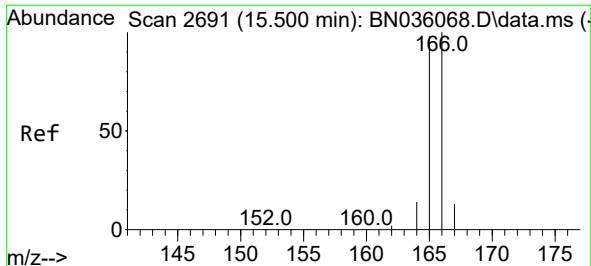

#12
Fluorene
Concen: 0.088 ng/ul
RT: 15.445 min Scan# 2679
Delta R.T. -0.056 min
Lab File: BN036091.D
Acq: 29 Jan 2025 02:17

Instrument :
BNA_N
ClientSampleId :
E2949

Tgt Ion:166 Resp: 1174
Ion Ratio Lower Upper
166 100
165 15.1 80.3 120.5#
167 39.4 12.3 18.5#

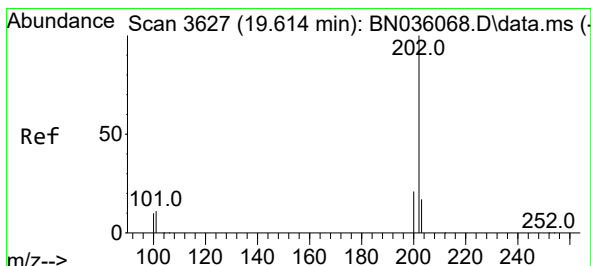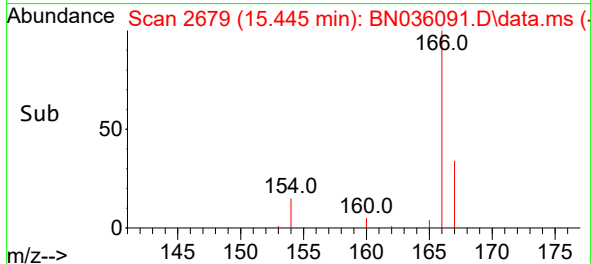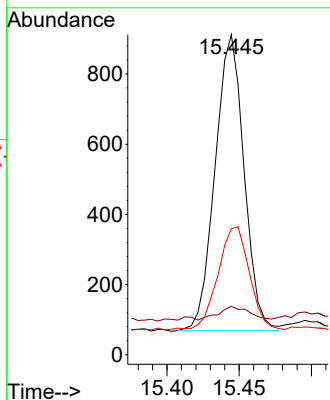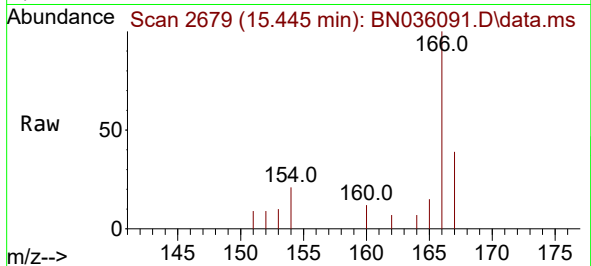

#20
Pyrene
Concen: 0.043 ng/ul
RT: 19.587 min Scan# 3621
Delta R.T. -0.023 min
Lab File: BN036091.D
Acq: 29 Jan 2025 02:17

Tgt Ion:202 Resp: 1293
Ion Ratio Lower Upper
202 100
101 173.5 9.3 13.9#
100 1273.3 7.5 11.3#

