

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012825\
 Data File : BN036094.D
 Acq On : 29 Jan 2025 04:06
 Operator : RC/JU
 Sample : Q1184-05
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E2957

Quant Time: Jan 29 08:08:32 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 21 23:52:22 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.808	152	2597	0.400	ng/ul	0.00
4) Naphthalene-d8	10.600	136	6173	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.450	164	3995	0.400	ng/ul	0.00
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-17.19
17) Chrysene-d12	21.378	240	8484	0.400	ng/ul	0.00
23) Perylene-d12	23.538	264	659775	0.400	ng/ul	#-0.13
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.268	96	13039	4.586	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.195	152	2822	0.362	ng/ul	0.00
18) Fluoranthene-d10	19.220	212	10247	0.440	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.587	202	1524	0.045	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012825\
Data File : BN036094.D
Acq On : 29 Jan 2025 04:06
Operator : RC/JU
Sample : Q1184-05
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E2957

Quant Time: Jan 29 08:08:32 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 21 23:52:22 2025
Response via : Initial Calibration

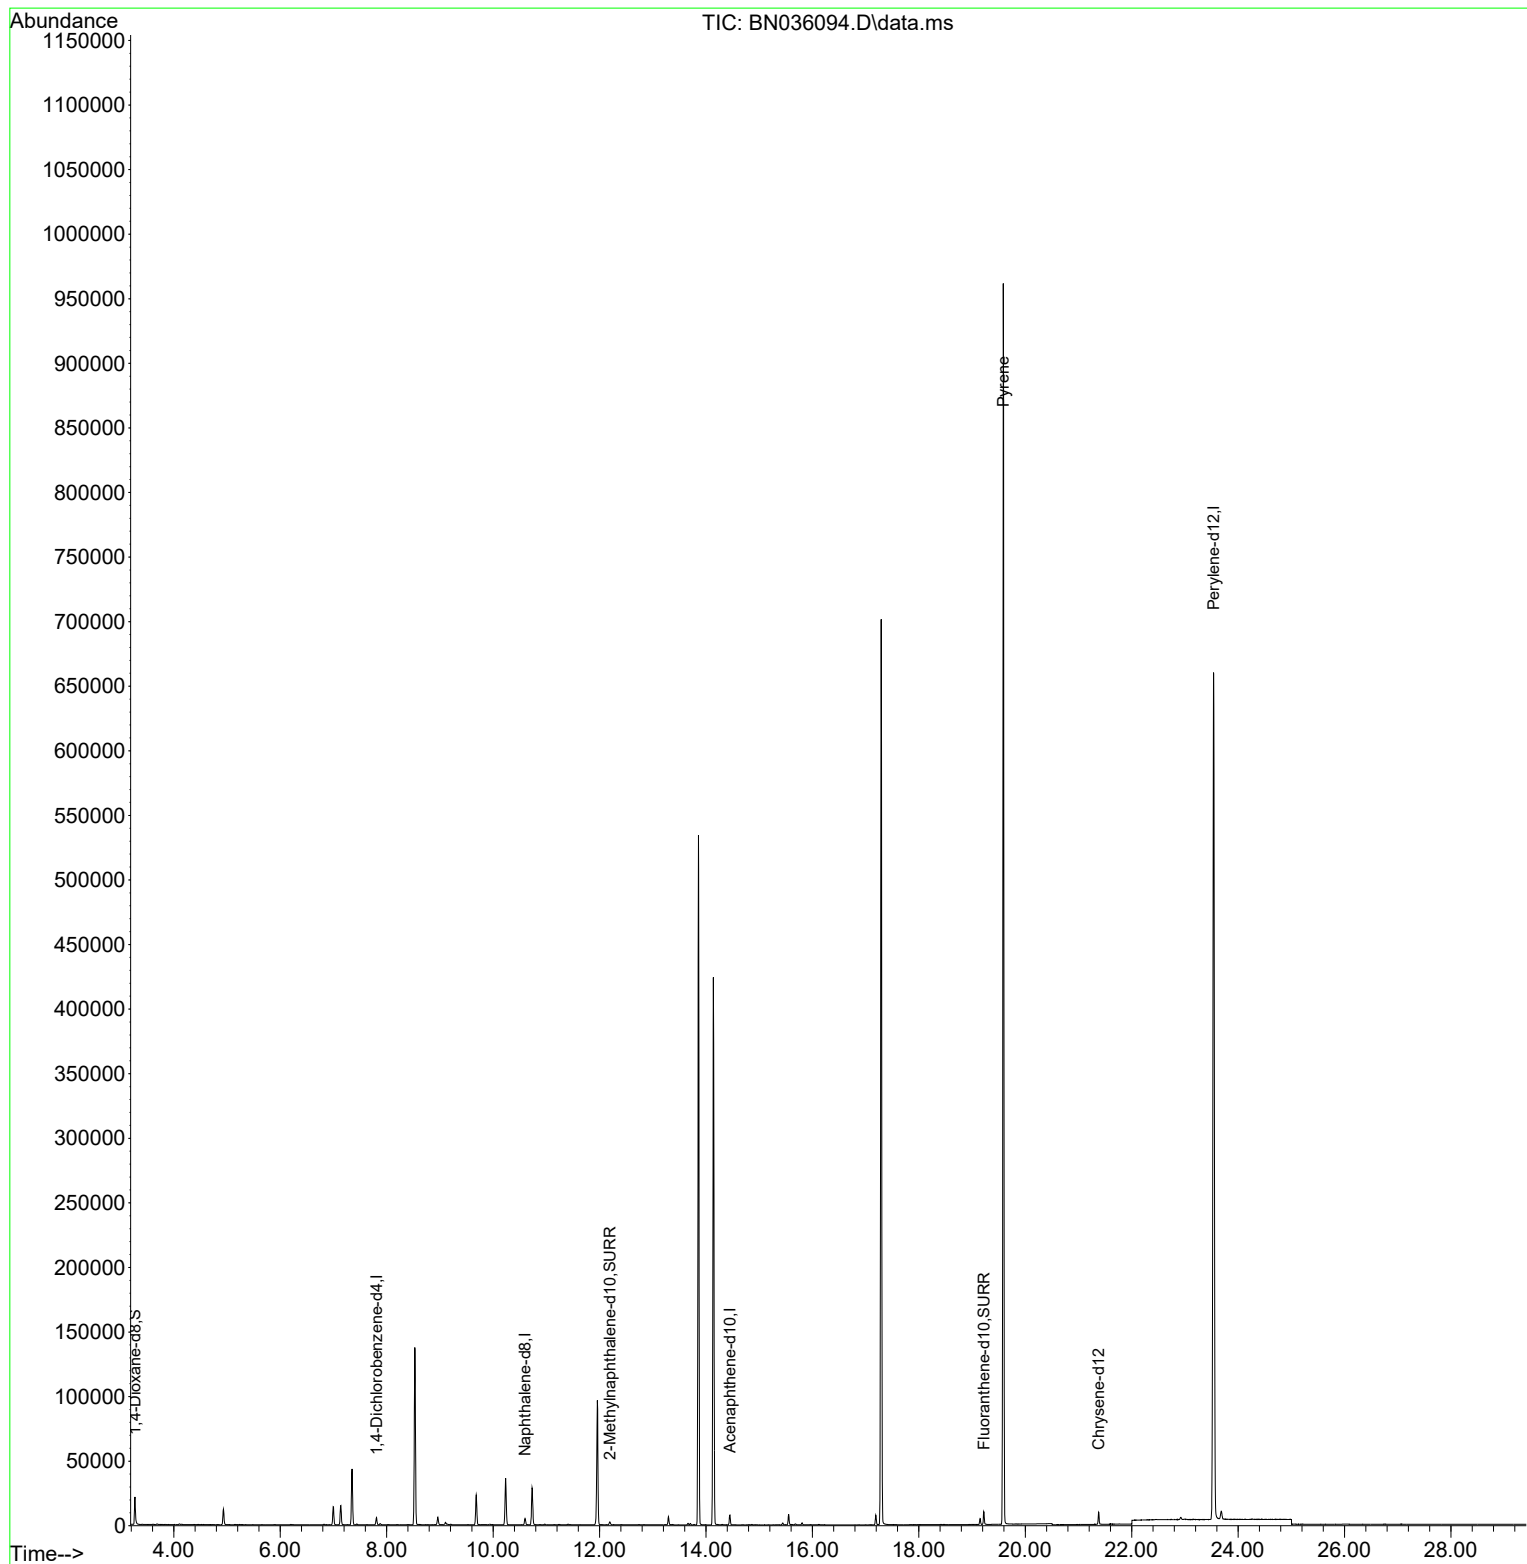

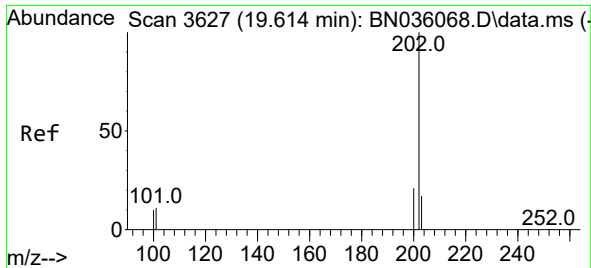

#20

Pyrene

Concen: 0.045 ng/ul

RT: 19.587 min Scan# 30

Delta R.T. -0.023 min

Lab File: BN036094.D


Acq: 29 Jan 2025 04:06

Instrument :

BNA_N

ClientSampleId :

E2957

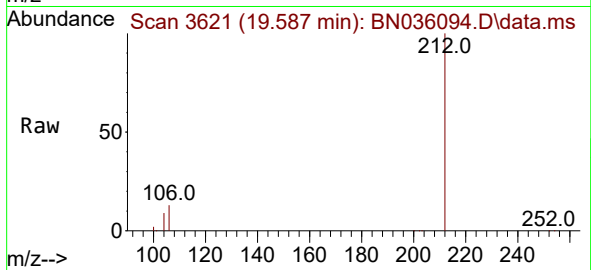

Tgt Ion:202 Resp: 1524

Ion Ratio Lower Upper

202 100

101 169.7 9.3 13.9#

100 1245.2 7.5 11.3#

