

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012825\
Data File : BN036091.D
Acq On : 29 Jan 2025 02:17
Operator : RC/JU
Sample : Q1184-02
Misc :
ALS Vial : 26 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
E2949

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/29/2025
Supervised By :mohammad ahmed 02/04/2025

Quant Time: Jan 29 08:08:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 21 23:52:22 2025
Response via : Initial Calibration

Ion 188.00 (187.70 to 188.70): BN036091.D\data.ms
Ion 94.00 (93.70 to 94.70): BN036091.D\data.ms
Ion 80.00 (79.70 to 80.70): BN036091.D\data.ms

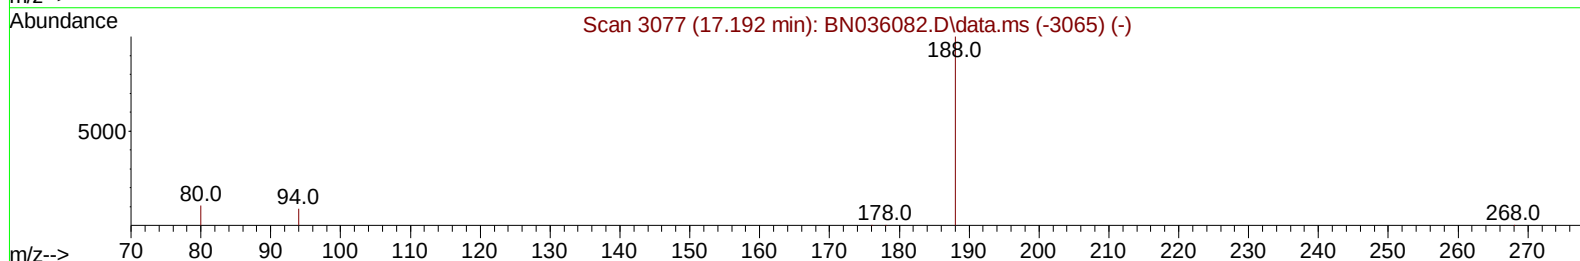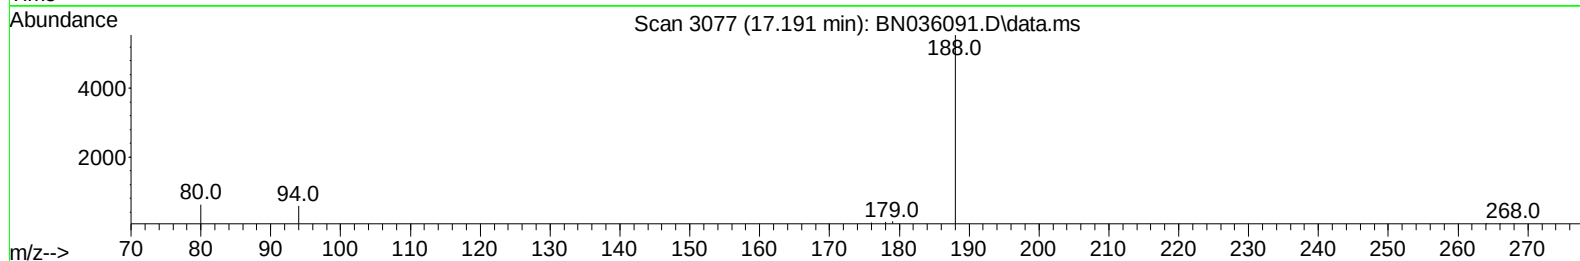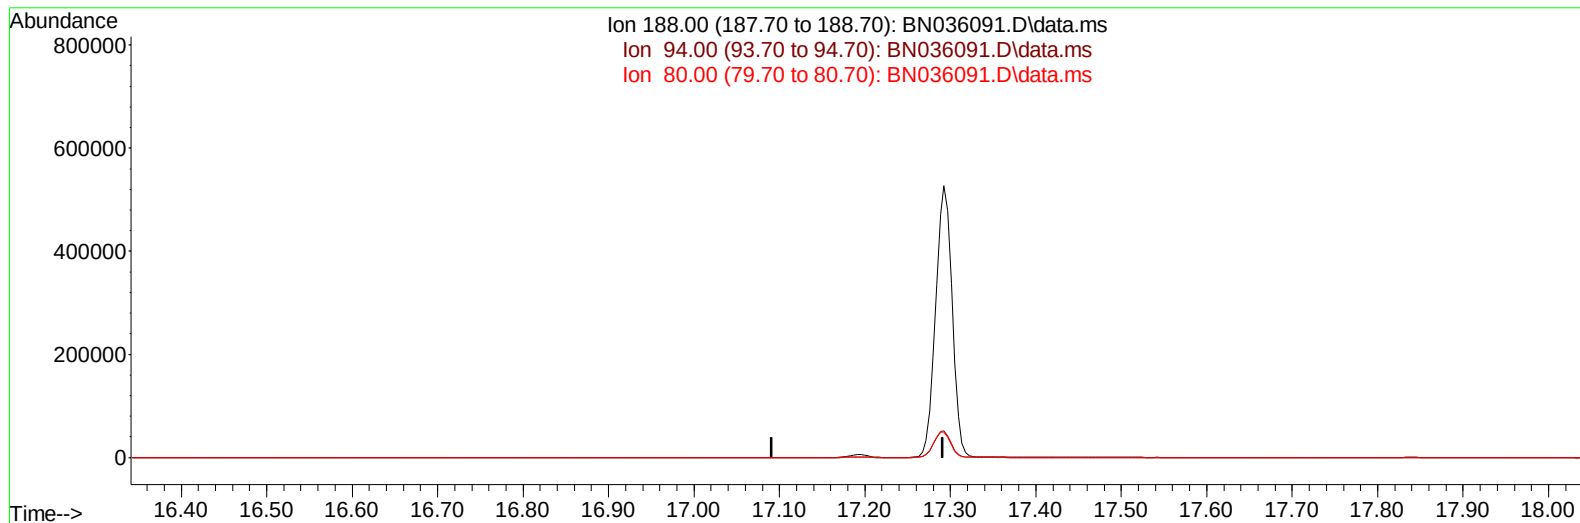

TIC: BN036091.D\data.ms

(13) Phenanthrene-d10 (I)

17.191min (-17.191) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	10.10	0.00#
80.00	10.90	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012825\
Data File : BN036091.D
Acq On : 29 Jan 2025 02:17
Operator : RC/JU
Sample : Q1184-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E2949

Manual IntegrationsAPPROVED

Quant Time: Jan 29 08:08:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 21 23:52:22 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/29/2025
Supervised By :mohammad ahmed 02/04/2025

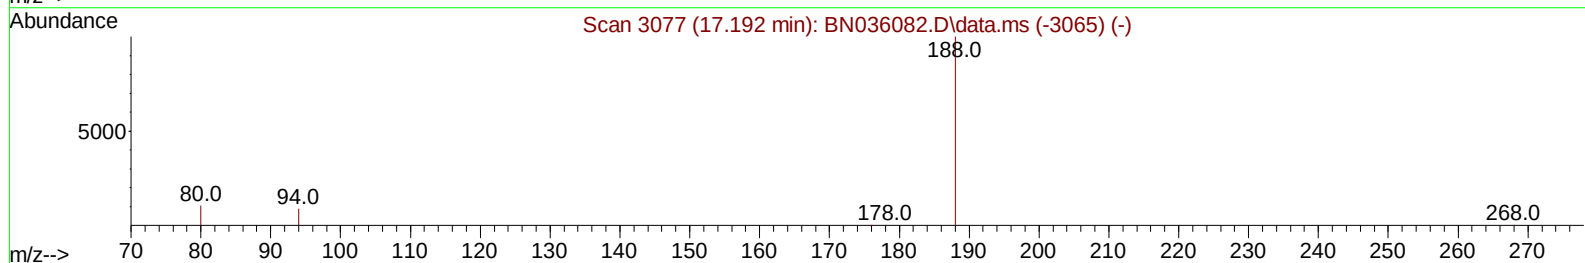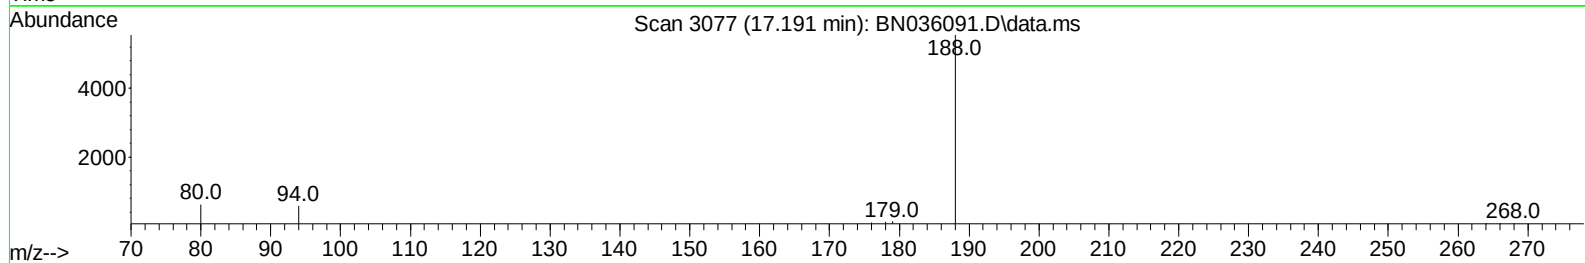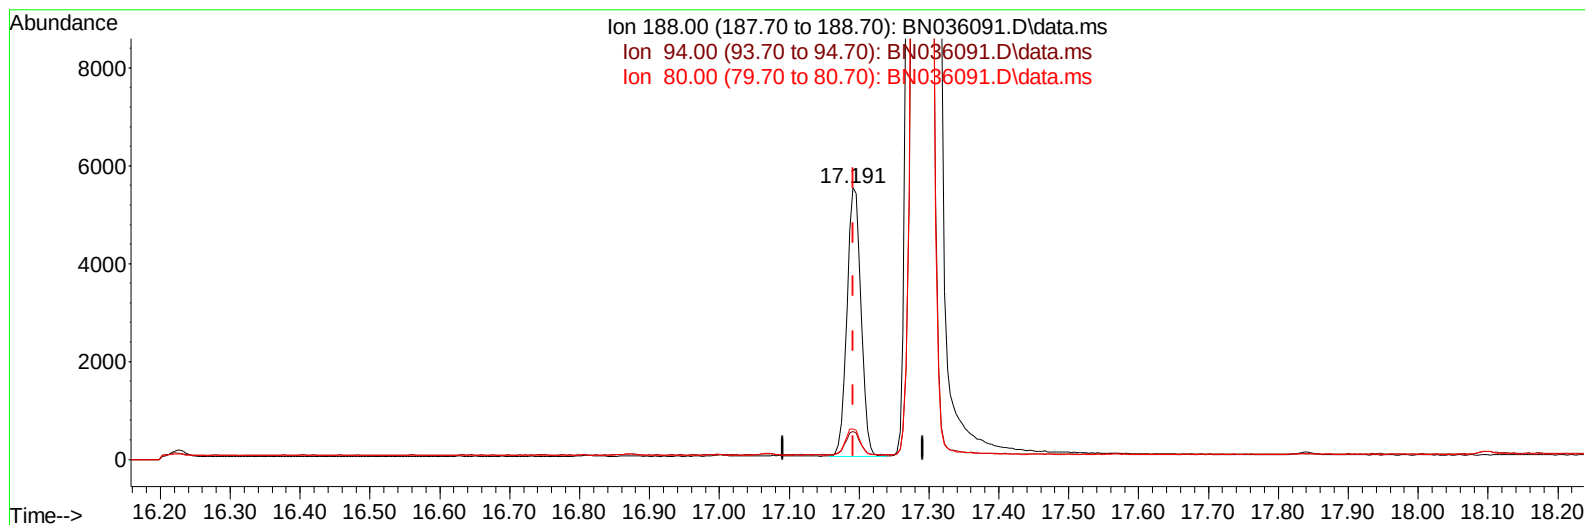

TIC: BN036091.D\data.ms

(13) Phenanthrene-d10 (I)

17.191min (+ 0.000) 0.40 ng/ul m

response 7605

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.10	10.38
80.00	10.90	11.21
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012825\
Data File : BN036091.D
Acq On : 29 Jan 2025 02:17
Operator : RC/JU
Sample : Q1184-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E2949

Manual IntegrationsAPPROVED

Quant Time: Jan 29 08:08:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 21 23:52:22 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/29/2025
Supervised By :mohammad ahmed 02/04/2025

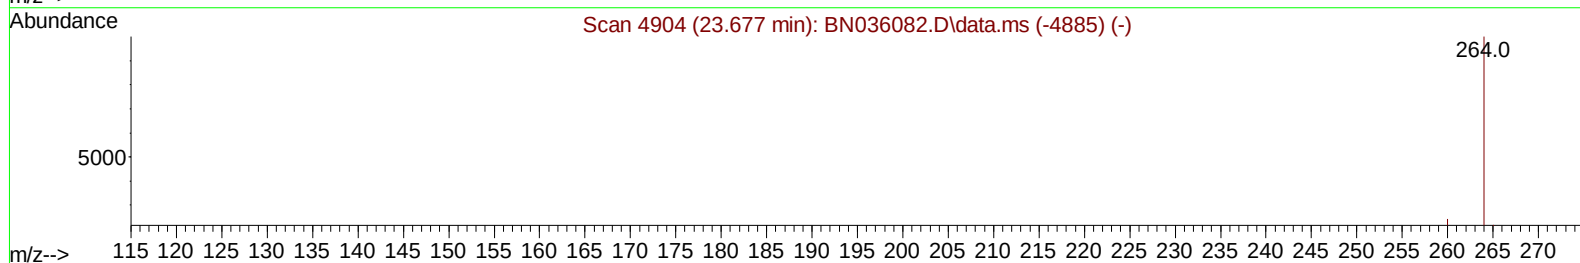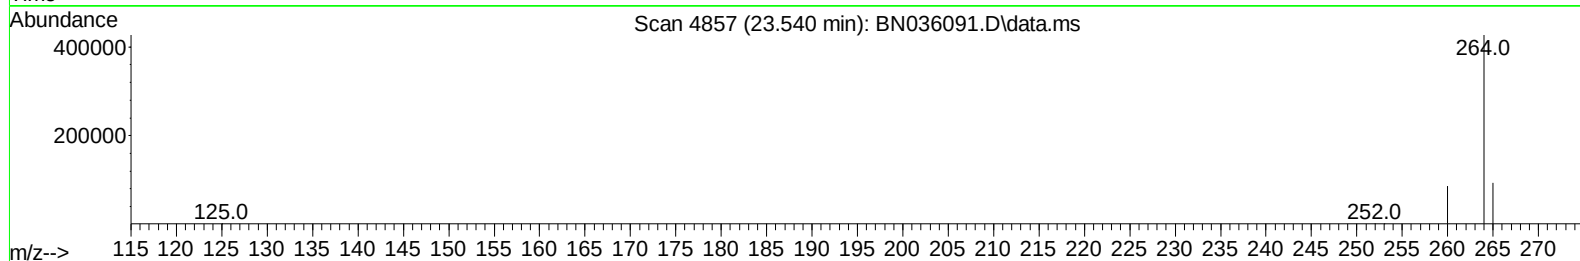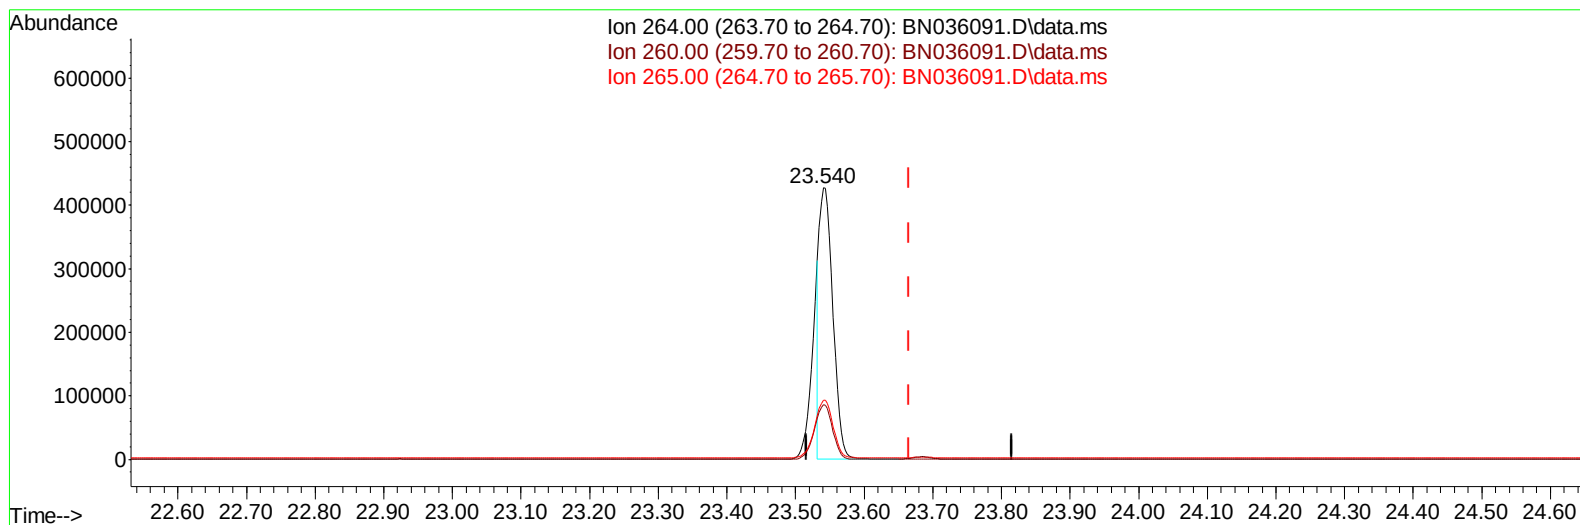

TIC: BN036091.D\data.ms

(23) Perylene-d12 (I)

23.540min (-0.125) 0.40 ng/u1

response 584581

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	20.22#
265.00	53.20	21.93#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012825\
Data File : BN036091.D
Acq On : 29 Jan 2025 02:17
Operator : RC/JU
Sample : Q1184-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E2949

Manual IntegrationsAPPROVED

Quant Time: Jan 29 08:08:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 21 23:52:22 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/29/2025
Supervised By :mohammad ahmed 02/04/2025

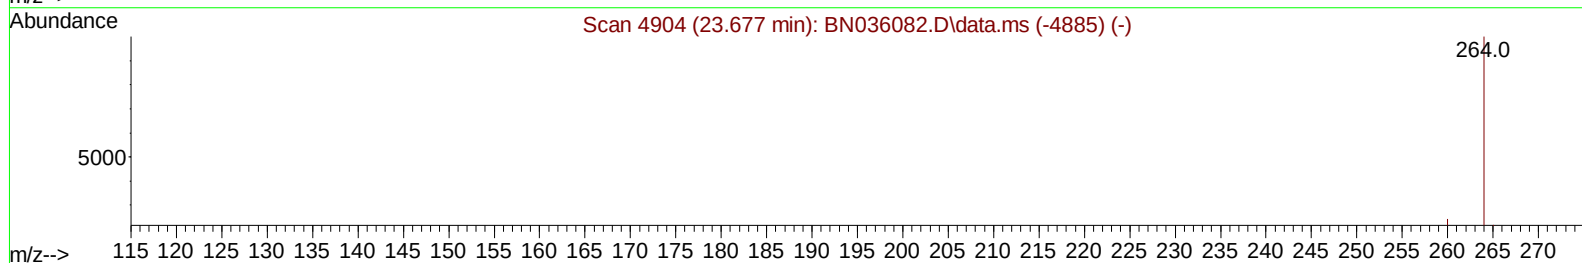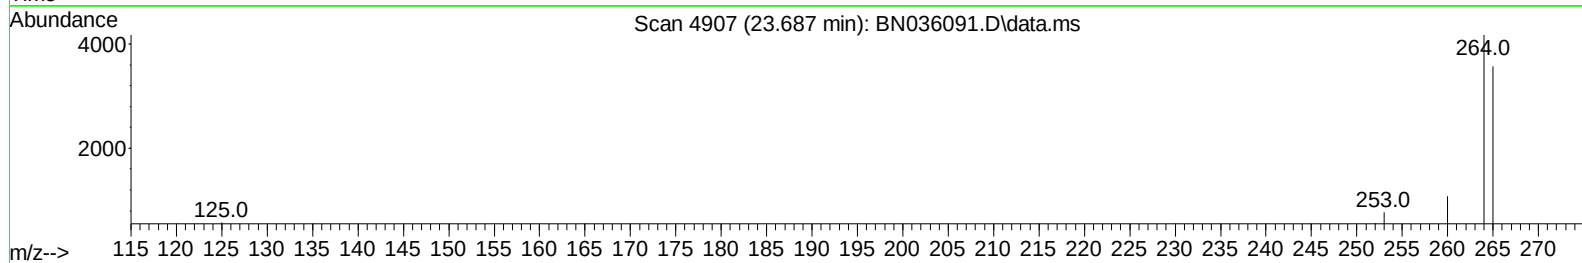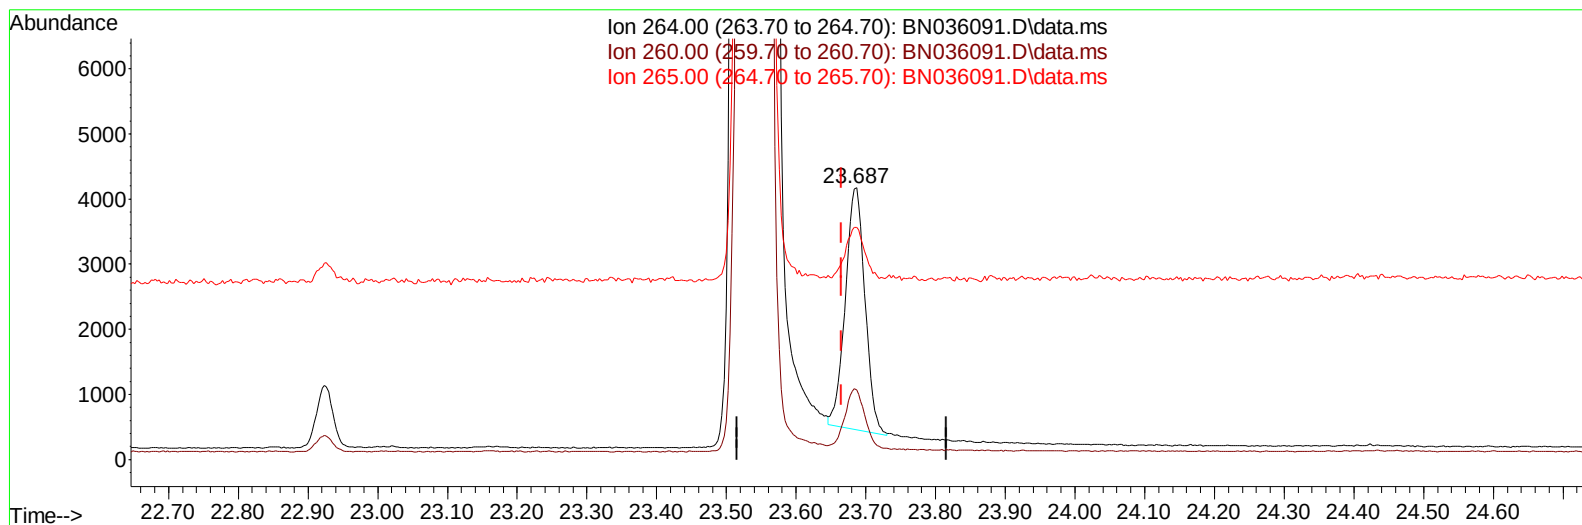

TIC: BN036091.D\data.ms

(23) Perylene-d12 (I)

23.687min (+ 0.021) 0.40 ng/ul m

response 7237

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	25.68
265.00	53.20	85.52#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012825\
 Data File : BN036091.D
 Acq On : 29 Jan 2025 02:17
 Operator : RC/JU
 Sample : Q1184-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E2949

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/29/2025
 Supervised By :mohammad ahmed 02/04/2025

Quant Time: Jan 29 08:08:12 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 21 23:52:22 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.807	152	2238	0.400	ng/ul	0.00
4) Naphthalene-d8	10.600	136	5397	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.450	164	3465	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.191	188	7605m	0.400	ng/ul	0.00
17) Chrysene-d12	21.380	240	7569	0.400	ng/ul	0.00
23) Perylene-d12	23.687	264	7237m	0.400	ng/ul	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.268	96	12399	5.060	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.195	152	2609	0.383	ng/ul	0.00
18) Fluoranthene-d10	19.224	212	9330	0.449	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012825\
Data File : BN036091.D
Acq On : 29 Jan 2025 02:17
Operator : RC/JU
Sample : Q1184-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E2949

Manual IntegrationsAPPROVED

Quant Time: Jan 29 08:08:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 21 23:52:22 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/29/2025
Supervised By :mohammad ahmed 02/04/2025

