

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN012921\
 Data File : BN013541.D
 Acq On : 29 Jan 2021 16:29
 Operator : CG/JU
 Sample : M1274-06
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD0

Quant Time: Jan 29 21:52:46 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012921MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 29 21:10:00 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	268242	20.00	ng/ul	0.00
18) Naphthalene-d8	10.32	136	1143128	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.19	164	691665	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.94	188	1418582	20.00	ng/ul	0.00
78) Chrysene-d12	21.15	240	1427334	20.00	ng/ul	0.00
86) Perylene-d12	23.31	264	1412388	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.16	96	35856	5.74	ng/uL	0.00
5) Phenol-d5	6.73	99	163221	8.19	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.90	67	435419	37.98	ng/ul	0.00
9) 2-Chlorophenol-d4	7.09	132	529805	31.83	ng/ul	0.00
13) 4-Methylphenol-d8	8.25	113	311312	19.63	ng/ul	0.00
19) Nitrobenzene-d5	8.70	128	300306	38.81	ng/ul	0.00
22) 2-Nitrophenol-d4	9.41	143	318640	39.91	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.95	165	582371	36.87	ng/ul	0.00
29) 4-Chloroaniline-d4	10.46	131	48974	2.58	ng/ul	0.00
44) Dimethylphthalate-d6	13.61	166	1994762	43.05	ng/ul	0.00
47) Acenaphthylene-d8	13.88	160	2532224	41.58	ng/ul	0.00
52) 4-Nitrophenol-d4	14.39	143	58519	6.51	ng/ul	0.00
58) Fluorene-d10	15.19	176	1824145	44.93	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.31	200	267065	35.20	ng/ul	0.00
71) Anthracene-d10	17.04	188	2943956	47.87	ng/ul	0.00
79) Pyrene-d10	19.35	212	3238153	47.75	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.17	264	3438593	49.86	ng/ul	0.00


Target Compounds				Ovalue	
45) Dimethylphthalate	13.66	163	103489	2.149	ng/ul 99




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN012921\
Data File : BN013541.D
Acq On : 29 Jan 2021 16:29
Operator : CG/JU
Sample : M1274-06
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD0

Quant Time: Jan 29 21:52:46 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012921MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 29 21:10:00 2021
Response via : Initial Calibration

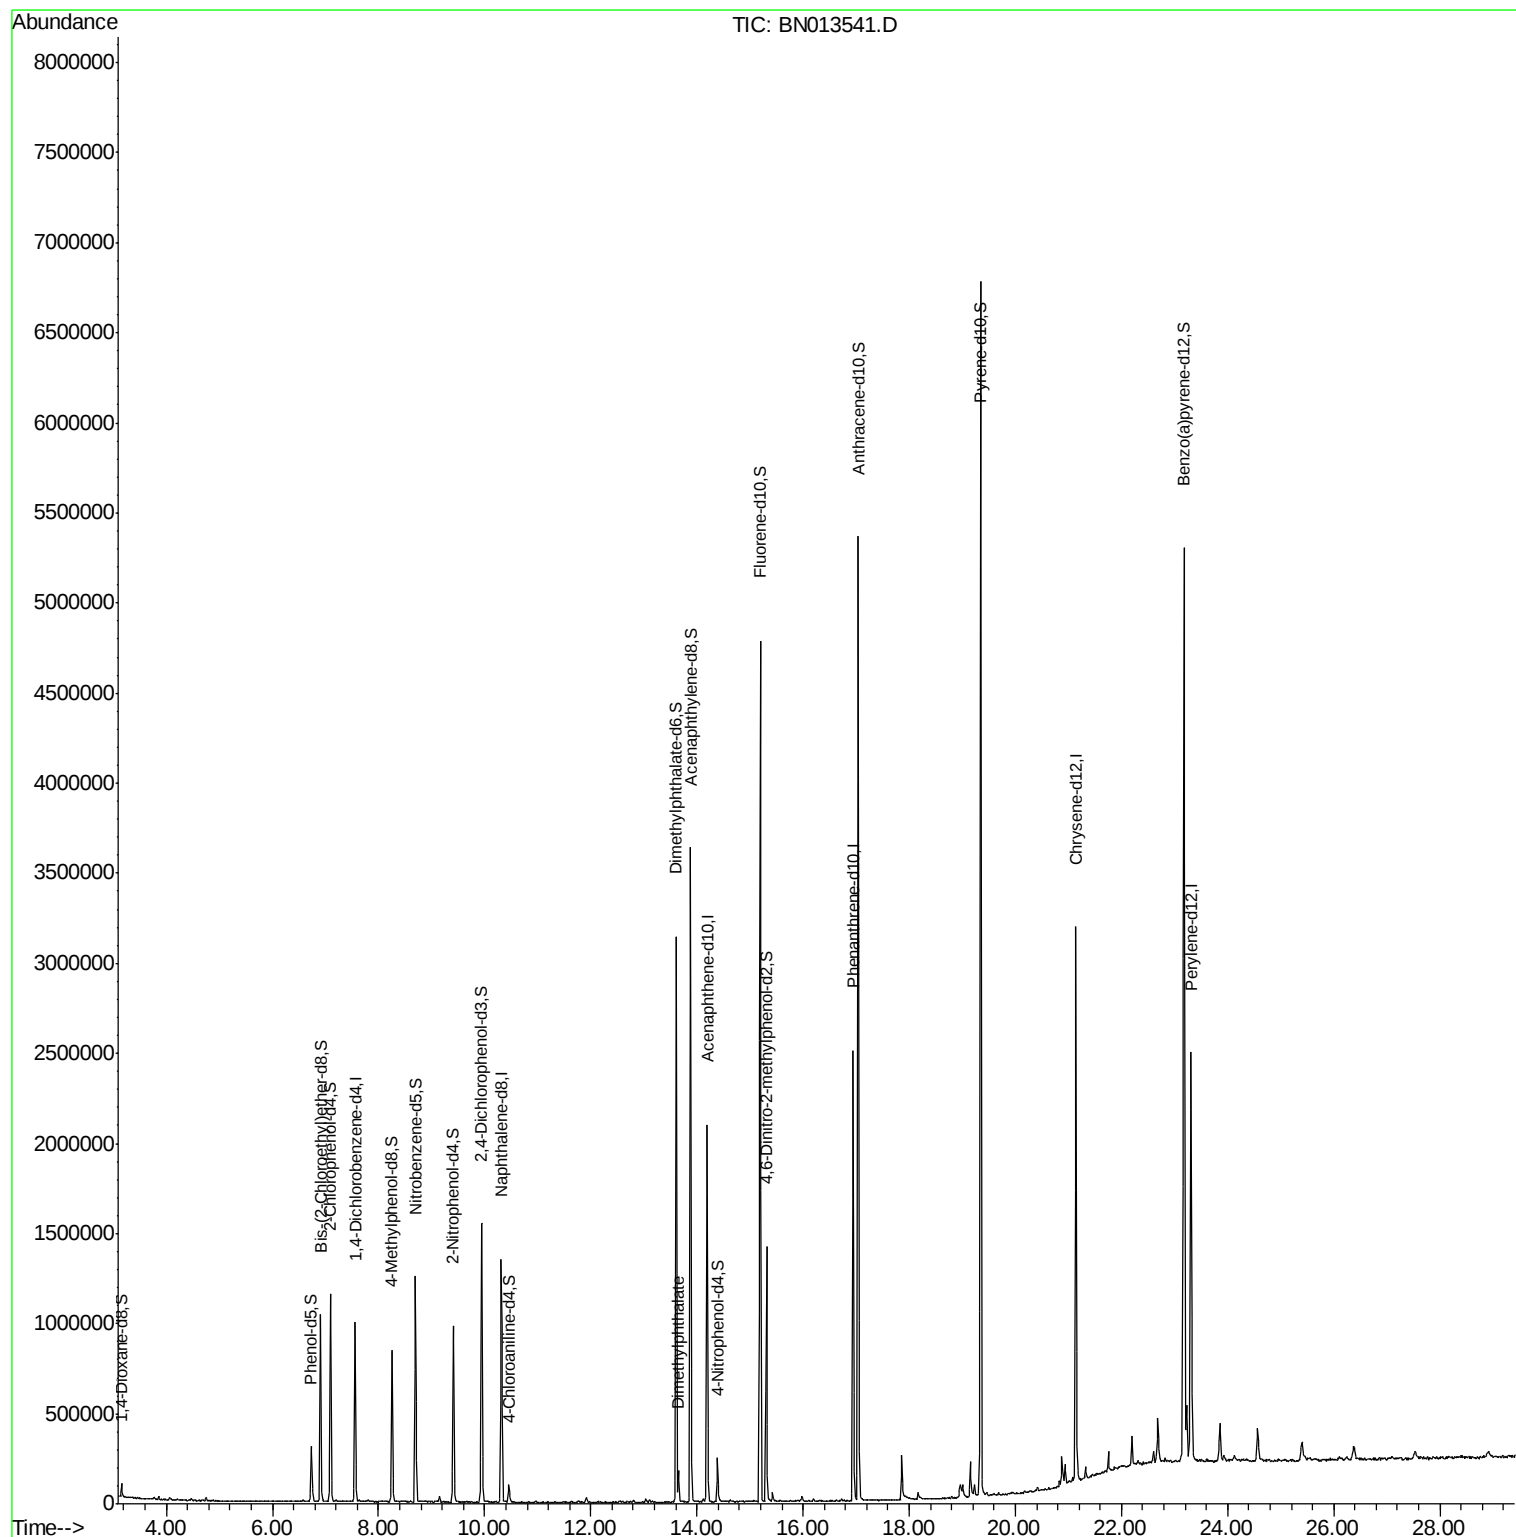

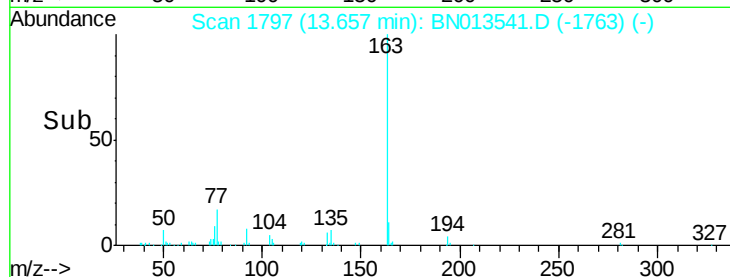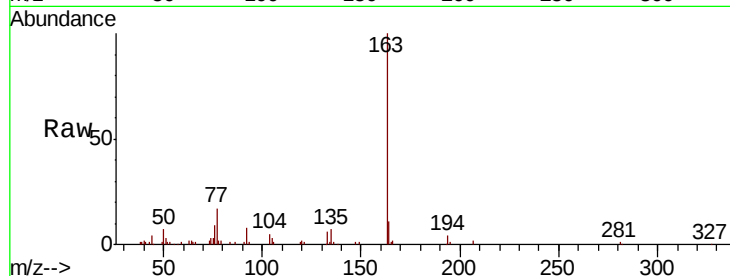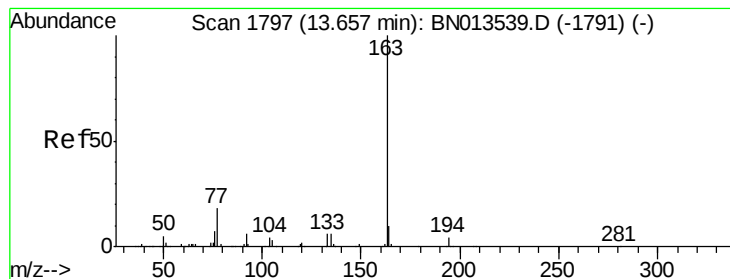

#45

Dimethylphthalate

Concen: 2.149 ng/ul

RT: 13.66 min Scan# 1797

Delta R.T. 0.00 min

Lab File: BN013541.D

Acq: 29 Jan 2021 16:29

Instrument :

BNA_N

ClientSampleId :

C0AD0

Tot Ion:163 Resp: 103489

Ion Ratio Lower Upper

163 100

194 4.3 3.4 5.0

164 10.9 8.3 12.5

