

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN012921\
 Data File : BN013542.D
 Acq On : 29 Jan 2021 17:05
 Operator : CG/JU
 Sample : M1274-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD3

Quant Time: Jan 29 21:56:29 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012921MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 29 21:10:00 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	292624	20.00	ng/ul	0.00
18) Naphthalene-d8	10.32	136	1240921	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.19	164	749735	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.94	188	1533930	20.00	ng/ul	0.00
78) Chrysene-d12	21.15	240	1487879	20.00	ng/ul	0.00
86) Perylene-d12	23.31	264	1493091	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.16	96	30246	4.44	ng/uL	0.00
5) Phenol-d5	6.73	99	148956	6.85	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.90	67	420873	33.65	ng/ul	0.00
9) 2-Chlorophenol-d4	7.09	132	492122	27.10	ng/ul	0.00
13) 4-Methylphenol-d8	8.26	113	294688	17.03	ng/ul	0.00
19) Nitrobenzene-d5	8.70	128	289530	34.47	ng/ul	0.00
22) 2-Nitrophenol-d4	9.41	143	310097	35.78	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.95	165	539718	31.48	ng/ul	0.00
29) 4-Chloroaniline-d4	10.46	131	44212	2.15	ng/ul	0.00
44) Dimethylphthalate-d6	13.61	166	1931851	38.47	ng/ul	0.00
47) Acenaphthylene-d8	13.88	160	2426218	36.76	ng/ul	0.00
52) 4-Nitrophenol-d4	14.39	143	51676	5.30	ng/ul	0.00
58) Fluorene-d10	15.19	176	1717493	39.03	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.31	200	253019	30.84	ng/ul	0.00
71) Anthracene-d10	17.04	188	2823756	42.46	ng/ul	0.00
79) Pyrene-d10	19.35	212	3066695	43.38	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.18	264	3204141	43.95	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.66	163	115375	2.210	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN012921\
Data File : BN013542.D
Acq On : 29 Jan 2021 17:05
Operator : CG/JU
Sample : M1274-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD3

Quant Time: Jan 29 21:56:29 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012921MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 29 21:10:00 2021
Response via : Initial Calibration

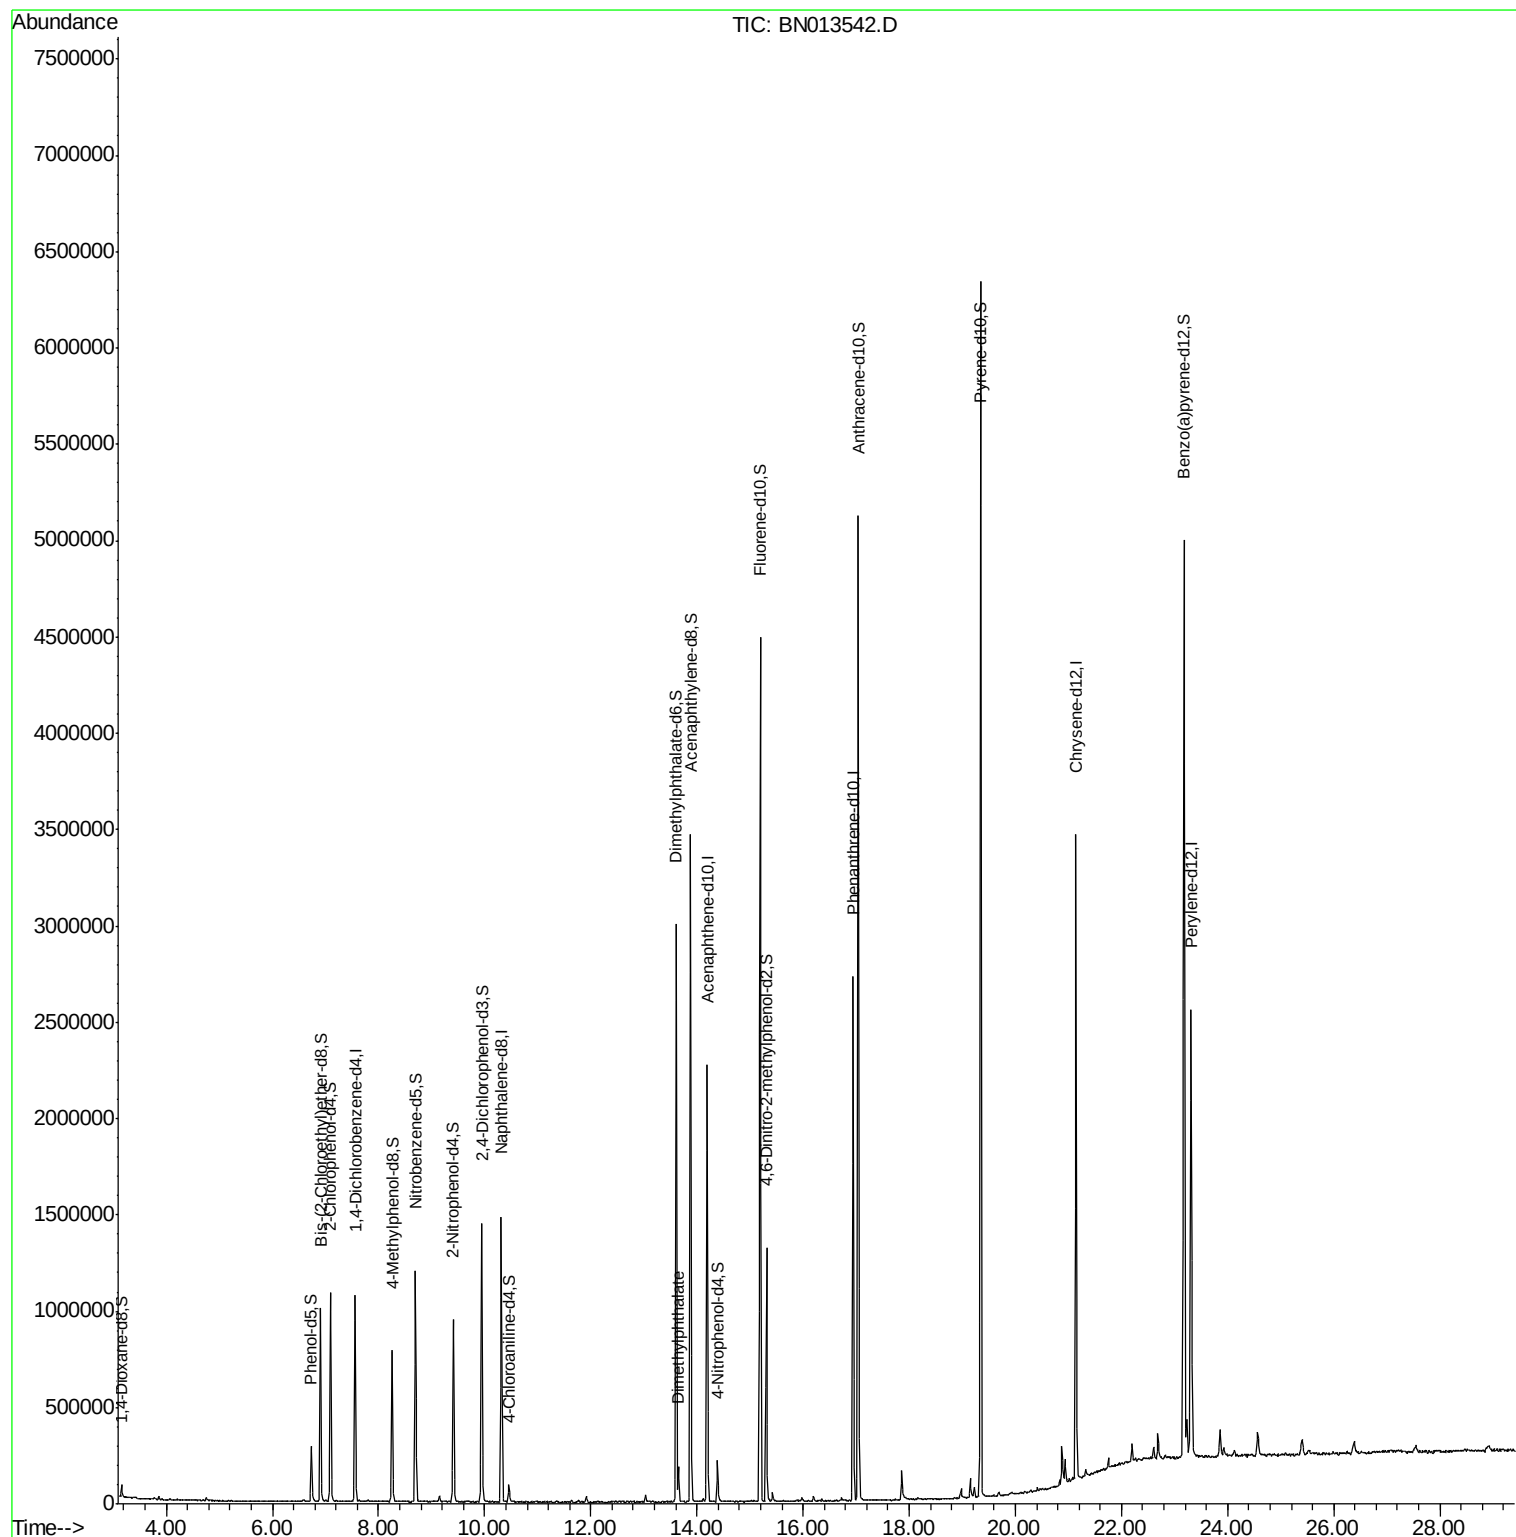

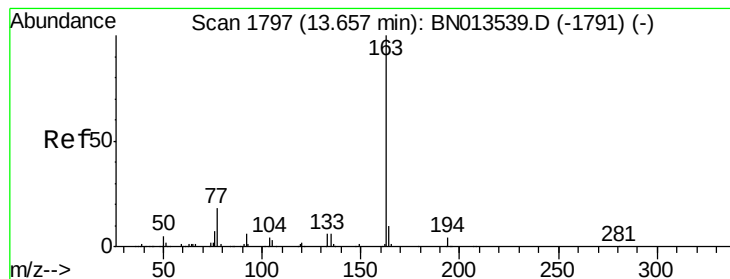

#45

Dimethylphthalate

Concen: 2.210 ng/ul

RT: 13.66 min Scan# 1797

Delta R.T. 0.00 min

Lab File: BN013542.D

Acq: 29 Jan 2021 17:05

Instrument :

BNA_N

ClientSampleId :

C0AD3


Tot Ion:163 Resp: 115375

Ion Ratio Lower Upper

163 100

194 3.9 3.4 5.0

164 10.1 8.3 12.5

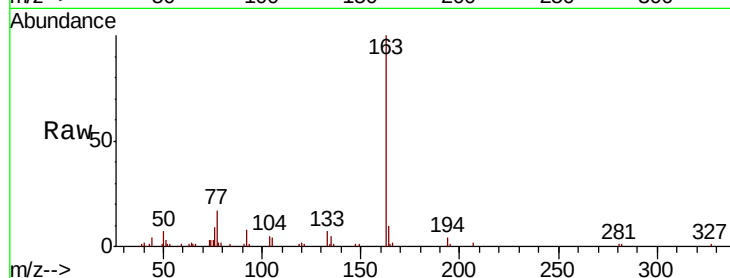

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

