

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN012921\
 Data File : BN013543.D
 Acq On : 29 Jan 2021 17:41
 Operator : CG/JU
 Sample : M1274-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012921MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.158	8	12	22	rVB	64077	85494	0.92%	0.111%
2	3.858	127	131	138	rVB2	18225	24513	0.26%	0.032%
3	6.581	587	594	596	rBV7	5308	10527	0.11%	0.014%
4	6.734	614	620	630	rBV2	294063	511222	5.50%	0.665%
5	6.905	643	649	659	rBV	993128	1552512	16.71%	2.019%
6	7.093	674	681	691	rVB	1101028	1688372	18.17%	2.196%
7	7.181	693	696	705	rVB4	14237	29640	0.32%	0.039%
8	7.557	753	760	767	rBV	1025723	1551941	16.70%	2.018%
9	7.634	769	773	776	rVB4	7856	11475	0.12%	0.015%
10	7.787	795	799	805	rBV6	7892	15866	0.17%	0.021%
11	8.257	871	879	889	rBV	789212	1233149	13.27%	1.604%
12	8.699	944	954	963	rBV	1207790	1894505	20.39%	2.464%
13	9.151	1025	1031	1037	rVB	56885	83921	0.90%	0.109%
14	9.410	1068	1075	1090	rVB	958691	1509852	16.25%	1.964%
15	9.940	1158	1165	1178	rBV	1463558	2401002	25.84%	3.123%
16	10.322	1222	1230	1237	rBV	1348169	2287186	24.61%	2.975%
17	10.457	1245	1253	1261	rBV	86930	148037	1.59%	0.193%
18	11.634	1447	1453	1461	rVB2	18868	32146	0.35%	0.042%
19	11.775	1472	1477	1481	rVB4	5990	10356	0.11%	0.013%
20	11.910	1496	1500	1507	rBV	31569	49131	0.53%	0.064%
21	12.804	1648	1652	1659	rVB6	9583	15715	0.17%	0.020%
22	13.034	1687	1691	1697	rVB	20861	29901	0.32%	0.039%
23	13.098	1697	1702	1708	rBV6	8955	17182	0.18%	0.022%
24	13.610	1782	1789	1794	rBV	3104612	4103817	44.16%	5.337%
25	13.657	1794	1797	1802	rVB	198928	252923	2.72%	0.329%
26	13.881	1828	1835	1845	rBV	3521750	5143907	55.35%	6.690%
27	14.116	1871	1875	1881	rBV4	11041	16013	0.17%	0.021%
28	14.192	1881	1888	1896	rBV	2164562	3095586	33.31%	4.026%
29	14.392	1916	1922	1930	rBV	234543	332897	3.58%	0.433%
30	15.028	2026	2030	2034	rBV6	6286	12061	0.13%	0.016%
31	15.075	2034	2038	2041	rVV3	8915	10050	0.11%	0.013%
32	15.192	2051	2058	2066	rBV	4581854	6667644	71.75%	8.671%
33	15.310	2071	2078	2088	rBV	1430465	1869470	20.12%	2.431%
34	15.428	2093	2098	2103	rVV2	52752	72329	0.78%	0.094%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN012921\
 Data File : BN013543.D
 Acq On : 29 Jan 2021 17:41
 Operator : CG/JU
 Sample : M1274-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012921MA.M
 Title : SVOA CALIBRATION

35	15.981	2188	2192	2197	rVB3	18684	29190	0.31%	0.038%
36	16.204	2225	2230	2233	rBV6	10078	16194	0.17%	0.021%
37	16.733	2313	2320	2324	rBV4	14552	28099	0.30%	0.037%
38	16.945	2349	2356	2365	rBV	2446079	3535725	38.05%	4.598%
39	17.039	2365	2372	2386	rBV2	5340417	7729597	83.18%	10.052%
40	17.863	2507	2512	2521	rBV	191275	297683	3.20%	0.387%
41	18.157	2559	2562	2567	rVB7	7735	12614	0.14%	0.016%
42	18.804	2669	2672	2677	rVB4	8700	10546	0.11%	0.014%
43	18.910	2686	2690	2693	rVB5	7265	9505	0.10%	0.012%
44	18.974	2695	2701	2708	rBV2	64603	110432	1.19%	0.144%
45	19.151	2727	2731	2740	rBV	119088	176828	1.90%	0.230%
46	19.233	2740	2745	2750	rVB	54941	81868	0.88%	0.106%
47	19.345	2758	2764	2776	rVB	6730970	8965945	96.48%	11.660%
48	19.686	2820	2822	2827	rVB4	25322	22673	0.24%	0.029%
49	20.833	3013	3017	3021	rBV2	32374	55573	0.60%	0.072%
50	20.880	3021	3025	3031	rBV2	237965	383494	4.13%	0.499%
51	20.933	3031	3034	3039	rVB	105006	134650	1.45%	0.175%
52	21.145	3064	3070	3079	rBV	3203320	4088153	43.99%	5.317%
53	21.327	3098	3101	3107	rBV3	48334	51792	0.56%	0.067%
54	21.751	3170	3173	3180	rVB2	73304	83800	0.90%	0.109%
55	22.198	3246	3249	3254	rBV2	112099	127707	1.37%	0.166%
56	22.686	3329	3332	3338	rVB	150501	206255	2.22%	0.268%
57	23.174	3408	3415	3422	rBV	5179356	9292707	100.00%	12.085%
58	23.233	3422	3425	3430	rVV	203067	319792	3.44%	0.416%
59	23.310	3432	3438	3446	rVB2	2418741	4131771	44.46%	5.373%
60	23.857	3527	3531	3536	rVB	140997	219557	2.36%	0.286%


Sum of corrected areas: 76892492

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN012921\
Data File : BN013543.D
Acq On : 29 Jan 2021 17:41
Operator : CG/JU
Sample : M1274-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012921MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

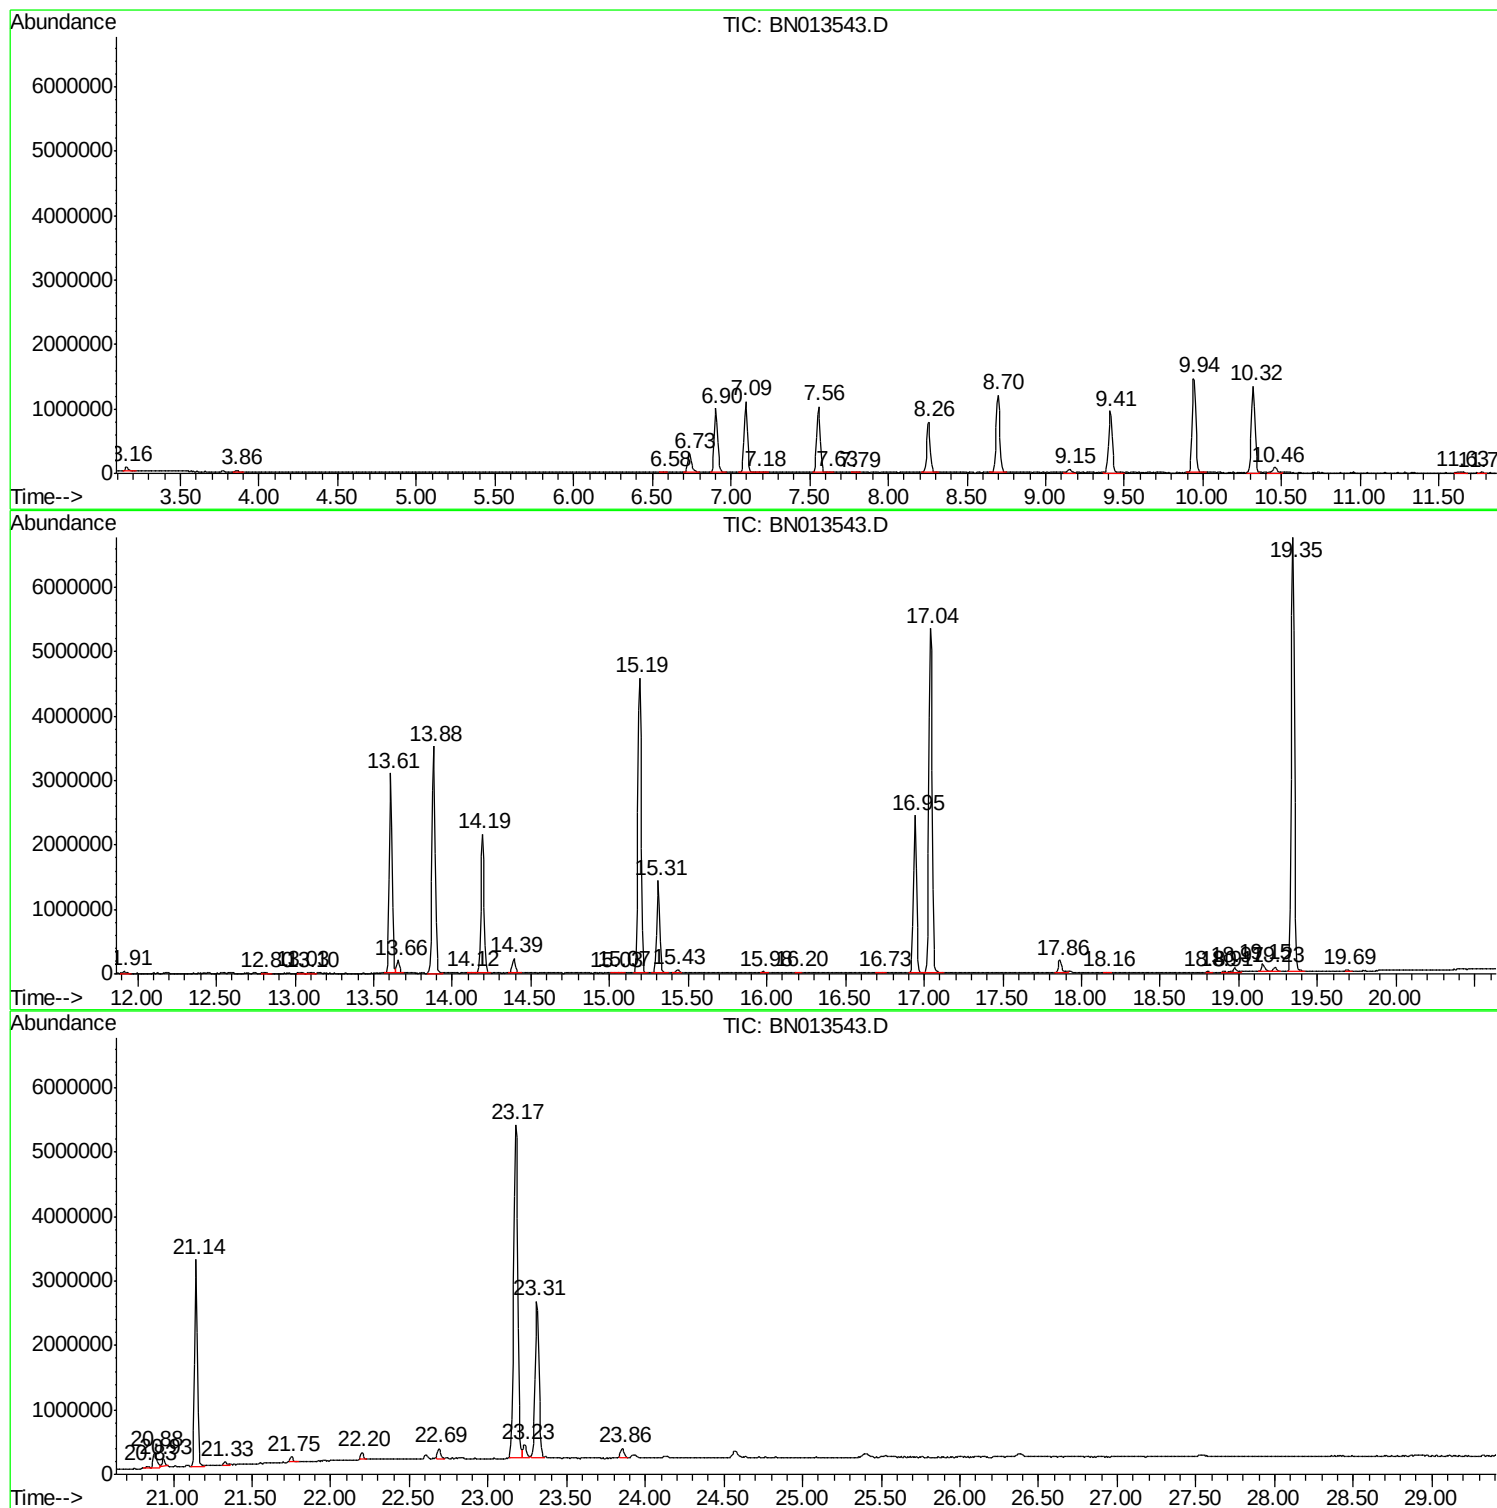

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN012921\
Data File : BN013543.D
Acq On : 29 Jan 2021 17:41
Operator : CG/JU
Sample : M1274-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012921MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN012921\
Data File : BN013543.D
Acq On : 29 Jan 2021 17:41
Operator : CG/JU
Sample : M1274-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012921MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc