
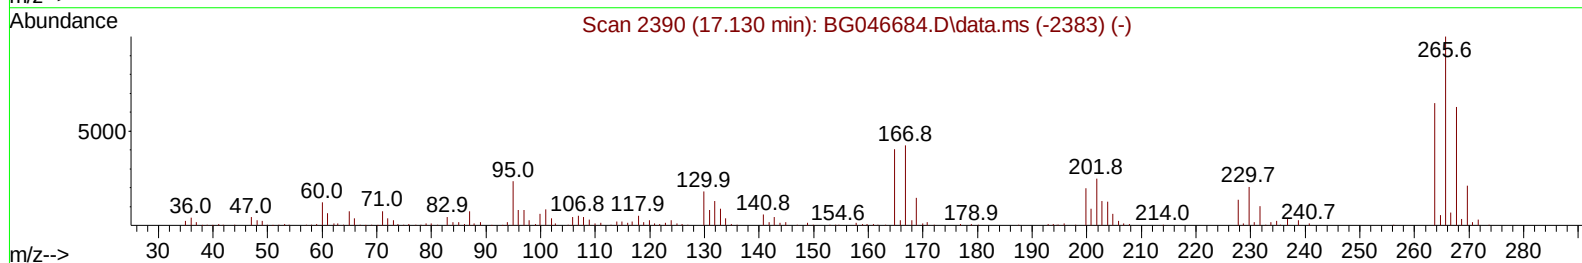
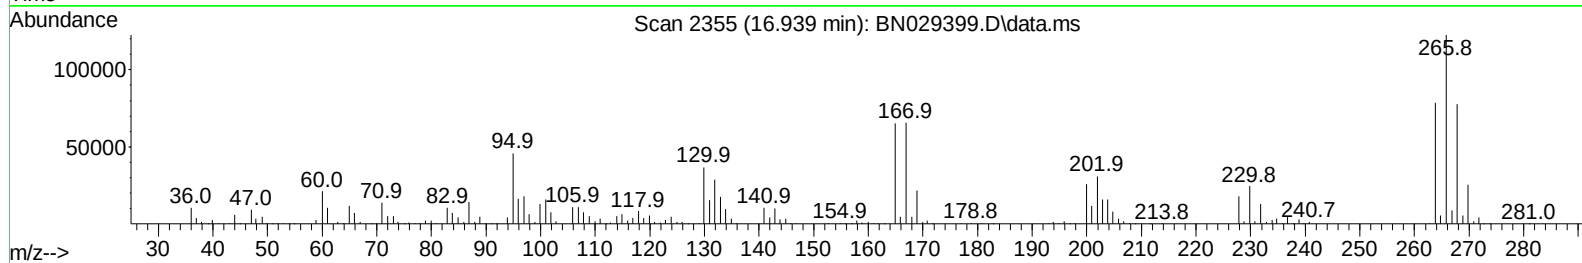


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012924\
Data File : BN029399.D
Acq On : 29 Jan 2024 14:01
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 30 04:03:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 30 04:03:06 2024
Response via : Initial Calibration

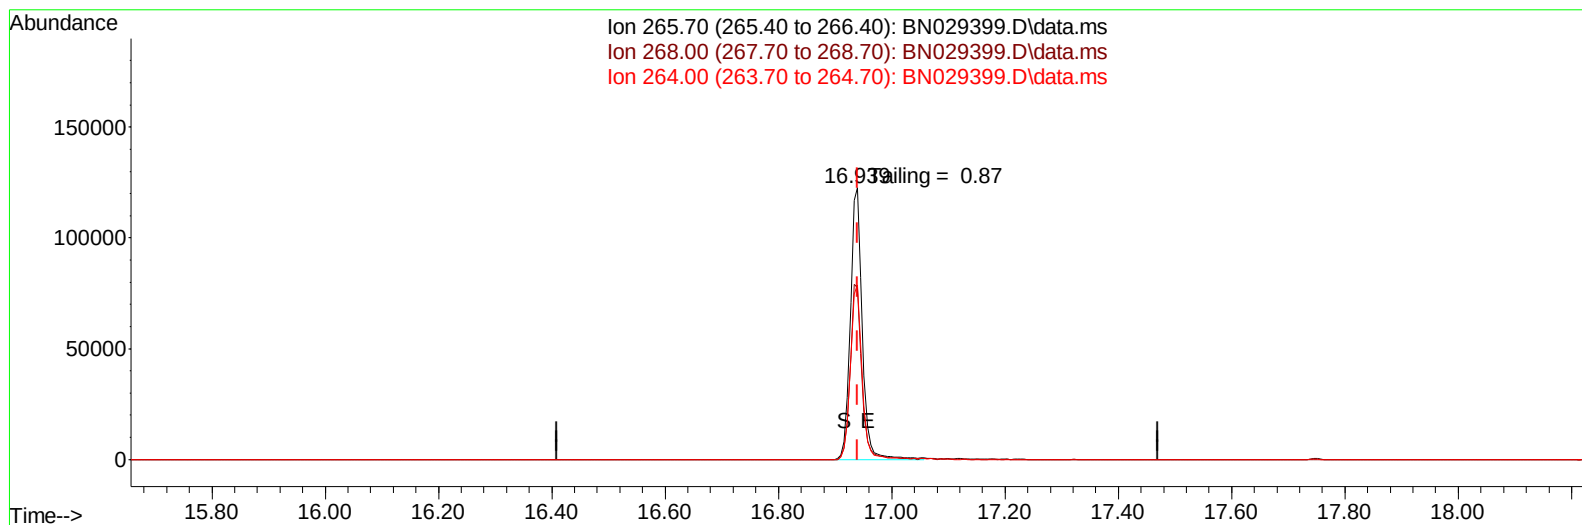




TIC: BN029399.D\data.ms

(70) Pentachlorophenol (C)**16.939min (0.000) 15921.44 ng****response 178300**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.42
264.00	61.60	64.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012924\
Data File : BN029399.D
Acq On : 29 Jan 2024 14:01
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 30 04:03:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 30 04:03:06 2024
Response via : Initial Calibration

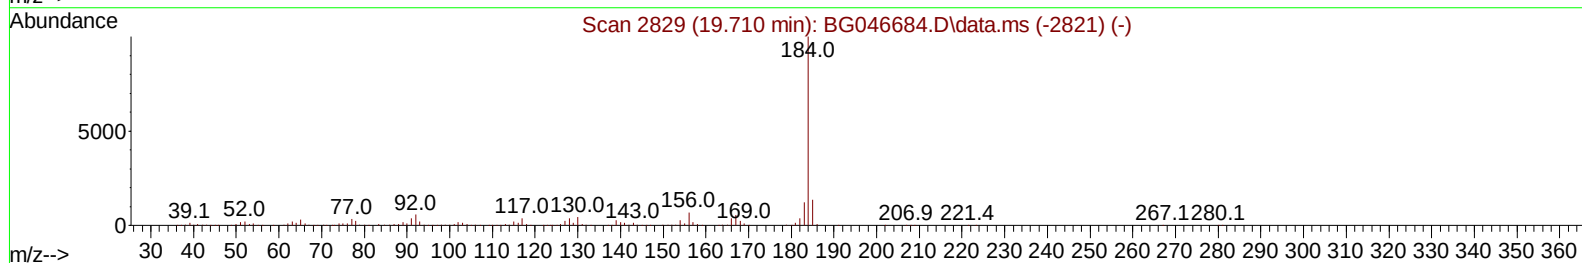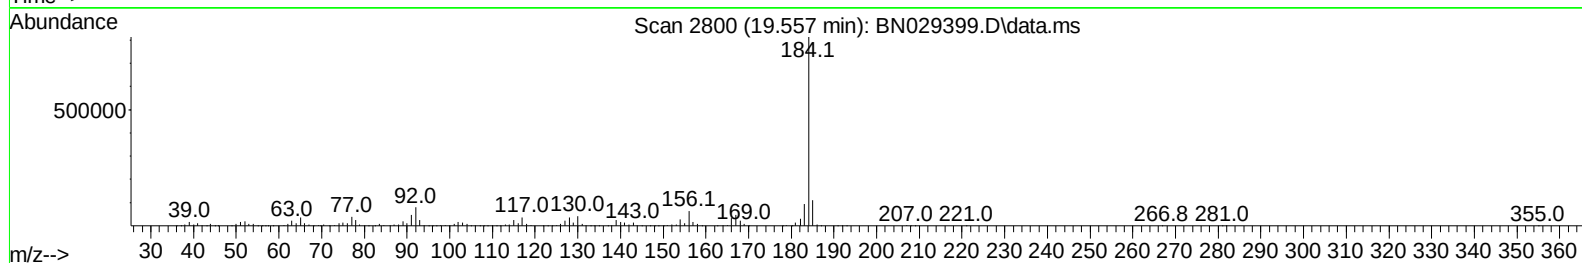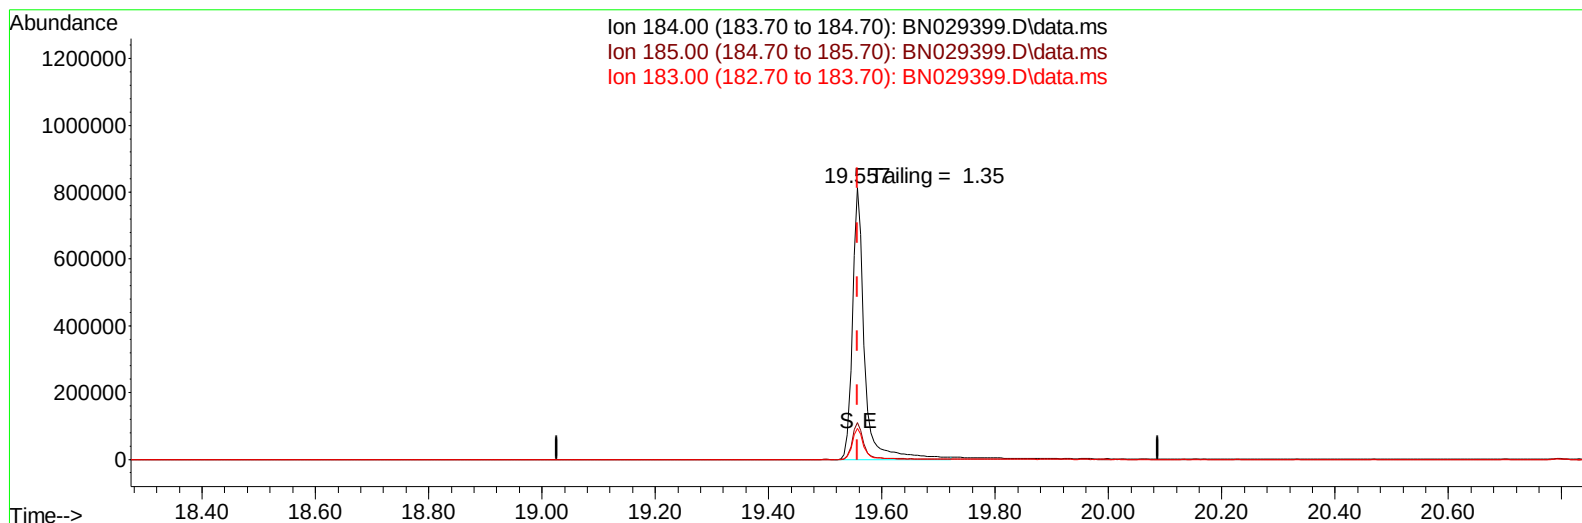

TIC: BN029399.D\data.ms

(77) Benzidine

19.557min (0.000) 0.00 ng

response 1210270

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.47
183.00	13.20	11.56
0.00	0.00	0.00