


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012924\
Data File : BN029399.D
Acq On : 29 Jan 2024 14:01
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN012924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jan 30 03:38:24 2024

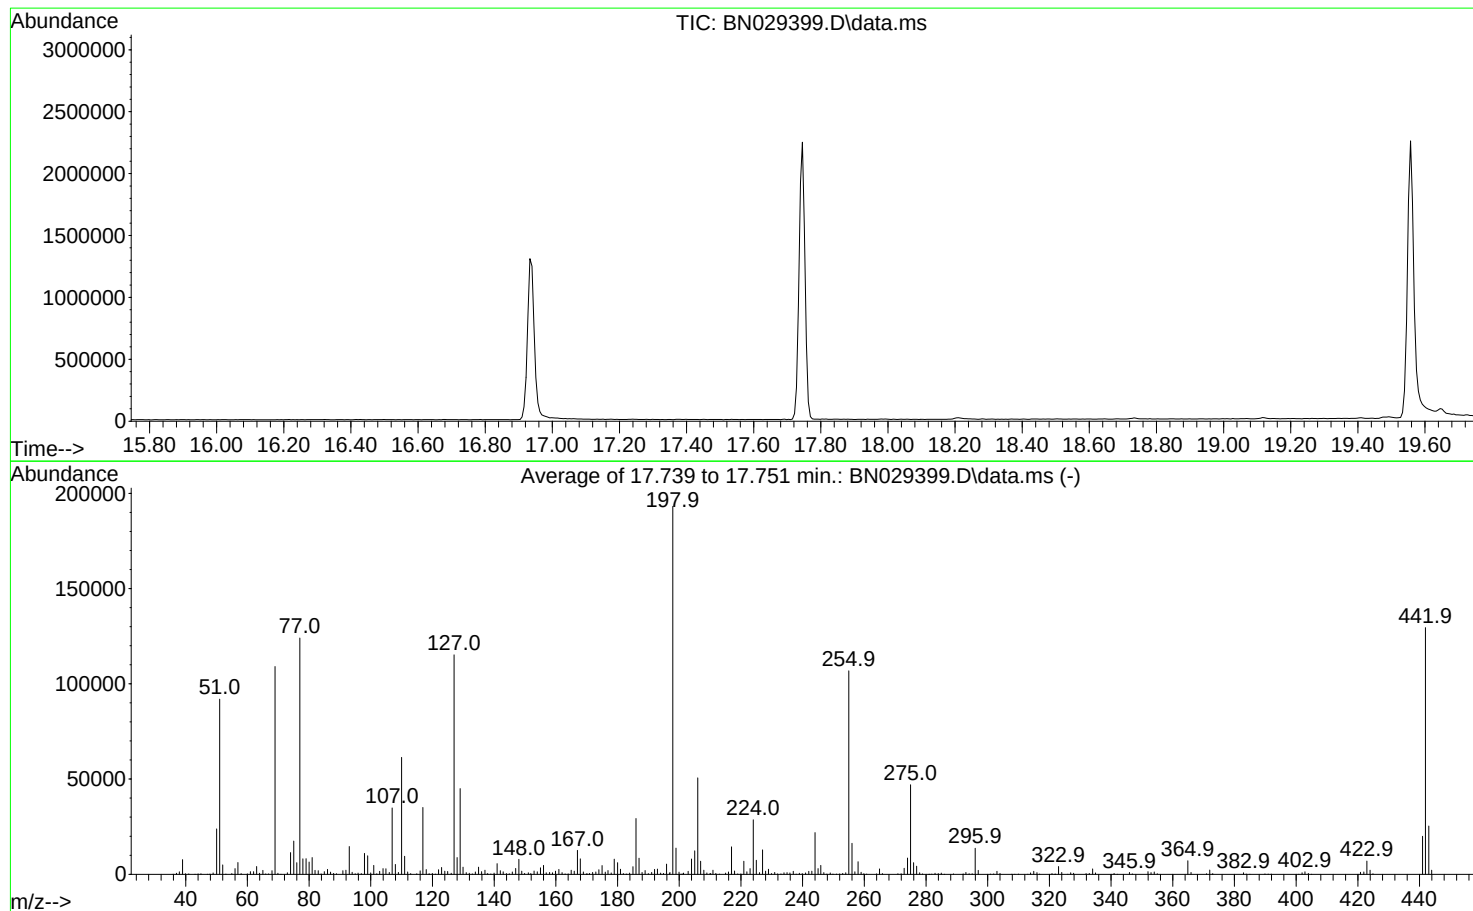




AutoFind: Scans 2491, 2492, 2493; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.6	91941	PASS
68	69	0.00	2	1.8	1922	PASS
69	198	0.00	100	56.5	109077	PASS
70	69	0.00	2	0.5	540	PASS
127	198	10	80	59.7	115267	PASS
197	198	0.00	2	0.5	958	PASS
198	198	100	100	100.0	193173	PASS
199	198	5	9	7.1	13732	PASS
275	198	10	60	24.3	46992	PASS
365	198	1	100	3.7	7144	PASS
441	198	0.01	100	10.3	19987	PASS
442	442	50	100	100.0	129517	PASS
443	442	15	24	19.5	25296	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012924\
Data File : BN029399.D
Acq On : 29 Jan 2024 14:01
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 30 04:03:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 30 04:03:06 2024
Response via : Initial Calibration

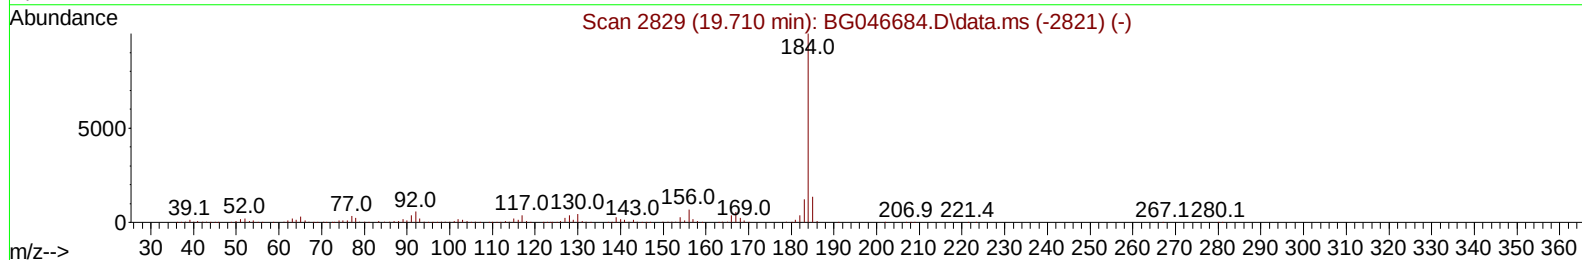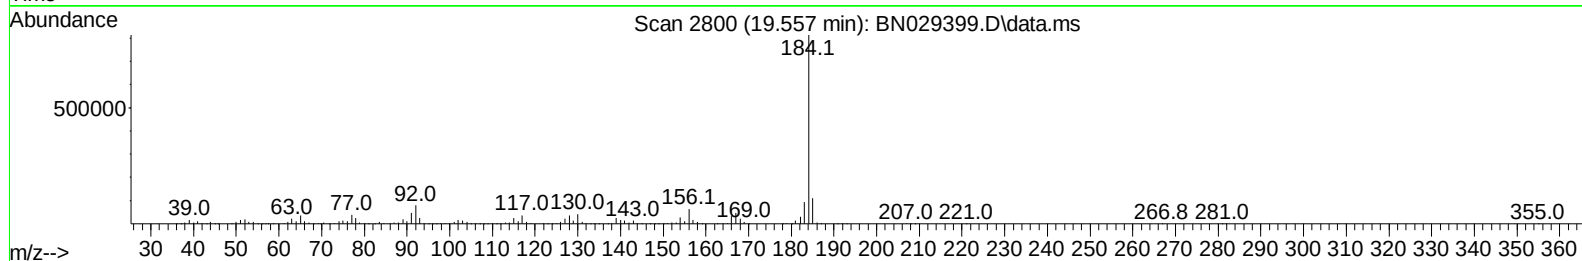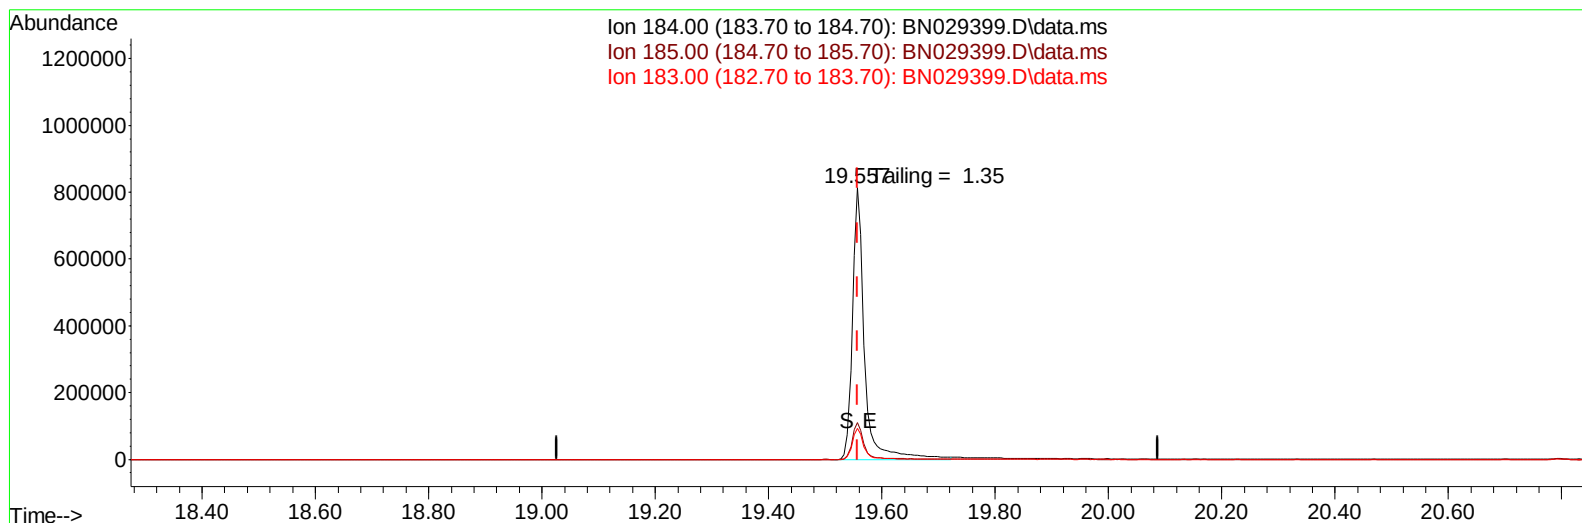

TIC: BN029399.D\data.ms

(77) Benzidine

19.557min (0.000) 0.00 ng

response 1210270

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.47
183.00	13.20	11.56
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/29/2024	BNA_N	<u>BN029399.D</u>
Compound Name	Response	Retention Time
DDT	566313	20.792
DDD	4584	20.404
DDE	0	20.004
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4584	570897	0.80

Instrument :
BNA_N
ClientSampleId :
DFTPP