

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012925\
 Data File : BN036113.D
 Acq On : 29 Jan 2025 18:42
 Operator : RC/JU
 Sample : PB166297BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB166297BL

Quant Time: Jan 30 00:35:33 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN012225.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 23 00:34:56 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.803	152	2136	0.400	ng	-0.01
7) Naphthalene-d8	10.600	136	4915	0.400	ng	-0.01
13) Acenaphthene-d10	14.442	164	2707	0.400	ng	0.00
19) Phenanthrene-d10	17.186	188	5606	0.400	ng	0.00
29) Chrysene-d12	21.376	240	4293	0.400	ng	0.00
35) Perylene-d12	23.678	264	4681	0.400	ng	# 0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.419	112	2354	0.424	ng	0.03
5) Phenol-d6	7.023	99	2714	0.416	ng	0.05
8) Nitrobenzene-d5	8.956	82	1959	0.422	ng	0.00
11) 2-Methylnaphthalene-d10	12.192	152	2885	0.432	ng	0.00
14) 2,4,6-Tribromophenol	15.945	330	538	0.310	ng	0.02
15) 2-Fluorobiphenyl	13.073	172	4491	0.372	ng	0.00
27) Fluoranthene-d10	19.220	212	6282	0.433	ng	0.00
31) Terphenyl-d14	19.820	244	5035	0.565	ng	0.00
Target Compounds						
6) bis(2-Chloroethyl)ether	7.138	93	127	0.024	ng	# 25
24) Pentachlorophenol	16.864	266	96	0.042	ng	# 73
34) Bis(2-ethylhexyl)phtha...	21.286	149	253	0.030	ng	# 75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012925\
Data File : BN036113.D
Acq On : 29 Jan 2025 18:42
Operator : RC/JU
Sample : PB166297BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB166297BL


Quant Time: Jan 30 00:35:33 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN012225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 23 00:34:56 2025
Response via : Initial Calibration

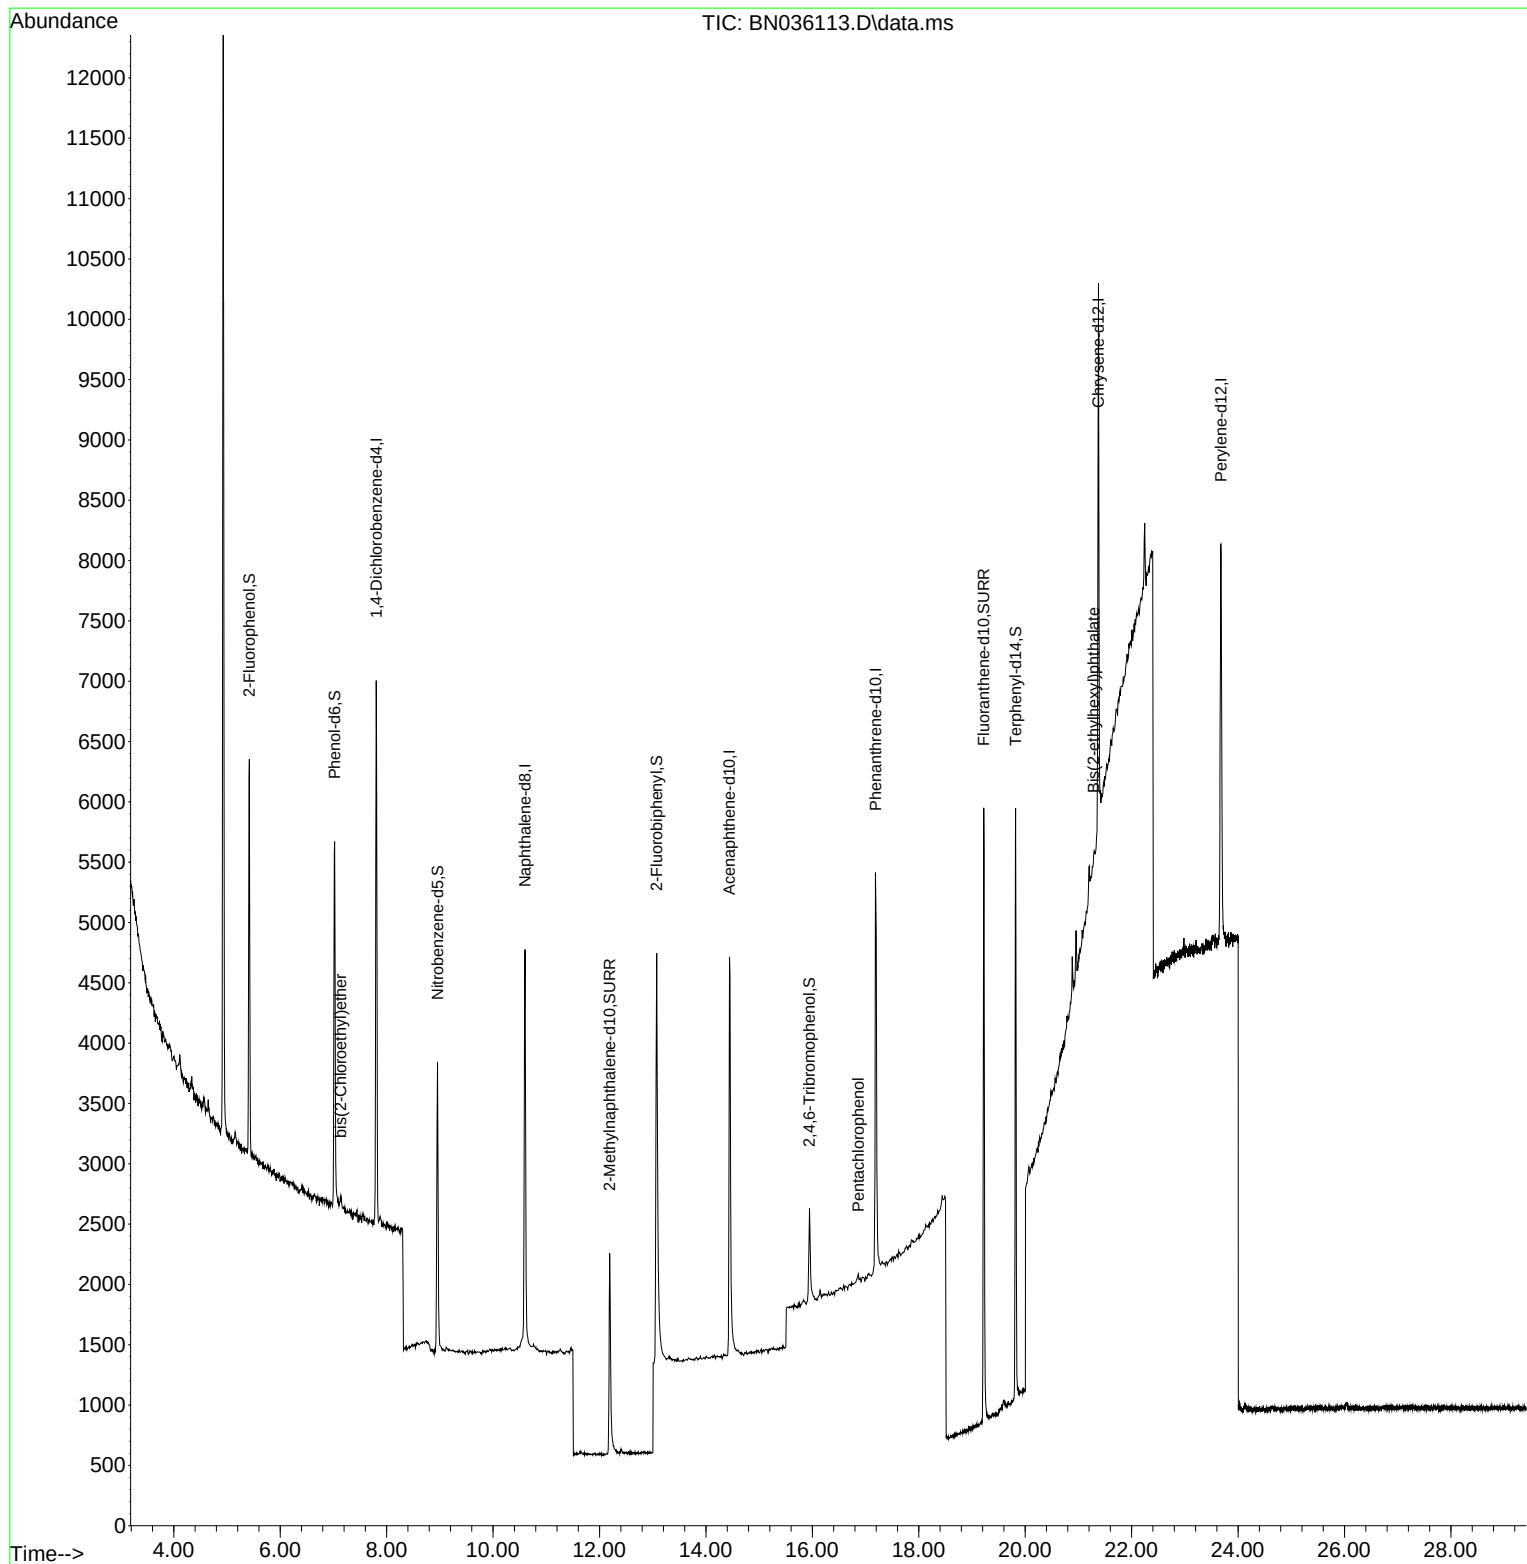



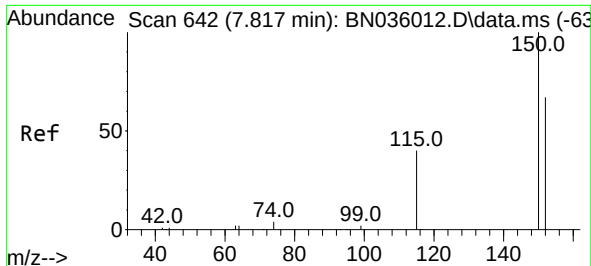


#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.803 min Scan# 64
 Delta R.T. -0.014 min
 Lab File: BN036113.D
 Acq: 29 Jan 2025 18:42

Instrument :
 BNA_N
 ClientSampleId :
 PB166297BL



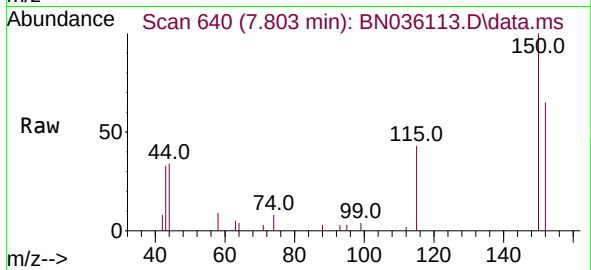



Tgt Ion:152 Resp: 2136
 Ion Ratio Lower Upper
 152 100
 150 153.7 117.4 176.2
 115 65.7 51.0 76.4

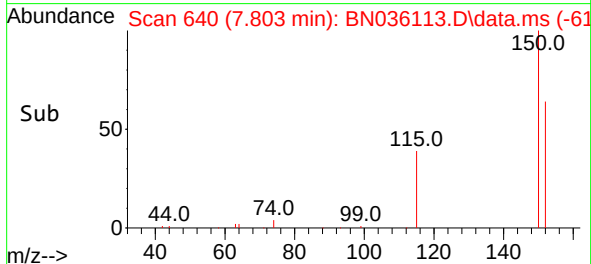

#4
 2-Fluorophenol
 Concen: 0.424 ng
 RT: 5.419 min Scan# 310
 Delta R.T. 0.029 min
 Lab File: BN036113.D
 Acq: 29 Jan 2025 18:42

Tgt Ion:112 Resp: 2354
 Ion Ratio Lower Upper
 112 100
 64 64.1 50.0 75.0
 63 37.8 30.7 46.1


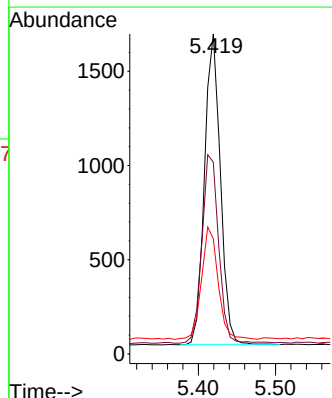

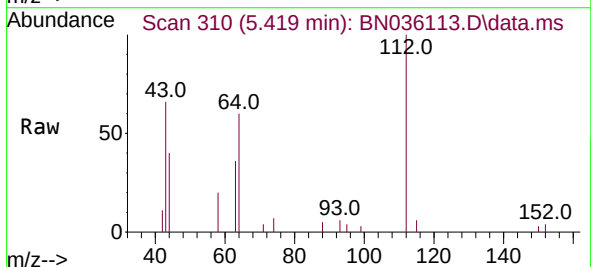


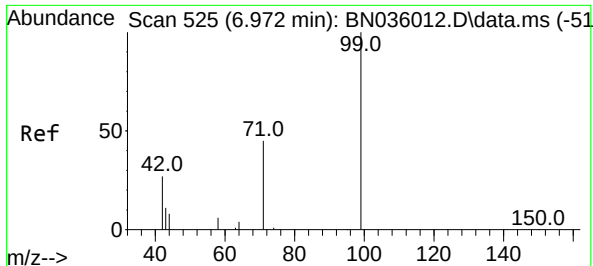

#5
Phenol-d6
Concen: 0.416 ng
RT: 7.023 min Scan# 51
Delta R.T. 0.051 min
Lab File: BN036113.D
Acq: 29 Jan 2025 18:42




Instrument :
BNA_N
ClientSampleId :
PB166297BL


Tgt Ion: 99 Resp: 2714
Ion Ratio Lower Upper
99 100
42 25.2 26.8 40.2#
71 43.1 36.6 55.0

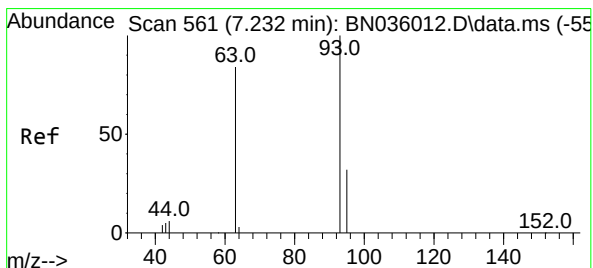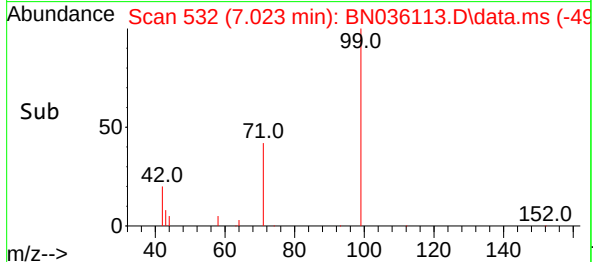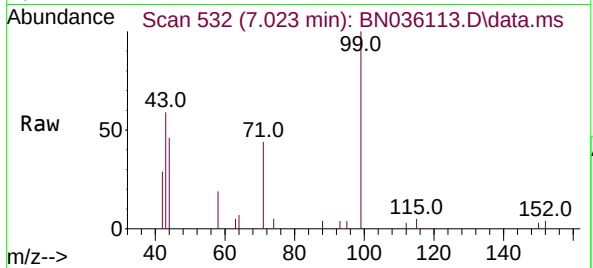

#6
bis(2-Chloroethyl)ether
Concen: 0.024 ng
RT: 7.138 min Scan# 548
Delta R.T. -0.094 min
Lab File: BN036113.D
Acq: 29 Jan 2025 18:42

Tgt Ion: 93 Resp: 127
Ion Ratio Lower Upper
93 100
63 8.7 65.8 98.6#
95 0.0 25.8 38.6#


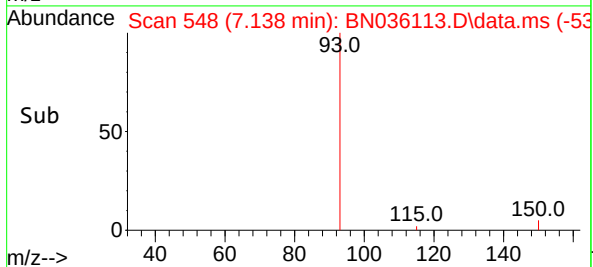

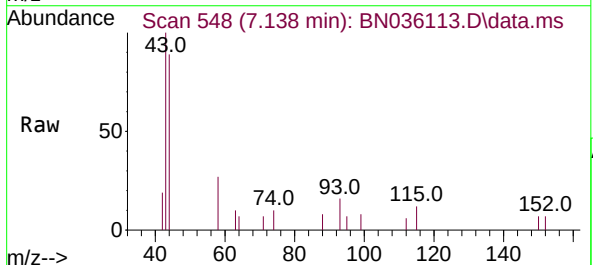


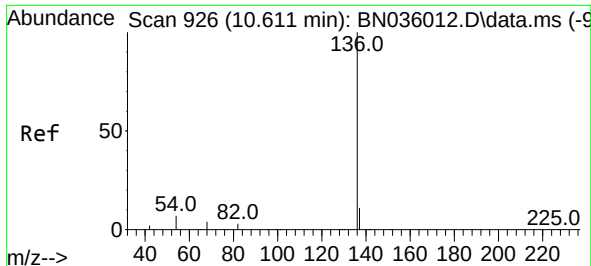

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.600 min Scan# 91
Delta R.T. -0.011 min
Lab File: BN036113.D
Acq: 29 Jan 2025 18:42




Instrument :
BNA_N
ClientSampleId :
PB166297BL


Tgt Ion:136	Resp:	4915
Ion	Ratio	Lower Upper
136	100	
137	12.4	10.4 15.6
54	9.5	7.7 11.5
68	6.7	5.4 8.0

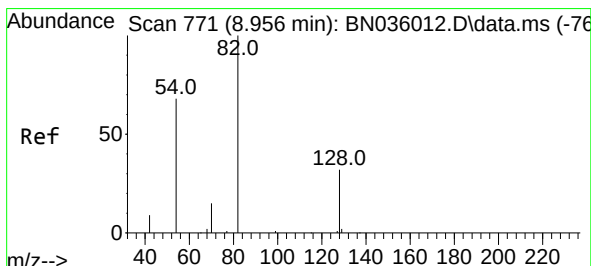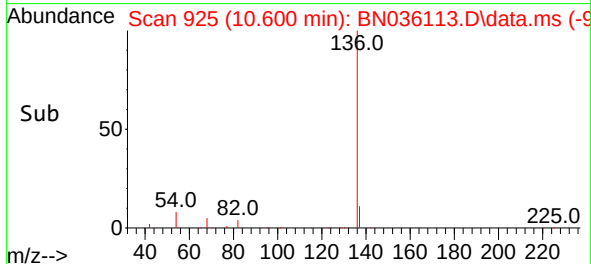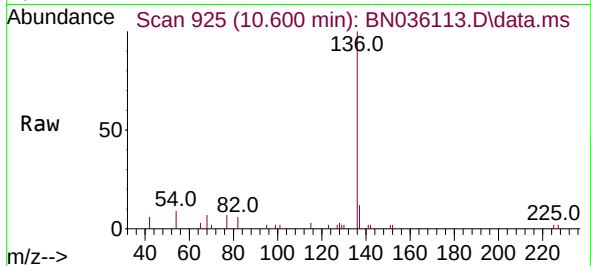

#8
Nitrobenzene-d5
Concen: 0.422 ng
RT: 8.956 min Scan# 771
Delta R.T. -0.000 min
Lab File: BN036113.D
Acq: 29 Jan 2025 18:42

Tgt Ion: 82	Resp:	1959
Ion	Ratio	Lower Upper
82	100	
128	41.8	28.8 43.2
54	59.0	55.8 83.8


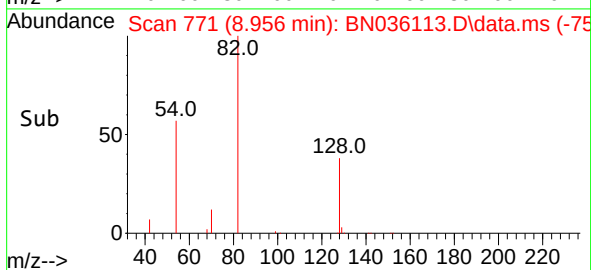

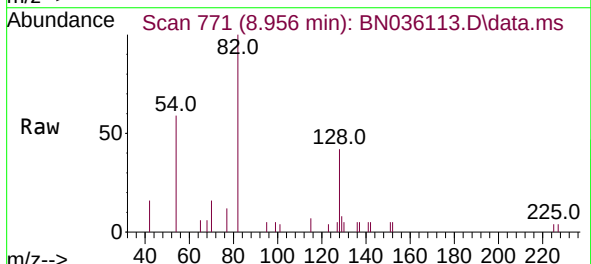


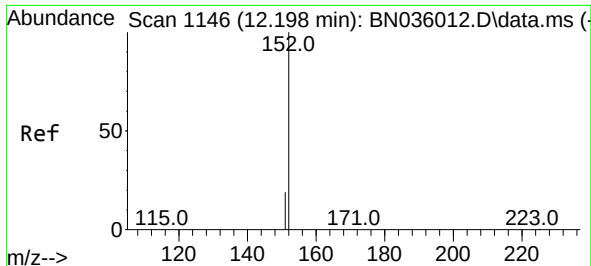

#11
2-Methylnaphthalene-d10
Concen: 0.432 ng
RT: 12.192 min Scan# 1145
Delta R.T. -0.005 min
Lab File: BN036113.D
Acq: 29 Jan 2025 18:42




Instrument :
BNA_N
ClientSampleId :
PB166297BL


Tgt Ion:152 Resp: 2885
Ion Ratio Lower Upper
152 100
151 20.6 16.6 25.0

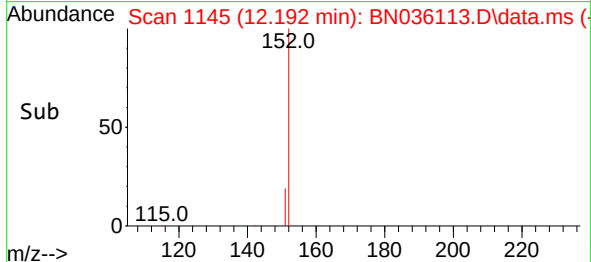

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.442 min Scan# 1440
Delta R.T. -0.006 min
Lab File: BN036113.D
Acq: 29 Jan 2025 18:42


Tgt Ion:164 Resp: 2707
Ion Ratio Lower Upper
164 100
162 101.9 84.1 126.1
160 51.3 43.8 65.8

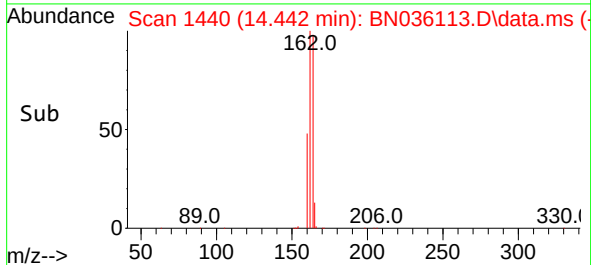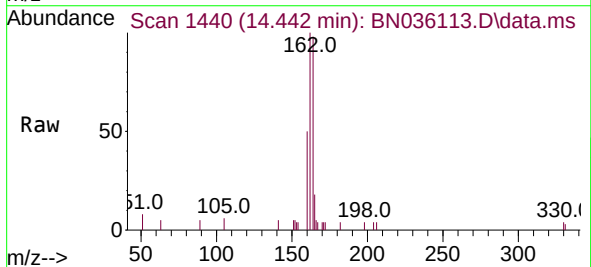






#14
2,4,6-Tribromophenol
Concen: 0.310 ng
RT: 15.945 min Scan# 1575
Delta R.T. 0.017 min
Lab File: BN036113.D
Acq: 29 Jan 2025 18:42

Instrument :
BNA_N
ClientSampleId :
PB166297BL







Tgt Ion:330 Resp: 538
Ion Ratio Lower Upper
330 100
332 94.6 81.0 121.4
141 50.2 36.7 55.1

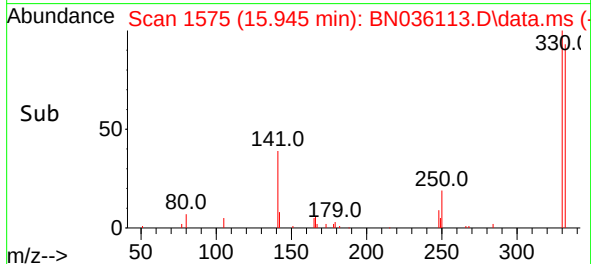

#15
2-Fluorobiphenyl
Concen: 0.372 ng
RT: 13.073 min Scan# 1312
Delta R.T. 0.005 min
Lab File: BN036113.D
Acq: 29 Jan 2025 18:42

Tgt Ion:172 Resp: 4491
Ion Ratio Lower Upper
172 100
171 36.9 30.9 46.3
170 24.5 21.2 31.8


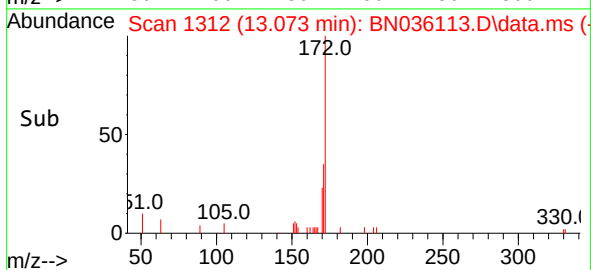

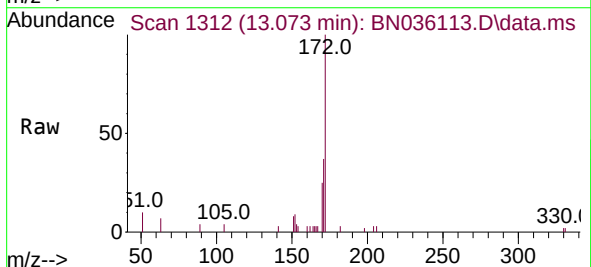




#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.186 min Scan# 11
Delta R.T. 0.005 min
Lab File: BN036113.D
Acq: 29 Jan 2025 18:42




Instrument :
BNA_N
ClientSampleId :
PB166297BL


Tgt Ion:188 Resp: 5606
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 13.8 12.3 18.5

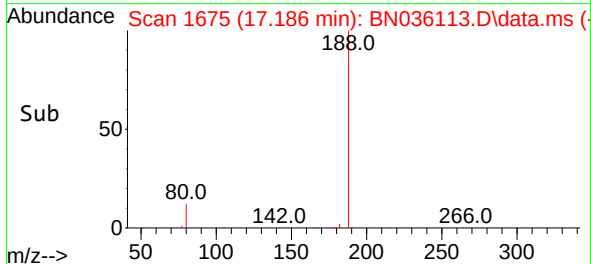

#24
Pentachlorophenol
Concen: 0.042 ng
RT: 16.864 min Scan# 1649
Delta R.T. 0.030 min
Lab File: BN036113.D
Acq: 29 Jan 2025 18:42

Tgt Ion:266 Resp: 96
Ion Ratio Lower Upper
266 100
264 35.4 48.2 72.2#
268 47.9 51.6 77.4#


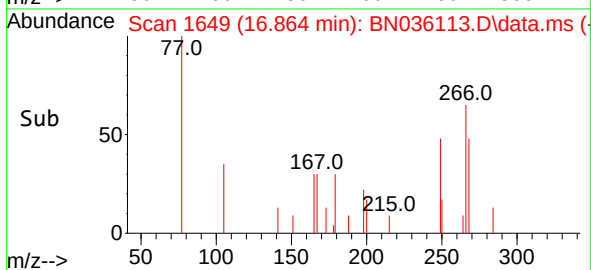

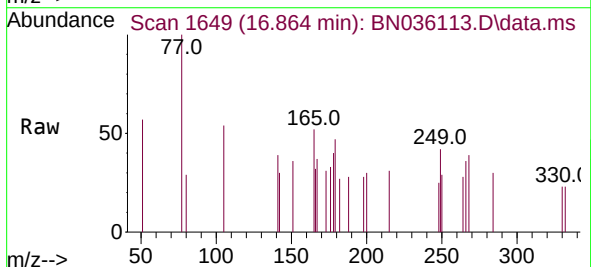


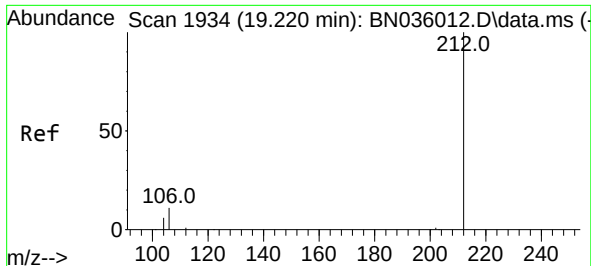

#27
Fluoranthene-d10
Concen: 0.433 ng
RT: 19.220 min Scan# 1934
Delta R.T. 0.000 min
Lab File: BN036113.D
Acq: 29 Jan 2025 18:42




Instrument :
BNA_N
ClientSampleId :
PB166297BL


Tgt Ion:212 Resp: 6282
Ion Ratio Lower Upper
212 100
106 11.6 9.7 14.5
104 7.3 6.0 9.0

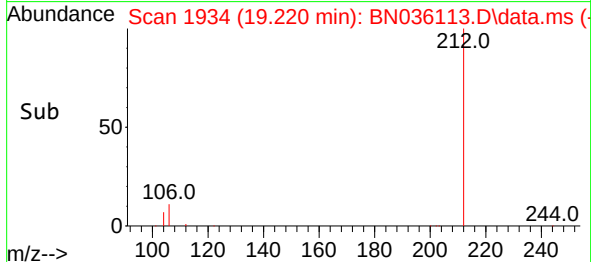

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.376 min Scan# 2256
Delta R.T. 0.009 min
Lab File: BN036113.D
Acq: 29 Jan 2025 18:42


Tgt Ion:240 Resp: 4293
Ion Ratio Lower Upper
240 100
120 16.6 13.9 20.9
236 30.1 23.7 35.5

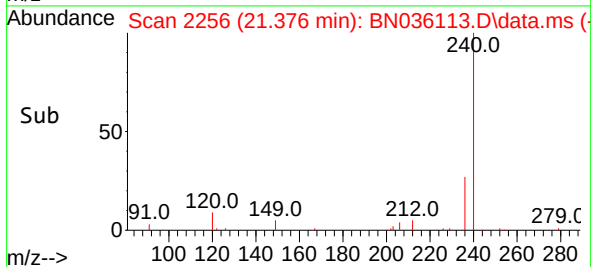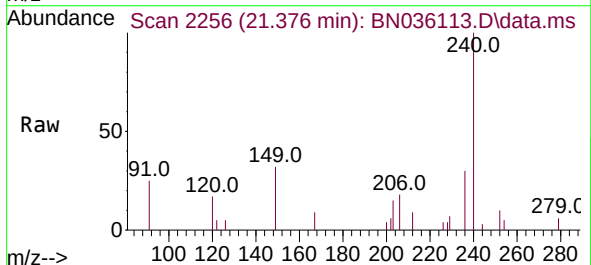



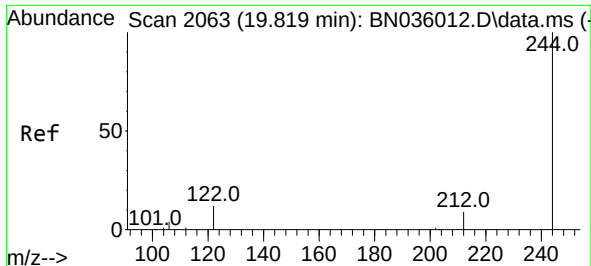


#31
 Terphenyl-d14
 Concen: 0.565 ng
 RT: 19.820 min Scan# 2063
 Delta R.T. 0.000 min
 Lab File: BN036113.D
 Acq: 29 Jan 2025 18:42

Instrument :
 BNA_N
 ClientSampleId :
 PB166297BL



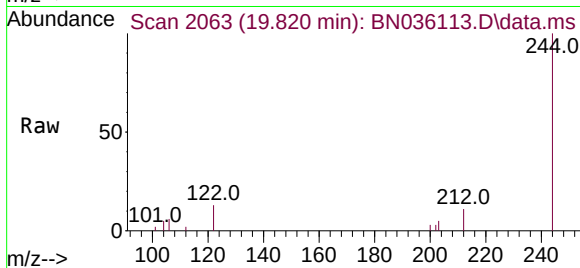



Tgt Ion:244 Resp: 5035
 Ion Ratio Lower Upper
 244 100
 212 10.8 9.1 13.7
 122 12.8 11.3 16.9

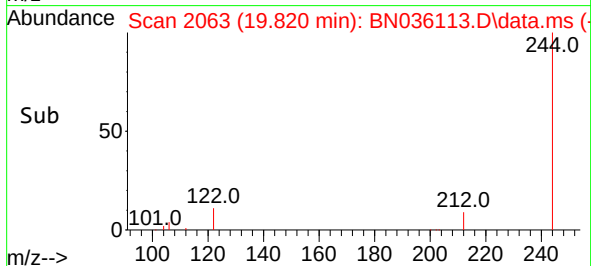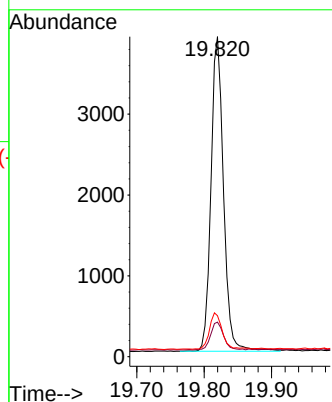

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.030 ng
 RT: 21.286 min Scan# 2246
 Delta R.T. -0.009 min
 Lab File: BN036113.D
 Acq: 29 Jan 2025 18:42

Tgt Ion:149 Resp: 253
 Ion Ratio Lower Upper
 149 100
 167 13.4 21.9 32.9#
 279 0.0 3.0 4.6#

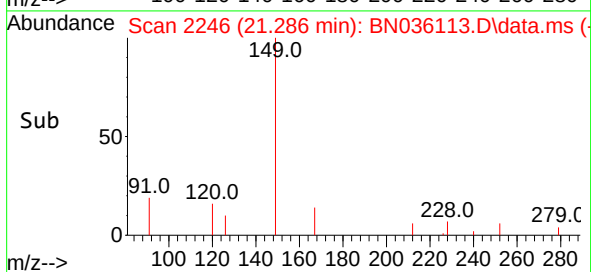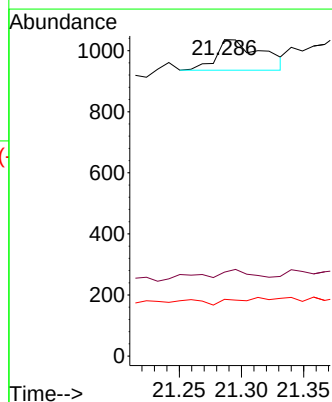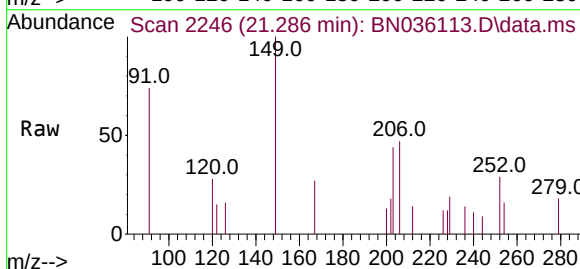

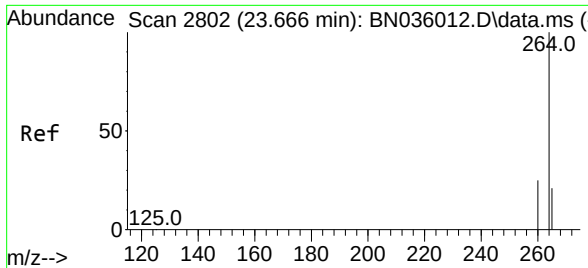

#35
Perylene-d12
Concen: 0.400 ng
RT: 23.678 min Scan# 21
Delta R.T. 0.012 min
Lab File: BN036113.D
Acq: 29 Jan 2025 18:42

Instrument :
BNA_N
ClientSampleId :
PB166297BL

Tgt Ion:264 Resp: 4681
Ion Ratio Lower Upper
264 100
260 26.9 21.8 32.6
265 135.9 56.6 84.8#

