
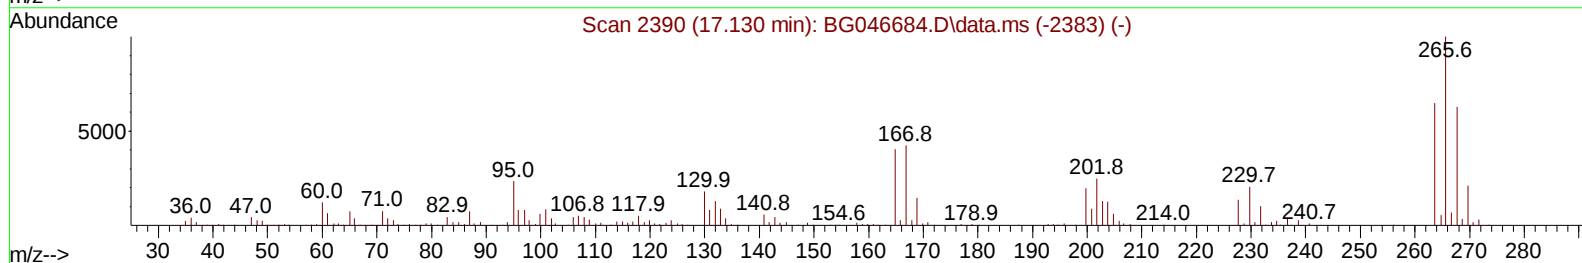
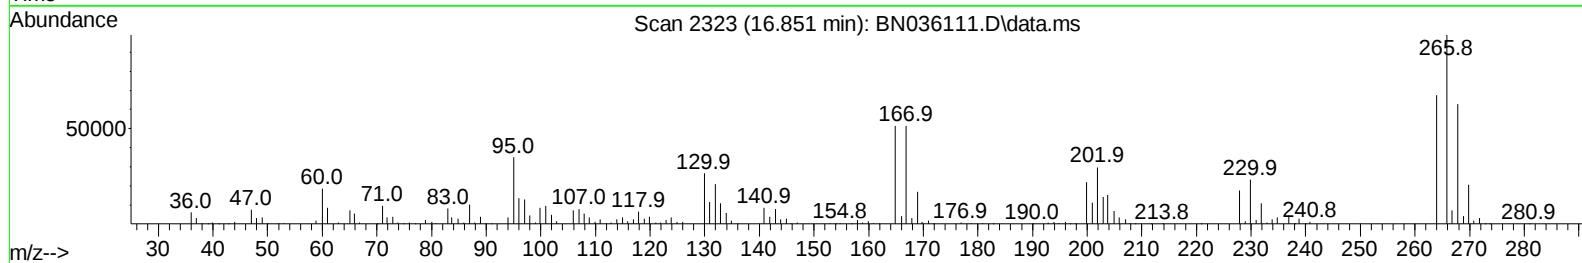


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012925\
Data File : BN036111.D
Acq On : 29 Jan 2025 17:27
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 30 04:00:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

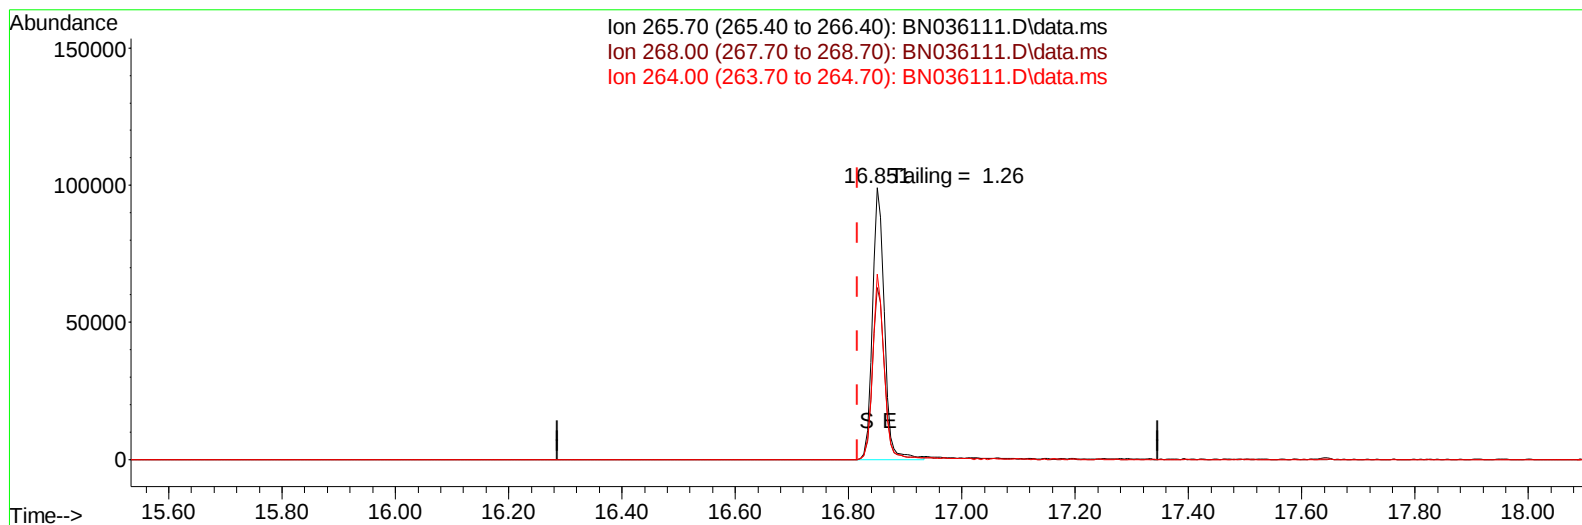




TIC: BN036111.D\data.ms

(70) Pentachlorophenol (C)**16.851min (+ 0.035) 14413.06 ng****response 143876**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.30
264.00	61.60	68.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012925\
Data File : BN036111.D
Acq On : 29 Jan 2025 17:27
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 30 04:00:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

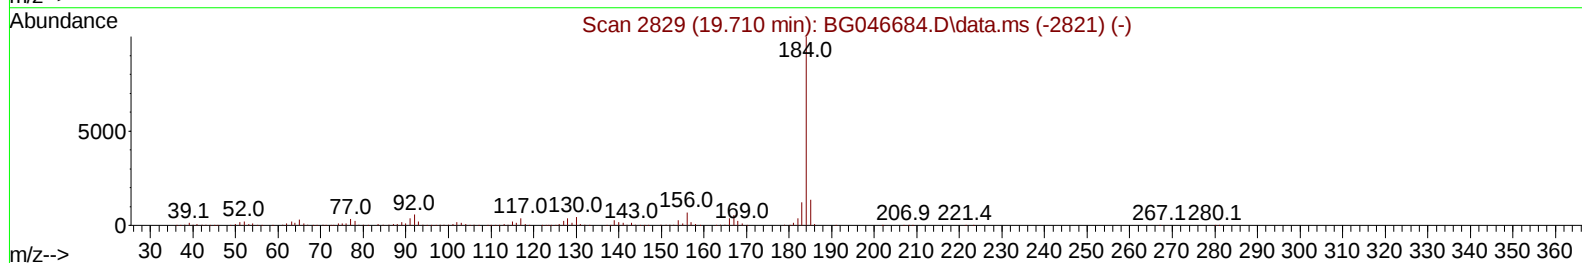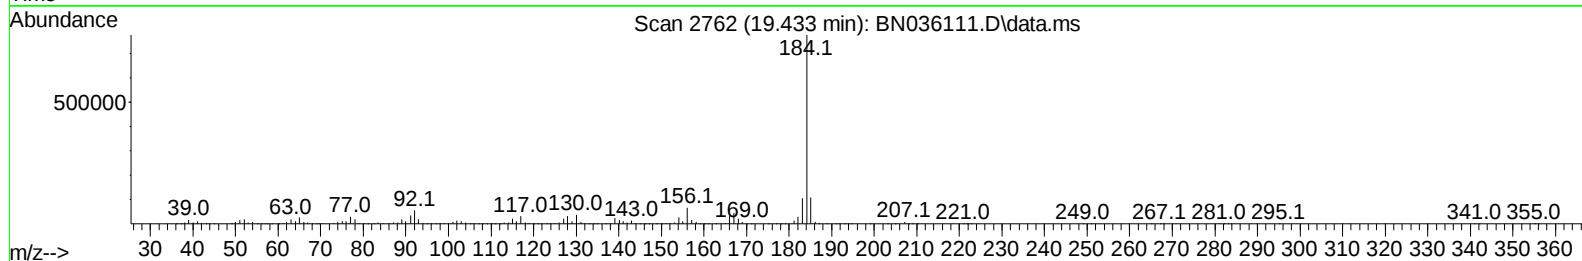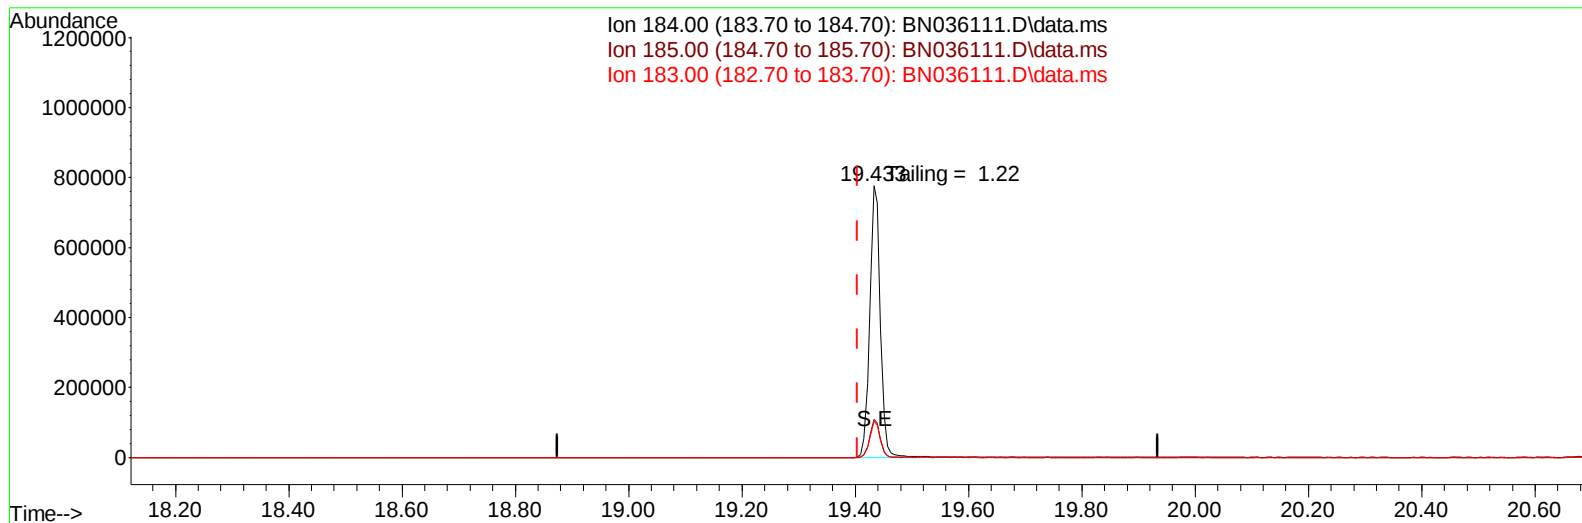

TIC: BN036111.D\data.ms

(77) Benzidine**19.433min (+ 0.029) 611311.00 ng****response 1017570**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.96
183.00	13.20	13.44
0.00	0.00	0.00