

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN013020\
 Data File : BN009486.D
 Acq On : 30 Jan 2020 22:05
 Operator : CG/JU
 Sample : L1300-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jan 31 00:32:54 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 22 15:13:20 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	183616	20.00	ng/ul	0.00
18) Naphthalene-d8	10.20	136	767052	20.00	ng/ul	-0.01
35) Acenaphthene-d10	14.09	164	486785	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.84	188	1018062	20.00	ng/ul	-0.01
77) Chrysene-d12	21.05	240	854264	20.00	ng/ul	0.00
85) Perylene-d12	23.16	264	950554	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.09	96	6513	1.47	ng/uL	0.00
5) Phenol-d5	6.66	99	116702	7.17	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.81	67	86452	7.48	ng/ul	0.00
9) 2-Chlorophenol-d4	7.00	132	89869	7.56	ng/ul	0.00
13) 4-Methylphenol-d8	8.17	113	90006	6.94	ng/ul	0.00
19) Nitrobenzene-d5	8.60	128	43651	7.82	ng/ul	0.00
22) 2-Nitrophenol-d4	9.31	143	47471	8.11	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.85	165	88096	7.60	ng/ul	0.00
29) 4-Chloroaniline-d4	10.36	131	112393	8.02	ng/ul	0.00
43) Dimethylphthalate-d6	13.52	166	311043	8.63	ng/ul	0.00
46) Acenaphthylene-d8	13.78	160	350625	8.20	ng/ul	0.00
51) 4-Nitrophenol-d4	14.33	143	27580	4.11	ng/ul	0.00
57) Fluorene-d10	15.09	176	269102	8.51	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.23	200	31399	5.09	ng/ul	0.00
70) Anthracene-d10	16.94	188	403419	8.57	ng/ul	0.00
78) Pyrene-d10	19.25	212	463513	10.09	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.03	264	446600	9.31	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
6) Phenol	6.68	94	23168	1.358	ng/ul	96
44) Dimethylphthalate	13.56	163	72948	1.967	ng/ul#	98
69) Phenanthrene	16.89	178	72878	1.269	ng/ul	97
76) Fluoranthene	18.91	202	223769	3.398	ng/ul	98
79) Pyrene	19.27	202	272809	4.410	ng/ul	98
82) Benzo(a)anthracene	21.03	228	143513	2.467	ng/ul	99
84) Chrysene	21.09	228	173275	3.058	ng/ul	98
87) Benzo(b)fluoranthene	22.54	252	162004	2.695	ng/ul	98
88) Benzo(k)fluoranthene	22.54	252	162004	2.741	ng/ul	99
90) Benzo(a)pyrene	23.07	252	124644	2.310	ng/ul	99
91) Indeno(1,2,3-cd)pyrene	25.23	276	73333	1.122	ng/ul	93
93) Benzo(g,h,i)perylene	25.85	276	72576	1.335	ng/ul	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN013020\
Data File : BN009486.D
Acq On : 30 Jan 2020 22:05
Operator : CG/JU
Sample : L1300-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jan 31 00:32:54 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 22 15:13:20 2020
Response via : Initial Calibration

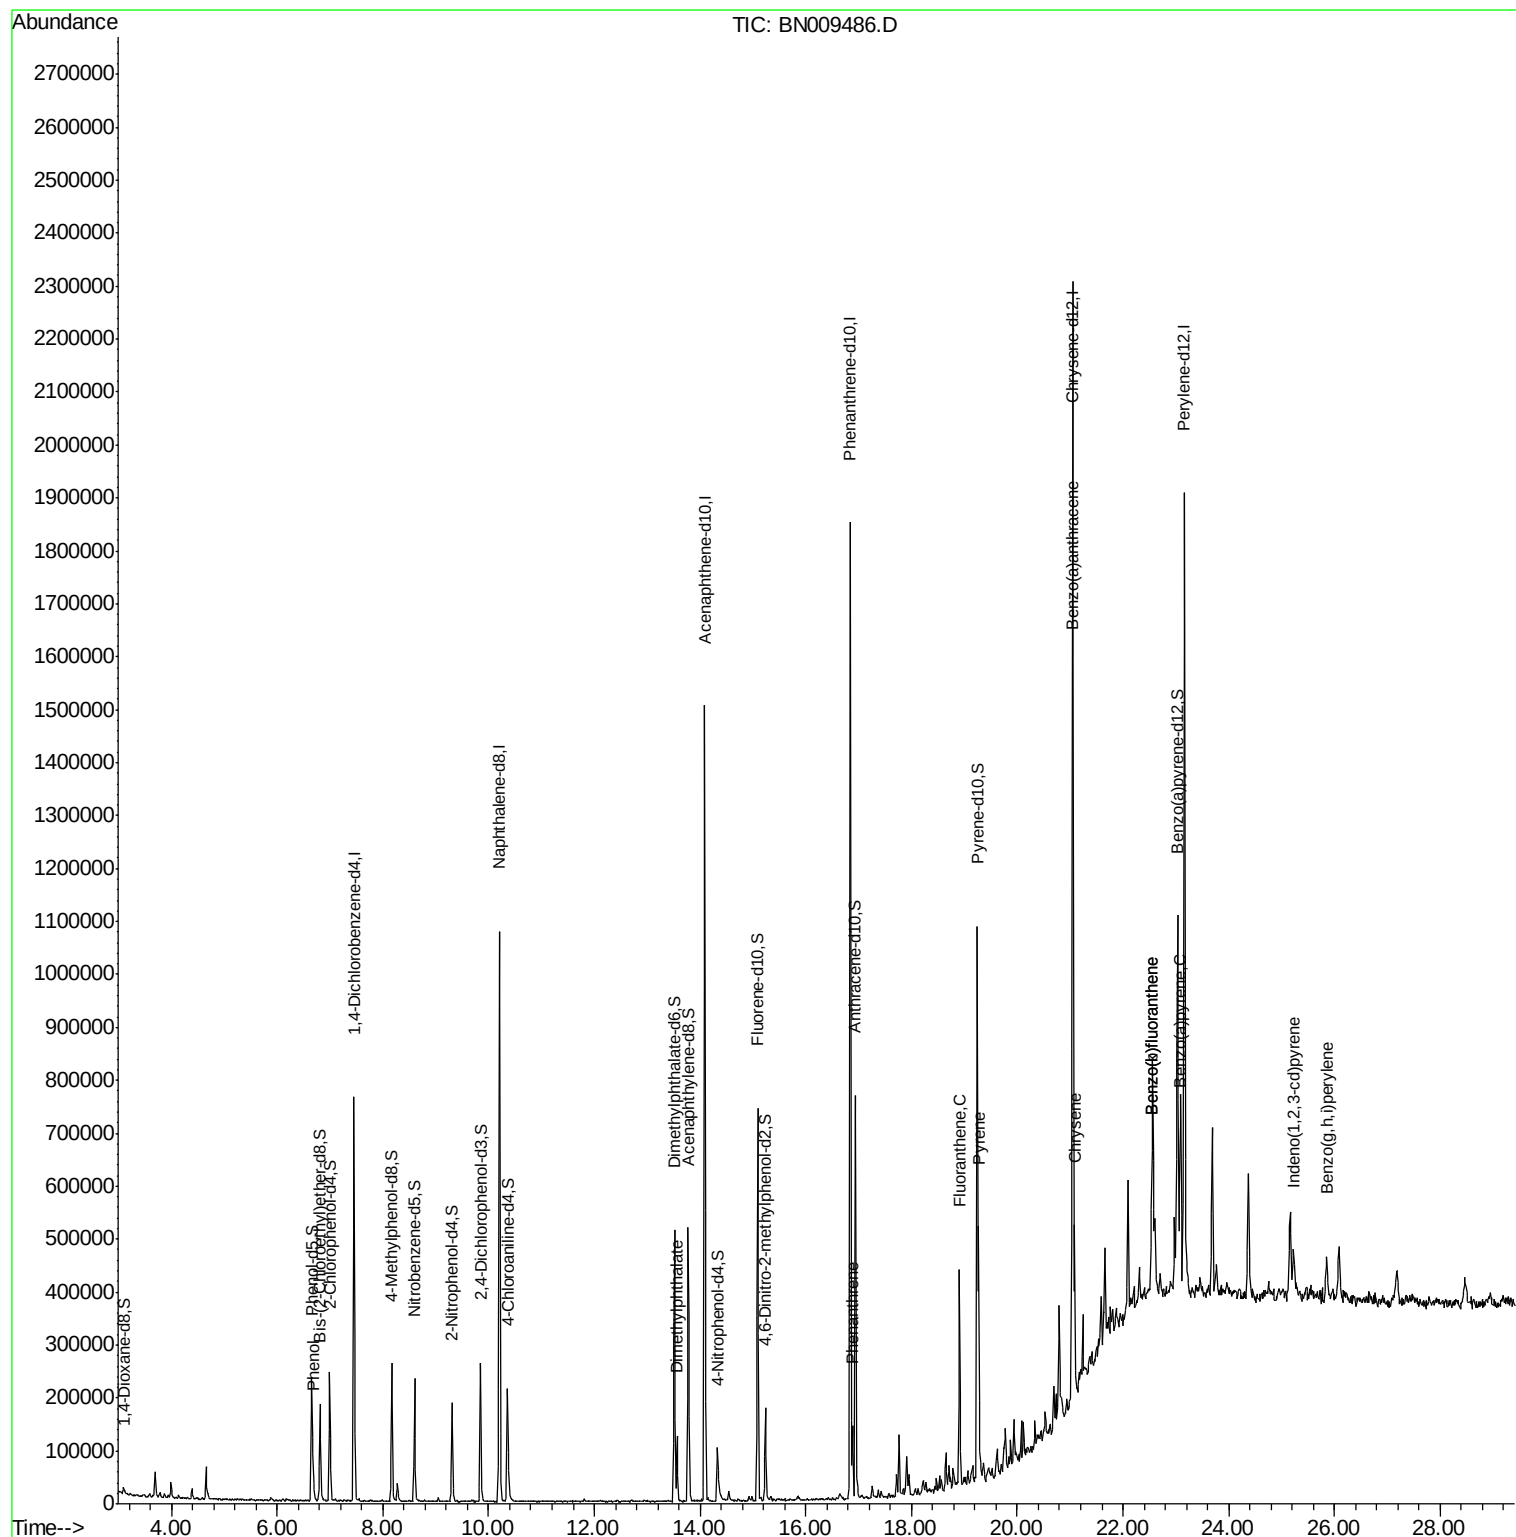

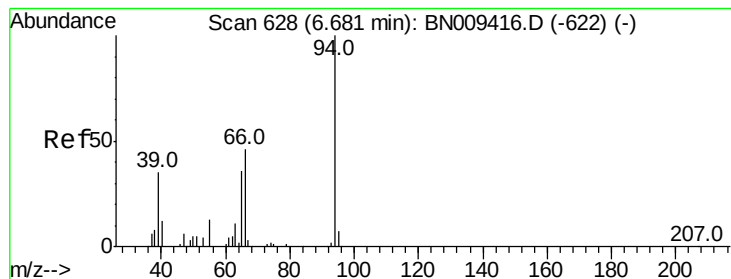

#6

Phenol

Concen: 1.358 ng/ul

RT: 6.68 min Scan# 628

Delta R.T. -0.00 min

Lab File: BN009486.D

Acq: 30 Jan 2020 22:05

Instrument :

BNA_N

ClientSampleId :


Tot Ion: 94 Resp: 23168

Ion Ratio Lower Upper

94 100

65 42.8 29.4 44.0




66 49.7 39.8 59.8

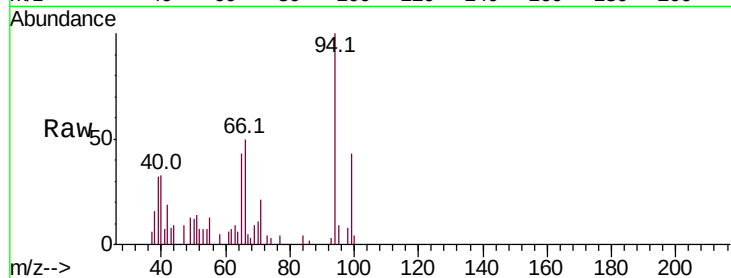

Abundance Ion 94.00 (93.70 to 94.70): BN009416.D (-622) (-)

Ion 65.00 (64.70 to 65.70): BN009416.D (-622) (-)

Ion 66.00 (65.70 to 66.70): BN009416.D (-622) (-)

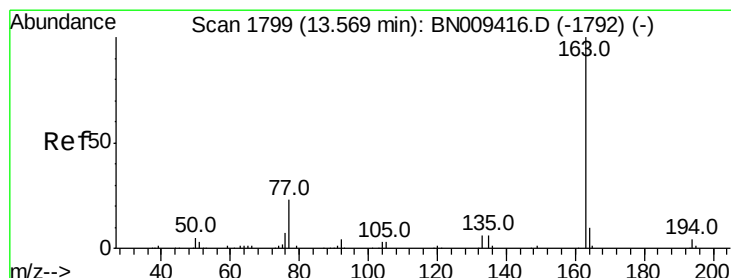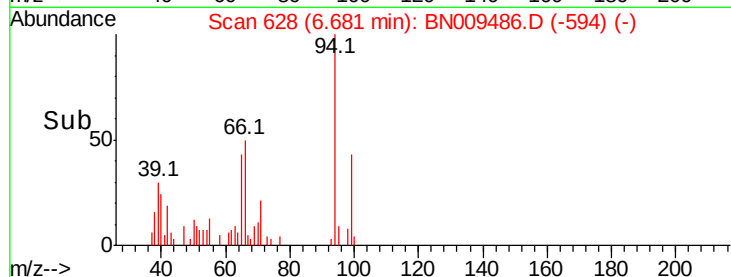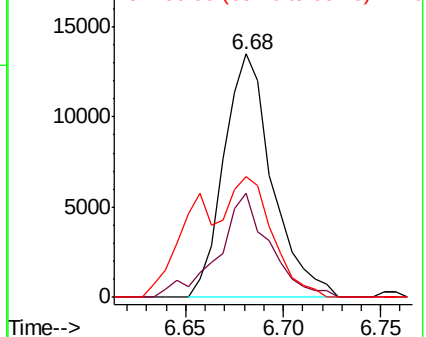

#44

Dimethylphthalate

Concen: 1.967 ng/ul

RT: 13.56 min Scan# 1798

Delta R.T. -0.01 min

Lab File: BN009486.D

Acq: 30 Jan 2020 22:05


Tgt Ion:163 Resp: 72948

Ion Ratio Lower Upper

163 100

194 5.1 3.1 4.7#



164 9.9 8.3 12.5

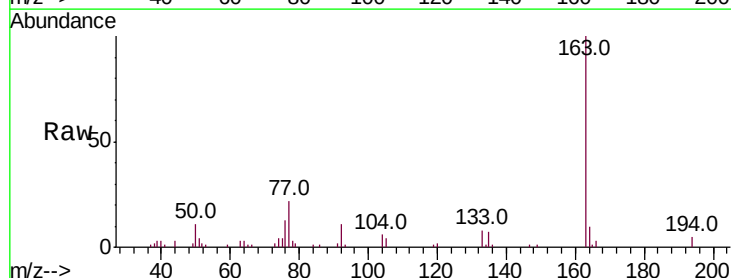


Abundance Ion 163.00 (162.70 to 163.70): BN009416.D (-1792) (-)

Ion 194.00 (193.70 to 194.70): BN009416.D (-1792) (-)

Ion 164.00 (163.70 to 164.70): BN009416.D (-1792) (-)

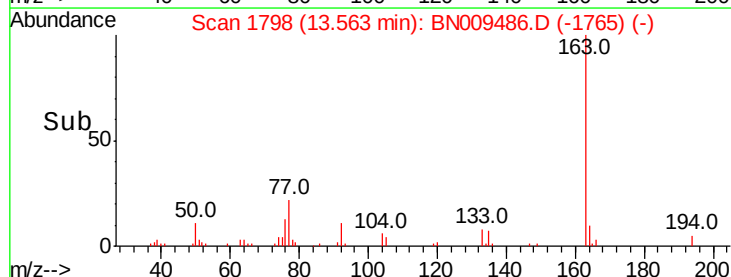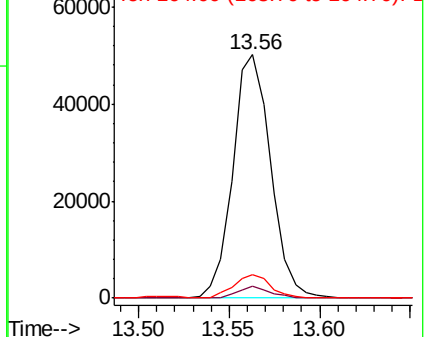

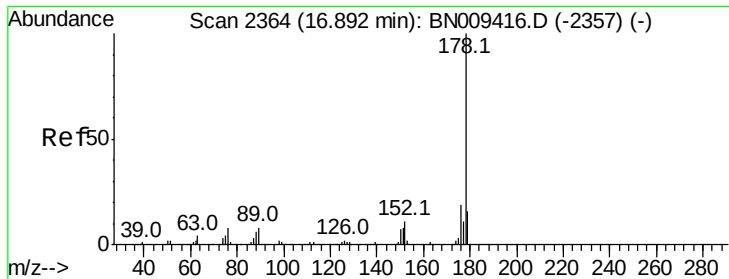

#69

Phenanthrene

Concen: 1.269 ng/ul

RT: 16.89 min Scan# 2363

Delta R.T. -0.01 min

Lab File: BN009486.D

Acq: 30 Jan 2020 22:05

Instrument :

BNA_N

ClientSampleId :


Tot Ion:178 Resp: 72878

Ion Ratio Lower Upper

178 100

179 16.1 13.3 19.9




176 17.1 15.5 23.3

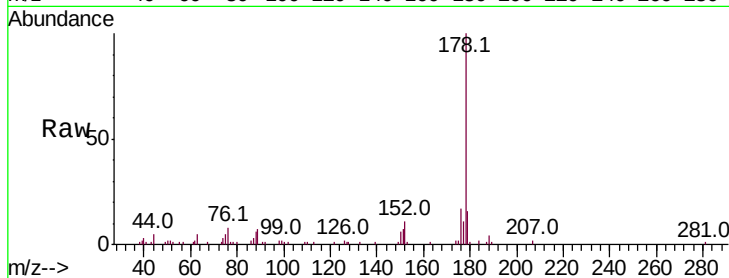

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

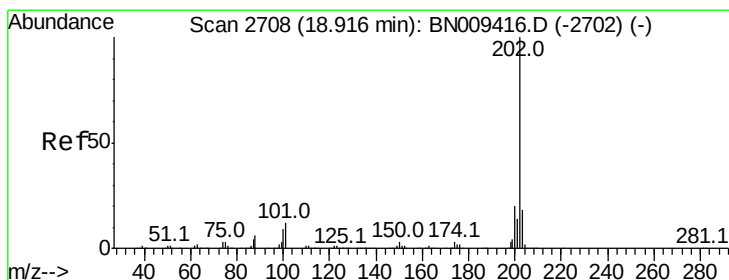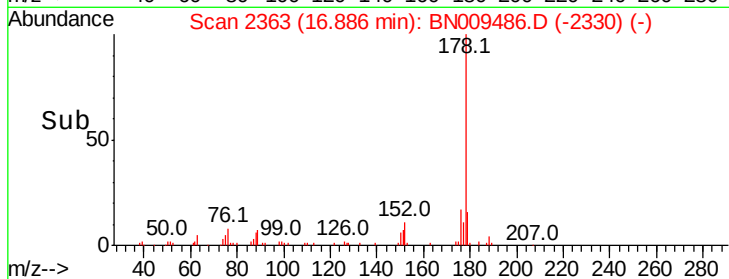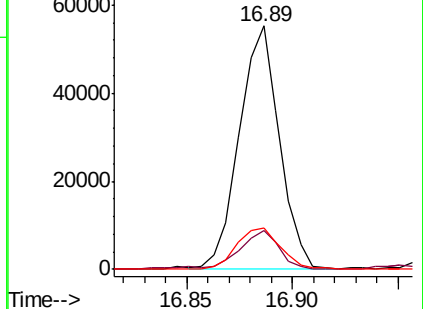

#76

Fluoranthene

Concen: 3.398 ng/ul

RT: 18.91 min Scan# 2707

Delta R.T. -0.01 min

Lab File: BN009486.D

Acq: 30 Jan 2020 22:05


Tgt Ion:202 Resp: 223769

Ion Ratio Lower Upper

202 100

101 10.9 9.7 14.5



100 8.9 7.1 10.7

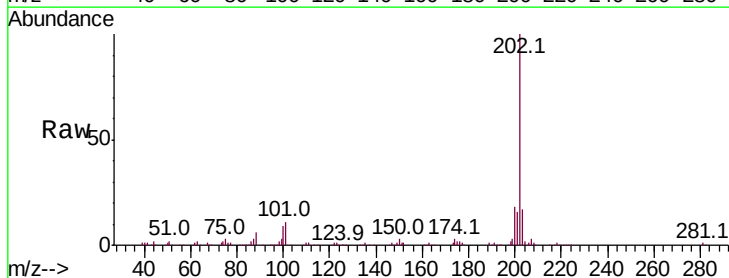


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B



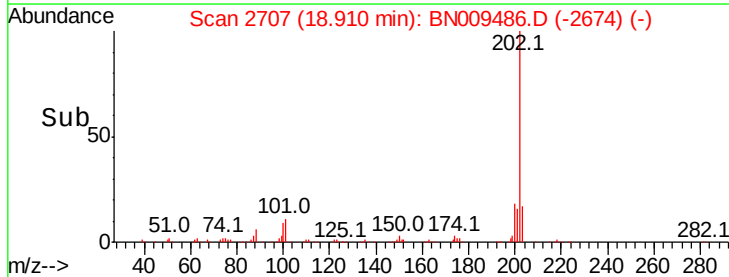
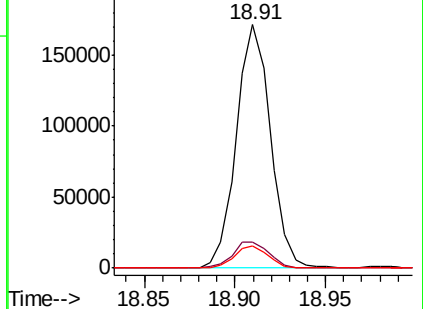


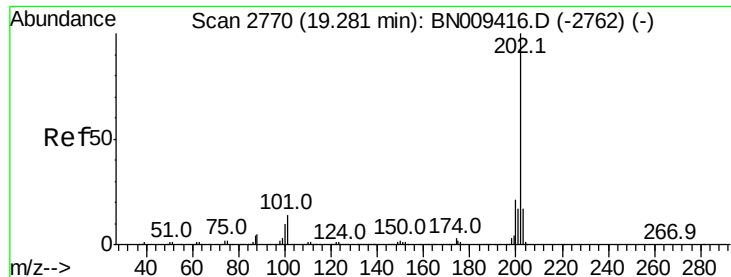

#79
Pvrene
Concen: 4.410 ng/ul
RT: 19.27 min Scan# 2769
Delta R.T. -0.01 min
Lab File: BN009486.D
Acq: 30 Jan 2020 22:05




Instrument :
BNA_N
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
202	100		
101	12.1	10.9	16.3
100	10.9	8.6	12.8

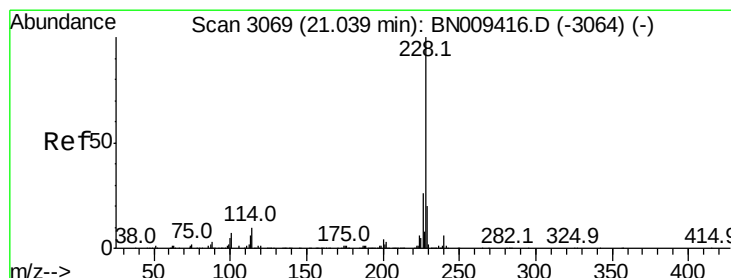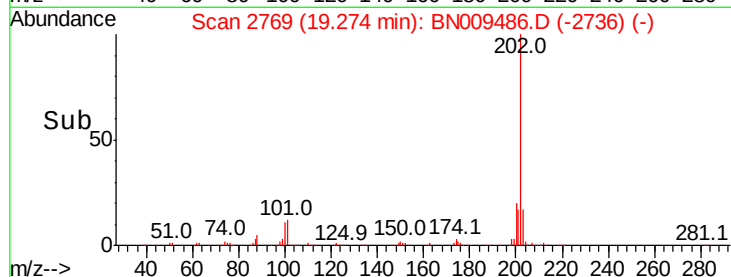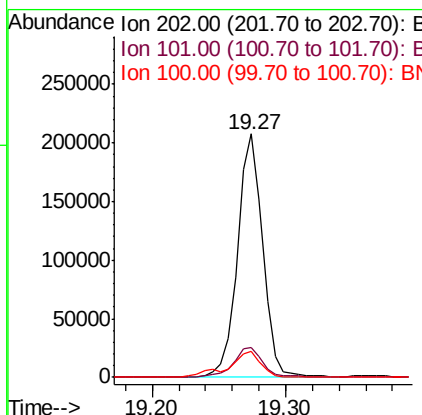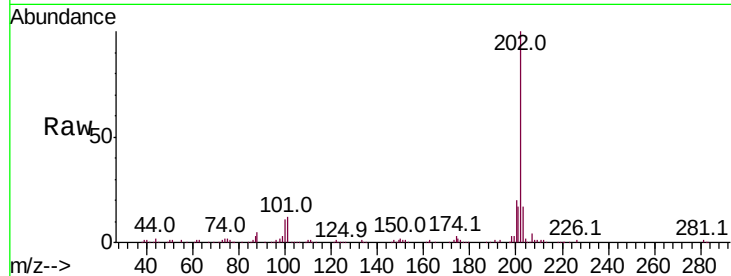

#82
Benzo(a)anthracene
Concen: 2.467 ng/ul
RT: 21.03 min Scan# 3068
Delta R.T. -0.01 min
Lab File: BN009486.D
Acq: 30 Jan 2020 22:05

Tgt Ion	Ratio	Lower	Upper
228	100		
229	19.9	15.9	23.9
226	26.6	20.9	31.3

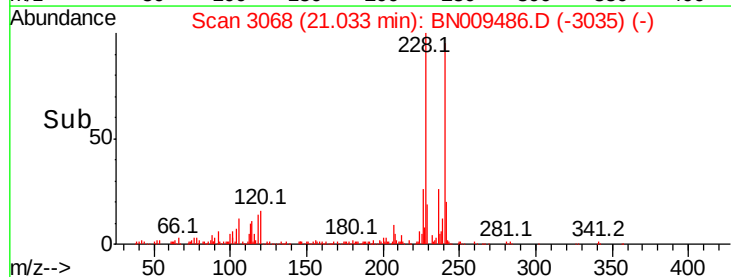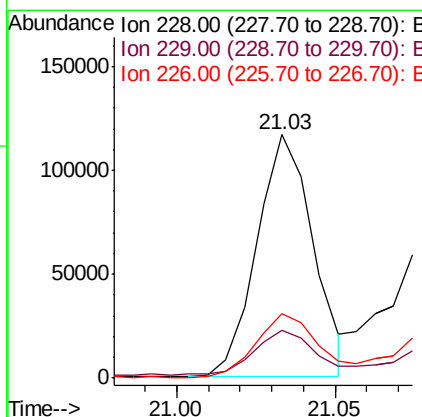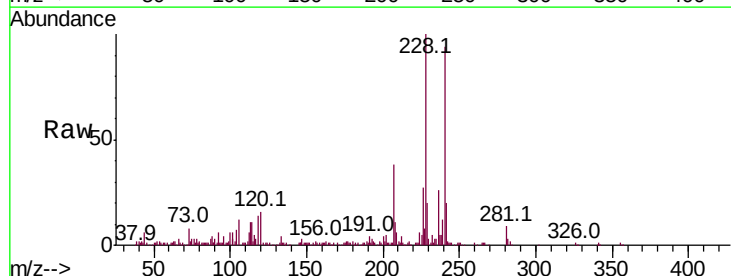

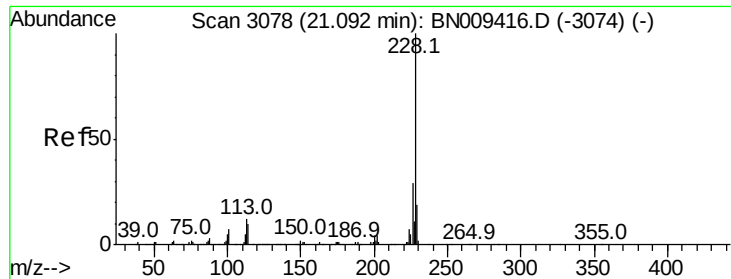

#84

Chrysene

Concen: 3.058 ng/ul

RT: 21.09 min Scan# 3077

Delta R.T. -0.01 min

Lab File: BN009486.D

Acq: 30 Jan 2020 22:05


Instrument :

BNA_N

ClientSampleId :

Tot Ion:228 Resp: 173275




Ion	Ratio	Lower	Upper
228	100		
226	29.8	22.9	34.3
229	20.2	15.4	23.0

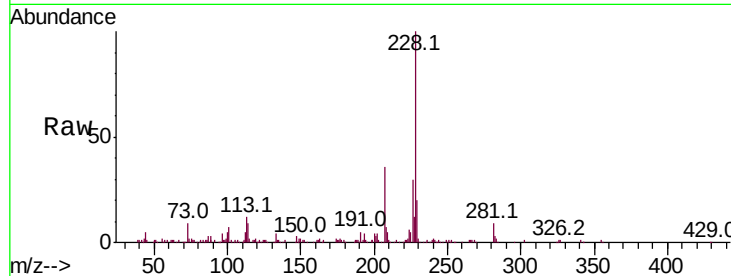

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

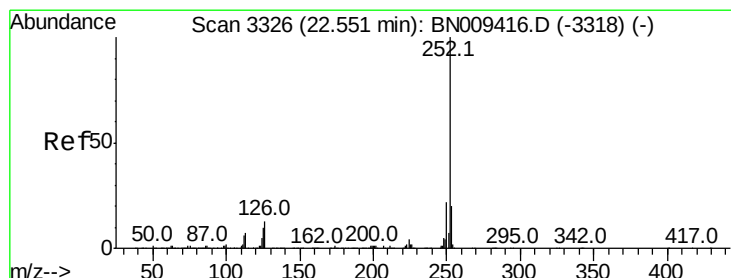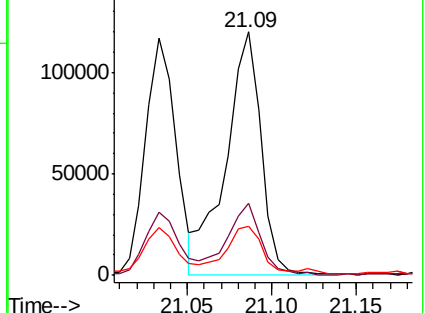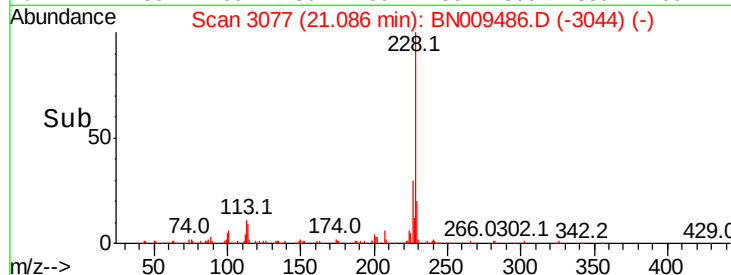

#87

Benzo(b)fluoranthene

Concen: 2.695 ng/ul

RT: 22.54 min Scan# 3325


Delta R.T. -0.01 min

Lab File: BN009486.D

Acq: 30 Jan 2020 22:05

Tgt Ion:252 Resp: 162004



Ion	Ratio	Lower	Upper
252	100		
253	21.4	16.5	24.7
125	10.9	8.2	12.2

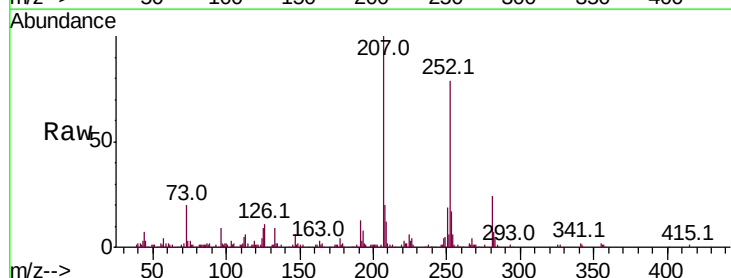


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

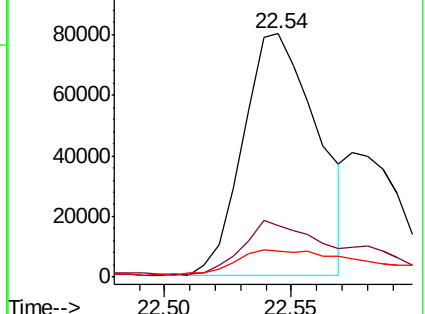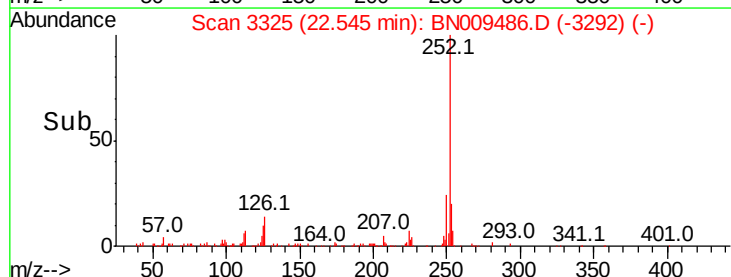

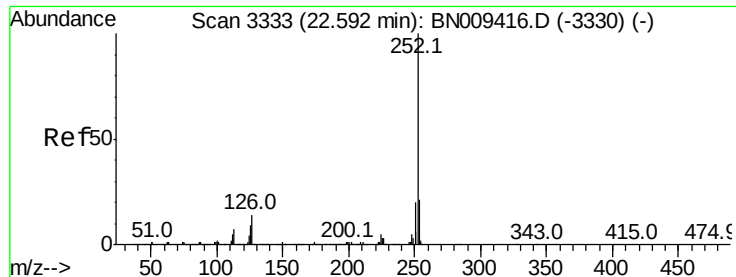

#88

Benzo(k)fluoranthene

Concen: 2.741 ng/ul

RT: 22.54 min Scan# 3325

Delta R.T. -0.05 min

Lab File: BN009486.D

Acq: 30 Jan 2020 22:05

Instrument :

BNA_N

ClientSampleId :


Tot Ion:252 Resp: 162004

Ion Ratio Lower Upper

252 100

253 21.4 17.0 25.4




125 10.9 7.8 11.8

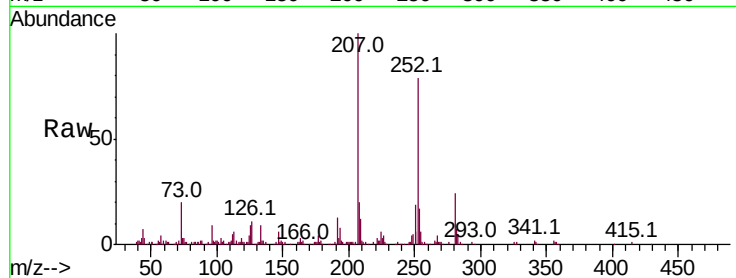

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

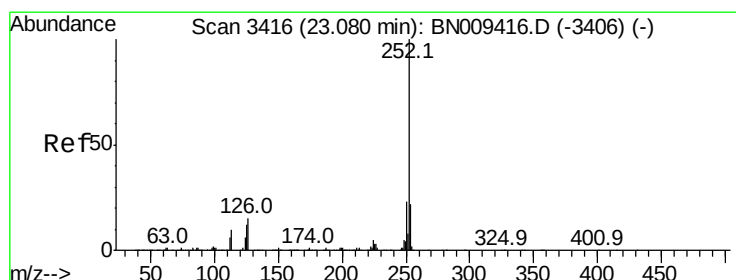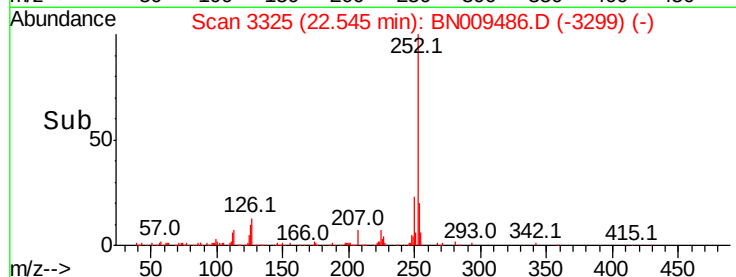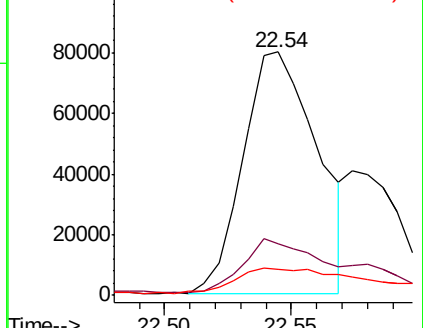

#90

Benzo(a)pyrene

Concen: 2.310 ng/ul

RT: 23.07 min Scan# 3415

Delta R.T. -0.01 min

Lab File: BN009486.D

Acq: 30 Jan 2020 22:05


Tgt Ion:252 Resp: 124644

Ion Ratio Lower Upper

252 100

253 22.2 18.0 27.0



125 12.5 9.8 14.6

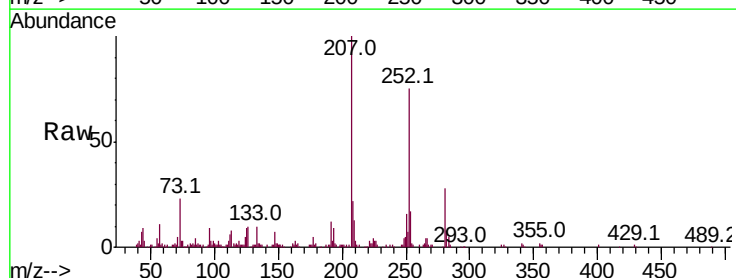


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

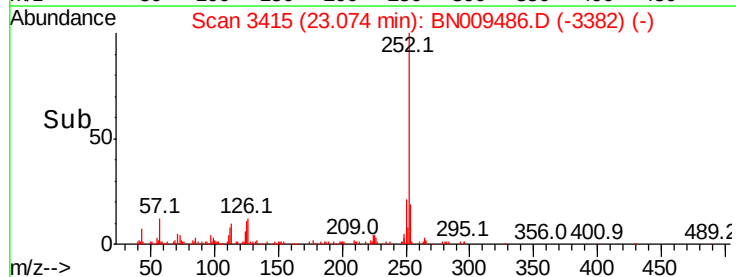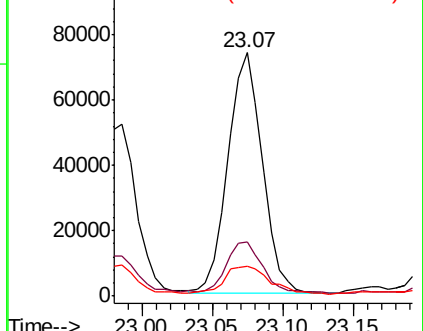




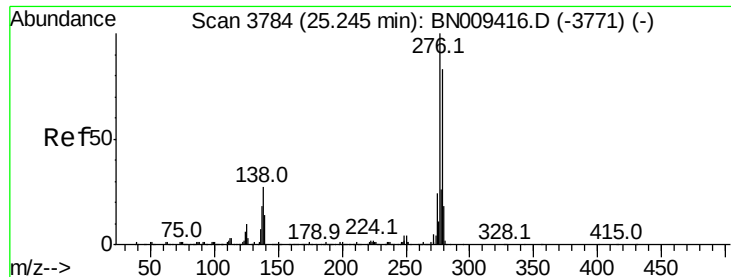


#91

Indeno(1,2,3-cd)pyrene
Concen: 1.122 ng/ul
RT: 25.23 min Scan# 3781
Delta R.T. -0.02 min
Lab File: BN009486.D
Acq: 30 Jan 2020 22:05

Instrument :
BNA_N
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
276	100		
138	24.0	21.4	32.0
277	21.2	20.4	30.6

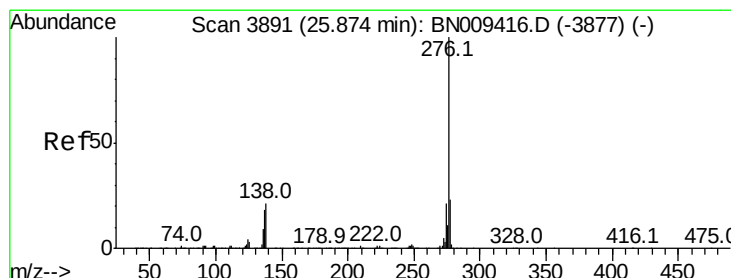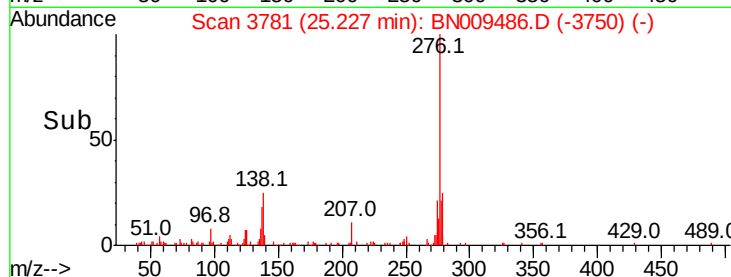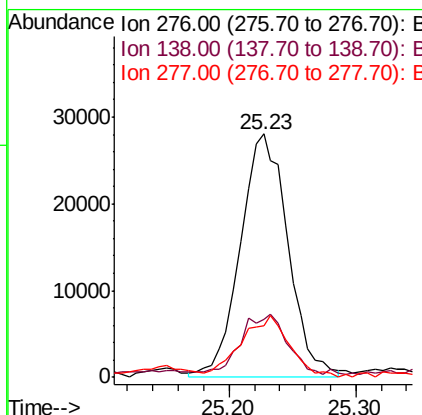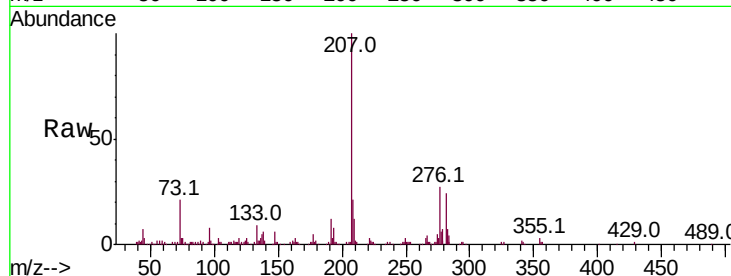

#93

Benzo(g,h,i)perylene
Concen: 1.335 ng/ul
RT: 25.85 min Scan# 3887
Delta R.T. -0.02 min
Lab File: BN009486.D
Acq: 30 Jan 2020 22:05

Tgt Ion	Ratio	Lower	Upper
276	100		
138	24.6	16.6	24.8
277	22.6	18.7	28.1

