

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN013020\
 Data File : BN009502.D
 Acq On : 31 Jan 2020 09:42
 Operator : CG/JU
 Sample : PB126501BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jan 31 22:17:55 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 22 15:13:20 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.45	152	183712	20.00	ng/ul	-0.02
18) Naphthalene-d8	10.20	136	823482	20.00	ng/ul	-0.02
35) Acenaphthene-d10	14.09	164	533779	20.00	ng/ul	-0.01
61) Phenanthrene-d10	16.84	188	1108019	20.00	ng/ul	-0.01
77) Chrysene-d12	21.05	240	959442	20.00	ng/ul	0.00
85) Perylene-d12	23.17	264	1014531	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.08	96	28482	6.41	ng/uL	0.00
5) Phenol-d5	6.64	99	518082	31.79	ng/ul	-0.02
7) Bis-(2-Chloroethyl)ether-d	6.80	67	373360	32.28	ng/ul	-0.02
9) 2-Chlorophenol-d4	6.99	132	412400	34.67	ng/ul	-0.02
13) 4-Methylphenol-d8	8.15	113	419073	32.32	ng/ul	-0.02
19) Nitrobenzene-d5	8.59	128	204562	34.15	ng/ul	-0.02
22) 2-Nitrophenol-d4	9.30	143	234375	37.31	ng/ul	-0.02
26) 2,4-Dichlorophenol-d3	9.83	165	394699	31.70	ng/ul	-0.02
29) 4-Chloroaniline-d4	10.34	131	574916	38.22	ng/ul	-0.02
43) Dimethylphthalate-d6	13.51	166	1333202	33.75	ng/ul	-0.01
46) Acenaphthylene-d8	13.77	160	1543026	32.91	ng/ul	-0.02
51) 4-Nitrophenol-d4	14.32	143	204319	27.79	ng/ul	0.00
57) Fluorene-d10	15.09	176	1127409	32.52	ng/ul	-0.01
62) 4,6-Dinitro-2-methylphenol	15.23	200	180729	26.94	ng/ul	0.00
70) Anthracene-d10	16.94	188	1613915	31.48	ng/ul	0.00
78) Pyrene-d10	19.25	212	1812229	35.11	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.04	264	1782002	34.80	ng/ul	0.00

Target Compounds


				Ovalue	
15) N-Nitroso-di-n-propylamine	8.15	70	12039	1.058	ng/ul# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN013020\
Data File : BN009502.D
Acq On : 31 Jan 2020 09:42
Operator : CG/JU
Sample : PB126501BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jan 31 22:17:55 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 22 15:13:20 2020
Response via : Initial Calibration

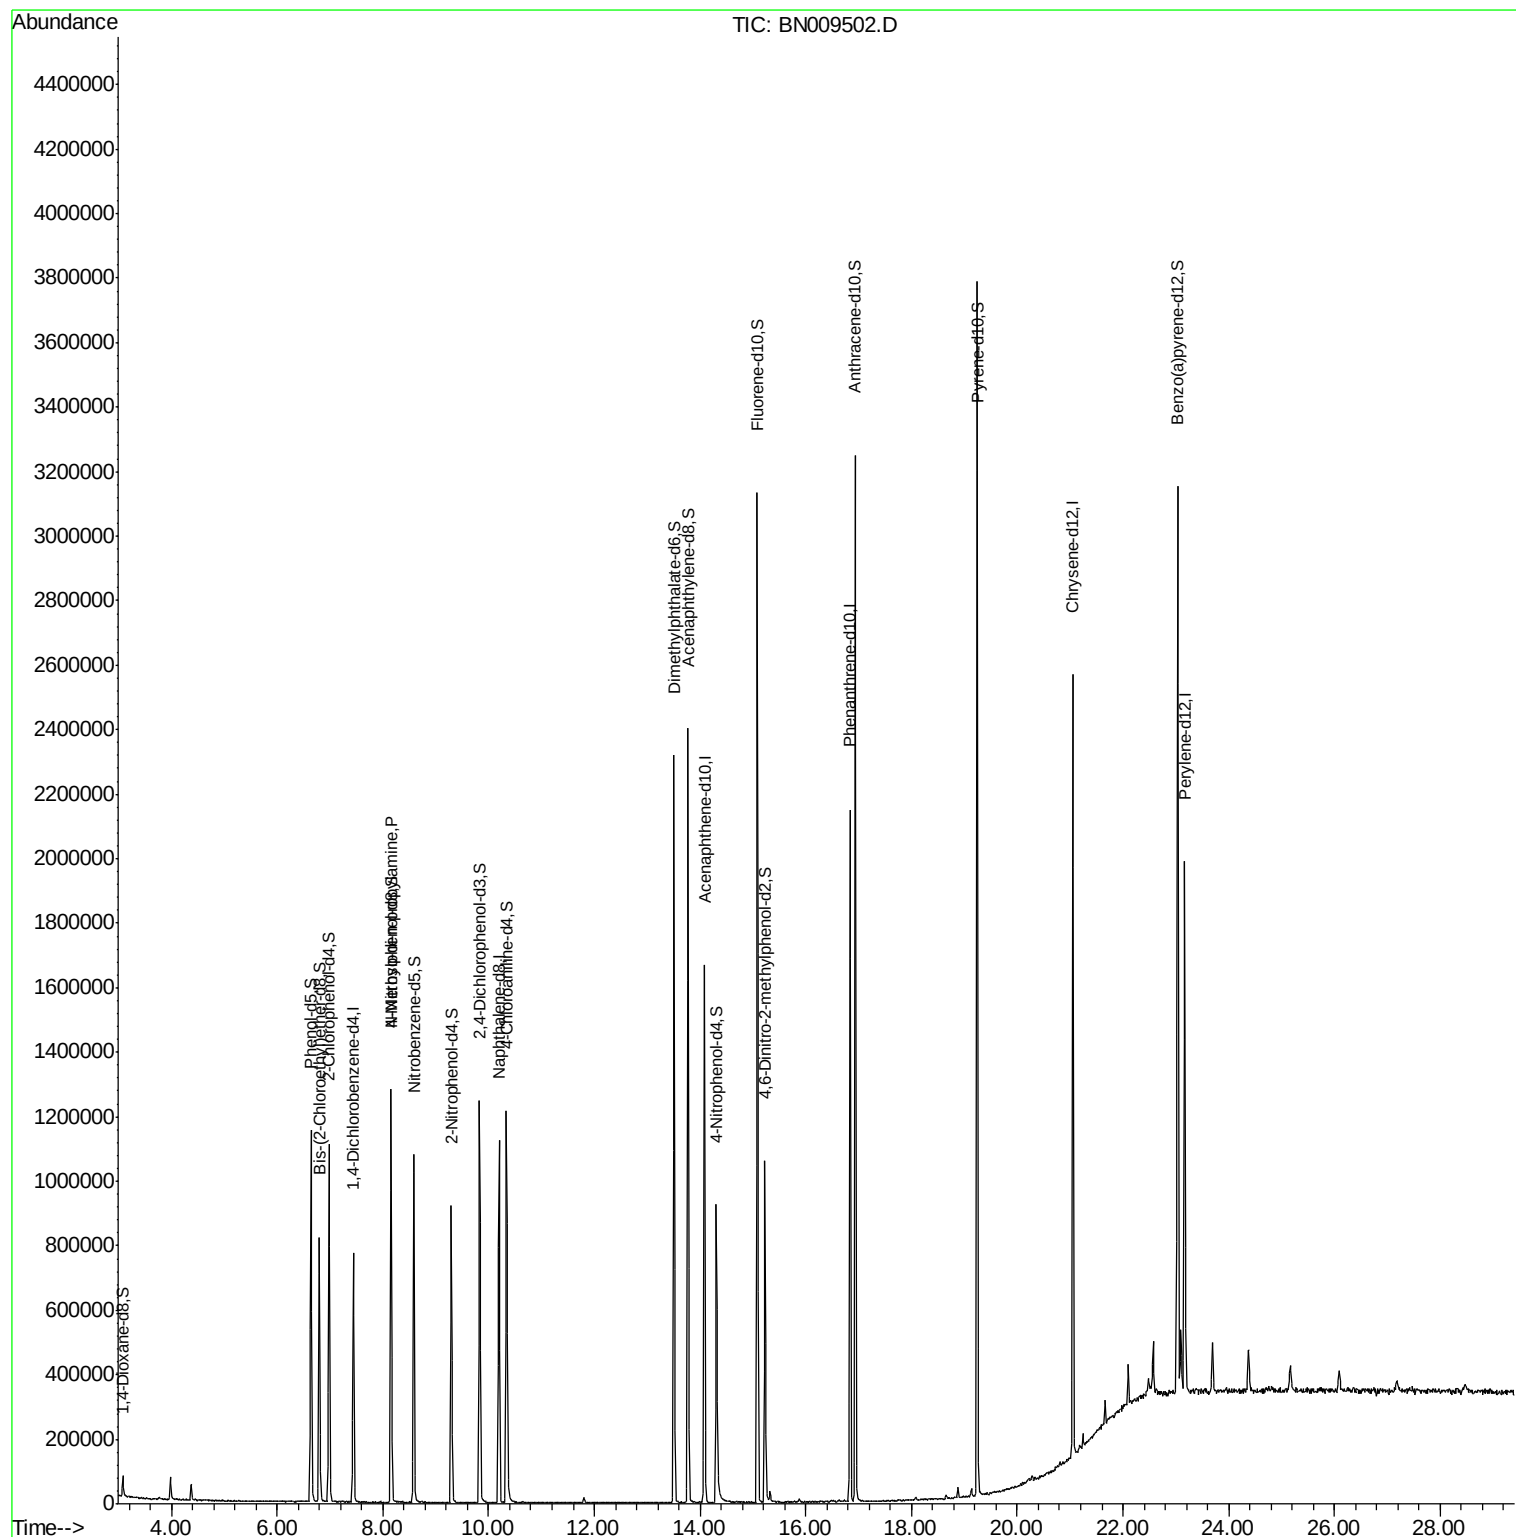

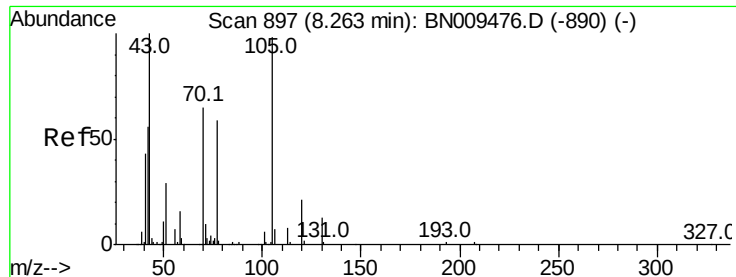

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.058 ng/ul
 RT: 8.15 min Scan# 878
 Delta R.T. -0.11 min
 Lab File: BN009502.D
 Acq: 31 Jan 2020 09:42

Instrument :
 BNA_N
 ClientSampleId :

Tot Ion: 70 Resp: 12039
 Ion Ratio Lower Upper
 70 100
 42 561.1 73.6 110.4#
 101 0.0 7.5 11.3#
 130 0.0 14.2 21.4#

