

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013024\
 Data File : BN029410.D
 Acq On : 30 Jan 2024 10:10
 Operator : MA/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Quant Time: Jan 30 10:48:31 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN012924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 30 03:38:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.898	152	4598	0.400	ng	0.00
7) Naphthalene-d8	10.701	136	12398	0.400	ng	0.00
13) Acenaphthene-d10	14.533	164	5703	0.400	ng	-0.01
19) Phenanthrene-d10	17.293	188	11161	0.400	ng	# 0.00
29) Chrysene-d12	21.492	240	7690	0.400	ng	# 0.00
35) Perylene-d12	23.876	264	7639	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.464	112	4193	0.380	ng	0.00
5) Phenol-d6	7.060	99	4721	0.370	ng	0.00
8) Nitrobenzene-d5	9.057	82	3929	0.381	ng	-0.01
11) 2-Methylnaphthalene-d10	12.291	152	6546	0.388	ng	0.00
14) 2,4,6-Tribromophenol	16.027	330	638	0.349	ng	-0.01
15) 2-Fluorobiphenyl	13.164	172	9624	0.393	ng	-0.01
27) Fluoranthene-d10	19.327	212	9959	0.368	ng	0.00
31) Terphenyl-d14	19.935	244	7576	0.397	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.369	88	2323	0.359	ng	92
3) n-Nitrosodimethylamine	3.709	42	1956	0.371	ng	# 98
6) bis(2-Chloroethyl)ether	7.335	93	4737	0.390	ng	99
9) Naphthalene	10.744	128	13825	0.391	ng	99
10) Hexachlorobutadiene	11.021	225	2627	0.392	ng	# 99
12) 2-Methylnaphthalene	12.363	142	8068	0.389	ng	99
16) Acenaphthylene	14.255	152	10105	0.373	ng	99
17) Acenaphthene	14.597	154	7019	0.386	ng	100
18) Fluorene	15.580	166	8726	0.383	ng	100
20) 4,6-Dinitro-2-methylph...	15.667	198	572	0.349	ng	83
21) 4-Bromophenyl-phenylether	16.486	248	2566	0.386	ng	# 87
22) Hexachlorobenzene	16.585	284	3325	0.408	ng	98
23) Atrazine	16.759	200	1778	0.376	ng	94
24) Pentachlorophenol	16.933	266	875	0.339	ng	96
25) Phenanthrene	17.330	178	12683	0.384	ng	99
26) Anthracene	17.417	178	10465	0.372	ng	99
28) Fluoranthene	19.355	202	13345	0.360	ng	99
30) Pyrene	19.722	202	13975	0.395	ng	100
32) Benzo(a)anthracene	21.474	228	9661	0.368	ng	98
33) Chrysene	21.528	228	11900	0.399	ng	99
34) Bis(2-ethylhexyl)phtha...	21.429	149	6058	0.338	ng	99
36) Indeno(1,2,3-cd)pyrene	26.344	276	11169	0.364	ng	# 91
37) Benzo(b)fluoranthene	23.154	252	10346	0.379	ng	99
38) Benzo(k)fluoranthene	23.201	252	10622	0.371	ng	100
39) Benzo(a)pyrene	23.771	252	8985	0.377	ng	98
40) Dibenzo(a,h)anthracene	26.373	278	8993	0.368	ng	95
41) Benzo(g,h,i)perylene	27.095	276	10988	0.369	ng	97




(#) = qualifier out of range (m) = manual integration (+) = signals summed



#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.898 min Scan# 6
 Delta R.T. -0.007 min
 Lab File: BN029410.D
 Acq: 30 Jan 2024 10:10




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Tgt Ion:152 Resp: 4598
 Ion Ratio Lower Upper
 152 100
 150 156.8 123.0 184.4
 115 66.1 51.4 77.0



#2
 1,4-Dioxane
 Concen: 0.359 ng
 RT: 3.369 min Scan# 40
 Delta R.T. -0.007 min
 Lab File: BN029410.D
 Acq: 30 Jan 2024 10:10

Tgt Ion: 88 Resp: 2323
 Ion Ratio Lower Upper
 88 100
 43 31.6 23.3 34.9
 58 74.2 53.8 80.6









#3
n-Nitrosodimethylamine
Concen: 0.371 ng
RT: 3.709 min Scan# 81
Delta R.T. 0.000 min
Lab File: BN029410.D
Acq: 30 Jan 2024 10:10




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion: 42 Resp: 1956
Ion Ratio Lower Upper
42 100
74 116.7 93.7 140.5
44 11.3 13.0 19.4#



#4
2-Fluorophenol
Concen: 0.380 ng
RT: 5.464 min Scan# 330
Delta R.T. -0.007 min
Lab File: BN029410.D
Acq: 30 Jan 2024 10:10

Tgt Ion: 112 Resp: 4193
Ion Ratio Lower Upper
112 100
64 57.7 47.2 70.8
63 30.5 25.8 38.6








#5
Phenol-d6
Concen: 0.370 ng
RT: 7.060 min Scan# 51
Delta R.T. -0.007 min
Lab File: BN029410.D
Acq: 30 Jan 2024 10:10

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion: 99 Resp: 4721




Ion	Ratio	Lower	Upper
99	100		
42	21.1	16.9	25.3
71	36.6	30.0	45.0



#6
bis(2-Chloroethyl)ether
Concen: 0.390 ng
RT: 7.335 min Scan# 589
Delta R.T. -0.007 min
Lab File: BN029410.D
Acq: 30 Jan 2024 10:10

Tgt Ion: 93 Resp: 4737

Ion	Ratio	Lower	Upper
93	100		
63	77.9	63.1	94.7
95	33.9	27.1	40.7








#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.701 min Scan# 948
Delta R.T. 0.000 min
Lab File: BN029410.D
Acq: 30 Jan 2024 10:10




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	136	Resp:	12398
Ion	Ratio	Lower	Upper
136	100		
137	11.5	9.7	14.5
54	6.9	6.6	10.0
68	6.1	5.7	8.5



#8
Nitrobenzene-d5
Concen: 0.381 ng
RT: 9.057 min Scan# 794
Delta R.T. -0.011 min
Lab File: BN029410.D
Acq: 30 Jan 2024 10:10

Tgt Ion:	82	Resp:	3929
Ion	Ratio	Lower	Upper
82	100		
128	34.8	31.6	47.4
54	53.7	38.2	57.4





#9

Naphthalene

Concen: 0.391 ng

RT: 10.744 min Scan# 91

Delta R.T. -0.011 min

Lab File: BN029410.D

Acq: 30 Jan 2024 10:10

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4





Tgt Ion:128 Resp: 13825

Ion Ratio Lower Upper

128 100

129 11.4 9.5 14.3

127 13.7 10.8 16.2



#10

Hexachlorobutadiene

Concen: 0.392 ng

RT: 11.021 min Scan# 978

Delta R.T. -0.011 min

Lab File: BN029410.D

Acq: 30 Jan 2024 10:10




Tgt Ion:225 Resp: 2627


Ion Ratio Lower Upper

225 100

223 0.0 0.0 0.0

227 64.4 51.1 76.7







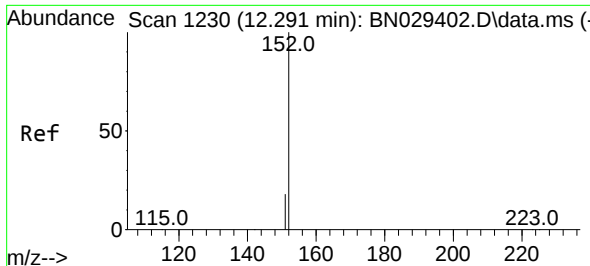

#11
2-Methylnaphthalene-d10
Concen: 0.388 ng
RT: 12.291 min Scan# 11
Delta R.T. 0.000 min
Lab File: BN029410.D
Acq: 30 Jan 2024 10:10




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:152 Resp: 6546
Ion Ratio Lower Upper
152 100
151 20.9 17.1 25.7



#12
2-Methylnaphthalene
Concen: 0.389 ng
RT: 12.363 min Scan# 1249
Delta R.T. -0.004 min
Lab File: BN029410.D
Acq: 30 Jan 2024 10:10

Tgt Ion:142 Resp: 8068
Ion Ratio Lower Upper
142 100
141 89.5 71.9 107.9
115 41.7 33.9 50.9








#13
 Acenaphthene-d10
 Concen: 0.400 ng
 RT: 14.533 min Scan# 1545
 Delta R.T. -0.011 min
 Lab File: BN029410.D
 Acq: 30 Jan 2024 10:10




Instrument :
 BNA_N
 ClientSampleId :
 SSTCCCC0.4


Tgt Ion:164 Resp: 5703
 Ion Ratio Lower Upper
 164 100
 162 106.8 82.6 123.8
 160 53.3 41.5 62.3



#14
 2,4,6-Tribromophenol
 Concen: 0.349 ng
 RT: 16.027 min Scan# 1678
 Delta R.T. -0.012 min
 Lab File: BN029410.D
 Acq: 30 Jan 2024 10:10

Tgt Ion:330 Resp: 638
 Ion Ratio Lower Upper
 330 100
 332 99.5 76.0 114.0
 141 56.4 43.4 65.2









#15
2-Fluorobiphenyl
Concen: 0.393 ng
RT: 13.164 min Scan# 1418
Delta R.T. -0.011 min
Lab File: BN029410.D
Acq: 30 Jan 2024 10:10




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:172 Resp: 9624
Ion Ratio Lower Upper
172 100
171 35.8 28.0 42.0
170 24.6 18.7 28.1



#16
Acenaphthylene
Concen: 0.373 ng
RT: 14.255 min Scan# 1519
Delta R.T. -0.011 min
Lab File: BN029410.D
Acq: 30 Jan 2024 10:10

Tgt Ion:152 Resp: 10105
Ion Ratio Lower Upper
152 100
151 19.3 15.9 23.9
153 13.4 10.5 15.7









#17
Acenaphthene
Concen: 0.386 ng
RT: 14.597 min Scan# 1551
Delta R.T. -0.011 min
Lab File: BN029410.D
Acq: 30 Jan 2024 10:10




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:154 Resp: 7019
Ion Ratio Lower Upper
154 100
153 117.1 93.6 140.4
152 61.0 48.6 73.0



#18
Fluorene
Concen: 0.383 ng
RT: 15.580 min Scan# 1642
Delta R.T. -0.012 min
Lab File: BN029410.D
Acq: 30 Jan 2024 10:10

Tgt Ion:166 Resp: 8726
Ion Ratio Lower Upper
166 100
165 99.8 79.9 119.9
167 13.5 11.3 16.9









#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.293 min Scan# 11
Delta R.T. 0.000 min
Lab File: BN029410.D
Acq: 30 Jan 2024 10:10




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:188 Resp: 11161
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 9.7 10.0 15.0#



#20
4,6-Dinitro-2-methylphenol
Concen: 0.349 ng
RT: 15.667 min Scan# 1649
Delta R.T. 0.000 min
Lab File: BN029410.D
Acq: 30 Jan 2024 10:10

Tgt Ion:198 Resp: 572
Ion Ratio Lower Upper
198 100
51 118.2 111.0 166.6
105 69.4 67.0 100.6









#21
4-Bromophenyl-phenylether
Concen: 0.386 ng
RT: 16.486 min Scan# 1715
Delta R.T. 0.000 min
Lab File: BN029410.D
Acq: 30 Jan 2024 10:10




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:248 Resp: 2566
Ion Ratio Lower Upper
248 100
250 98.0 75.0 112.4
141 74.9 77.0 115.6#



#22
Hexachlorobenzene
Concen: 0.408 ng
RT: 16.585 min Scan# 1723
Delta R.T. 0.000 min
Lab File: BN029410.D
Acq: 30 Jan 2024 10:10

Tgt Ion:284 Resp: 3325
Ion Ratio Lower Upper
284 100
142 48.0 39.4 59.2
249 32.2 26.9 40.3







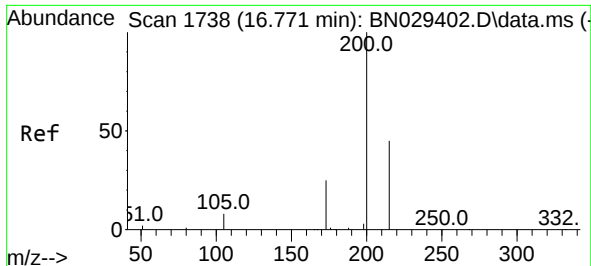

#23
Atrazine
Concen: 0.376 ng
RT: 16.759 min Scan# 1737
Delta R.T. -0.012 min
Lab File: BN029410.D
Acq: 30 Jan 2024 10:10




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:200 Resp: 1778
Ion Ratio Lower Upper
200 100
173 33.7 23.4 35.0
215 45.1 38.4 57.6



#24
Pentachlorophenol
Concen: 0.339 ng
RT: 16.933 min Scan# 1751
Delta R.T. 0.000 min
Lab File: BN029410.D
Acq: 30 Jan 2024 10:10

Tgt Ion:266 Resp: 875
Ion Ratio Lower Upper
266 100
264 60.8 50.8 76.2
268 60.5 51.5 77.3







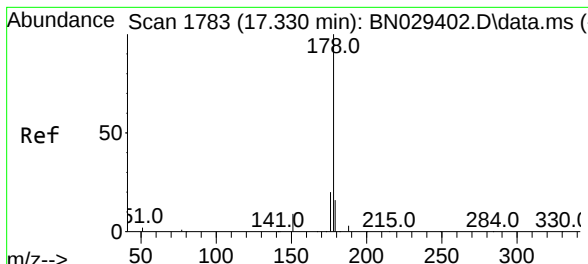

#25
 Phenanthrene
 Concen: 0.384 ng
 RT: 17.330 min Scan# 1783
 Delta R.T. 0.000 min
 Lab File: BN029410.D
 Acq: 30 Jan 2024 10:10




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Tgt Ion:	178	Resp:	12683
Ion Ratio	Lower	Upper	
178	100		
176	19.2	15.8	23.6
179	15.4	12.6	19.0



#26
 Anthracene
 Concen: 0.372 ng
 RT: 17.417 min Scan# 1790
 Delta R.T. -0.012 min
 Lab File: BN029410.D
 Acq: 30 Jan 2024 10:10

Tgt Ion:	178	Resp:	10465
Ion Ratio	Lower	Upper	
178	100		
176	18.8	15.0	22.4
179	15.0	12.3	18.5









#27
Fluoranthene-d10
Concen: 0.368 ng
RT: 19.327 min Scan# 2054
Delta R.T. -0.005 min
Lab File: BN029410.D
Acq: 30 Jan 2024 10:10




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:212 Resp: 9959
Ion Ratio Lower Upper
212 100
106 16.7 13.2 19.8
104 10.2 7.7 11.5

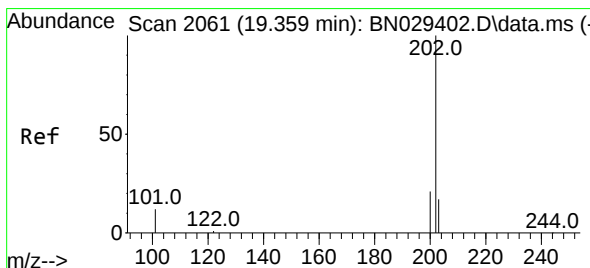

#28
Fluoranthene
Concen: 0.360 ng
RT: 19.355 min Scan# 2060
Delta R.T. -0.005 min
Lab File: BN029410.D
Acq: 30 Jan 2024 10:10

Tgt Ion:202 Resp: 13345
Ion Ratio Lower Upper
202 100
101 13.1 10.5 15.7
203 17.3 13.5 20.3





#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.492 min Scan# 2470

Delta R.T. 0.000 min

Lab File: BN029410.D

Acq: 30 Jan 2024 10:10

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4





Tgt Ion:240 Resp: 7690

Ion Ratio Lower Upper

240 100

120 15.1 16.7 25.1#

236 28.0 23.9 35.9



#30

Pyrene

Concen: 0.395 ng

RT: 19.722 min Scan# 2139

Delta R.T. 0.000 min

Lab File: BN029410.D

Acq: 30 Jan 2024 10:10




Tgt Ion:202 Resp: 13975

Ion Ratio Lower Upper

202 100

200 20.8 16.6 25.0

203 18.0 14.2 21.4









#31
 Terphenyl-d14
 Concen: 0.397 ng
 RT: 19.935 min Scan# 2185
 Delta R.T. 0.000 min
 Lab File: BN029410.D
 Acq: 30 Jan 2024 10:10




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Tgt Ion:244 Resp: 7576
 Ion Ratio Lower Upper
 244 100
 212 9.8 8.2 12.4
 122 17.9 15.6 23.4



#32
 Benzo(a)anthracene
 Concen: 0.368 ng
 RT: 21.474 min Scan# 2468
 Delta R.T. -0.009 min
 Lab File: BN029410.D
 Acq: 30 Jan 2024 10:10

Tgt Ion:228 Resp: 9661
 Ion Ratio Lower Upper
 228 100
 226 28.6 22.2 33.4
 229 19.8 16.5 24.7





#33

Chrysene

Concen: 0.399 ng

RT: 21.528 min Scan# 2474

Delta R.T. 0.000 min

Lab File: BN029410.D

Acq: 30 Jan 2024 10:10

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4





Tgt Ion:228 Resp: 11900

Ion Ratio Lower Upper

228 100

226 30.3 24.9 37.3

229 19.5 15.9 23.9



#34

Bis(2-ethylhexyl)phthalate

Concen: 0.338 ng

RT: 21.429 min Scan# 2463

Delta R.T. 0.000 min

Lab File: BN029410.D

Acq: 30 Jan 2024 10:10




Tgt Ion:149 Resp: 6058

Ion Ratio Lower Upper

149 100

167 24.7 20.1 30.1

279 2.8 2.5 3.7





#35

Perylene-d12

Concen: 0.400 ng

RT: 23.876 min Scan# 3075

Delta R.T. -0.009 min

Lab File: BN029410.D


Acq: 30 Jan 2024 10:10

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4






Tgt Ion:264 Resp: 7639

Ion Ratio Lower Upper

264 100

260 26.6 21.2 31.8

265 47.2 41.5 62.3



#36

Indeno(1,2,3-cd)pyrene

Concen: 0.364 ng

RT: 26.344 min Scan# 3919

Delta R.T. -0.009 min

Lab File: BN029410.D

Acq: 30 Jan 2024 10:10




Tgt Ion:276 Resp: 11169

Ion Ratio Lower Upper

276 100

138 31.4 20.5 30.7#

277 24.1 17.0 25.4





#37

Benzo(b)fluoranthene

Concen: 0.379 ng

RT: 23.154 min Scan# 2828

Delta R.T. -0.003 min

Lab File: BN029410.D

Acq: 30 Jan 2024 10:10

Instrument :

BN029410.D

ClientSampleId :

SSTDCCC0.4





Tgt Ion:252 Resp: 10346

Ion Ratio Lower Upper

252 100

253 26.7 21.7 32.5

125 15.8 13.3 19.9



#38

Benzo(k)fluoranthene

Concen: 0.371 ng

RT: 23.201 min Scan# 2844

Delta R.T. -0.006 min

Lab File: BN029410.D

Acq: 30 Jan 2024 10:10




Tgt Ion:252 Resp: 10622

Ion Ratio Lower Upper

252 100

253 27.4 21.8 32.8

125 17.5 13.9 20.9









#39
Benzo(a)pyrene
Concen: 0.377 ng
RT: 23.771 min Scan# 3041
Delta R.T. -0.006 min
Lab File: BN029410.D
Acq: 30 Jan 2024 10:10




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:252 Resp: 8985
Ion Ratio Lower Upper
252 100
253 30.0 24.9 37.3
125 19.3 16.6 25.0



#40
Dibenzo(a,h)anthracene
Concen: 0.368 ng
RT: 26.373 min Scan# 3929
Delta R.T. -0.006 min
Lab File: BN029410.D
Acq: 30 Jan 2024 10:10


Tgt Ion:278 Resp: 8993
Ion Ratio Lower Upper
278 100
139 22.9 20.4 30.6
279 28.3 25.0 37.6





#41
Benzo(g,h,i)perylene
Concen: 0.369 ng
RT: 27.095 min Scan# 41
Delta R.T. -0.009 min
Lab File: BN029410.D
Acq: 30 Jan 2024 10:10

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4



Tgt Ion:	276	Resp:	10988
Ion Ratio	Lower	Upper	
276	100		
277	25.9	19.4	29.2
138	28.3	23.5	35.3

