
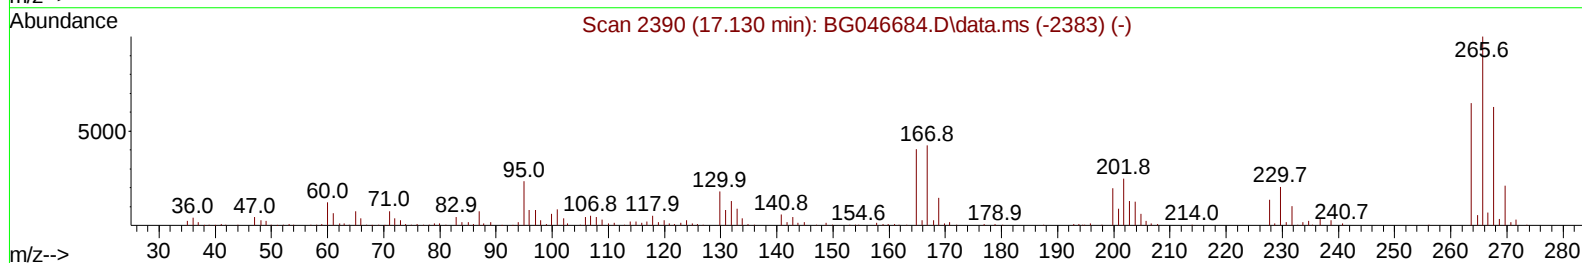
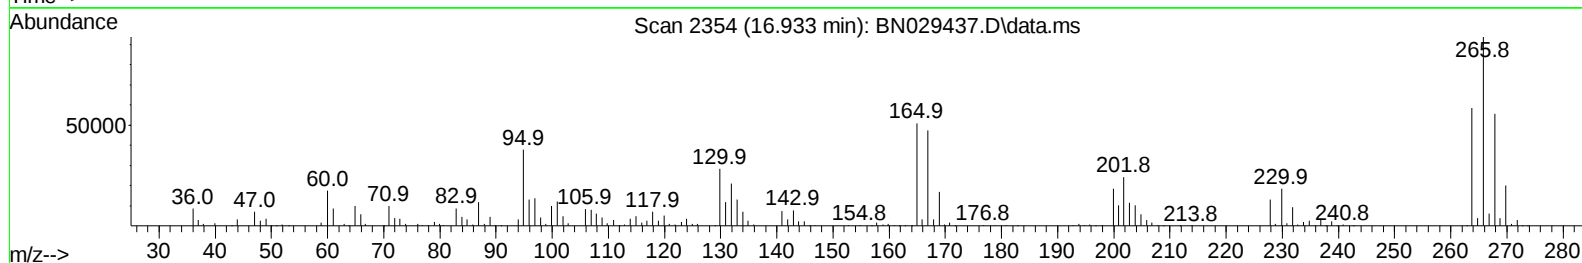


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013024\
Data File : BN029437.D
Acq On : 31 Jan 2024 06:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 31 07:30:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 07:30:14 2024
Response via : Initial Calibration

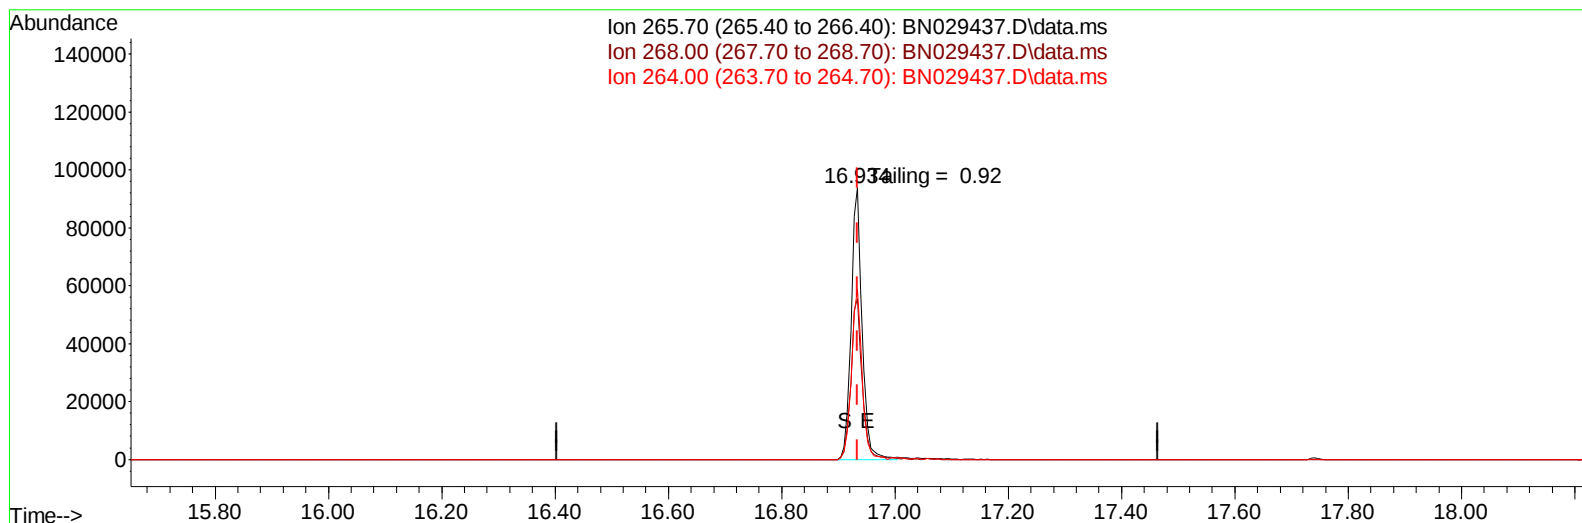

TIC: BN029437.D\data.ms

(70) Pentachlorophenol (C)




16.933min (0.000) 15476.01 ng

response 126067

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.42
264.00	61.60	62.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013024\
Data File : BN029437.D
Acq On : 31 Jan 2024 06:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 31 07:30:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 07:30:14 2024
Response via : Initial Calibration

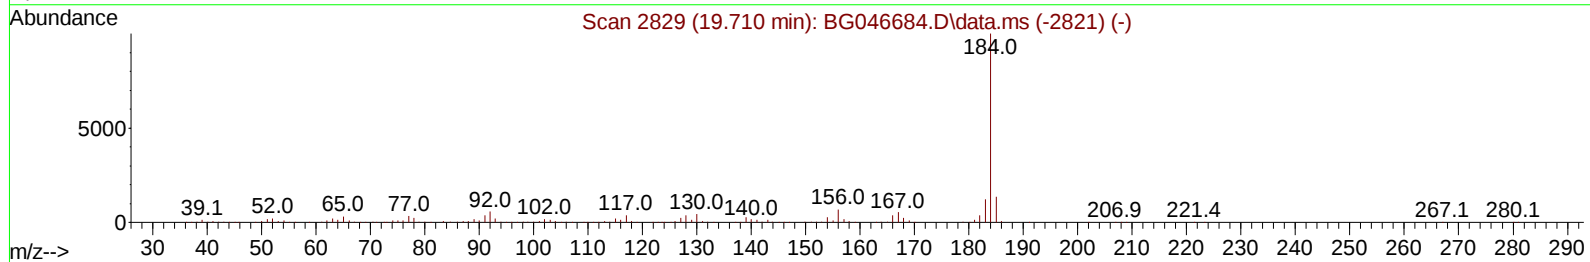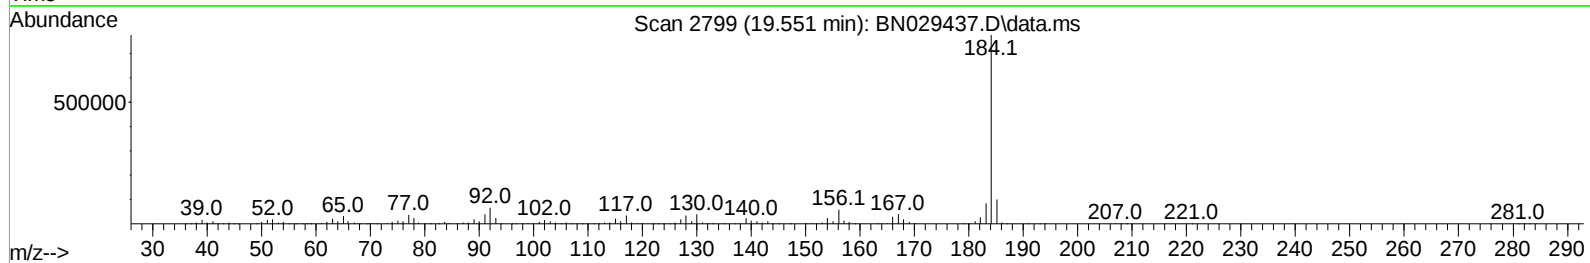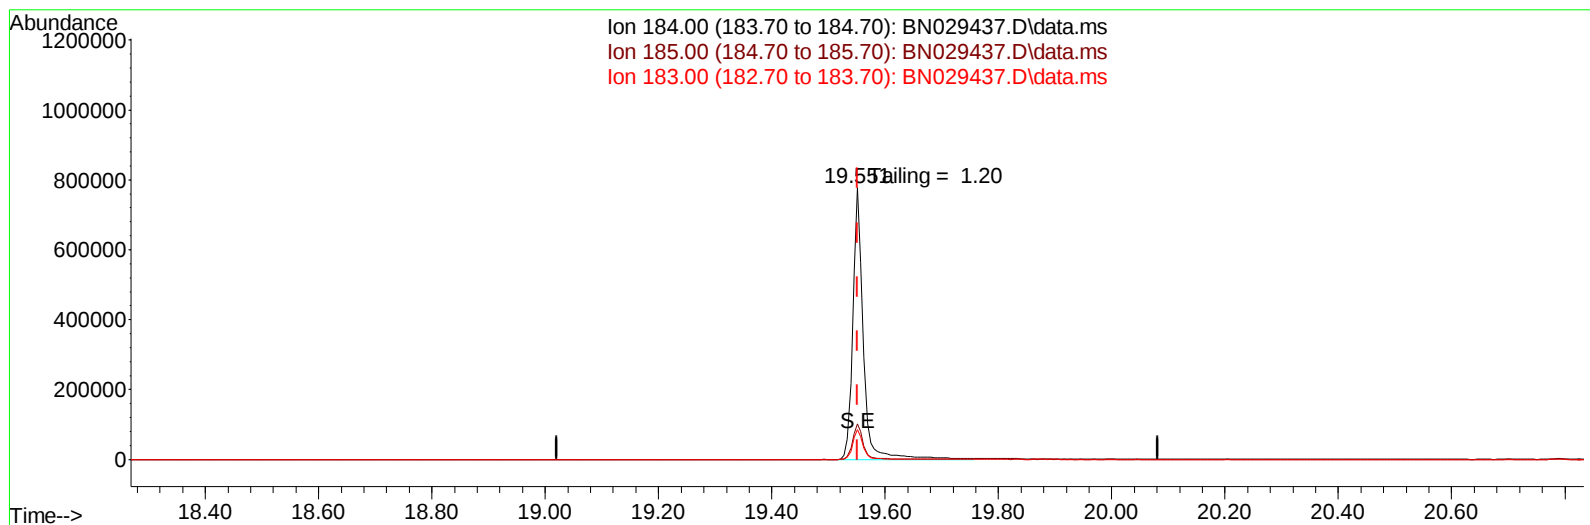

TIC: BN029437.D\data.ms

(77) Benzidine

19.551min (0.000) 0.00 ng

response 1018014

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.01
183.00	13.20	10.97
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/30/2024	BNA_N	<u>BN029437.D</u>
Compound Name	Response	Retention Time
DDT	477573	20.792
DDD	4266	20.398
DDE	0	20.004
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4266	481839	0.89