

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013024\
Data File : BN029418.D
Acq On : 30 Jan 2024 18:56
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 31 06:53:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN012924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 30 03:38:24 2024
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	0.000	152	0	0.000	ng	-7.91
7) Naphthalene-d8	0.000	136	0	0.000	ng	-10.70
13) Acenaphthene-d10	0.000	164	0	0.000	ng	-14.54
19) Phenanthrene-d10	0.000	188	0	0.000	ng	-17.29
29) Chrysene-d12	0.000	240	0	0.000	ng	-21.49
35) Perylene-d12	0.000	264	0	0.000	ng	-23.88
System Monitoring Compounds						
4) 2-Fluorophenol	0.000	112	0	0.000	ng	
5) Phenol-d6	0.000	99	0	0.000	ng	
8) Nitrobenzene-d5	0.000	82	0	0.000	ng	
11) 2-Methylnaphthalene-d10	0.000	152	0	0.000	ng	
14) 2,4,6-Tribromophenol	0.000	330	0	0.000	ng	
15) 2-Fluorobiphenyl	0.000	172	0	0.000	ng	
27) Fluoranthene-d10	0.000	212	0	0.000	ng	
31) Terphenyl-d14	0.000	244	0	0.000	ng	


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013024\
Data File : BN029418.D
Acq On : 30 Jan 2024 18:56
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 31 06:53:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN012924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 30 03:38:24 2024
Response via : Initial Calibration

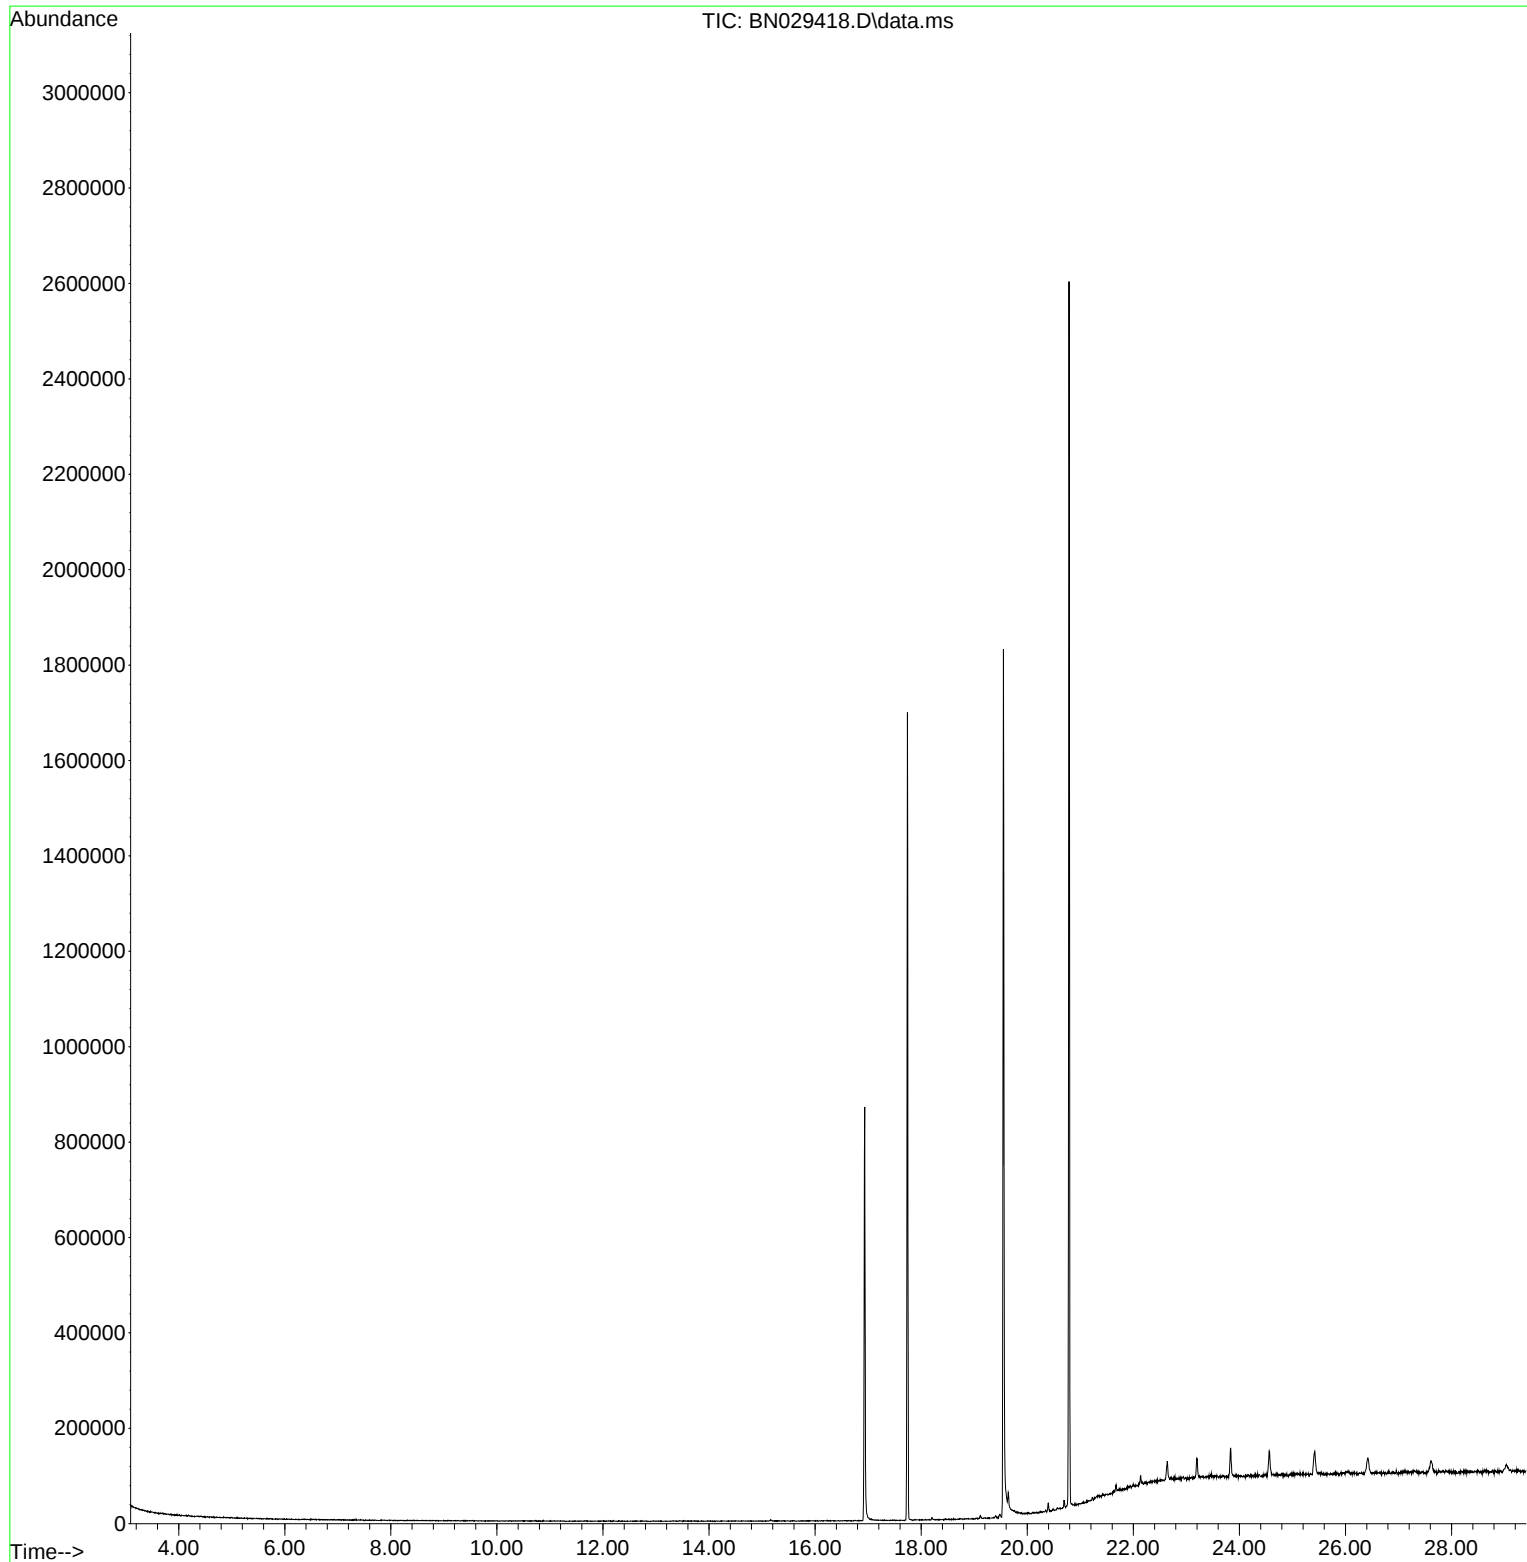


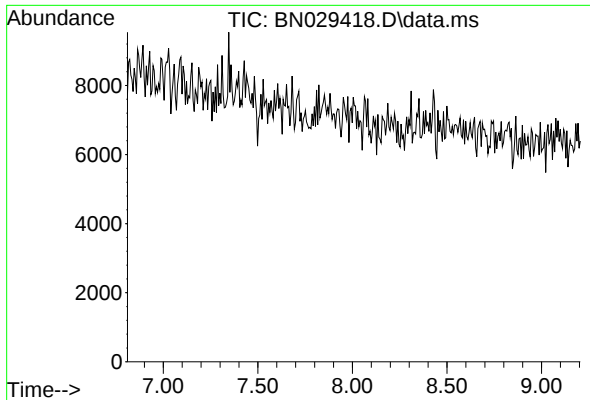


#1
1,4-Dichlorobenzene-d4
Concen: 0.000 ng
Expected RT: 7.91 min

Lab File: BN029418.D
Acq: 30 Jan 2024 18:56

Instrument :
BNA_N
ClientSampleId :
DFTPP


Tgt Ion: 152
Sig Exp Ratio
152 100
150 153.7
115 64.2

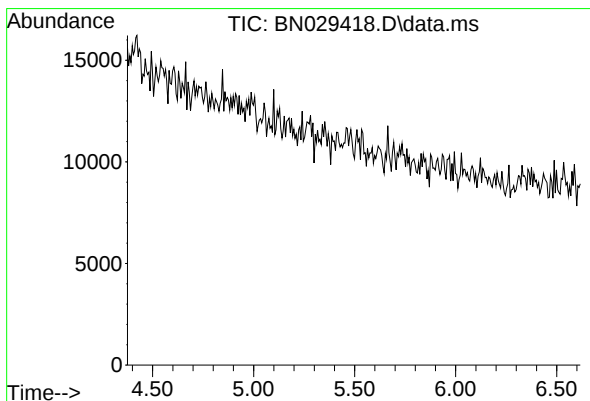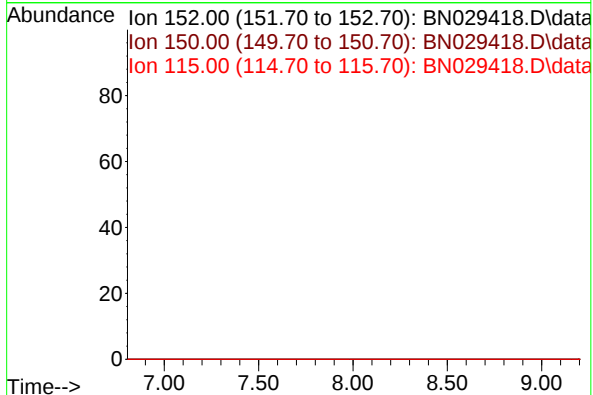


#4
2-Fluorophenol
Concen: 0.000 ng
Expected RT: 5.47 min

Lab File: BN029418.D
Acq: 30 Jan 2024 18:56

Tgt Ion: 112
Sig Exp Ratio
112 100
64 59.0
63 32.2

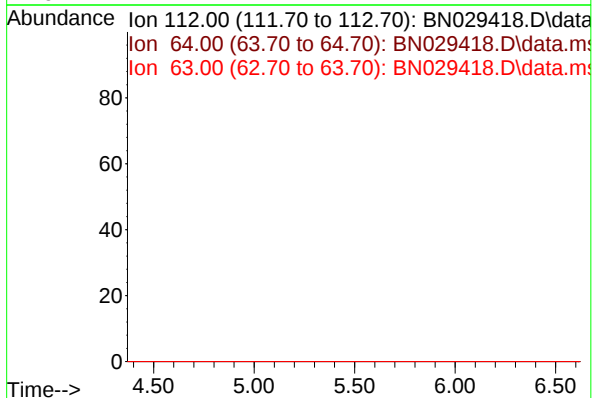


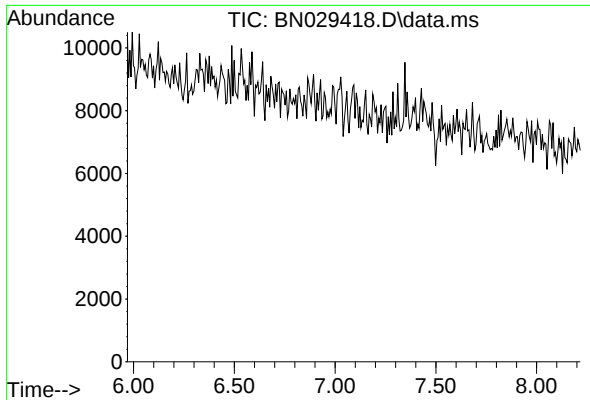


#5
 Phenol-d6
 Concen: 0.000 ng
 Expected RT: 7.07 min
 Lab File: BN029418.D
 Acq: 30 Jan 2024 18:56

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Tgt Ion: 99


Sig	Exp Ratio
99	100
42	21.1
71	37.5

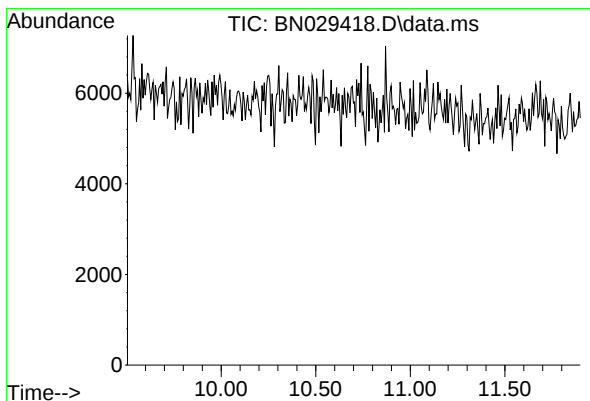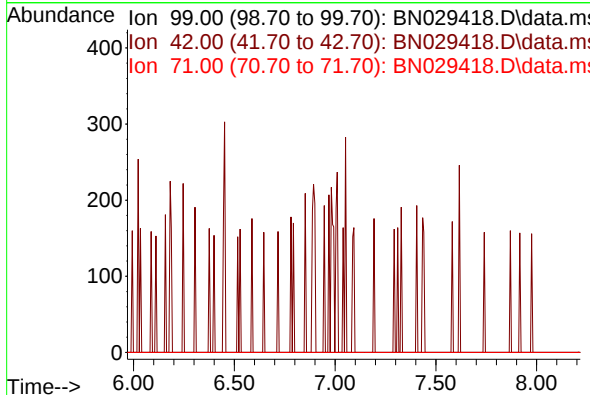


#7
 Naphthalene-d8
 Concen: 0.000 ng
 Expected RT: 10.70 min
 Lab File: BN029418.D
 Acq: 30 Jan 2024 18:56

Tgt Ion: 136

Sig	Exp Ratio
136	100
137	12.1
54	8.3
68	7.1

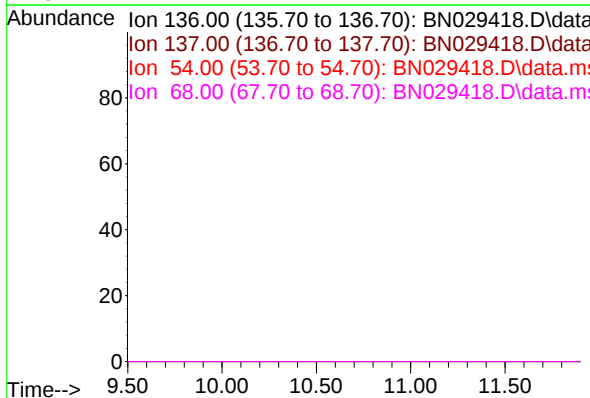


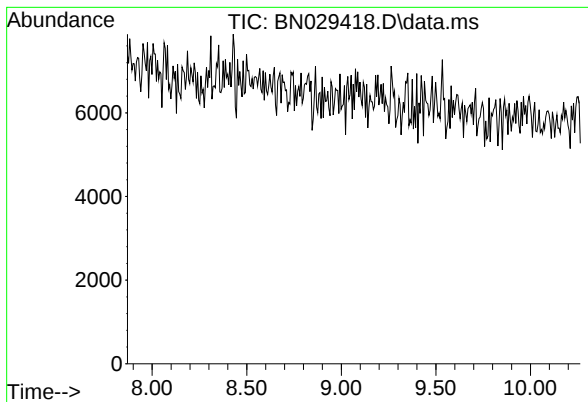


#8
 Nitrobenzene-d5
 Concen: 0.000 ng
 Expected RT: 9.07 min
 Lab File: BN029418.D
 Acq: 30 Jan 2024 18:56

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Tgt Ion: 82


Sig	Exp Ratio
82	100
128	39.5
54	47.8

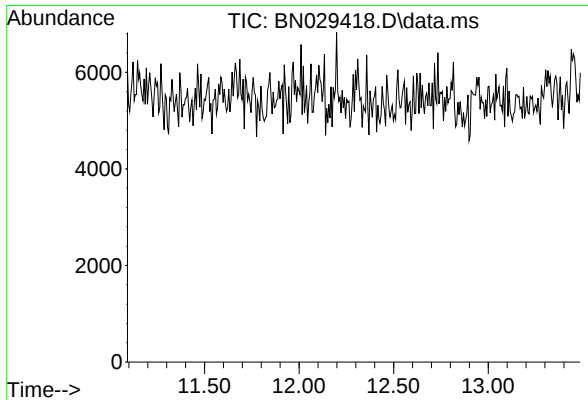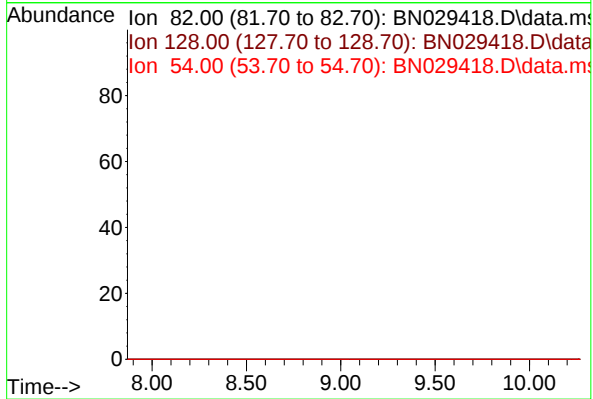


#11
 2-Methylnaphthalene-d10
 Concen: 0.000 ng
 Expected RT: 12.29 min
 Lab File: BN029418.D
 Acq: 30 Jan 2024 18:56

Tgt Ion: 152

Sig	Exp Ratio
152	100
151	21.4

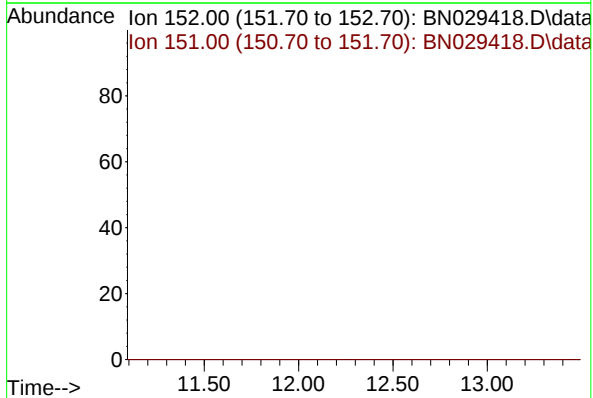


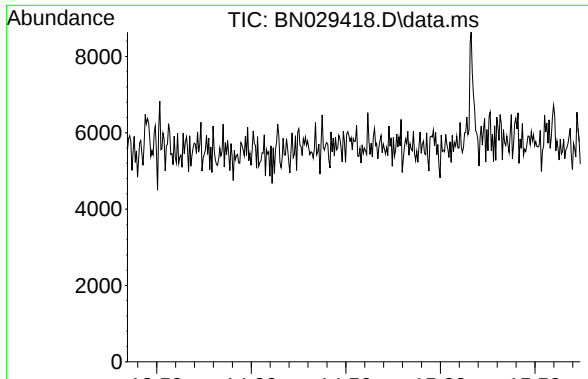


#13
 Acenaphthene-d10
 Concen: 0.000 ng
 Expected RT: 14.54 min
 Lab File: BN029418.D
 Acq: 30 Jan 2024 18:56

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Tgt Ion: 164


Sig	Exp Ratio
164	100
162	103.2
160	51.9

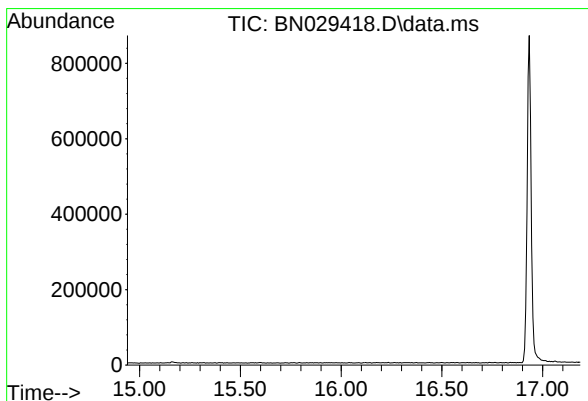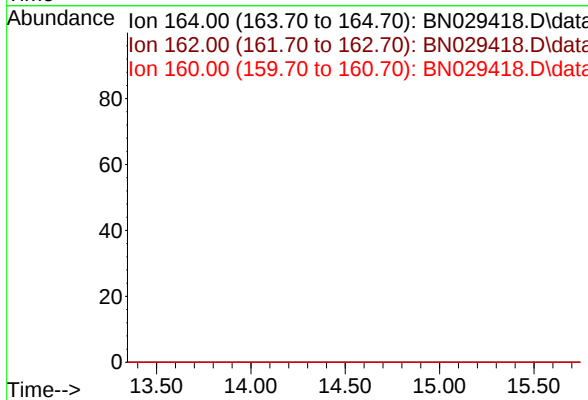


#14
 2,4,6-Tribromophenol
 Concen: 0.000 ng
 Expected RT: 16.04 min
 Lab File: BN029418.D
 Acq: 30 Jan 2024 18:56

Tgt Ion: 330

Sig	Exp Ratio
330	100
332	95.0
141	54.3

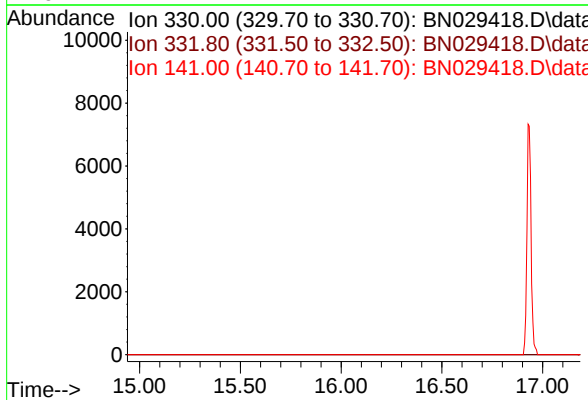


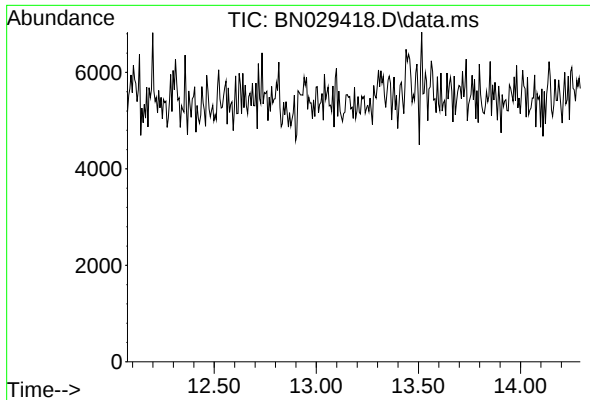


#15
 2-Fluorobiphenyl
 Concen: 0.000 ng
 Expected RT: 13.17 min
 Lab File: BN029418.D
 Acq: 30 Jan 2024 18:56

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Tgt Ion: 172


Sig	Exp Ratio
172	100
171	35.0
170	23.4

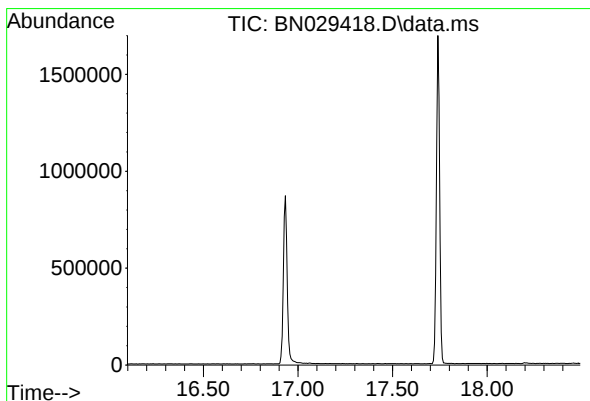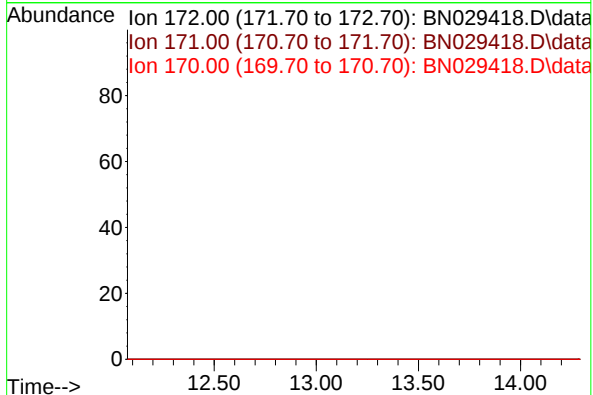


#19
 Phenanthrene-d10
 Concen: 0.000 ng
 Expected RT: 17.29 min
 Lab File: BN029418.D
 Acq: 30 Jan 2024 18:56

Tgt Ion: 188

Sig	Exp Ratio
188	100
94	0.0
80	12.5

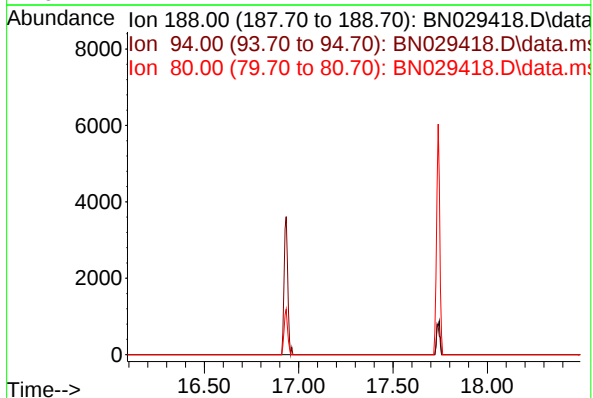


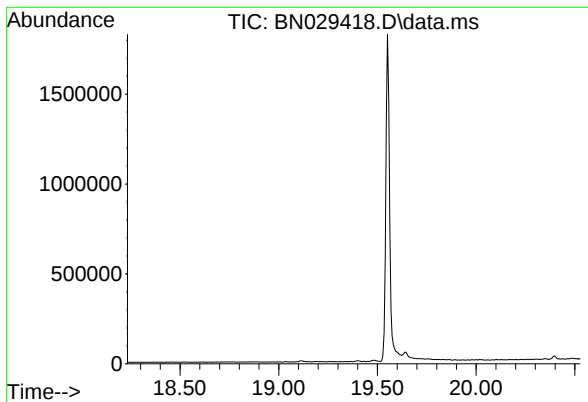


#27
 Fluoranthene-d10
 Concen: 0.000 ng
 Expected RT: 19.33 min
 Lab File: BN029418.D
 Acq: 30 Jan 2024 18:56

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Tgt Ion: 212


Sig	Exp Ratio
212	100
106	16.5
104	9.6

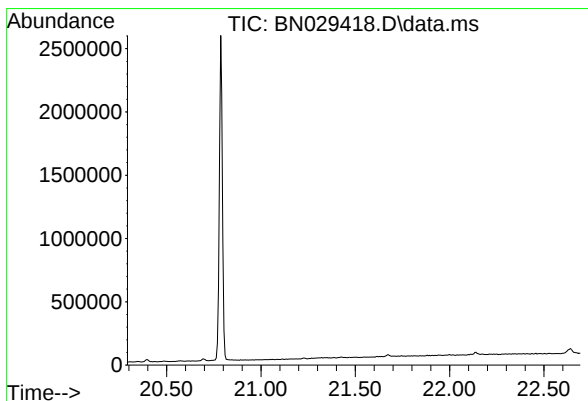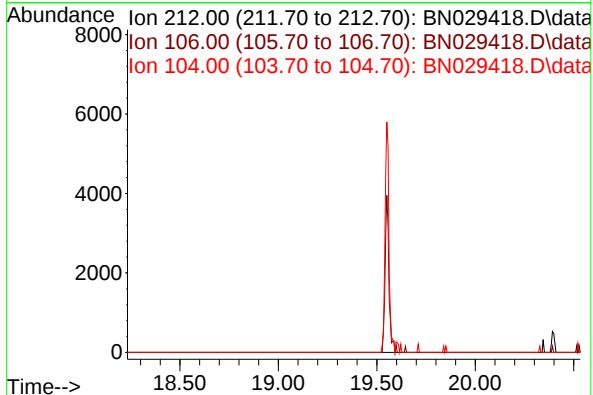


#29
 Chrysene-d12
 Concen: 0.000 ng
 Expected RT: 21.49 min
 Lab File: BN029418.D
 Acq: 30 Jan 2024 18:56

Tgt Ion: 240

Sig	Exp Ratio
240	100
120	20.9
236	29.9

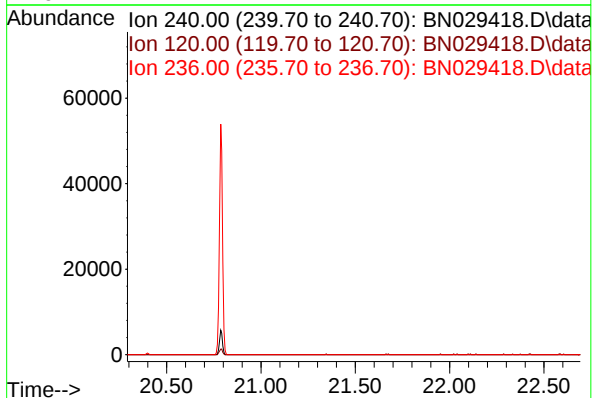


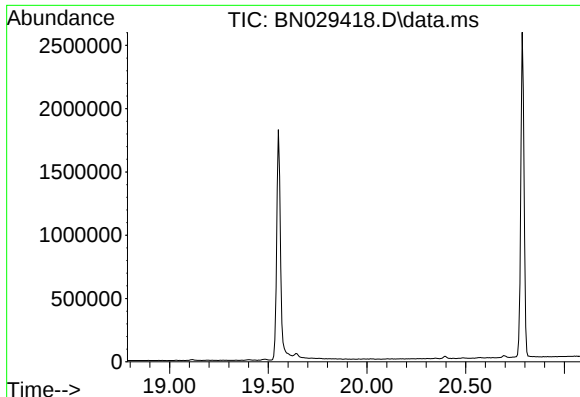


#31
 Terphenyl-d14
 Concen: 0.000 ng
 Expected RT: 19.94 min
 Lab File: BN029418.D
 Acq: 30 Jan 2024 18:56

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Tgt Ion: 244

Sig	Exp Ratio
244	100
212	10.3
122	19.5

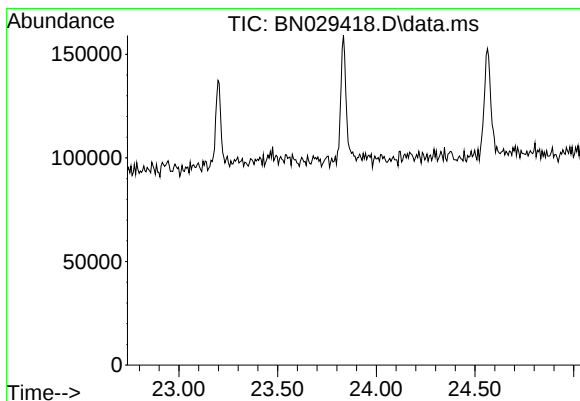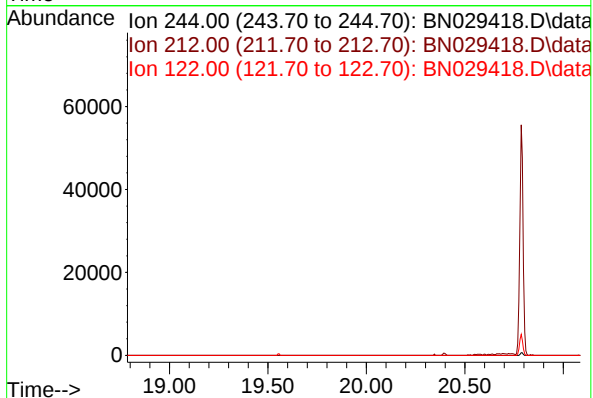

#35
 Perylene-d12
 Concen: 0.000 ng
 Expected RT: 23.88 min
 Lab File: BN029418.D
 Acq: 30 Jan 2024 18:56

Tgt Ion: 264

Sig	Exp Ratio
264	100
260	26.5
265	51.9

