

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013024\
 Data File : BN029432.D
 Acq On : 31 Jan 2024 03:21
 Operator : MA/JU
 Sample : 04699-08
 Misc : LOQ-WATER-0.1NG
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 LOQ-WATER-02-QT4-2023

Quant Time: Jan 31 03:48:29 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN012924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 30 03:38:24 2024
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By :Jagrut Upadhyay 01/31/2024
 Supervised By :Sohil Jodhani 02/02/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.898	152	3680	0.400	ng	0.00
7) Naphthalene-d8	10.701	136	9861	0.400	ng	0.00
13) Acenaphthene-d10	14.532	164	4553	0.400	ng	-0.01
19) Phenanthrene-d10	17.293	188	8996	0.400	ng	0.00
29) Chrysene-d12	21.492	240	6280	0.400	ng	# 0.00
35) Perylene-d12	23.870	264	6674	0.400	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.464	112	3043	0.344	ng	0.00
5) Phenol-d6	7.060	99	3700	0.363	ng	0.00
8) Nitrobenzene-d5	9.067	82	2789	0.340	ng	0.00
11) 2-Methylnaphthalene-d10	12.291	152	7221	0.538	ng	0.00
14) 2,4,6-Tribromophenol	16.027	330	466	0.319	ng	-0.01
15) 2-Fluorobiphenyl	13.164	172	6599	0.338	ng	-0.01
27) Fluoranthene-d10	19.322	212	12374	0.568	ng	0.00
31) Terphenyl-d14	19.931	244	5173	0.332	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.377	88	701	0.135	ng	Qvalue 94
3) n-Nitrosodimethylamine	3.723	42	371	0.088	ng	# 89
6) bis(2-Chloroethyl)ether	7.342	93	867	0.089	ng	97
9) Naphthalene	10.744	128	2716	0.097	ng	# 94
10) Hexachlorobutadiene	11.021	225	500	0.094	ng	# 100
12) 2-Methylnaphthalene	12.363	142	1559	0.094	ng	96
16) Acenaphthylene	14.254	152	2093	0.097	ng	98
17) Acenaphthene	14.597	154	1371	0.094	ng	98
18) Fluorene	15.592	166	1755	0.096	ng	100
20) 4,6-Dinitro-2-methylph...	15.679	198	94	0.071	ng	# 17
21) 4-Bromophenyl-phenylether	16.486	248	491	0.092	ng	94
22) Hexachlorobenzene	16.585	284	629	0.096	ng	99
23) Atrazine	16.771	200	359	0.094	ng	# 81
24) Pentachlorophenol	16.933	266	112	0.054	ng	89
25) Phenanthrene	17.330	178	2569	0.097	ng	100
26) Anthracene	17.429	178	2076	0.092	ng	98
28) Fluoranthene	19.355	202	2578	0.086	ng	98
30) Pyrene	19.717	202	2638	0.091	ng	99
32) Benzo(a)anthracene	21.474	228	1849	0.086	ng	96
33) Chrysene	21.528	228	2163	0.089	ng	98
34) Bis(2-ethylhexyl)phtha...	21.420	149	1622	0.111	ng	99
36) Indeno(1,2,3-cd)pyrene	26.338	276	2052	0.076	ng	# 76
37) Benzo(b)fluoranthene	23.151	252	1885	0.079	ng	# 71
38) Benzo(k)fluoranthene	23.198	252	1938	0.078	ng	# 47
39) Benzo(a)pyrene	23.765	252	1603m	0.077	ng	
40) Dibenzo(a,h)anthracene	26.373	278	1716m	0.080	ng	
41) Benzo(g,h,i)perylene	27.089	276	1948	0.075	ng	# 85

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013024\
 Data File : BN029432.D
 Acq On : 31 Jan 2024 03:21
 Operator : MA/JU
 Sample : 04699-08
 Misc : LOQ-WATER-0.1NG
 ALS Vial : 15 Sample Multiplier: 1


Instrument :
 BNA_N
 ClientSampleId :
 LOQ-WATER-02-QT4-2023

Quant Time: Jan 31 03:48:29 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN012924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 30 03:38:24 2024
 Response via : Initial Calibration

Manual Integrations APPROVED


Reviewed By :Jagrut Upadhyay 01/31/2024
 Supervised By :Sohil Jodhani 02/02/2024

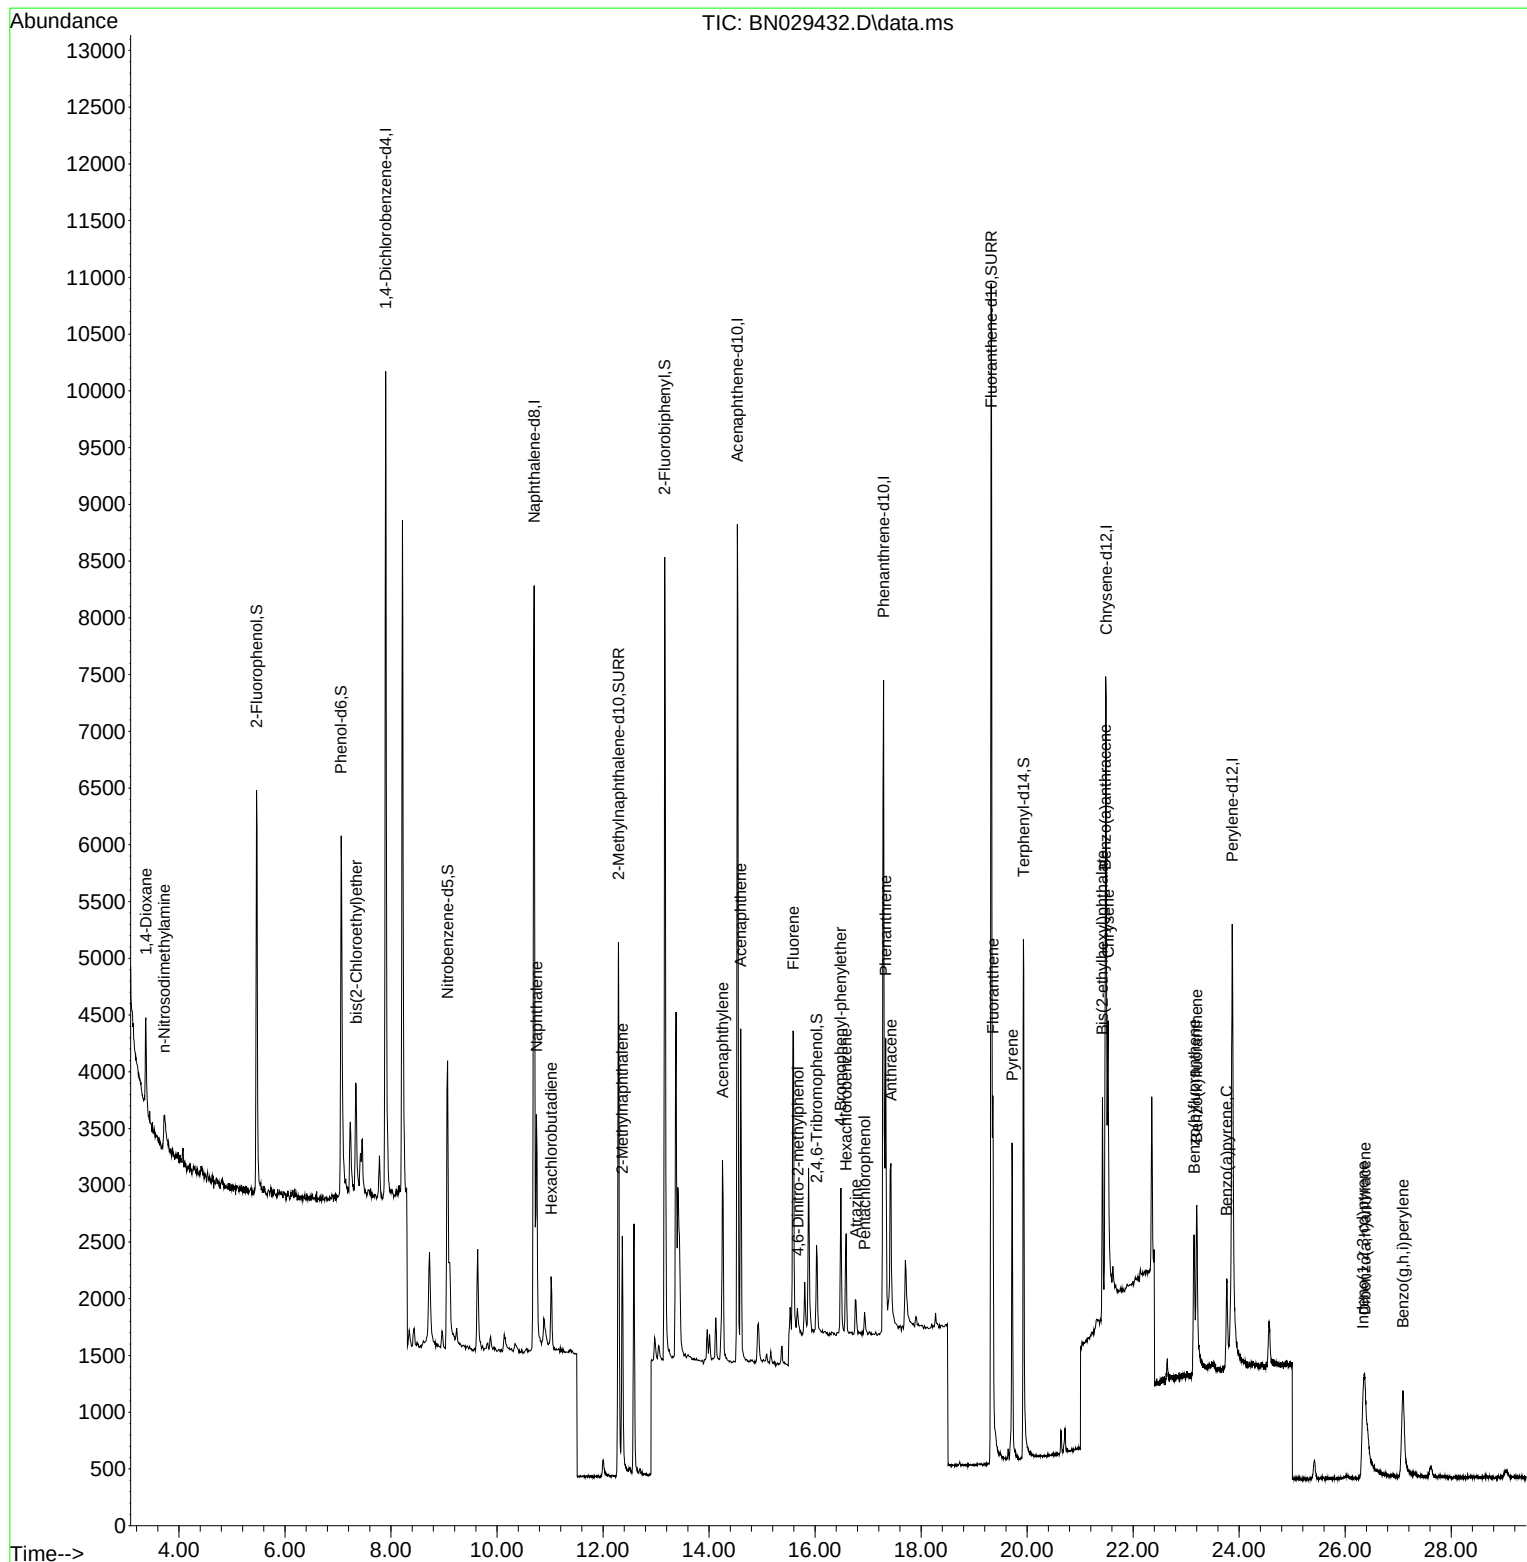



#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.898 min Scan# 668
Delta R.T. -0.007 min
Lab File: BN029432.D
Acq: 31 Jan 2024 03:21




Instrument : BNA_N
ClientSampleId : LOQ-WATER-02-QT4-2023



Tgt Ion: 152 Resp: 3680
Ion Ratio Lower Upper
152 100
150 157.2 123.0 184.4
115 67.3 51.4 77.0




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 01/31/2024
Supervised By :Sohil Jodhani 02/02/2024

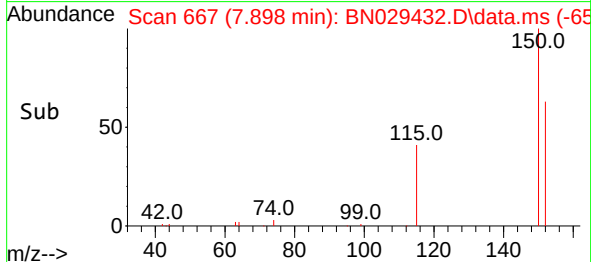

#2
1,4-Dioxane
Concen: 0.135 ng
RT: 3.377 min Scan# 41
Delta R.T. -0.000 min
Lab File: BN029432.D
Acq: 31 Jan 2024 03:21


Tgt Ion: 88 Resp: 701
Ion Ratio Lower Upper
88 100
43 26.1 23.3 34.9
58 61.9 53.8 80.6

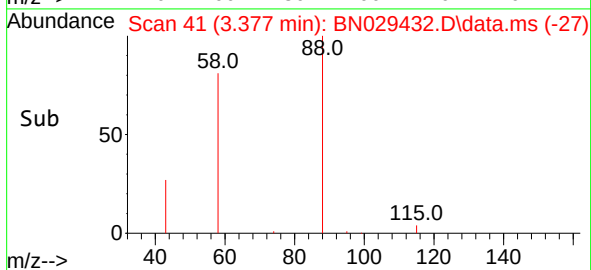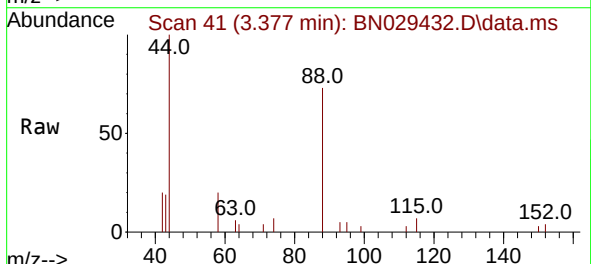

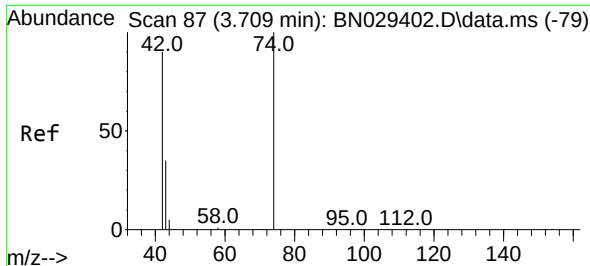

#3
n-Nitrosodimethylamine
Concen: 0.088 ng
RT: 3.723 min Scan# 89
Delta R.T. 0.014 min
Lab File: BN029432.D
Acq: 31 Jan 2024 03:21




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT4-2023



Tgt Ion: 42 Resp: 37
Ion Ratio Lower Upper
42 100
74 109.7 93.7 140.5
44 0.0 13.0 19.4




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 01/31/2024
Supervised By :Sohil Jodhani 02/02/2024

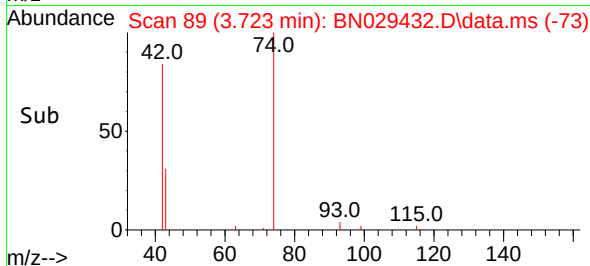

#4
2-Fluorophenol
Concen: 0.344 ng
RT: 5.464 min Scan# 330
Delta R.T. -0.007 min
Lab File: BN029432.D
Acq: 31 Jan 2024 03:21


Tgt Ion:112 Resp: 3043
Ion Ratio Lower Upper
112 100
64 59.3 47.2 70.8
63 32.0 25.8 38.6

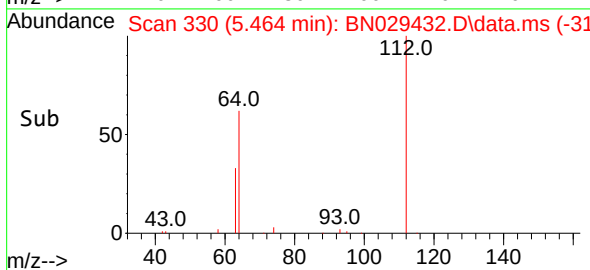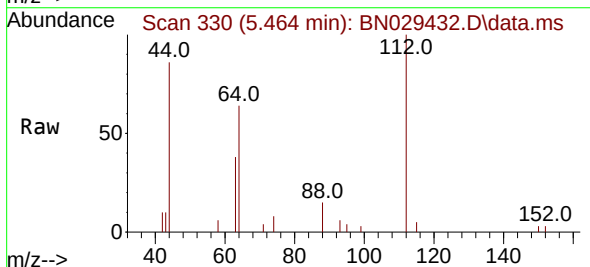



#5
Phenol-d6
Concen: 0.363 ng
RT: 7.060 min Scan# 51
Delta R.T. -0.007 min
Lab File: BN029432.D
Acq: 31 Jan 2024 03:21




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT4-2023



Tgt Ion: 99 Resp: 3700
Ion Ratio Lower Upper
99 100
42 20.7 16.9 25.3
71 38.0 30.0 45.0




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 01/31/2024
Supervised By :Sohil Jodhani 02/02/2024

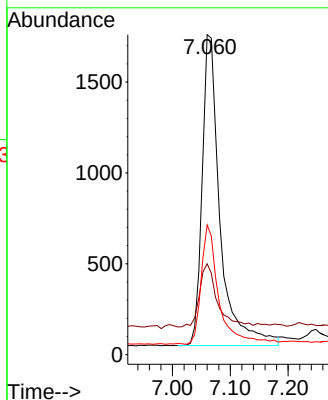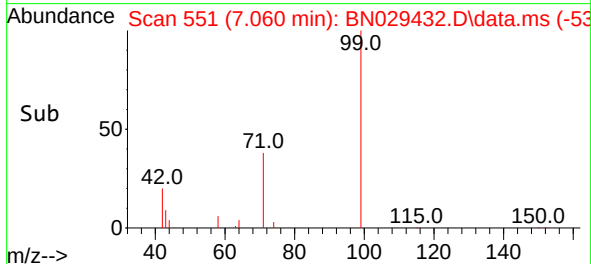

#6
bis(2-Chloroethyl)ether
Concen: 0.089 ng
RT: 7.342 min Scan# 590
Delta R.T. -0.000 min
Lab File: BN029432.D
Acq: 31 Jan 2024 03:21


Tgt Ion: 93 Resp: 867
Ion Ratio Lower Upper
93 100
63 81.1 63.1 94.7
95 35.5 27.1 40.7

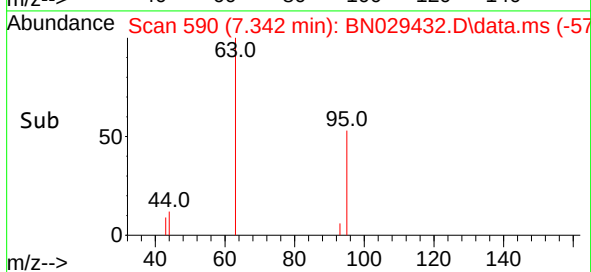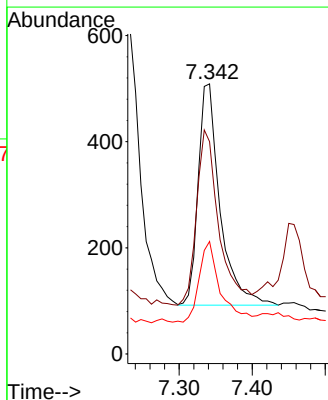



#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.701 min Scan# 948
Delta R.T. -0.000 min
Lab File: BN029432.D
Acq: 31 Jan 2024 03:21




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT4-2023



Tgt Ion:	136	Resp:	986
Ion Ratio	Lower	Upper	
136	100		
137	11.8	9.7	14.5
54	7.6	6.6	10.0
68	6.3	5.7	8.5




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 01/31/2024
Supervised By :Sohil Jodhani 02/02/2024

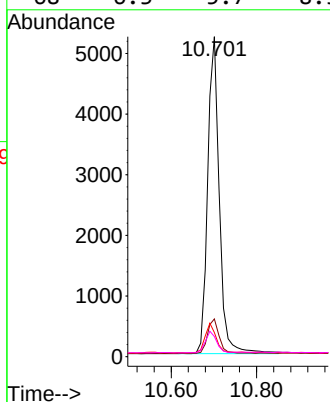

#8
Nitrobenzene-d5
Concen: 0.340 ng
RT: 9.067 min Scan# 795
Delta R.T. -0.000 min
Lab File: BN029432.D
Acq: 31 Jan 2024 03:21

Tgt Ion:	82	Resp:	2789
Ion Ratio	Lower	Upper	
82	100		
128	40.9	31.6	47.4
54	49.1	38.2	57.4

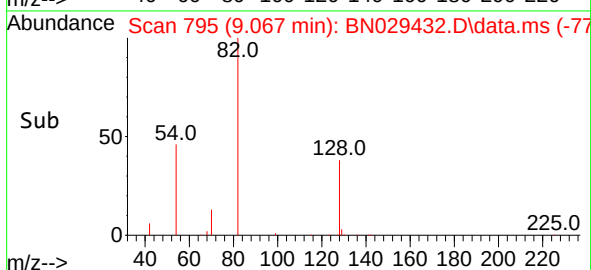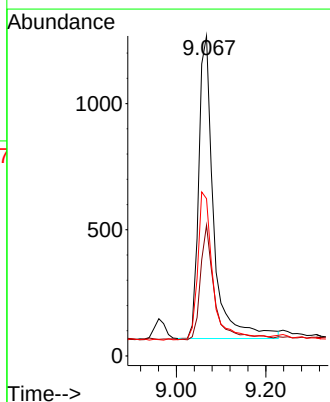

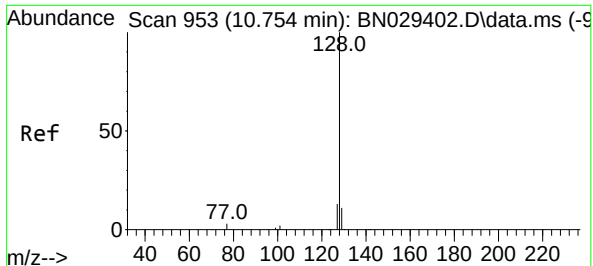





#9
Naphthalene
Concen: 0.097 ng
RT: 10.744 min Scan# 910
Delta R.T. -0.011 min
Lab File: BN029432.D
Acq: 31 Jan 2024 03:21

Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT4-2023

Tgt Ion:128 Resp: 2710
Ion Ratio Lower Upper
128 100
129 14.4 9.5 14.3
127 16.0 10.8 16.2




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 01/31/2024
Supervised By :Sohil Jodhani 02/02/2024

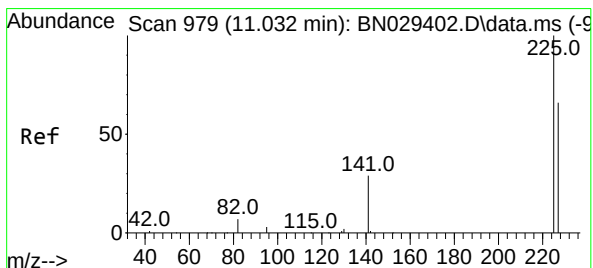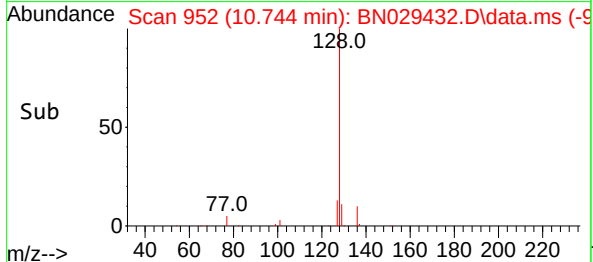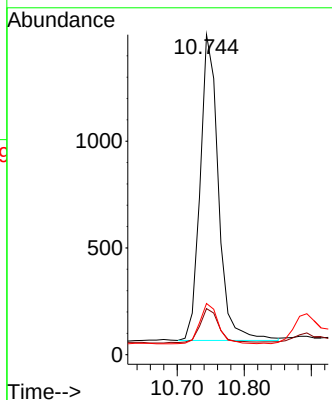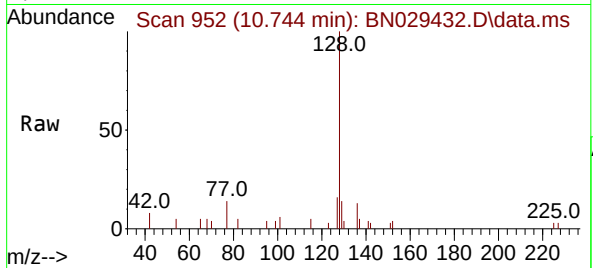

#10
Hexachlorobutadiene
Concen: 0.094 ng
RT: 11.021 min Scan# 978
Delta R.T. -0.011 min
Lab File: BN029432.D
Acq: 31 Jan 2024 03:21


Tgt Ion:225 Resp: 500
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 63.6 51.1 76.7

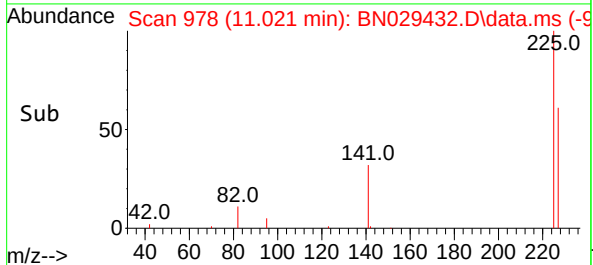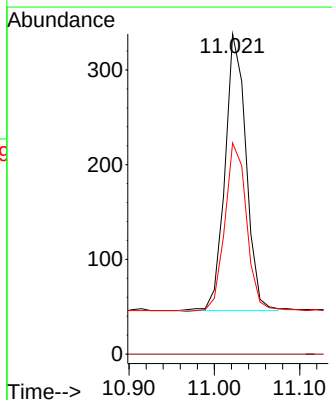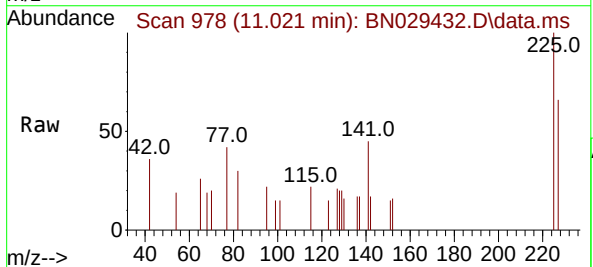

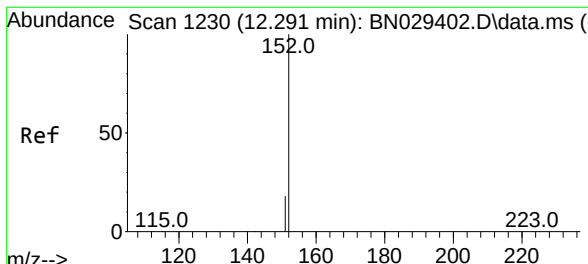

#11
2-Methylnaphthalene-d10
Concen: 0.538 ng
RT: 12.291 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN029432.D
Acq: 31 Jan 2024 03:21




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT4-2023

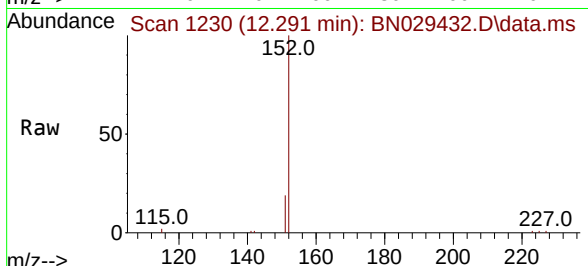


Tgt Ion:152 Resp: 722
Ion Ratio Lower Upper
152 100
151 19.4 17.1 25.7

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 01/31/2024
Supervised By :Sohil Jodhani 02/02/2024

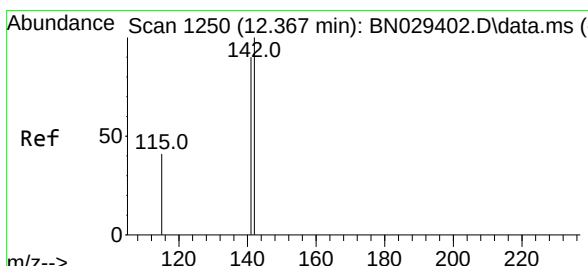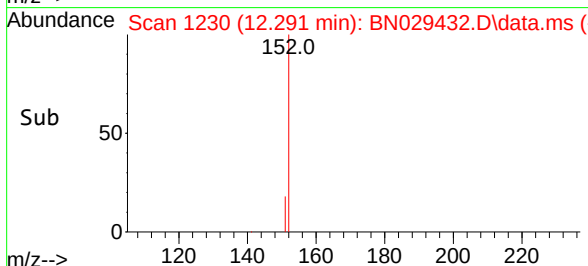


#12
2-Methylnaphthalene
Concen: 0.094 ng
RT: 12.363 min Scan# 1249
Delta R.T. -0.004 min
Lab File: BN029432.D
Acq: 31 Jan 2024 03:21

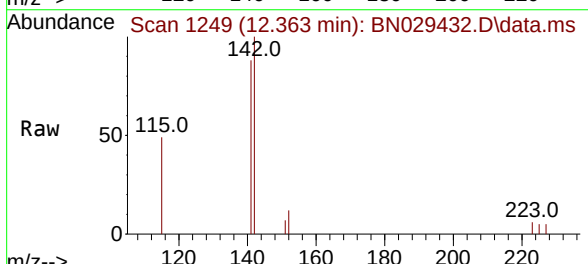


Tgt Ion:142 Resp: 1559
Ion Ratio Lower Upper
142 100
141 88.1 71.9 107.9
115 48.6 33.9 50.9

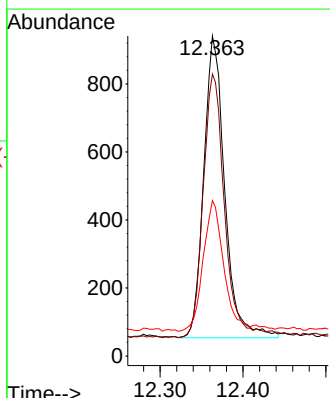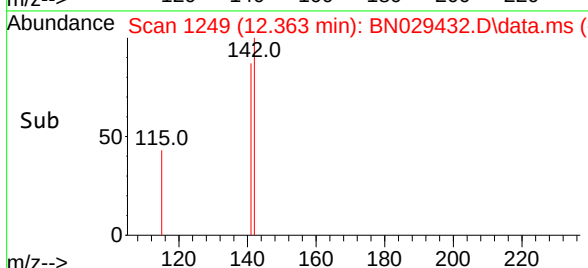



#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.532 min Scan# 11
Delta R.T. -0.011 min
Lab File: BN029432.D
Acq: 31 Jan 2024 03:21




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT4-2023




Tgt Ion:164 Resp: 455
Ion Ratio Lower Upper
164 100
162 106.1 82.6 123.8
160 54.0 41.5 62.3

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 01/31/2024
Supervised By :Sohil Jodhani 02/02/2024

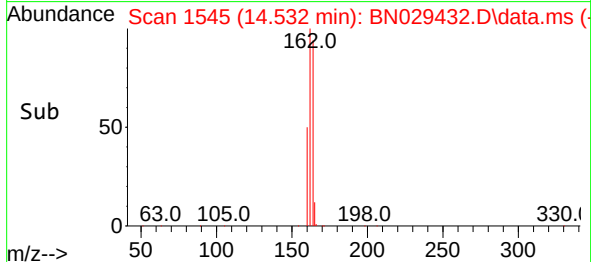


#14
2,4,6-Tribromophenol
Concen: 0.319 ng
RT: 16.027 min Scan# 1678
Delta R.T. -0.012 min
Lab File: BN029432.D
Acq: 31 Jan 2024 03:21

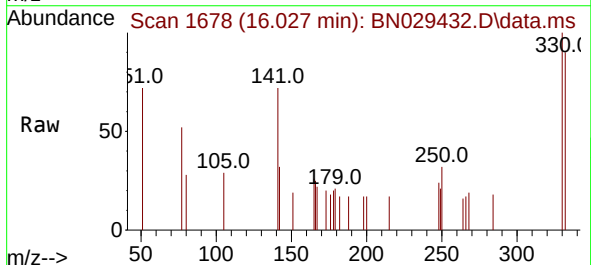


Tgt Ion:330 Resp: 466
Ion Ratio Lower Upper
330 100
332 99.8 76.0 114.0
141 57.7 43.4 65.2

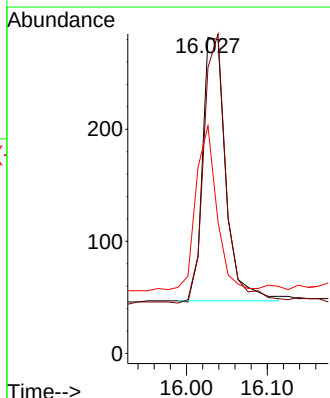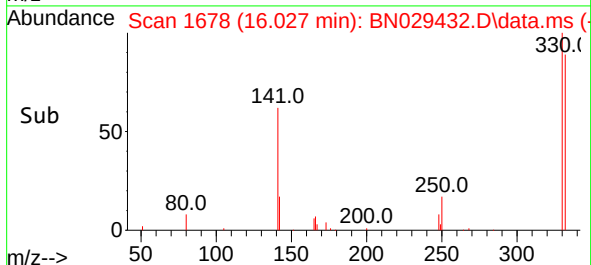

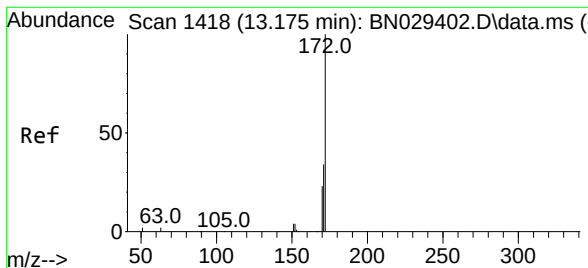

#15
2-Fluorobiphenyl
Concen: 0.338 ng
RT: 13.164 min Scan# 1418
Delta R.T. -0.011 min
Lab File: BN029432.D
Acq: 31 Jan 2024 03:21




Instrument : BNA_N
ClientSampleId : LOQ-WATER-02-QT4-2023

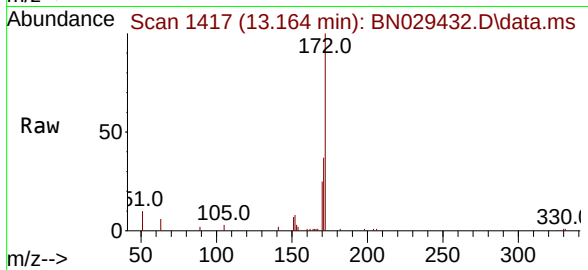

Tgt Ion:172 Resp: 6599
Ion Ratio Lower Upper
172 100
171 37.1 28.0 42.0
170 24.9 18.7 28.1




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 01/31/2024
Supervised By :Sohil Jodhani 02/02/2024

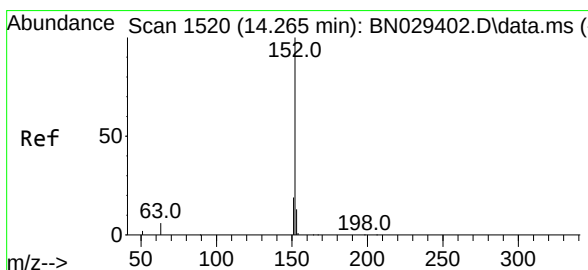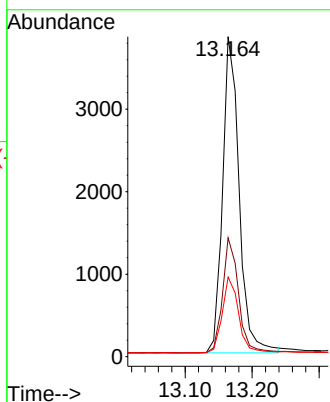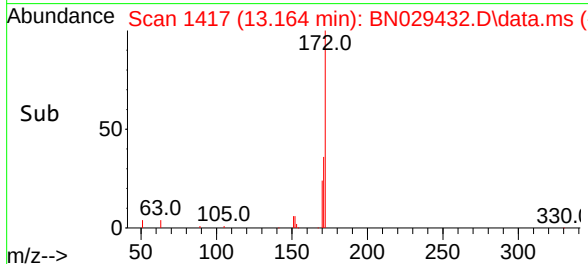

#16
Acenaphthylene
Concen: 0.097 ng
RT: 14.254 min Scan# 1519
Delta R.T. -0.011 min
Lab File: BN029432.D
Acq: 31 Jan 2024 03:21


Tgt Ion:152 Resp: 2093
Ion Ratio Lower Upper
152 100
151 20.1 15.9 23.9
153 14.7 10.5 15.7

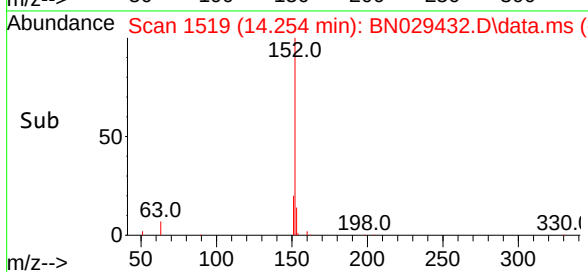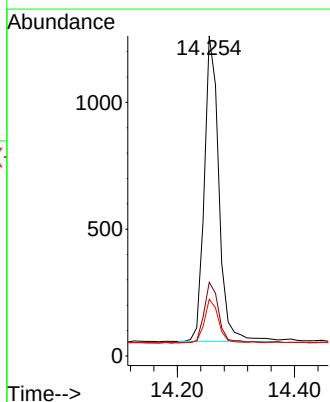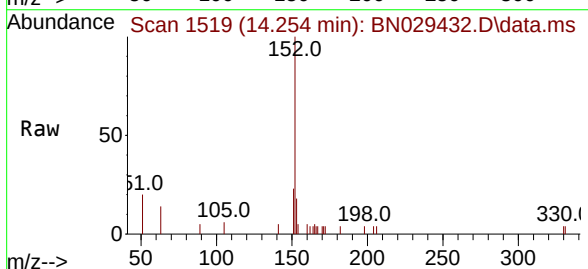



#17
Acenaphthene
Concen: 0.094 ng
RT: 14.597 min Scan# 1551
Delta R.T. -0.011 min
Lab File: BN029432.D
Acq: 31 Jan 2024 03:21




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT4-2023



Tgt Ion:154 Resp: 137
Ion Ratio Lower Upper
154 100
153 117.7 93.6 140.4
152 64.8 48.6 73.0




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 01/31/2024
Supervised By :Sohil Jodhani 02/02/2024

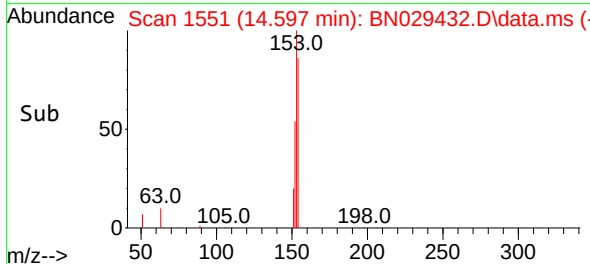

#18
Fluorene
Concen: 0.096 ng
RT: 15.592 min Scan# 1643
Delta R.T. -0.000 min
Lab File: BN029432.D
Acq: 31 Jan 2024 03:21

Tgt Ion:166 Resp: 1755
Ion Ratio Lower Upper
166 100
165 99.8 79.9 119.9
167 14.4 11.3 16.9

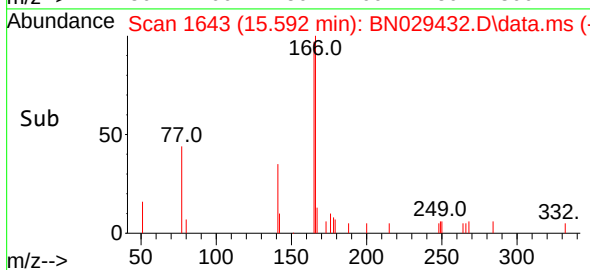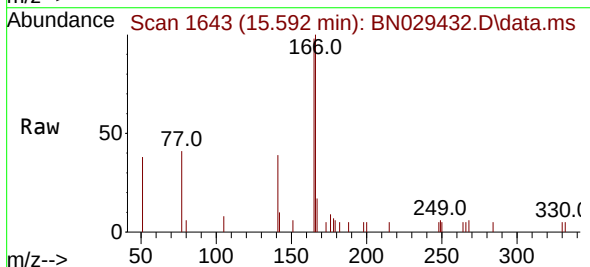



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.293 min Scan# 11

Delta R.T. -0.000 min

Lab File: BN029432.D

Acq: 31 Jan 2024 03:21

Instrument :

BNA_N

ClientSampleId :





LOQ-WATER-02-QT4-2023

Tgt Ion:	188	Resp:	8990
Ion Ratio	Lower	Upper	
188	100		
94	0.0	0.0	0.0
80	10.3	10.0	15.0

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 01/31/2024
Supervised By :Sohil Jodhani 02/02/2024

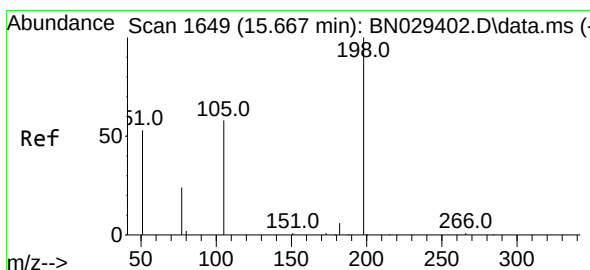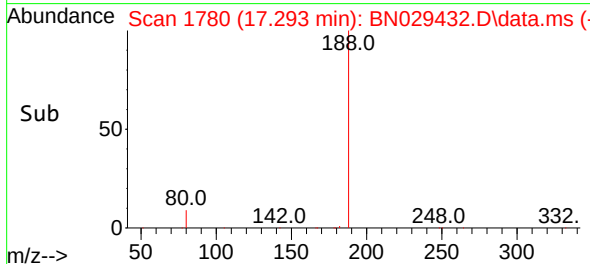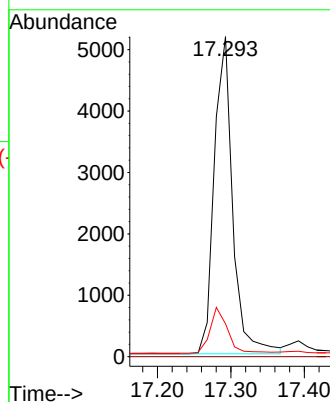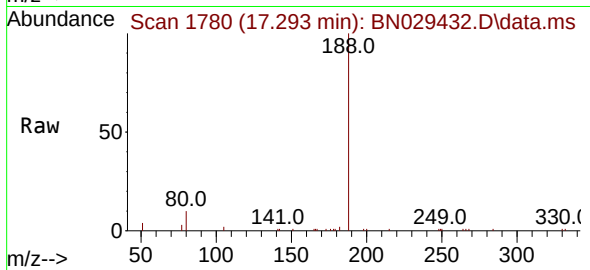

#20

4,6-Dinitro-2-methylphenol

Concen: 0.071 ng




RT: 15.679 min Scan# 1650


Delta R.T. 0.012 min

Lab File: BN029432.D

Acq: 31 Jan 2024 03:21


Tgt Ion:	198	Resp:	94
Ion Ratio	Lower	Upper	
198	100		
51	276.3	111.0	166.6#
105	113.8	67.0	100.6#

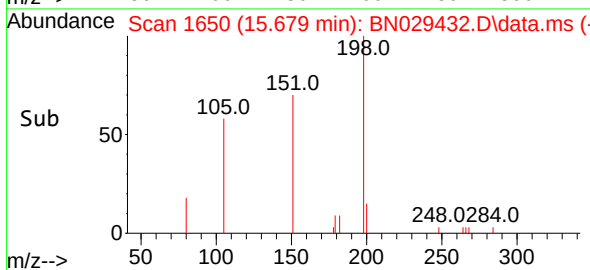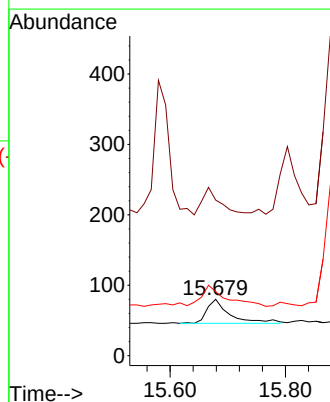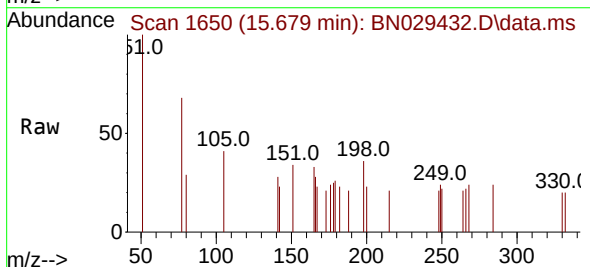



#21
4-Bromophenyl-phenylether
Concen: 0.092 ng
RT: 16.486 min Scan# 1715
Delta R.T. -0.000 min
Lab File: BN029432.D
Acq: 31 Jan 2024 03:21




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT4-2023




Tgt Ion:248 Resp: 491
Ion Ratio Lower Upper
248 100
250 98.3 75.0 112.4
141 88.6 77.0 115.6

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 01/31/2024
Supervised By :Sohil Jodhani 02/02/2024

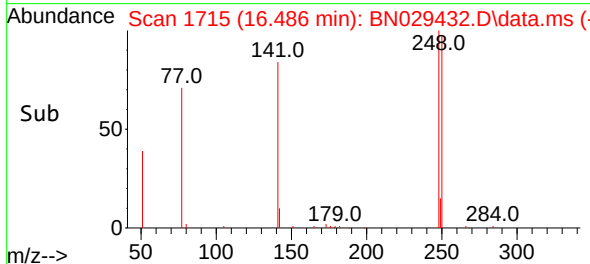


#22
Hexachlorobenzene
Concen: 0.096 ng
RT: 16.585 min Scan# 1723
Delta R.T. -0.000 min
Lab File: BN029432.D
Acq: 31 Jan 2024 03:21

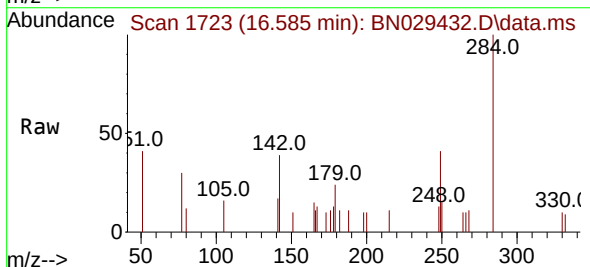


Tgt Ion:284 Resp: 629
Ion Ratio Lower Upper
284 100
142 49.4 39.4 59.2
249 34.8 26.9 40.3

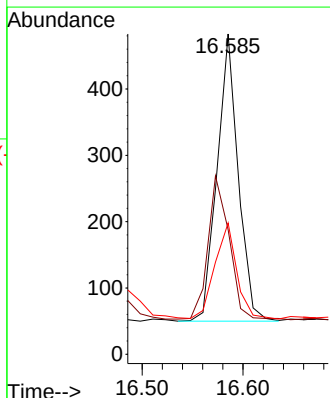

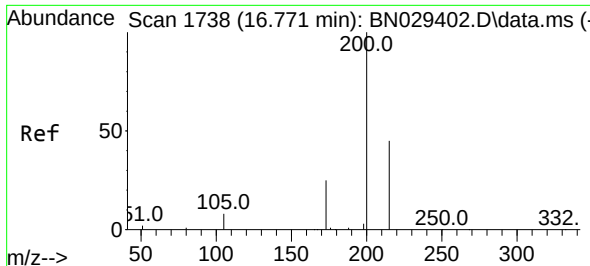

#23
Atrazine
Concen: 0.094 ng
RT: 16.771 min Scan# 1738
Delta R.T. -0.000 min
Lab File: BN029432.D
Acq: 31 Jan 2024 03:21




Instrument : BNA_N
ClientSampleId : LOQ-WATER-02-QT4-2023




Tgt Ion:200 Resp: 359
Ion Ratio Lower Upper
200 100
173 41.9 23.4 35.0
215 58.6 38.4 57.6

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 01/31/2024
Supervised By :Sohil Jodhani 02/02/2024

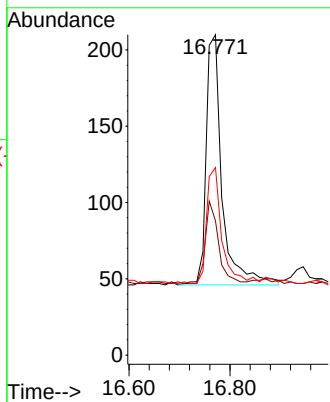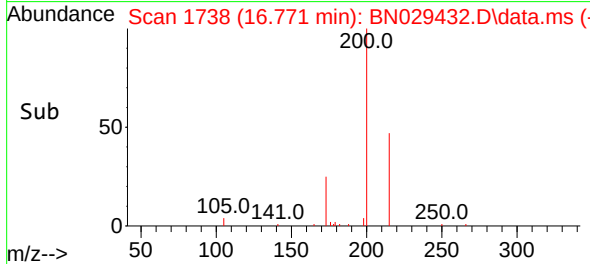


#24
Pentachlorophenol
Concen: 0.054 ng
RT: 16.933 min Scan# 1751
Delta R.T. -0.000 min
Lab File: BN029432.D
Acq: 31 Jan 2024 03:21

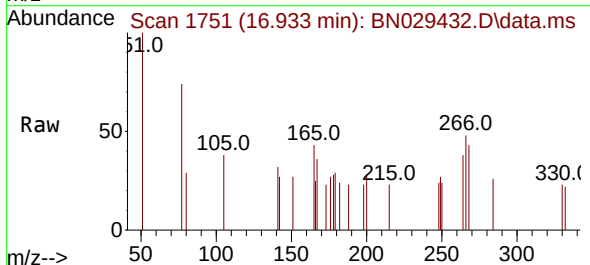


Tgt Ion:266 Resp: 112
Ion Ratio Lower Upper
266 100
264 58.9 50.8 76.2
268 76.8 51.5 77.3

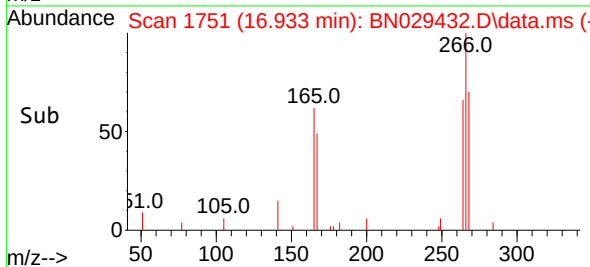



#25
Phenanthrene
Concen: 0.097 ng
RT: 17.330 min Scan# 1783
Delta R.T. -0.000 min
Lab File: BN029432.D
Acq: 31 Jan 2024 03:21




Instrument : BNA_N
ClientSampleId : LOQ-WATER-02-QT4-2023




Tgt Ion:178 Resp: 2569
Ion Ratio Lower Upper
178 100
176 19.7 15.8 23.6
179 15.9 12.6 19.0

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 01/31/2024
Supervised By :Sohil Jodhani 02/02/2024

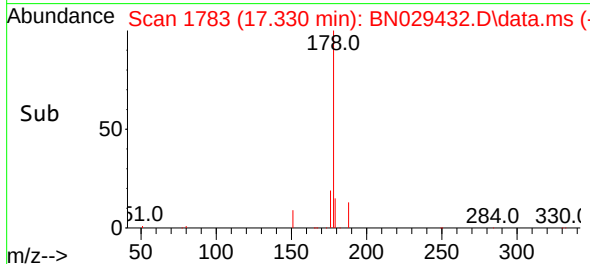


#26
Anthracene
Concen: 0.092 ng
RT: 17.429 min Scan# 1791
Delta R.T. -0.000 min
Lab File: BN029432.D
Acq: 31 Jan 2024 03:21

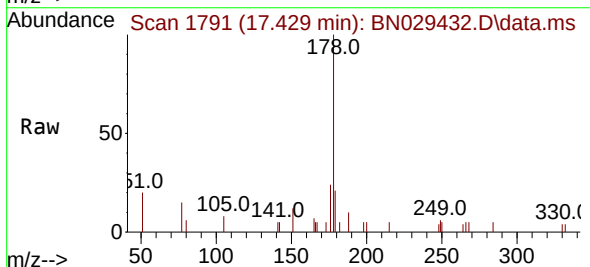


Tgt Ion:178 Resp: 2076
Ion Ratio Lower Upper
178 100
176 20.2 15.0 22.4
179 14.8 12.3 18.5

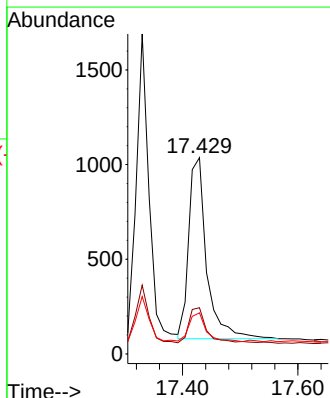

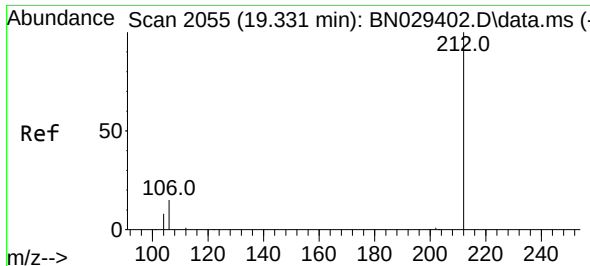

#27
Fluoranthene-d10
Concen: 0.568 ng
RT: 19.322 min Scan# 2053
Delta R.T. -0.009 min
Lab File: BN029432.D
Acq: 31 Jan 2024 03:21




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT4-2023



Tgt Ion:212 Resp: 12374
Ion Ratio Lower Upper
212 100
106 16.2 13.2 19.8
104 9.9 7.7 11.5




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 01/31/2024
Supervised By :Sohil Jodhani 02/02/2024

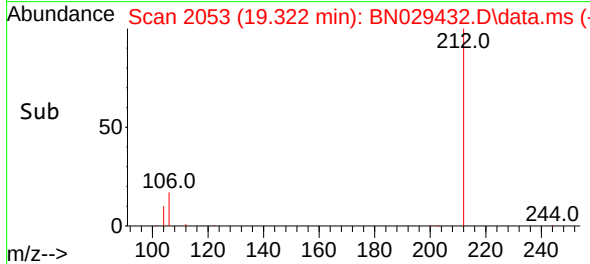

#28
Fluoranthene
Concen: 0.086 ng
RT: 19.355 min Scan# 2060
Delta R.T. -0.005 min
Lab File: BN029432.D
Acq: 31 Jan 2024 03:21


Tgt Ion:202 Resp: 2578
Ion Ratio Lower Upper
202 100
101 13.9 10.5 15.7
203 17.7 13.5 20.3

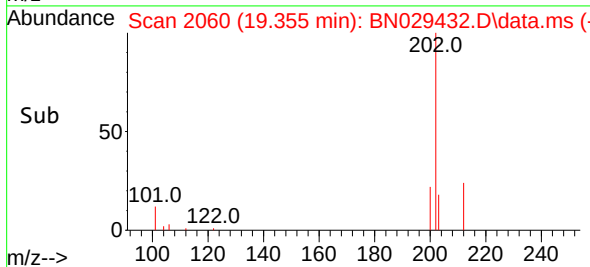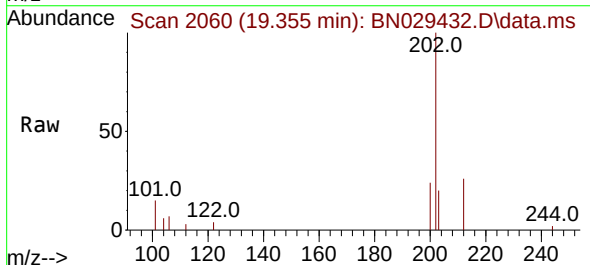



#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.492 min Scan# 2470
Delta R.T. -0.000 min
Lab File: BN029432.D
Acq: 31 Jan 2024 03:21




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT4-2023




Tgt Ion:240 Resp: 6280
Ion Ratio Lower Upper
240 100
120 14.0 16.7 25.1
236 29.1 23.9 35.9

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 01/31/2024
Supervised By :Sohil Jodhani 02/02/2024

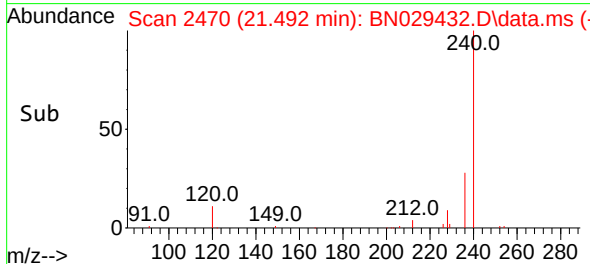


#30
Pyrene
Concen: 0.091 ng
RT: 19.717 min Scan# 2138
Delta R.T. -0.005 min
Lab File: BN029432.D
Acq: 31 Jan 2024 03:21

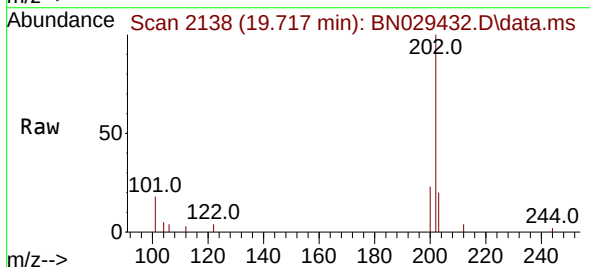


Tgt Ion:202 Resp: 2638
Ion Ratio Lower Upper
202 100
200 20.4 16.6 25.0
203 16.9 14.2 21.4

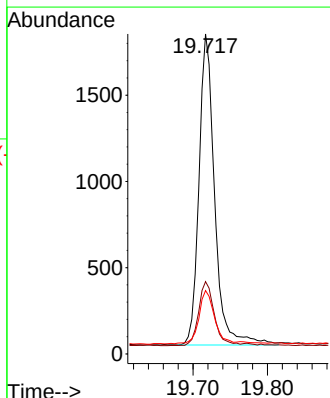



#31
 Terphenyl-d14
 Concen: 0.332 ng
 RT: 19.931 min Scan# 2185
 Delta R.T. -0.005 min
 Lab File: BN029432.D
 Acq: 31 Jan 2024 03:21




Instrument : BNA_N
 ClientSampleId : LOQ-WATER-02-QT4-2023



Tgt Ion:244 Resp: 517
 Ion Ratio Lower Upper
 244 100
 212 10.5 8.2 12.4
 122 19.0 15.6 23.4




Manual Integrations
 APPROVED


Reviewed By :Jagrut Upadhyay 01/31/2024
 Supervised By :Sohil Jodhani 02/02/2024

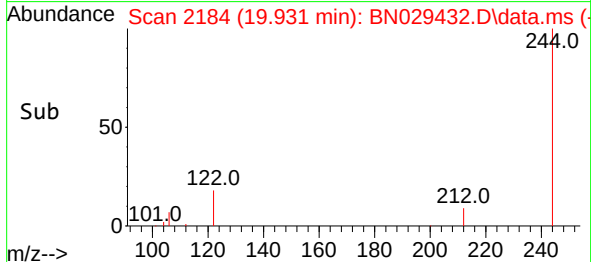

#32
 Benzo(a)anthracene
 Concen: 0.086 ng
 RT: 21.474 min Scan# 2468
 Delta R.T. -0.009 min
 Lab File: BN029432.D
 Acq: 31 Jan 2024 03:21

Tgt Ion:228 Resp: 1849
 Ion Ratio Lower Upper
 228 100
 226 29.4 22.2 33.4
 229 22.6 16.5 24.7

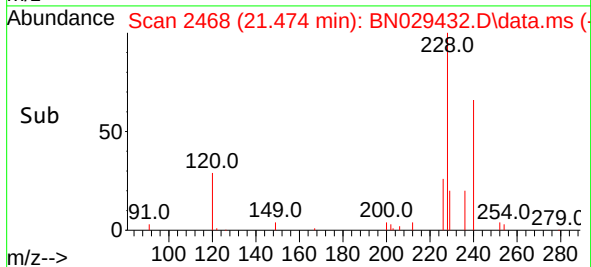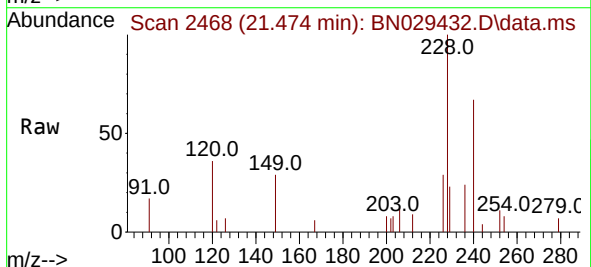



#33

Chrysene

Concen: 0.089 ng

RT: 21.528 min Scan# 2474

Delta R.T. -0.000 min

Lab File: BN029432.D

Acq: 31 Jan 2024 03:21

Instrument :

BNA_N

ClientSampleId :





LOQ-WATER-02-QT4-2023

Tgt Ion:	228	Resp:	216
Ion Ratio	Lower	Upper	
228	100		
226	31.1	24.9	37.3
229	22.6	15.9	23.9

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 01/31/2024
Supervised By :Sohil Jodhani 02/02/2024

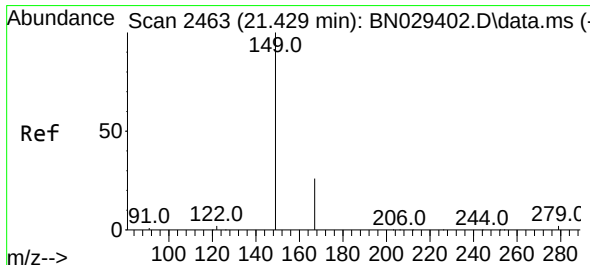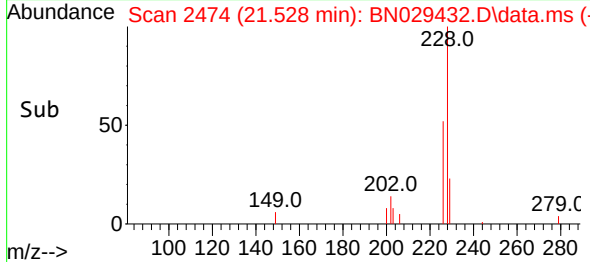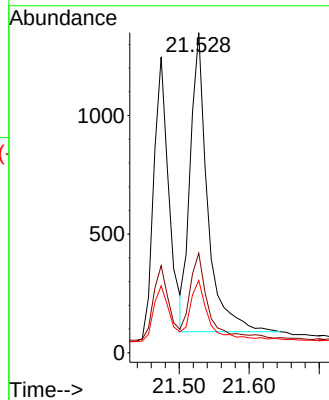

#34

Bis(2-ethylhexyl)phthalate

Concen: 0.111 ng




RT: 21.420 min Scan# 2462


Delta R.T. -0.009 min

Lab File: BN029432.D

Acq: 31 Jan 2024 03:21


Tgt Ion:	149	Resp:	1622
Ion Ratio	Lower	Upper	
149	100		
167	24.3	20.1	30.1
279	3.2	2.5	3.7

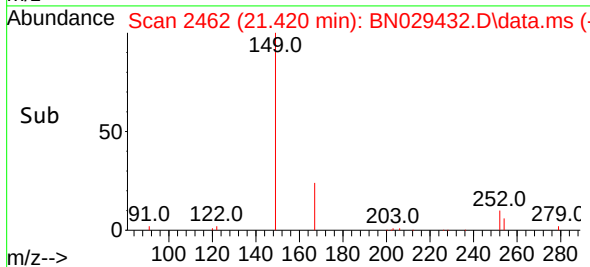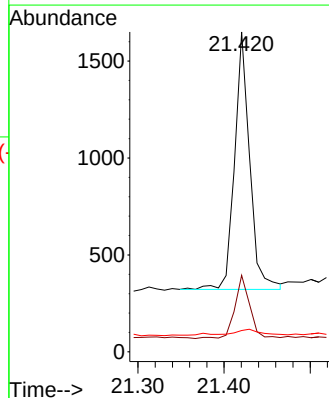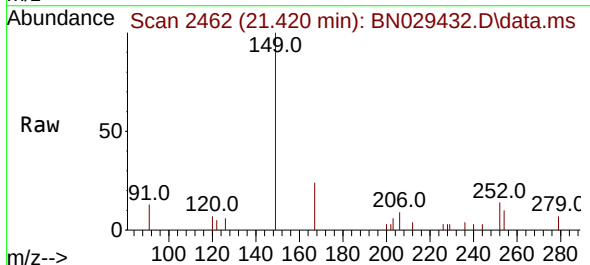



#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.870 min Scan# 3078
 Delta R.T. -0.015 min
 Lab File: BN029432.D
 Acq: 31 Jan 2024 03:21




Instrument : BNA_N
 ClientSampleId : LOQ-WATER-02-QT4-2023




Tgt Ion:264 Resp: 6674
 Ion Ratio Lower Upper
 264 100
 260 27.4 21.2 31.8
 265 46.1 41.5 62.3

Manual Integrations
 APPROVED



Reviewed By :Jagrut Upadhyay 01/31/2024
 Supervised By :Sohil Jodhani 02/02/2024

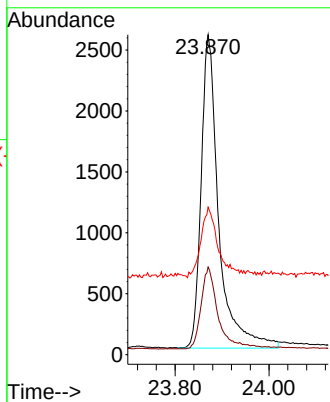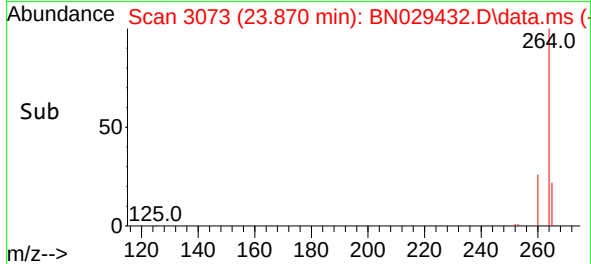


#36
 Indeno(1,2,3-cd)pyrene
 Concen: 0.076 ng
 RT: 26.338 min Scan# 3917
 Delta R.T. -0.015 min
 Lab File: BN029432.D
 Acq: 31 Jan 2024 03:21

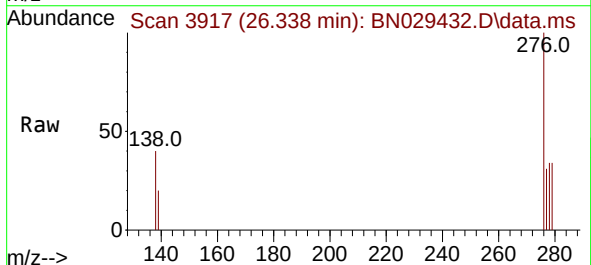

Tgt Ion:276 Resp: 2052
 Ion Ratio Lower Upper
 276 100
 138 15.0 20.5 30.7#
 277 8.6 17.0 25.4#

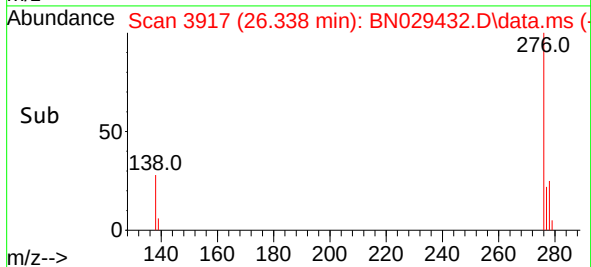



#37

Benzo(b)fluoranthene

Concen: 0.079 ng

RT: 23.151 min Scan# 2827

Delta R.T. -0.006 min

Lab File: BN029432.D

Acq: 31 Jan 2024 03:21

Instrument :

BNA_N

ClientSampleId :

LOQ-WATER-02-QT4-2023





Tgt Ion:252 Resp: 1885

Ion	Ratio	Lower	Upper
252	100		
253	44.7	21.7	32.5
125	26.1	13.3	19.9

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 01/31/2024
Supervised By :Sohil Jodhani 02/02/2024

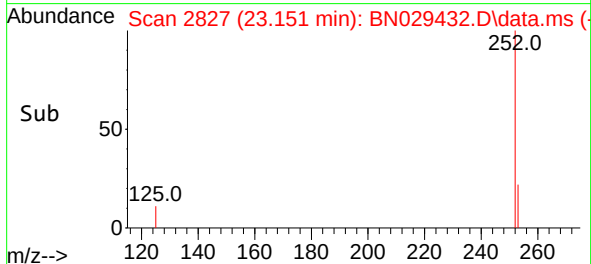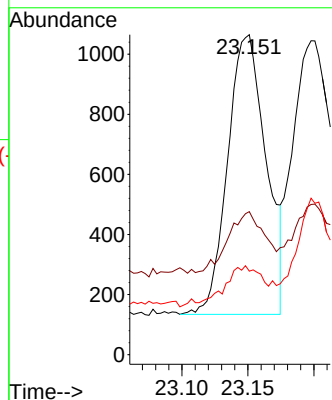

#38

Benzo(k)fluoranthene

Concen: 0.078 ng

RT: 23.198 min Scan# 2843




Delta R.T. -0.009 min


Lab File: BN029432.D

Acq: 31 Jan 2024 03:21

Tgt Ion:252 Resp: 1938


Ion	Ratio	Lower	Upper
252	100		
253	47.8	21.8	32.8
125	49.9	13.9	20.9

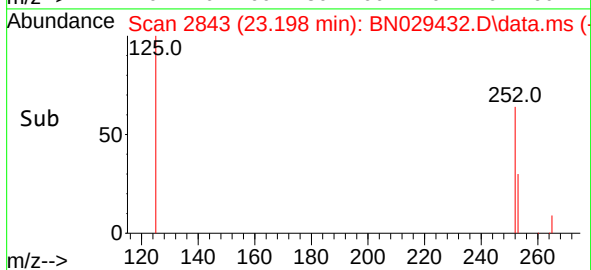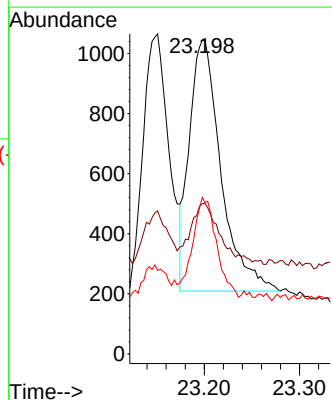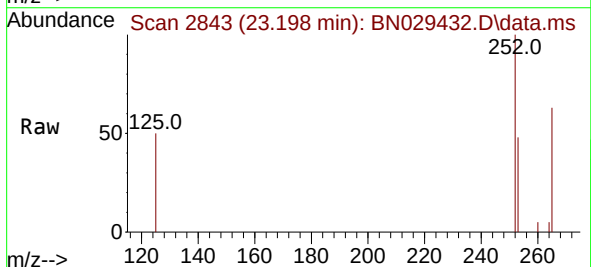



#39
Benzo(a)pyrene
Concen: 0.077 ng m
RT: 23.765 min Scan# 3041
Delta R.T. -0.012 min
Lab File: BN029432.D
Acq: 31 Jan 2024 03:21




Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT4-2023



Tgt Ion:252 Resp: 160
Ion Ratio Lower Upper
252 100
253 61.0 24.9 37.3#
125 36.0 16.6 25.0#




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 01/31/2024
Supervised By :Sohil Jodhani 02/02/2024



#40
Dibenzo(a,h)anthracene
Concen: 0.080 ng m
RT: 26.373 min Scan# 3929
Delta R.T. -0.006 min
Lab File: BN029432.D
Acq: 31 Jan 2024 03:21


Tgt Ion:278 Resp: 1716
Ion Ratio Lower Upper
278 100
139 34.3 20.4 30.6#
279 47.6 25.0 37.6#

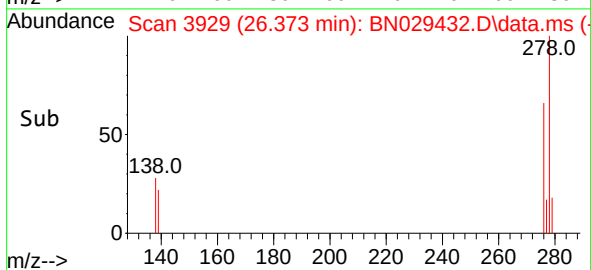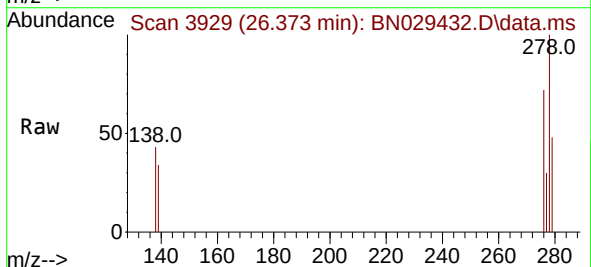

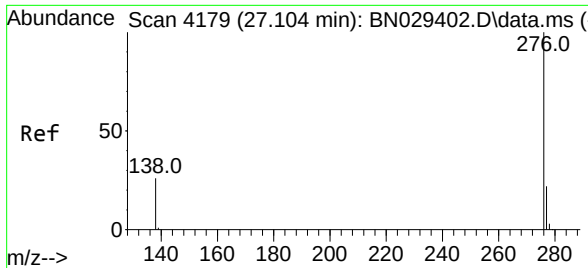

#41
Benzo(g,h,i)perylene
Concen: 0.075 ng
RT: 27.089 min Scan# 41
Delta R.T. -0.015 min
Lab File: BN029432.D
Acq: 31 Jan 2024 03:21

Instrument :
BNA_N
ClientSampleId :
LOQ-WATER-02-QT4-2023

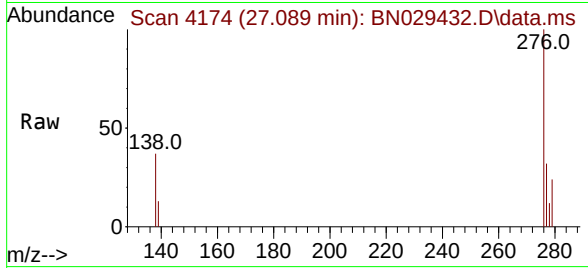

Tgt Ion:276 Resp: 1948
Ion Ratio Lower Upper
276 100
277 31.9 19.4 29.2
138 37.4 23.5 35.3

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 01/31/2024
Supervised By :Sohil Jodhani 02/02/2024

