


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013024\
Data File : BN029409.D
Acq On : 30 Jan 2024 09:35
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 01 03:26:31 2024

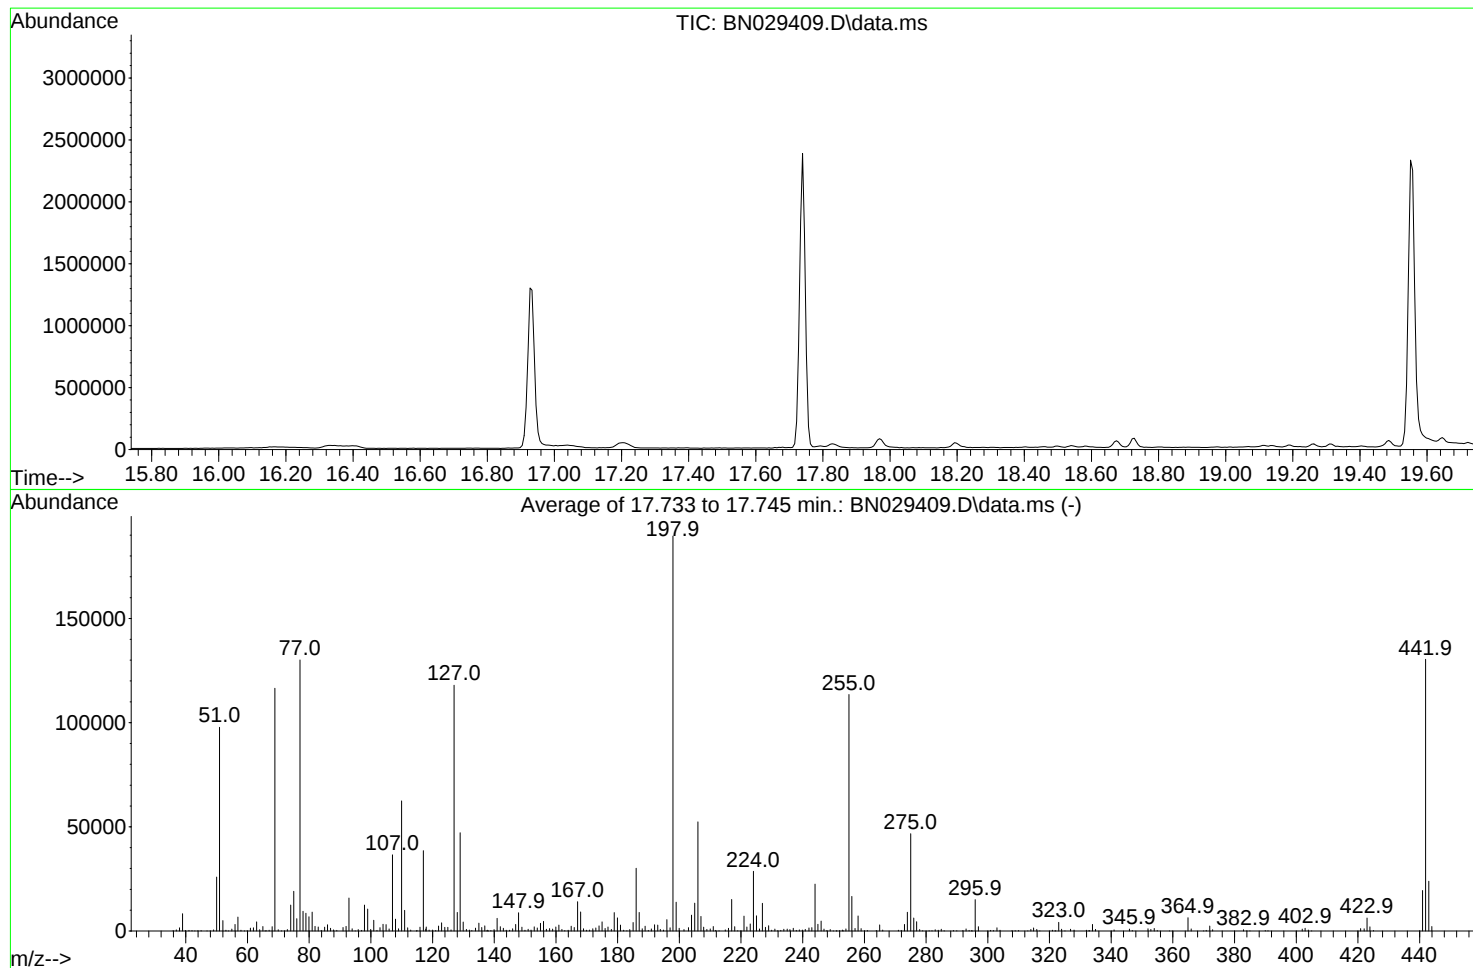

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2483

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.8	2060	PASS
69	69	100	100	100.0	116479	PASS
70	69	0.00	2	0.6	648	PASS
197	198	0.00	2	0.8	1518	PASS
198	198	100	100	100.0	189504	PASS
199	198	5	9	7.3	13847	PASS
365	198	1	100	3.4	6393	PASS
441	443	0.01	150	81.4	19428	PASS
442	442	100	100	100.0	130389	PASS
443	442	15	24	18.3	23869	PASS