
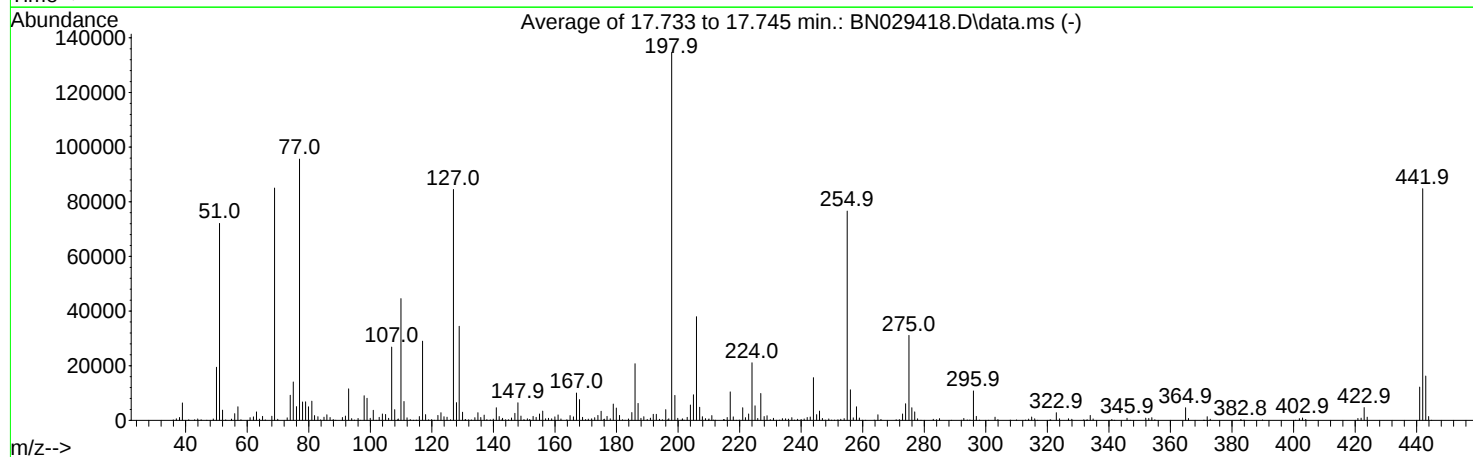


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013024\
Data File : BN029418.D
Acq On : 30 Jan 2024 18:56
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN012924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 01 01:51:59 2024

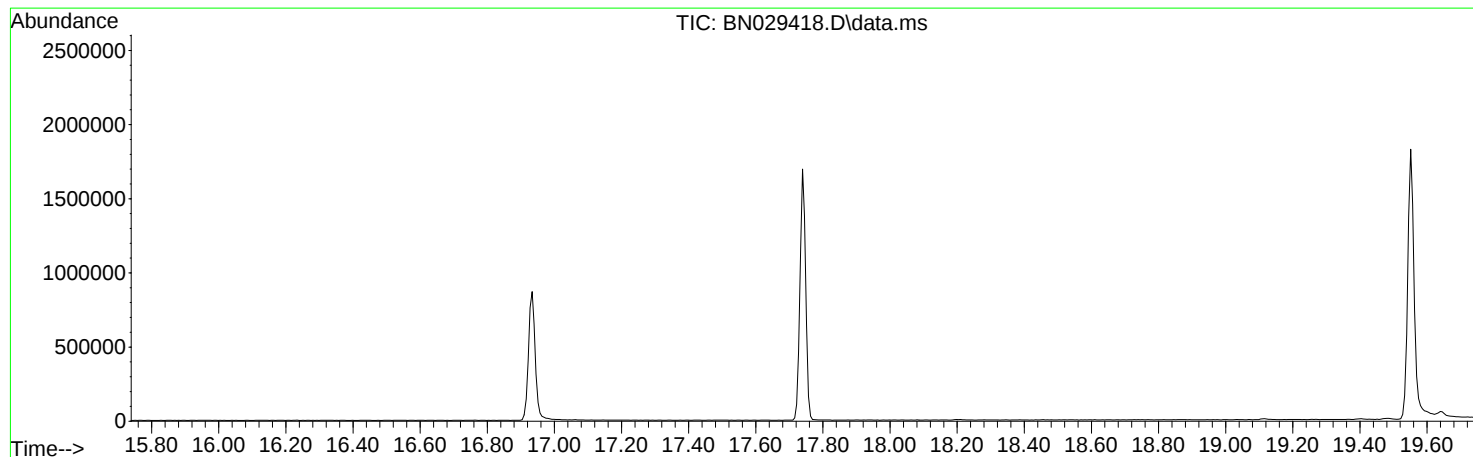

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2483

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	53.6	72109	PASS
68	69	0.00	2	1.8	1539	PASS
69	198	0.00	100	63.2	85043	PASS
70	69	0.00	2	0.5	441	PASS
127	198	10	80	62.8	84501	PASS
197	198	0.00	2	0.5	623	PASS
198	198	100	100	100.0	134643	PASS
199	198	5	9	6.8	9124	PASS
275	198	10	60	23.1	31099	PASS
365	198	1	100	3.4	4643	PASS
441	198	0.01	100	9.1	12197	PASS
442	442	50	100	100.0	84819	PASS
443	442	15	24	19.1	16217	PASS