
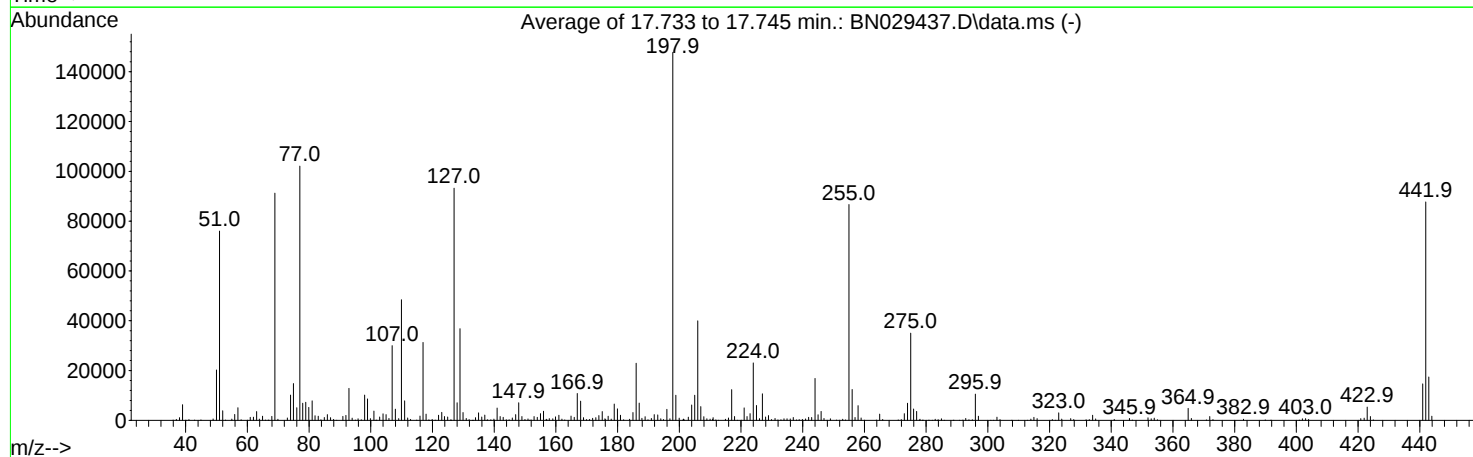


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013024\
Data File : BN029437.D
Acq On : 31 Jan 2024 06:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN012924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 01 01:51:59 2024

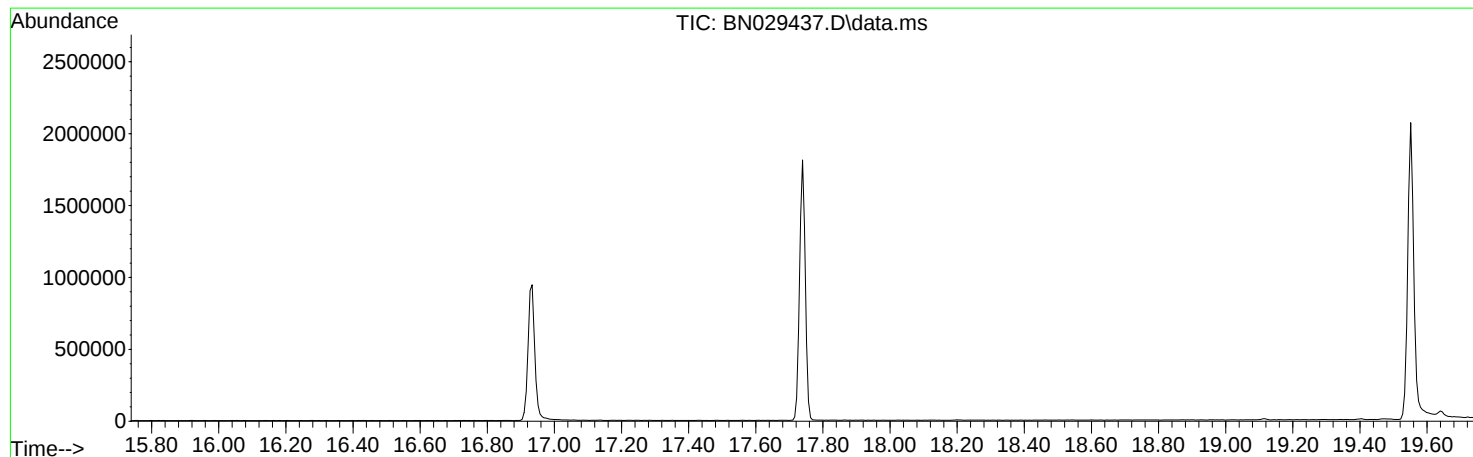

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.5	76016	PASS
68	69	0.00	2	1.7	1586	PASS
69	198	0.00	100	61.8	91243	PASS
70	69	0.00	2	0.5	425	PASS
127	198	10	80	63.1	93232	PASS
197	198	0.00	2	0.4	624	PASS
198	198	100	100	100.0	147712	PASS
199	198	5	9	6.8	10106	PASS
275	198	10	60	23.7	35016	PASS
365	198	1	100	3.2	4797	PASS
441	198	0.01	100	9.9	14675	PASS
442	442	50	100	100.0	87704	PASS
443	442	15	24	19.8	17403	PASS