

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013025\
 Data File : BN036141.D
 Acq On : 30 Jan 2025 20:21
 Operator : RC/JU
 Sample : PB166277TB 10X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SLEB277

Quant Time: Jan 31 07:34:00 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN013025.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 30 17:36:07 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.793	152	95026	20.000	ng/ul	0.00
20) Naphthalene-d8	10.587	136	347768	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.434	164	215996	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.181	188	435160	20.000	ng/ul	0.00
79) Chrysene-d12	21.427	240	384808	20.000	ng/ul	0.00
88) Perylene-d12	24.451	264	425104	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	20618	8.841	ng/uL	0.00
4) Pyridine-d5	3.675	84	207957	31.308	ng/ul	0.00
7) Phenol-d5	6.993	99	230348	29.253	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.122	67	148989	29.484	ng/ul	0.00
11) 2-Chlorophenol-d4	7.340	132	187102	30.349	ng/ul	0.00
15) 4-Methylphenol-d8	8.522	113	182358	28.827	ng/ul	0.00
21) Nitrobenzene-d5	8.946	128	85394	30.585	ng/ul	0.00
24) 2-Nitrophenol-d4	9.669	143	97106	30.653	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.228	165	169137	29.570	ng/ul	0.00
31) 4-Chloroaniline-d4	10.722	131	216790	28.850	ng/ul	0.00
46) Dimethylphthalate-d6	13.846	166	493530	30.298	ng/ul	0.00
49) Acenaphthylene-d8	14.128	160	552927	30.486	ng/ul	0.00
54) 4-Nitrophenol-d4	14.687	143	76023	27.043	ng/ul	0.00
60) Fluorene-d10	15.428	176	406448	29.809	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.540	200	69219	24.034	ng/ul	0.00
73) Anthracene-d10	17.281	188	658329	31.143	ng/ul	0.00
81) Pyrene-d10	19.575	212	690113	30.113	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.251	264	681285	30.479	ng/ul	0.00


Target Compounds					Qvalue
17) N-Nitroso-di-n-propyla...	8.516	70	5595	1.030 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013025\
Data File : BN036141.D
Acq On : 30 Jan 2025 20:21
Operator : RC/JU
Sample : PB166277TB 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SLEB277


Quant Time: Jan 31 07:34:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN013025.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jan 30 17:36:07 2025
Response via : Initial Calibration

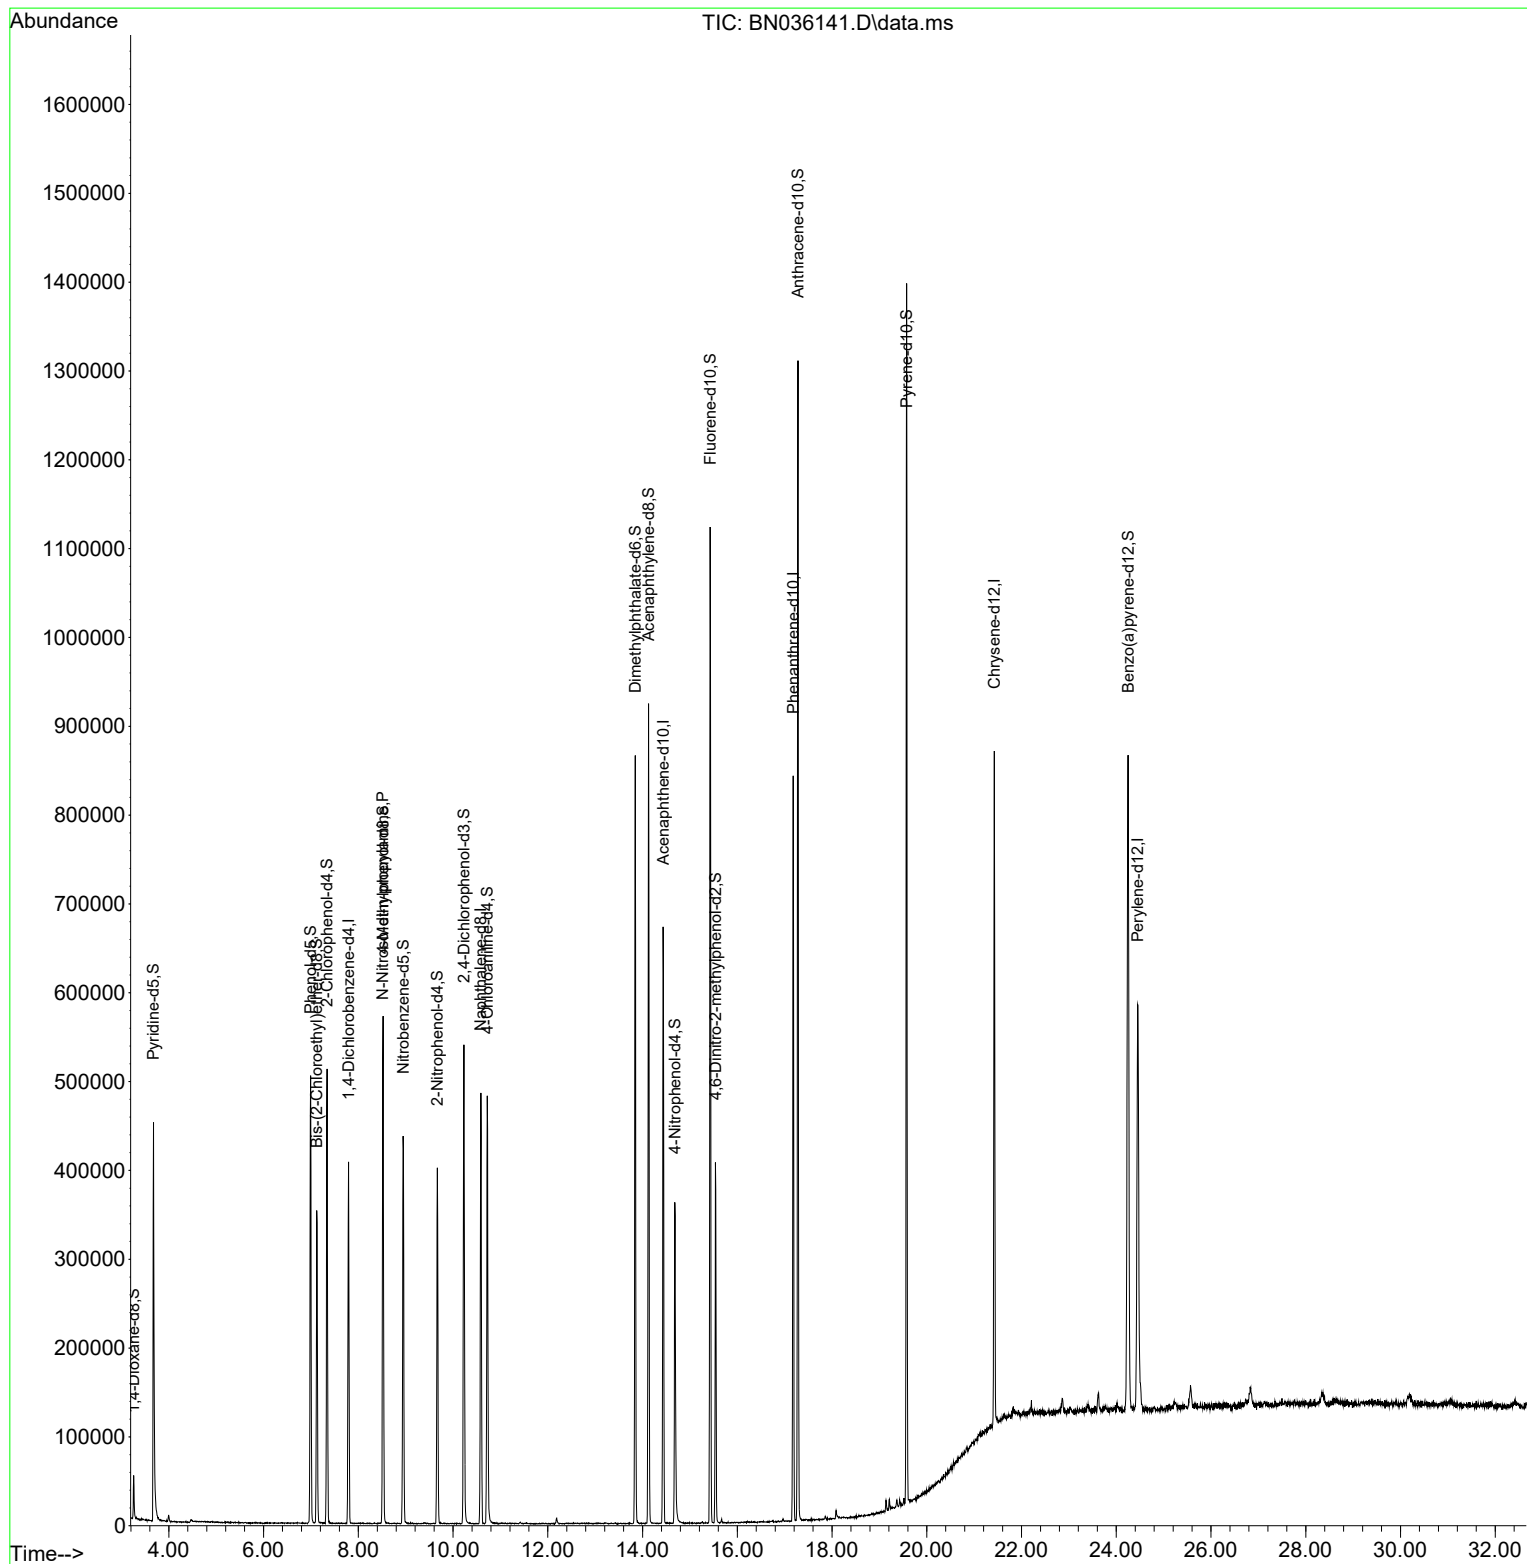

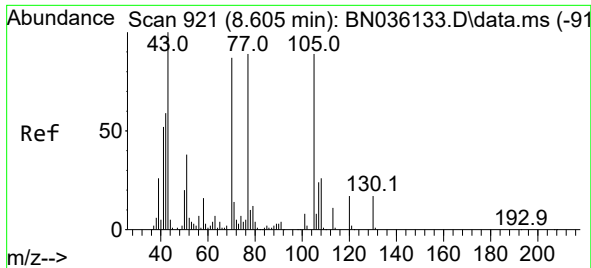

#17
 N-Nitroso-di-n-propylamine
 Concen: 1.030 ng/ul
 RT: 8.516 min Scan# 90
 Delta R.T. -0.088 min
 Lab File: BN036141.D
 Acq: 30 Jan 2025 20:21

Instrument :
 BNA_N
 ClientSampleId :
 SLEB277

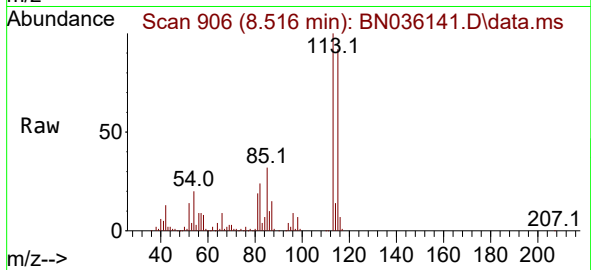

Tgt Ion: 70 Resp: 5595

Ion	Ratio	Lower	Upper
70	100		
42	388.8	54.7	82.1#
101	0.0	7.1	10.7#
130	0.0	15.7	23.5#

