

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013025\
 Data File : BN036143.D
 Acq On : 30 Jan 2025 21:39
 Operator : RC/JU
 Sample : Q1162-02 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E2947

Quant Time: Jan 31 07:34:18 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN013025.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 30 17:36:07 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.792	152	90938	20.000	ng/ul	0.00
20) Naphthalene-d8	10.586	136	365413	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.439	164	246088	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.180	188	483368	20.000	ng/ul	0.00
79) Chrysene-d12	21.427	240	459485	20.000	ng/ul	0.00
88) Perylene-d12	24.450	264	399059	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.257	96	11031	4.943	ng/uL	0.00
4) Pyridine-d5	3.675	84	69395	10.917	ng/ul	0.00
7) Phenol-d5	6.992	99	78072	10.360	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.122	67	158671	32.811	ng/ul	0.00
11) 2-Chlorophenol-d4	7.340	132	177575	30.099	ng/ul	0.00
15) 4-Methylphenol-d8	8.522	113	144022	23.790	ng/ul	0.00
21) Nitrobenzene-d5	8.951	128	100490	34.254	ng/ul	0.00
24) 2-Nitrophenol-d4	9.669	143	116445	34.983	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.228	165	193207	32.147	ng/ul	0.00
31) 4-Chloroaniline-d4	10.722	131	236120	29.905	ng/ul	0.00
46) Dimethylphthalate-d6	13.845	166	705847	38.034	ng/ul	0.00
49) Acenaphthylene-d8	14.127	160	679751	32.895	ng/ul	0.00
54) 4-Nitrophenol-d4	14.686	143	35777	11.171	ng/ul	0.00
60) Fluorene-d10	15.427	176	560350	36.071	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.545	200	111454	34.839	ng/ul	0.00
73) Anthracene-d10	17.280	188	939525	40.013	ng/ul	0.00
81) Pyrene-d10	19.574	212	1106897	40.449	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.250	264	798067	38.033	ng/ul	0.00
Target Compounds						
					Qvalue	
35) 4-Chloro-3-methylphenol	11.945	107	8343	1.199	ng/ul#	24
47) Dimethylphthalate	13.892	163	26803	1.442	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013025\
Data File : BN036143.D
Acq On : 30 Jan 2025 21:39
Operator : RC/JU
Sample : Q1162-02 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E2947

Quant Time: Jan 31 07:34:18 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN013025.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jan 30 17:36:07 2025
Response via : Initial Calibration




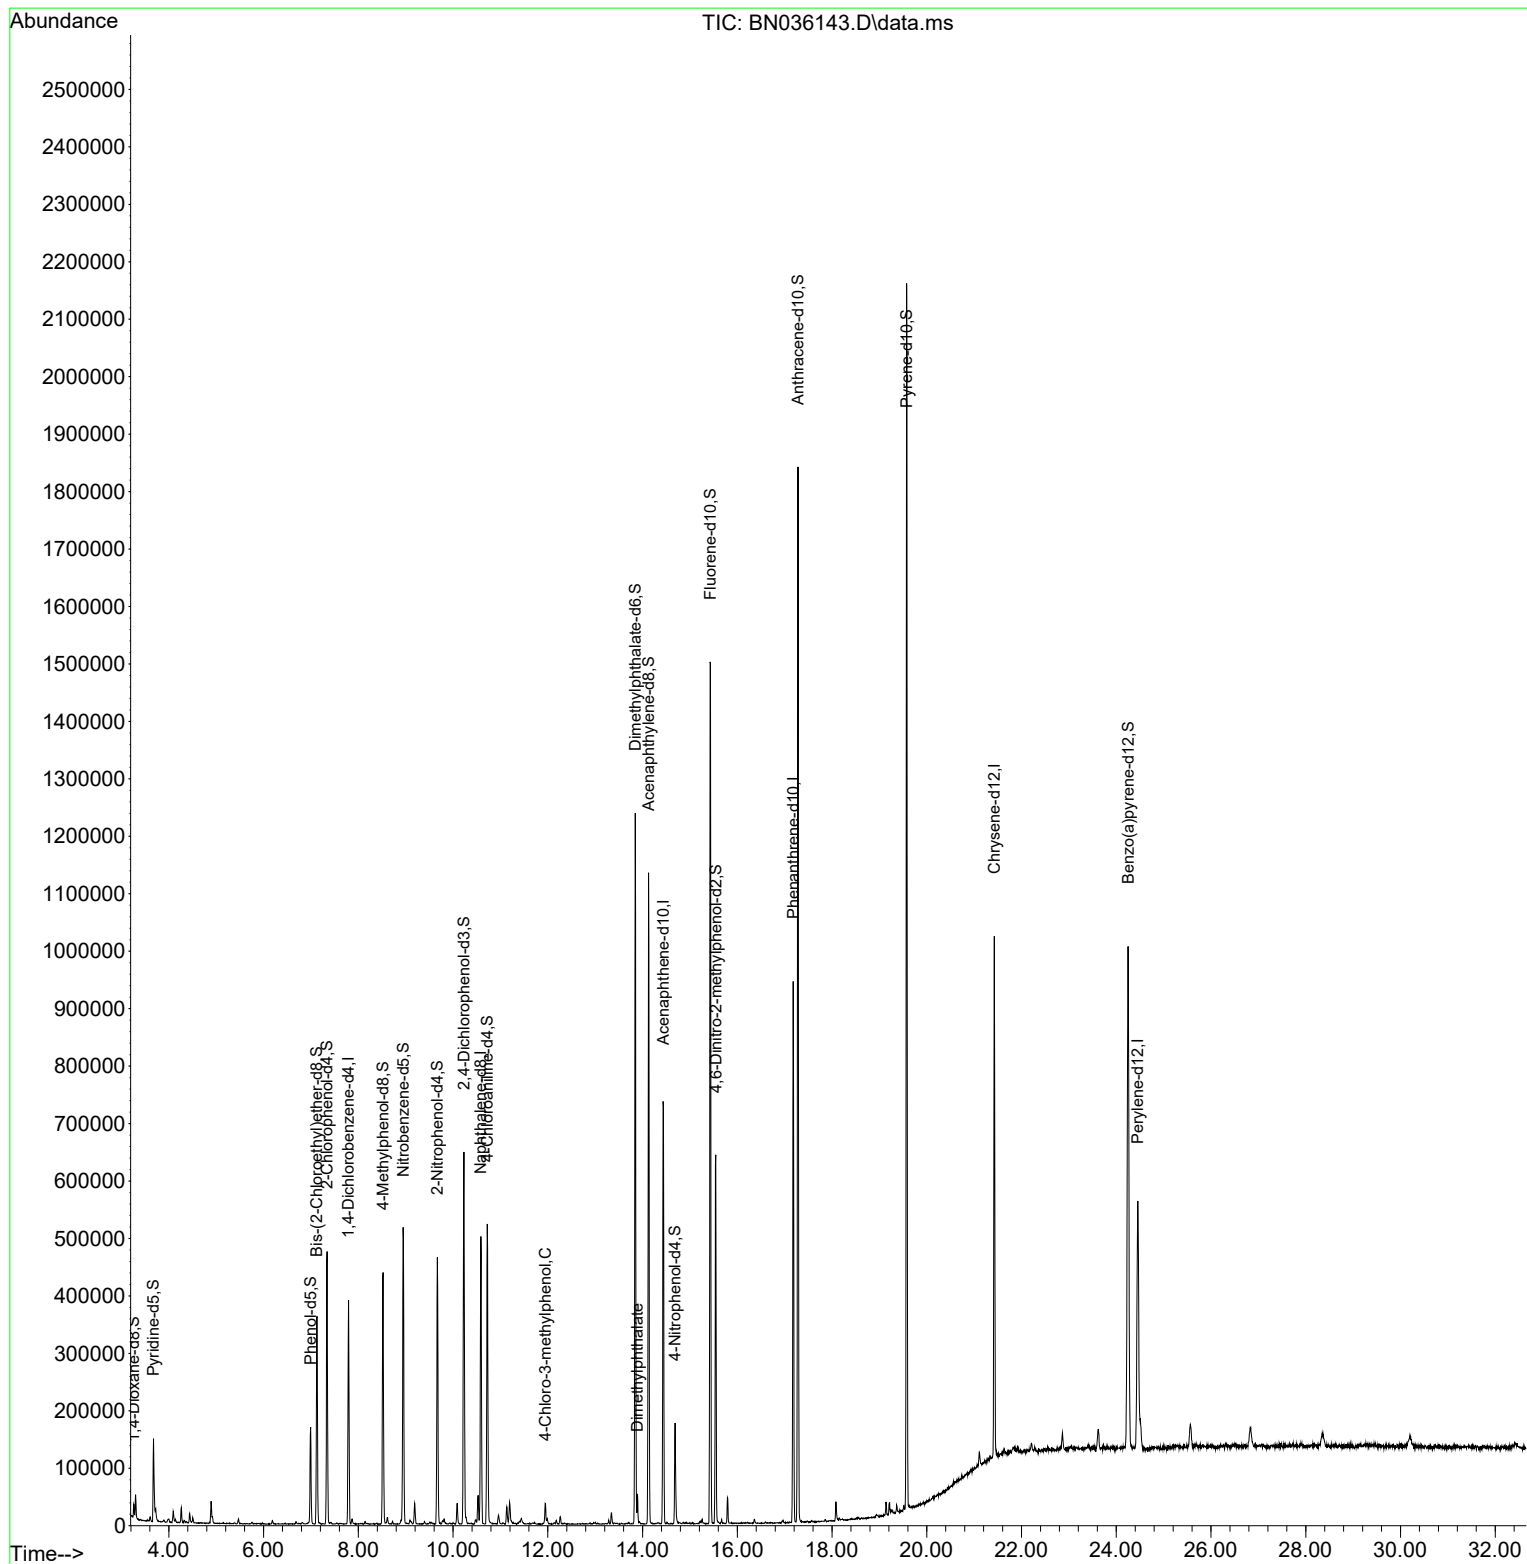


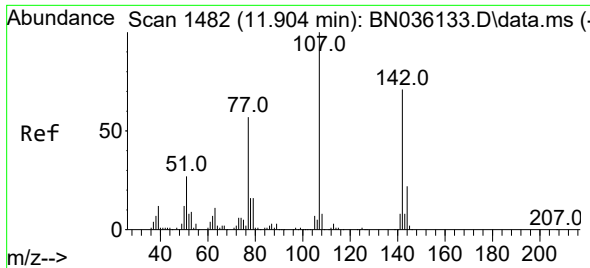

#35
 4-Chloro-3-methylphenol
 Concen: 1.199 ng/ul
 RT: 11.945 min Scan# 1489
 Delta R.T. 0.041 min
 Lab File: BN036143.D
 Acq: 30 Jan 2025 21:39

Instrument :
 BNA_N
 ClientSampleId :
 E2947

Tgt Ion:107 Resp: 8343
 Ion Ratio Lower Upper
 107 100
 144 0.0 17.5 26.3#
 142 0.0 56.7 85.1#

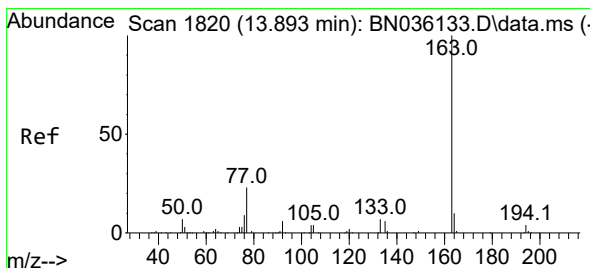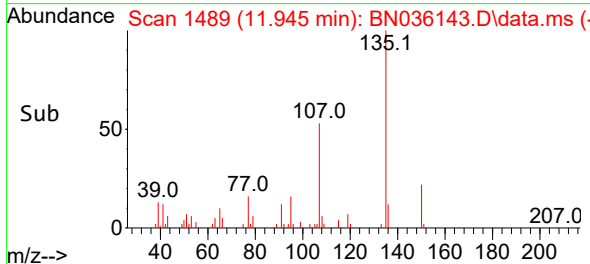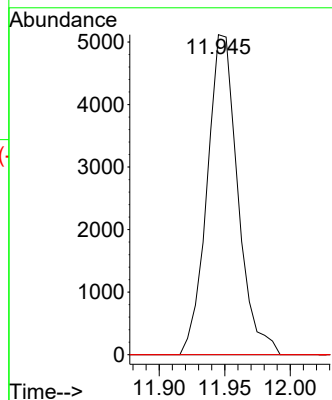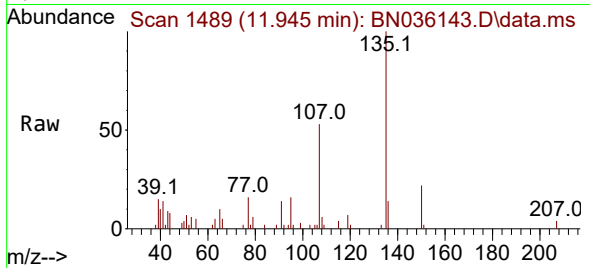

#47
 Dimethylphthalate
 Concen: 1.442 ng/ul
 RT: 13.892 min Scan# 1820
 Delta R.T. -0.000 min
 Lab File: BN036143.D
 Acq: 30 Jan 2025 21:39

Tgt Ion:163 Resp: 26803
 Ion Ratio Lower Upper
 163 100
 194 3.9 3.3 4.9
 164 9.1 8.4 12.6

