

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013025\
 Data File : BN036148.D
 Acq On : 31 Jan 2025 00:55
 Operator : RC/JU
 Sample : Q1191-06
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A44W6

Quant Time: Jan 31 07:35:57 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN013025.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 30 17:36:07 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.793	152	101304	20.000	ng/ul	0.00
20) Naphthalene-d8	10.587	136	395156	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.434	164	272977	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.181	188	567282	20.000	ng/ul	0.00
79) Chrysene-d12	21.428	240	530386	20.000	ng/ul	0.00
88) Perylene-d12	24.463	264	458240	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	10911	4.389	ng/uL	0.00
4) Pyridine-d5	3.676	84	28906	4.082	ng/ul	0.00
7) Phenol-d5	6.987	99	55601	6.623	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.122	67	155667	28.896	ng/ul	0.00
11) 2-Chlorophenol-d4	7.334	132	161431	24.563	ng/ul	0.00
15) 4-Methylphenol-d8	8.516	113	111550	16.541	ng/ul	0.00
21) Nitrobenzene-d5	8.946	128	91906	28.970	ng/ul	0.00
24) 2-Nitrophenol-d4	9.669	143	105847	29.406	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.228	165	178805	27.512	ng/ul	0.00
31) 4-Chloroaniline-d4	10.722	131	72685	8.513	ng/ul	0.00
46) Dimethylphthalate-d6	13.846	166	698168	33.914	ng/ul	0.00
49) Acenaphthylene-d8	14.128	160	671508	29.295	ng/ul	0.00
54) 4-Nitrophenol-d4	14.681	143	24444	6.880	ng/ul	0.00
60) Fluorene-d10	15.428	176	559745	32.483	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.540	200	105145	28.005	ng/ul	0.00
73) Anthracene-d10	17.281	188	921273	33.432	ng/ul	0.00
81) Pyrene-d10	19.575	212	1120554	35.475	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.251	264	802488	33.305	ng/ul	0.00
Target Compounds						
35) 4-Chloro-3-methylphenol	11.899	107	9423	1.253	ng/ul	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013025\
 Data File : BN036148.D
 Acq On : 31 Jan 2025 00:55
 Operator : RC/JU
 Sample : Q1191-06
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A44W6

Quant Time: Jan 31 07:35:57 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN013025.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 30 17:36:07 2025
 Response via : Initial Calibration

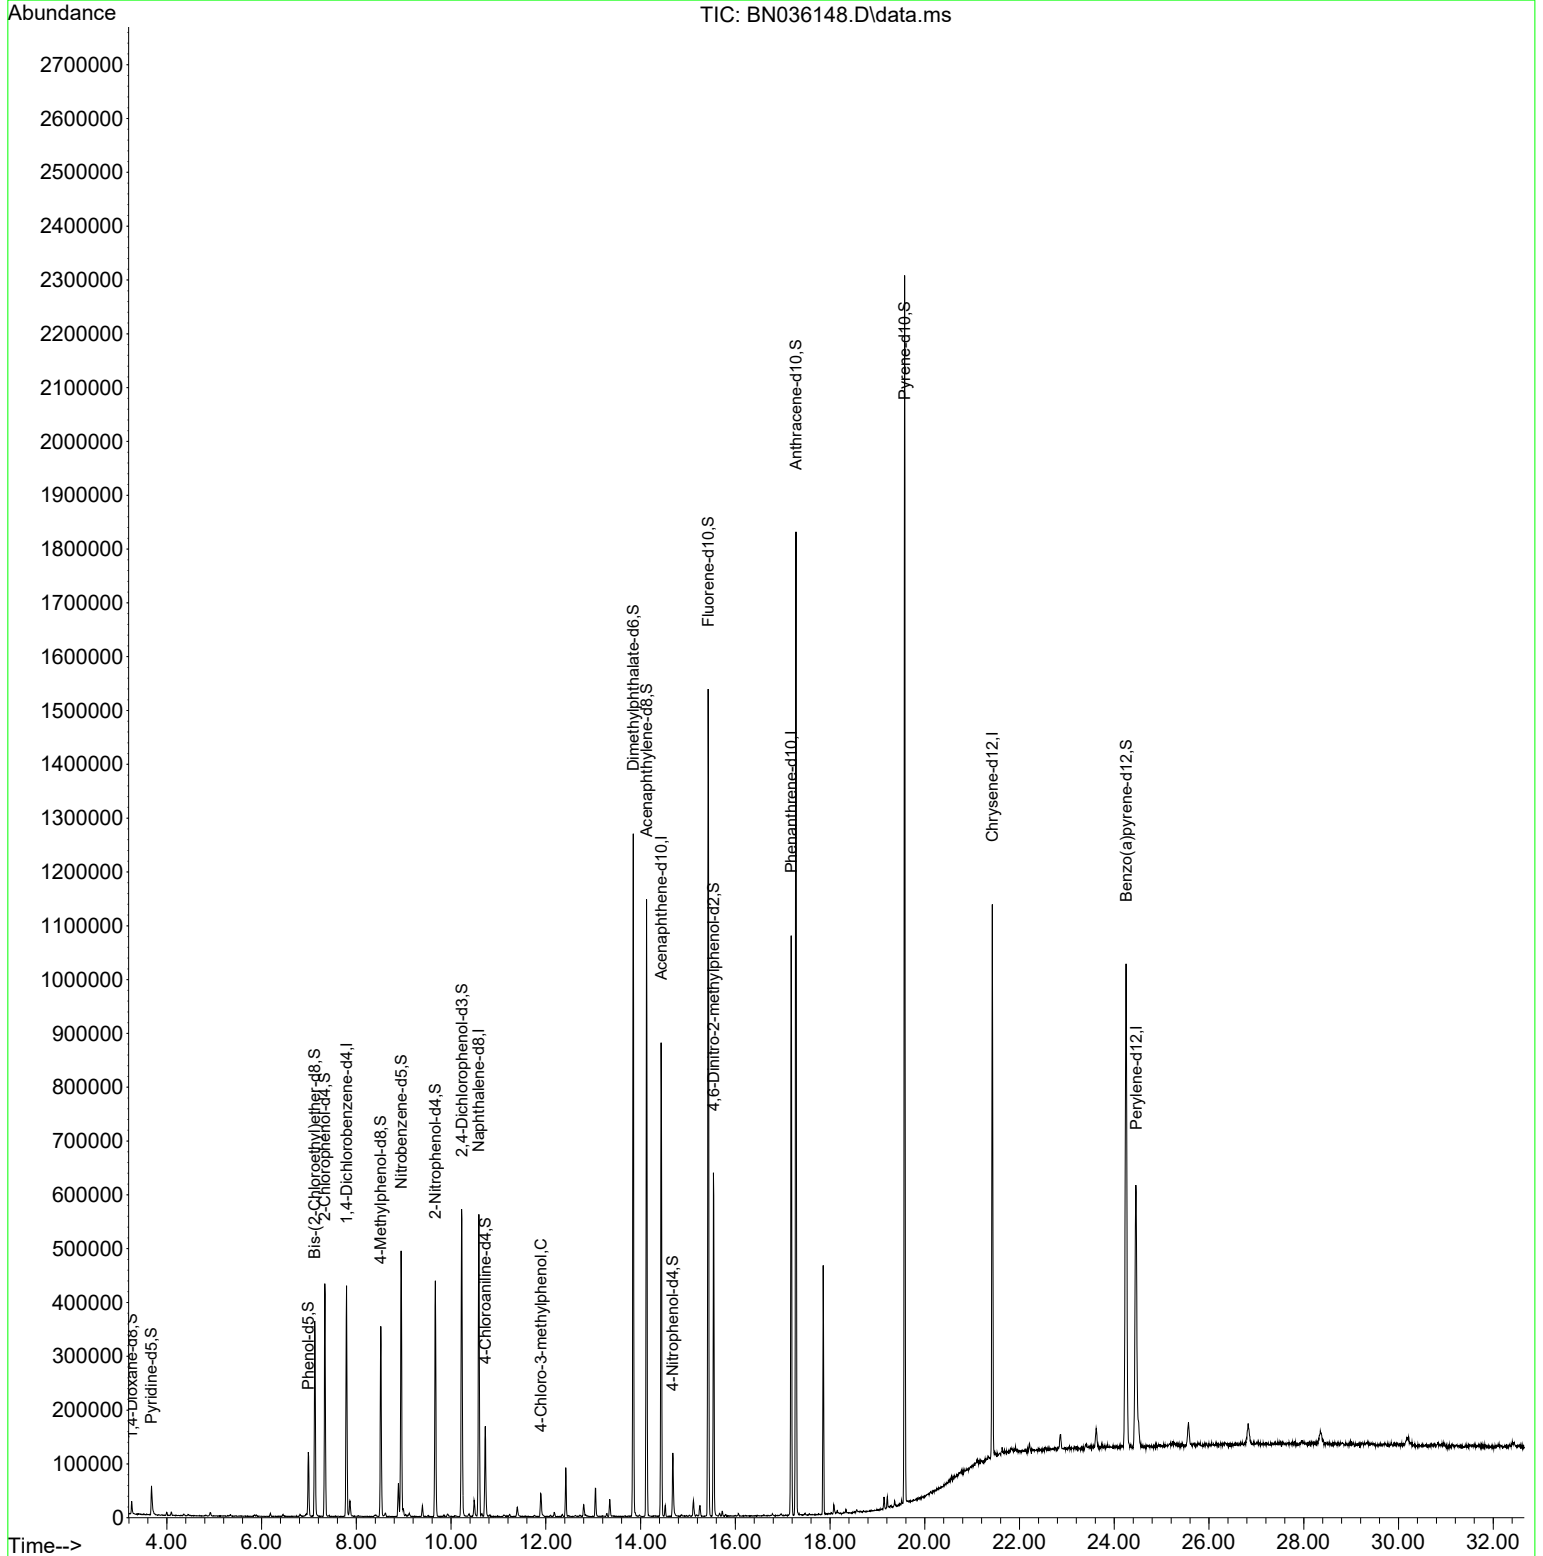

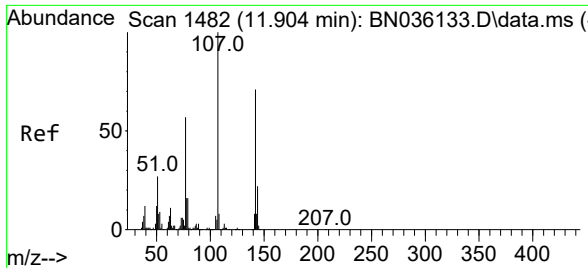

#35
 4-Chloro-3-methylphenol
 Concen: 1.253 ng/ul
 RT: 11.899 min Scan# 14
 Delta R.T. -0.006 min
 Lab File: BN036148.D
 Acq: 31 Jan 2025 00:55

Instrument :
 BNA_N
ClientSampleId :
 A44W6

Tgt Ion:107 Resp: 9423

Ion	Ratio	Lower	Upper
107	100		
144	24.5	17.5	26.3
142	67.4	56.7	85.1

