

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013025\
 Data File : BN036147.D
 Acq On : 31 Jan 2025 00:16
 Operator : RC/JU
 Sample : Q1191-05
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A44W5

Quant Time: Jan 31 07:35:47 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN013025.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 30 17:36:07 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.793	152	115693	20.000	ng/u1	0.00
20) Naphthalene-d8	10.587	136	444422	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.434	164	288127	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.181	188	588596	20.000	ng/u1	0.00
79) Chrysene-d12	21.428	240	489684	20.000	ng/u1	0.00
88) Perylene-d12	24.457	264	457058	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	11684	4.115	ng/uL	0.00
4) Pyridine-d5	3.693	84	1717	0.212	ng/u1	0.02
7) Phenol-d5	6.987	99	117004	12.204	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.122	67	181536	29.507	ng/u1	0.00
11) 2-Chlorophenol-d4	7.334	132	212638	28.330	ng/u1	0.00
15) 4-Methylphenol-d8	8.516	113	182858	23.742	ng/u1	0.00
21) Nitrobenzene-d5	8.946	128	110099	30.858	ng/u1	0.00
24) 2-Nitrophenol-d4	9.669	143	127366	31.462	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.228	165	217346	29.735	ng/u1	0.00
31) 4-Chloroaniline-d4	10.728	131	12629	1.315	ng/u1	0.00
46) Dimethylphthalate-d6	13.846	166	775907	35.709	ng/u1	0.00
49) Acenaphthylene-d8	14.128	160	759334	31.385	ng/u1	0.00
54) 4-Nitrophenol-d4	14.681	143	50747	13.533	ng/u1	0.00
60) Fluorene-d10	15.428	176	634986	34.912	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.545	200	120989	31.058	ng/u1	0.00
73) Anthracene-d10	17.281	188	997804	34.898	ng/u1	0.00
81) Pyrene-d10	19.575	212	1108463	38.009	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.251	264	822125	34.208	ng/u1	0.00
Target Compounds						
35) 4-Chloro-3-methylphenol	11.899	107	12507	1.478	ng/u1	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013025\
Data File : BN036147.D
Acq On : 31 Jan 2025 00:16
Operator : RC/JU
Sample : Q1191-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A44W5

Quant Time: Jan 31 07:35:47 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN013025.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jan 30 17:36:07 2025
Response via : Initial Calibration

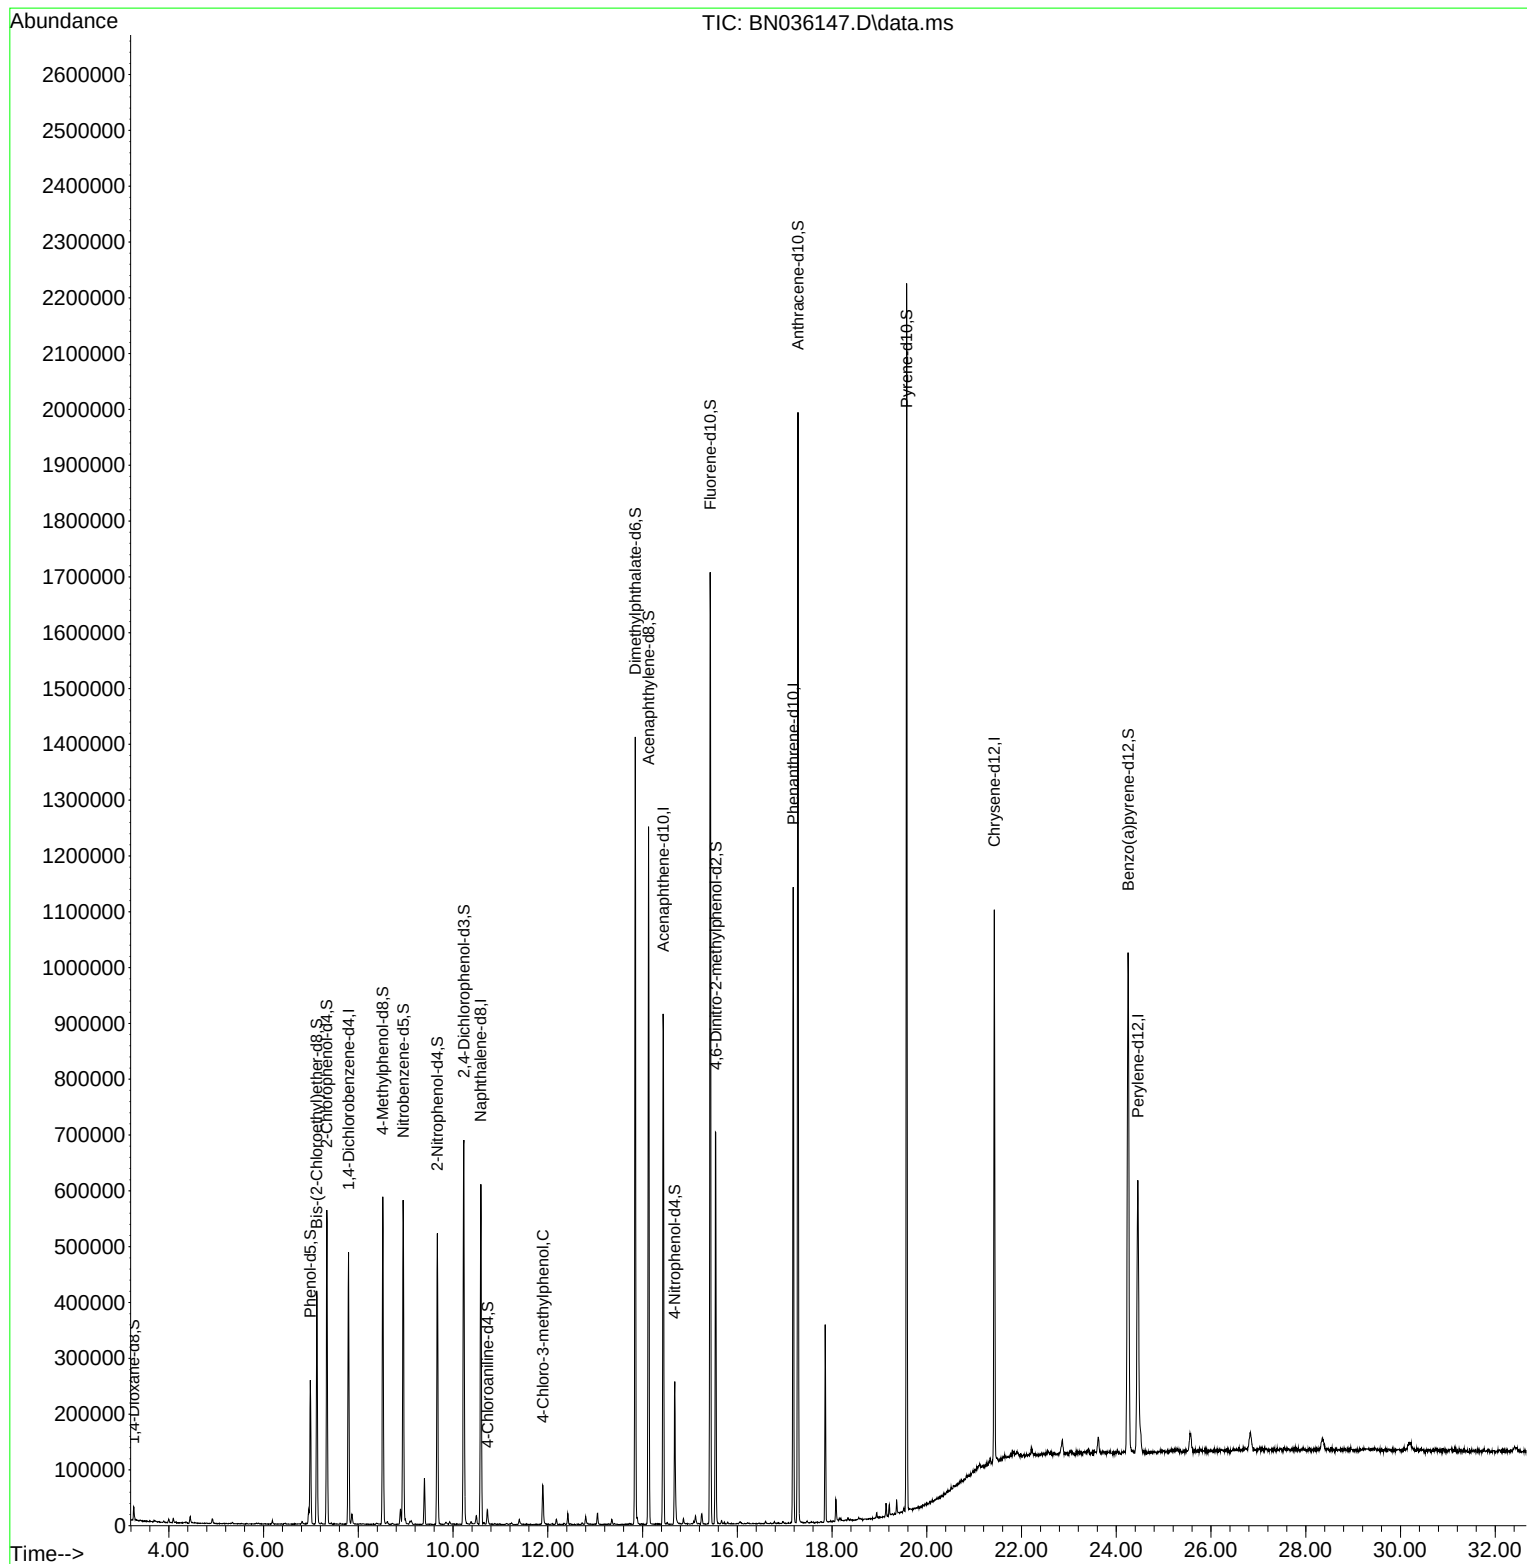

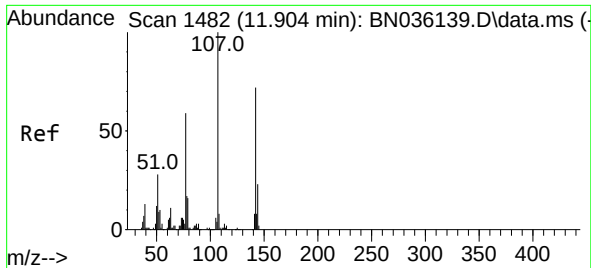

#35
 4-Chloro-3-methylphenol
 Concen: 1.478 ng/ul
 RT: 11.899 min Scan# 14
 Delta R.T. -0.006 min
 Lab File: BN036147.D
 Acq: 31 Jan 2025 00:16

Instrument :
 BNA_N
 ClientSampleId :
 A44W5

Tgt Ion:107 Resp: 12507
 Ion Ratio Lower Upper
 107 100
 144 20.9 17.5 26.3
 142 63.0 56.7 85.1

