

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013025\
 Data File : BN036140.D
 Acq On : 30 Jan 2025 19:42
 Operator : RC/JU
 Sample : PB166340BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK340

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN013025.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN036140.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	8	12	19	rVB	33279	44716	2.32%	0.186%
2	3.675	79	83	102	rBV	448642	664827	34.51%	2.765%
3	3.828	107	109	114	rVB3	1407	2191	0.11%	0.009%
4	3.993	132	137	142	rVB3	5529	8826	0.46%	0.037%
5	4.470	215	218	223	rBV3	2225	2687	0.14%	0.011%
6	6.993	636	647	658	rBV	506319	783798	40.69%	3.260%
7	7.122	662	669	679	rVV	345107	545066	28.29%	2.267%
8	7.340	699	706	716	rBV	505615	774641	40.21%	3.222%
9	7.793	777	783	790	rBV	408177	633418	32.88%	2.635%
10	7.875	792	797	798	rBV5	1361	2199	0.11%	0.009%
11	8.522	900	907	916	rBV	571389	904188	46.94%	3.761%
12	8.946	972	979	994	rBV	458331	747826	38.82%	3.111%
13	9.669	1094	1102	1114	rBV	404626	648311	33.65%	2.697%
14	10.228	1190	1197	1210	rBV	536574	897904	46.61%	3.735%
15	10.587	1251	1258	1266	rBV	483124	810849	42.09%	3.373%
16	10.722	1274	1281	1297	rBV	485149	849469	44.10%	3.533%
17	12.187	1525	1530	1536	rVB4	6505	11236	0.58%	0.047%
18	13.846	1805	1812	1821	rBV	829829	1146330	59.51%	4.768%
19	14.128	1853	1860	1870	rBV2	956130	1369637	71.10%	5.697%
20	14.434	1905	1912	1919	rBV	686101	991821	51.49%	4.125%
21	14.687	1948	1955	1975	rBV	348770	603267	31.32%	2.509%
22	15.263	2049	2053	2056	rBV3	2548	3096	0.16%	0.013%
23	15.428	2075	2081	2089	rBV	1147397	1597779	82.94%	6.646%
24	15.540	2095	2100	2108	rBV	408637	539551	28.01%	2.244%
25	15.669	2119	2122	2128	rBV4	3545	4793	0.25%	0.020%
26	16.545	2268	2271	2275	rBV4	1570	2744	0.14%	0.011%
27	16.969	2340	2343	2347	rVB4	2934	3909	0.20%	0.016%
28	17.181	2372	2379	2389	rBV2	864368	1183788	61.45%	4.924%
29	17.281	2389	2396	2407	rVV	1271630	1781400	92.47%	7.410%
30	17.463	2423	2427	2430	rVB6	2151	2515	0.13%	0.010%
31	17.857	2490	2494	2498	rVB5	2947	4411	0.23%	0.018%
32	18.098	2529	2535	2540	rBV6	7306	14766	0.77%	0.061%
33	19.139	2709	2712	2716	rBV3	13939	18308	0.95%	0.076%
34	19.210	2720	2724	2728	rBV3	13078	18122	0.94%	0.075%
35	19.369	2748	2751	2755	rBV4	6098	7019	0.36%	0.029%
36	19.433	2758	2762	2765	rBV	10978	14810	0.77%	0.062%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013025\
Data File : BN036140.D
Acq On : 30 Jan 2025 19:42
Operator : RC/JU
Sample : PB166340BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK340

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN013025.MA.M
Title : SVOA CALIBRATION

37	19.575	2780	2786	2792	rBV	1507984	1926078	99.98%	8.012%
38	21.427	3095	3101	3107	rBV	866208	1213693	63.00%	5.048%
39	24.251	3572	3581	3597	rVB	806214	1926375	100.00%	8.013%
40	24.457	3608	3616	3635	rVB2	491632	1334885	69.30%	5.552%




Sum of corrected areas: 24041249

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013025\
Data File : BN036140.D
Acq On : 30 Jan 2025 19:42
Operator : RC/JU
Sample : PB166340BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK340

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN013025.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

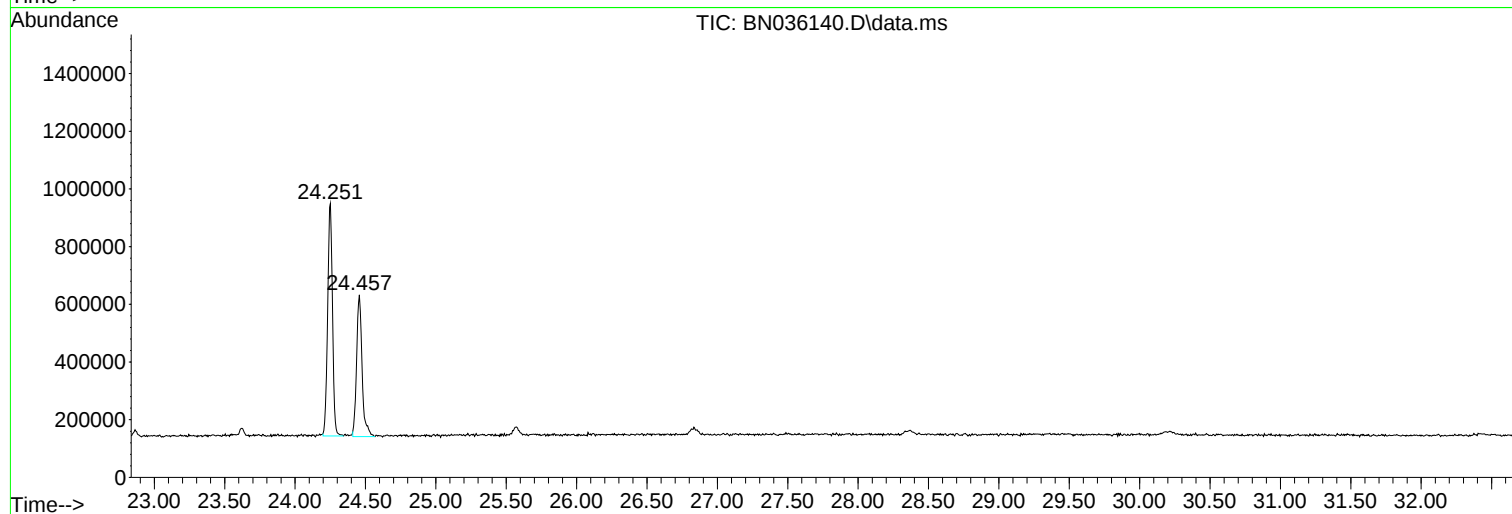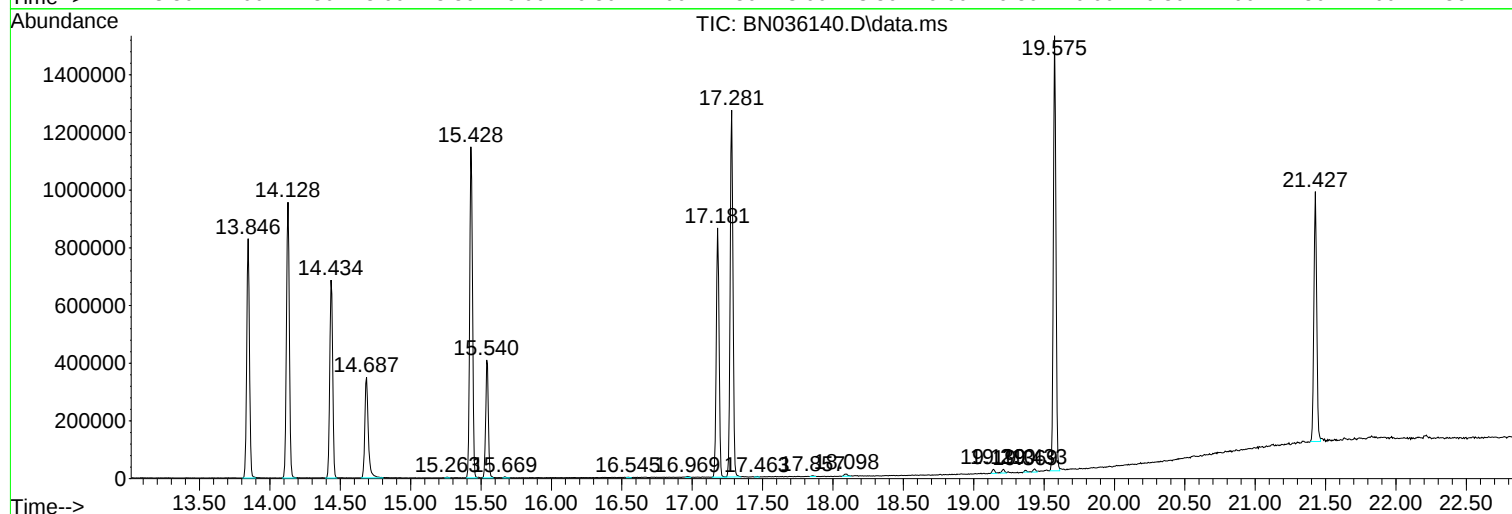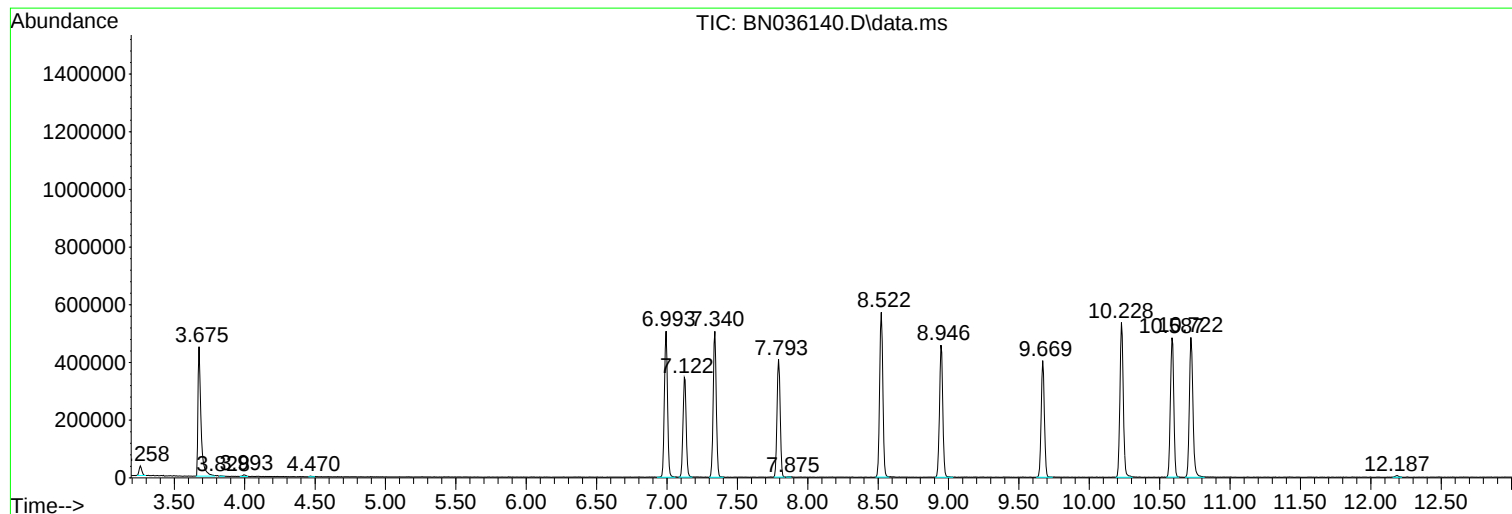

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013025\
Data File : BN036140.D
Acq On : 30 Jan 2025 19:42
Operator : RC/JU
Sample : PB166340BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK340

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN013025.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013025\
Data File : BN036140.D
Acq On : 30 Jan 2025 19:42
Operator : RC/JU
Sample : PB166340BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK340

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN013025.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc