

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013025\
 Data File : BN036141.D
 Acq On : 30 Jan 2025 20:21
 Operator : RC/JU
 Sample : PB166277TB 10X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SLEB277

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN013025.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN036141.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	8	12	20	rBV	48378	61248	3.38%	0.262%
2	3.370	28	31	33	rVB4	1732	2090	0.12%	0.009%
3	3.452	41	45	50	rBV5	1560	2325	0.13%	0.010%
4	3.675	79	83	99	rBV	448259	661081	36.44%	2.826%
5	3.999	132	138	143	rVB2	7084	11032	0.61%	0.047%
6	4.464	212	217	221	rBV4	3153	6402	0.35%	0.027%
7	6.993	635	647	657	rBV	504399	786284	43.34%	3.361%
8	7.122	663	669	678	rVB	351529	541058	29.82%	2.313%
9	7.340	699	706	713	rBV	511846	779160	42.94%	3.330%
10	7.793	777	783	791	rBV	406936	625621	34.48%	2.674%
11	8.522	900	907	917	rBV	570572	890884	49.10%	3.808%
12	8.946	971	979	988	rBV	436191	728049	40.13%	3.112%
13	9.405	1054	1057	1063	rVB3	1145	2071	0.11%	0.009%
14	9.669	1095	1102	1111	rBV	400540	634589	34.98%	2.712%
15	10.228	1188	1197	1217	rBV	539318	901108	49.67%	3.852%
16	10.587	1249	1258	1265	rBV	485122	781969	43.10%	3.342%
17	10.722	1274	1281	1295	rBV	481090	826151	45.53%	3.531%
18	11.416	1393	1399	1404	rBV2	1830	3351	0.18%	0.014%
19	12.187	1524	1530	1539	rVB5	6533	12885	0.71%	0.055%
20	13.846	1806	1812	1823	rBV	864182	1158838	63.87%	4.953%
21	14.128	1854	1860	1871	rVV2	922770	1350308	74.42%	5.772%
22	14.434	1906	1912	1920	rBV	671088	965120	53.19%	4.125%
23	14.681	1948	1954	1968	rBV	361258	612629	33.77%	2.619%
24	15.428	2075	2081	2089	rBV	1121205	1585707	87.40%	6.778%
25	15.540	2094	2100	2111	rBV	405732	543491	29.96%	2.323%
26	15.669	2116	2122	2125	rBV5	4212	4795	0.26%	0.020%
27	16.963	2339	2342	2347	rVB3	2696	3850	0.21%	0.016%
28	17.181	2373	2379	2386	rBV2	839113	1139683	62.82%	4.871%
29	17.281	2389	2396	2406	rBV	1305794	1768232	97.46%	7.558%
30	17.857	2491	2494	2499	rVB6	3858	5277	0.29%	0.023%
31	17.969	2510	2513	2516	rBV4	1564	1909	0.11%	0.008%
32	18.086	2529	2533	2542	rBV7	9535	17899	0.99%	0.077%
33	18.498	2600	2603	2604	rBV3	1878	2104	0.12%	0.009%
34	18.545	2607	2611	2612	rBV4	1886	2579	0.14%	0.011%
35	18.881	2666	2668	2671	rVB4	1978	1976	0.11%	0.008%
36	19.139	2708	2712	2717	rBV6	13411	21440	1.18%	0.092%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013025\
Data File : BN036141.D
Acq On : 30 Jan 2025 20:21
Operator : RC/JU
Sample : PB166277TB 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SLEB277

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN013025.MA.M
Title : SVOA CALIBRATION

37	19.210	2720	2724	2728	rBV3	12625	16640	0.92%	0.071%
38	19.369	2747	2751	2756	rBV6	7916	11910	0.66%	0.051%
39	19.428	2758	2761	2764	rBV	7405	8374	0.46%	0.036%
40	19.516	2774	2776	2778	rVB3	6412	4702	0.26%	0.020%
41	19.575	2780	2786	2792	rBV	1372956	1814329	100.00%	7.755%
42	21.427	3095	3101	3107	rBV	758501	1105546	60.93%	4.725%
43	24.251	3572	3581	3591	rVB	734080	1811886	99.87%	7.744%
44	24.451	3608	3615	3629	rVB2	450064	1179470	65.01%	5.041%




Sum of corrected areas: 23396052

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013025\
Data File : BN036141.D
Acq On : 30 Jan 2025 20:21
Operator : RC/JU
Sample : PB166277TB 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SLEB277

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN013025.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

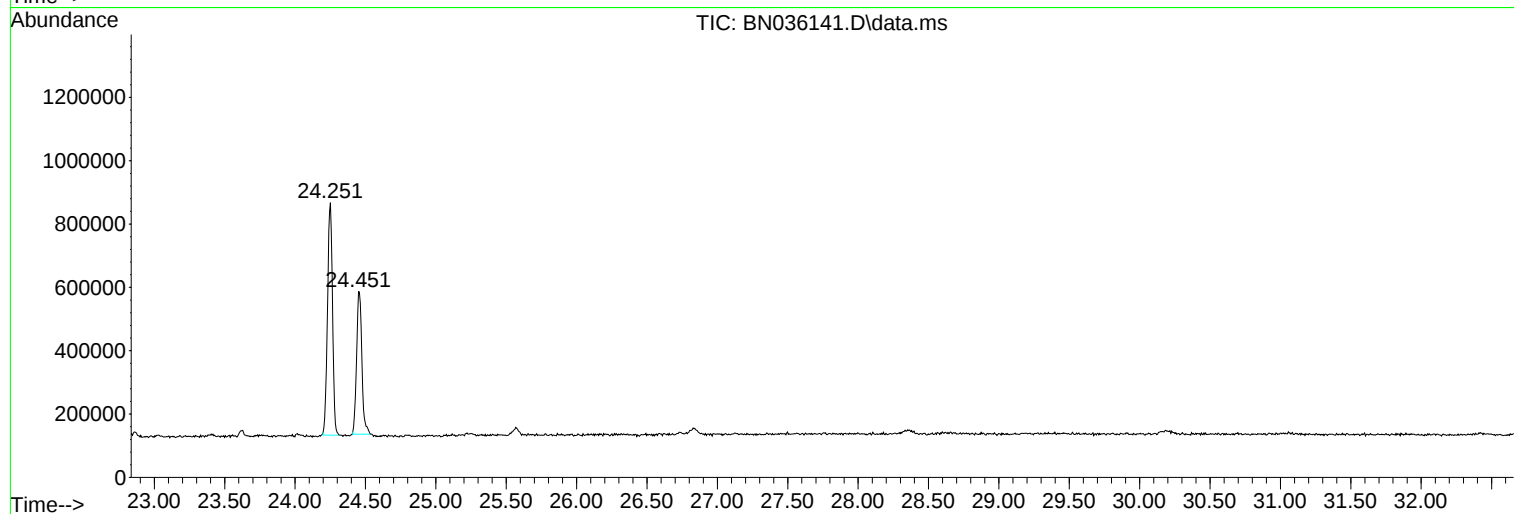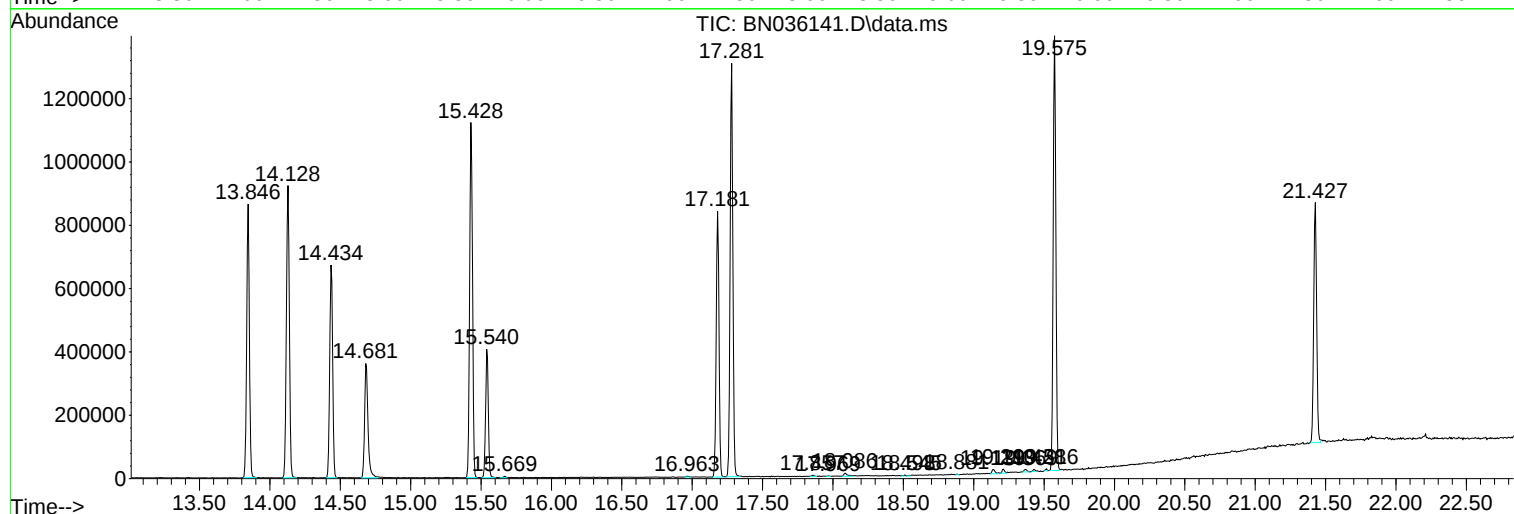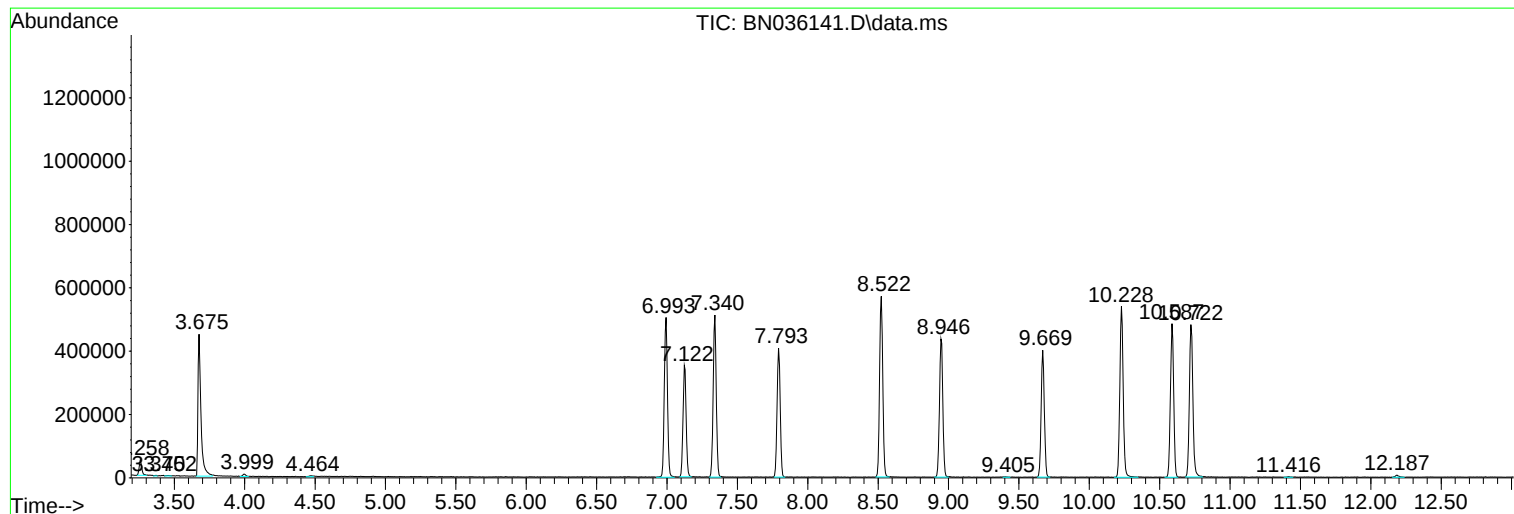

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013025\
Data File : BN036141.D
Acq On : 30 Jan 2025 20:21
Operator : RC/JU
Sample : PB166277TB 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SLEB277

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN013025.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013025\
Data File : BN036141.D
Acq On : 30 Jan 2025 20:21
Operator : RC/JU
Sample : PB166277TB 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SLEB277

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN013025.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc