

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013025\
 Data File : BN036155.D
 Acq On : 31 Jan 2025 06:08
 Operator : RC/JU
 Sample : PB166370BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK370

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN013025.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN036155.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	7	12	22	rBV	31613	47450	1.94%	0.174%
2	3.670	79	82	106	rBV	449376	717049	29.37%	2.628%
3	3.993	132	137	143	rVB2	4688	8414	0.34%	0.031%
4	6.987	639	646	653	rBV	543046	852409	34.91%	3.124%
5	7.122	661	669	679	rBV	382560	582131	23.84%	2.134%
6	7.334	697	705	713	rBV	551620	836180	34.25%	3.065%
7	7.793	776	783	791	rBV	448687	708641	29.03%	2.597%
8	8.516	899	906	921	rBV	639092	1005738	41.19%	3.686%
9	8.946	972	979	987	rBV	502838	786604	32.22%	2.883%
10	9.669	1094	1102	1111	rBV	429081	685951	28.10%	2.514%
11	10.222	1189	1196	1212	rBV	621942	1015617	41.60%	3.722%
12	10.587	1250	1258	1265	rBV	567876	924693	37.87%	3.389%
13	10.722	1273	1281	1296	rBV	532827	942248	38.59%	3.453%
14	12.181	1524	1529	1537	rBV4	6291	11422	0.47%	0.042%
15	13.846	1805	1812	1821	rBV	1062426	1430789	58.60%	5.244%
16	14.128	1853	1860	1873	rBV	1116776	1598212	65.46%	5.857%
17	14.434	1905	1912	1921	rBV	878702	1248779	51.15%	4.577%
18	14.669	1945	1952	1971	rBV	450486	735015	30.11%	2.694%
19	15.428	2074	2081	2088	rBV	1403587	1946790	79.74%	7.135%
20	15.540	2094	2100	2111	rBV	513067	667458	27.34%	2.446%
21	15.669	2117	2122	2126	rBV2	4484	5877	0.24%	0.022%
22	16.781	2305	2311	2314	rBV5	1810	3037	0.12%	0.011%
23	16.963	2336	2342	2347	rBV3	3568	6333	0.26%	0.023%
24	17.181	2373	2379	2388	rBV	1142811	1575132	64.52%	5.773%
25	17.281	2389	2396	2406	rVV	1570902	2234173	91.51%	8.188%
26	17.734	2469	2473	2475	rBV3	1441	2464	0.10%	0.009%
27	17.822	2486	2488	2491	rBV4	1999	2568	0.11%	0.009%
28	17.857	2491	2494	2497	rVB4	3078	3165	0.13%	0.012%
29	18.086	2530	2533	2535	rBV4	3032	2984	0.12%	0.011%
30	19.139	2708	2712	2715	rBV2	16577	23075	0.95%	0.085%
31	19.210	2720	2724	2729	rVV2	14542	21014	0.86%	0.077%
32	19.575	2780	2786	2793	rBV	1832601	2441465	100.00%	8.948%
33	21.427	3095	3101	3109	rBV	951441	1355557	55.52%	4.968%
34	24.251	3573	3581	3591	rVB	691641	1626884	66.64%	5.963%
35	24.457	3608	3616	3632	rVB	477669	1229744	50.37%	4.507%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013025\
Data File : BN036155.D
Acq On : 31 Jan 2025 06:08
Operator : RC/JU
Sample : PB166370BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK370

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN013025.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 27285062

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013025\
Data File : BN036155.D
Acq On : 31 Jan 2025 06:08
Operator : RC/JU
Sample : PB166370BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK370

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN013025.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

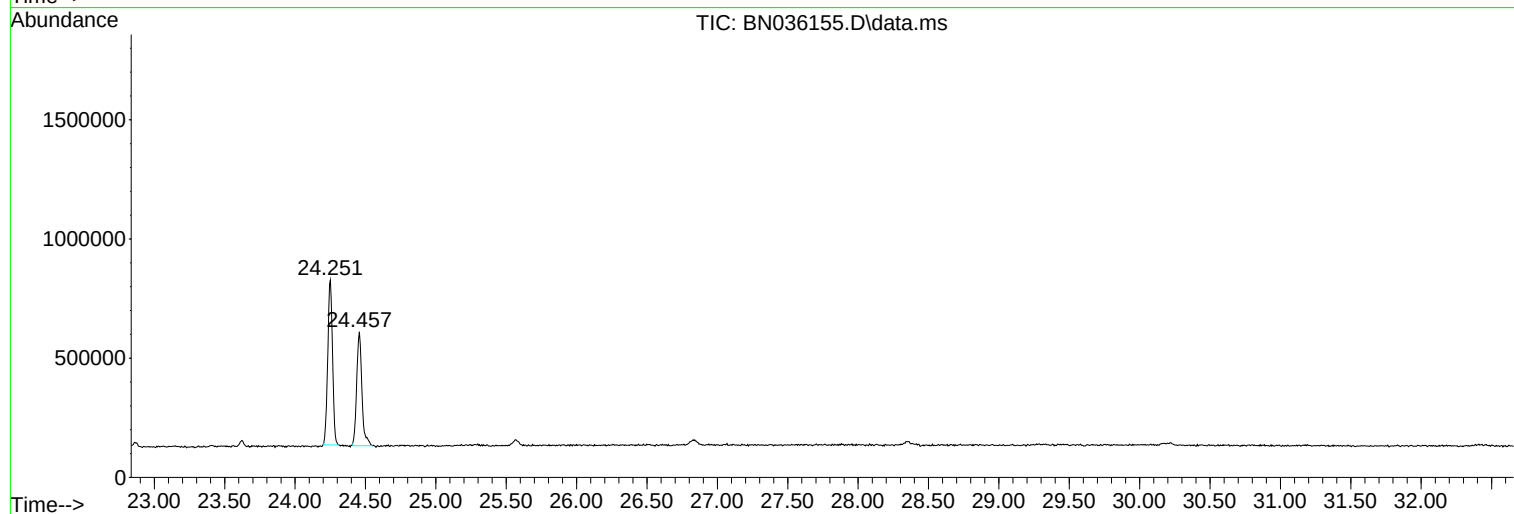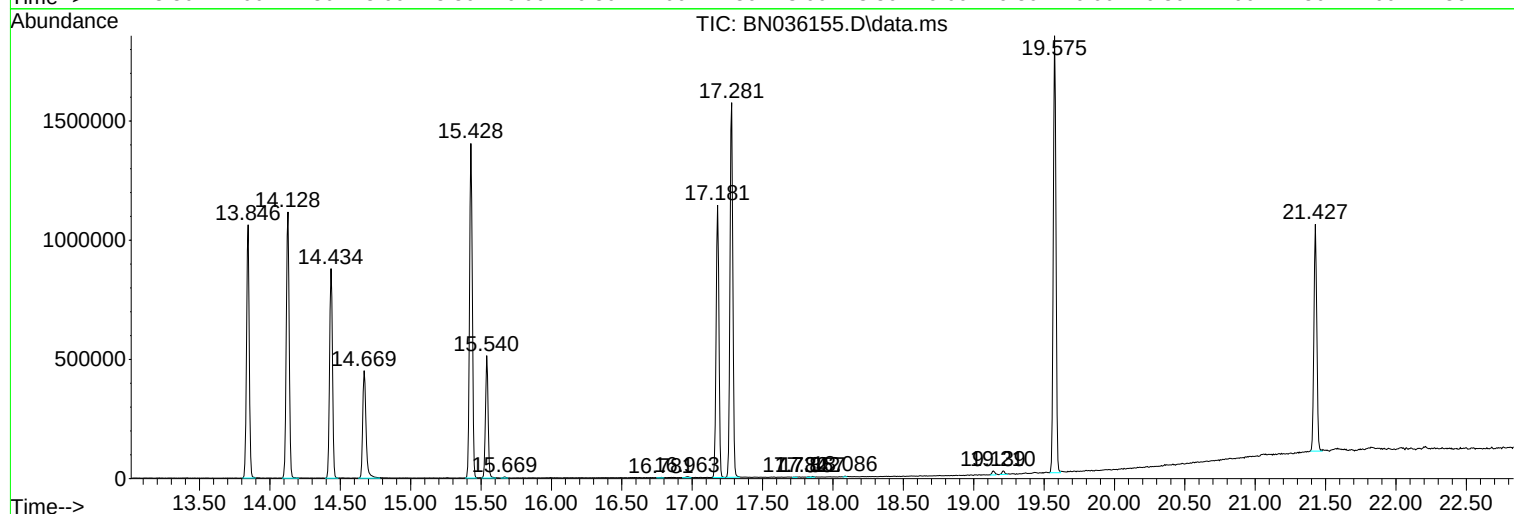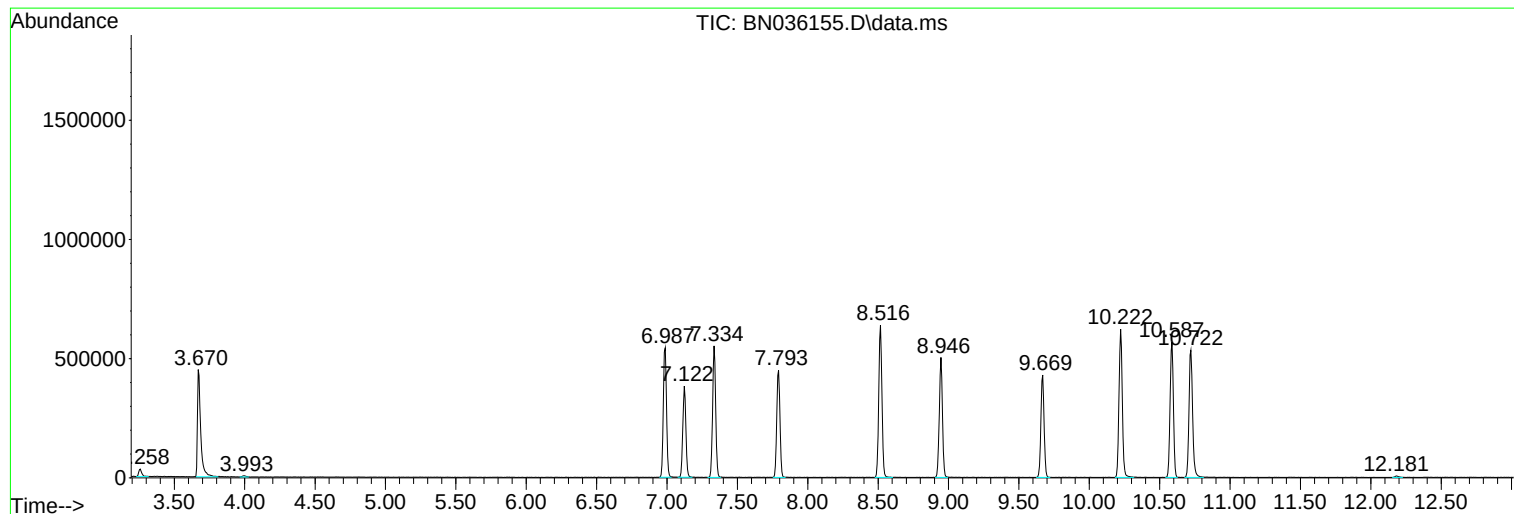

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013025\
Data File : BN036155.D
Acq On : 31 Jan 2025 06:08
Operator : RC/JU
Sample : PB166370BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK370

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN013025.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013025\
Data File : BN036155.D
Acq On : 31 Jan 2025 06:08
Operator : RC/JU
Sample : PB166370BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK370

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN013025.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
