
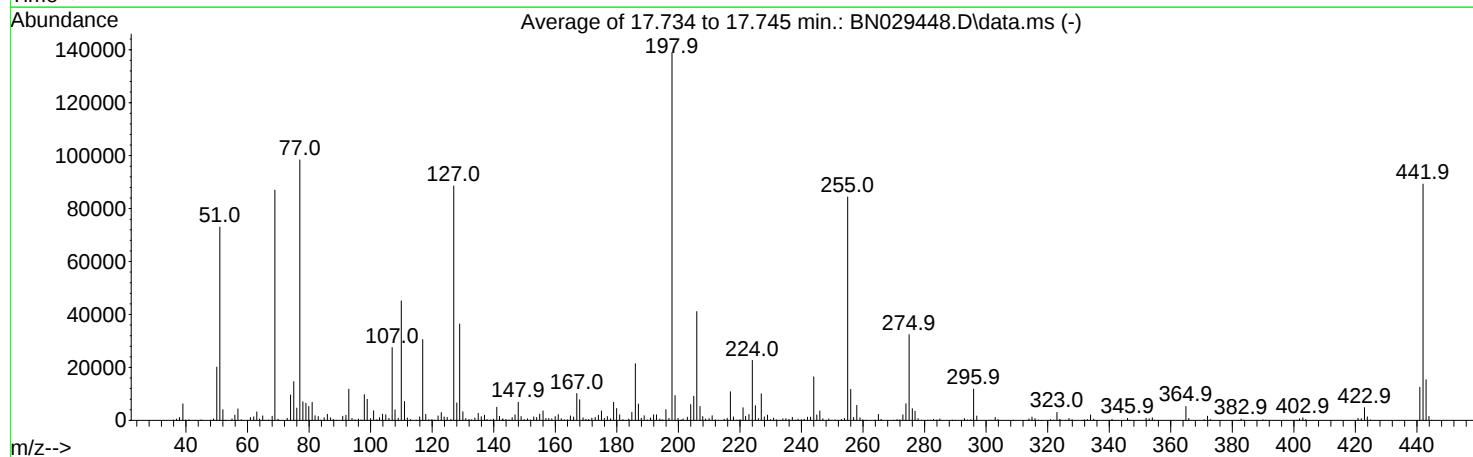


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013124\
Data File : BN029448.D
Acq On : 31 Jan 2024 13:47
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN012924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 01 01:51:59 2024

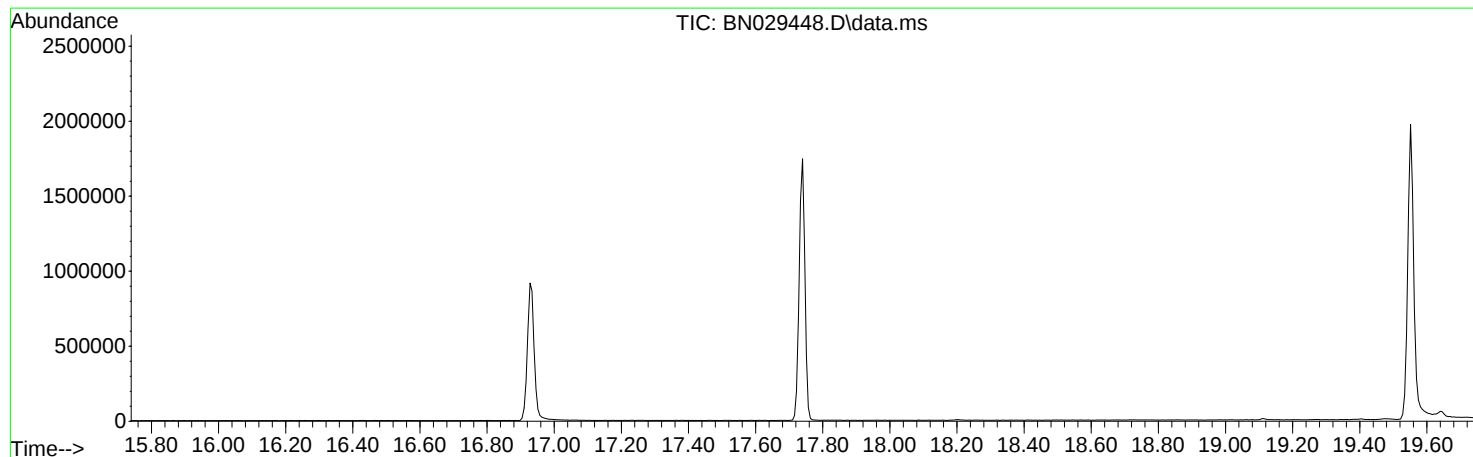




AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2483

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	52.5	72992	PASS
68	69	0.00	2	1.8	1573	PASS
69	198	0.00	100	62.6	86976	PASS
70	69	0.00	2	0.5	477	PASS
127	198	10	80	63.7	88523	PASS
197	198	0.00	2	0.6	818	PASS
198	198	100	100	100.0	138949	PASS
199	198	5	9	6.7	9379	PASS
275	198	10	60	23.3	32411	PASS
365	198	1	100	3.8	5269	PASS
441	198	0.01	100	9.0	12506	PASS
442	442	50	100	100.0	89280	PASS
443	442	15	24	17.2	15362	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013124\
Data File : BN029448.D
Acq On : 31 Jan 2024 13:47
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 01 03:24:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 03:24:38 2024
Response via : Initial Calibration

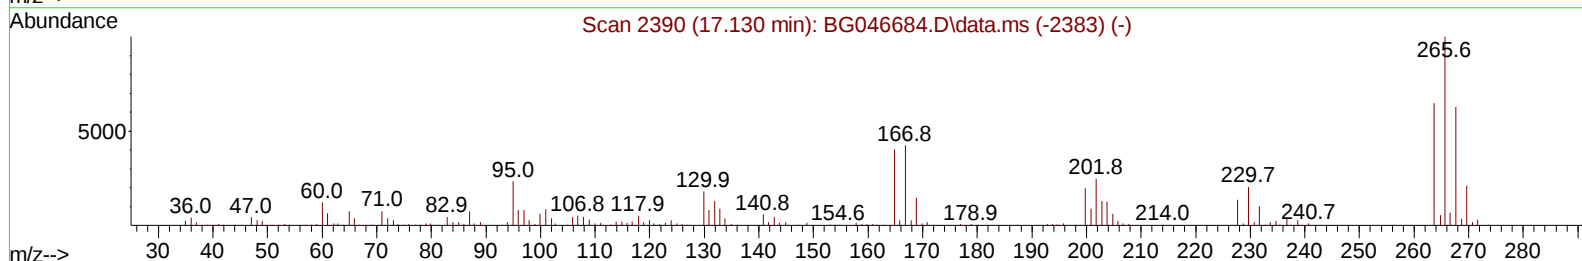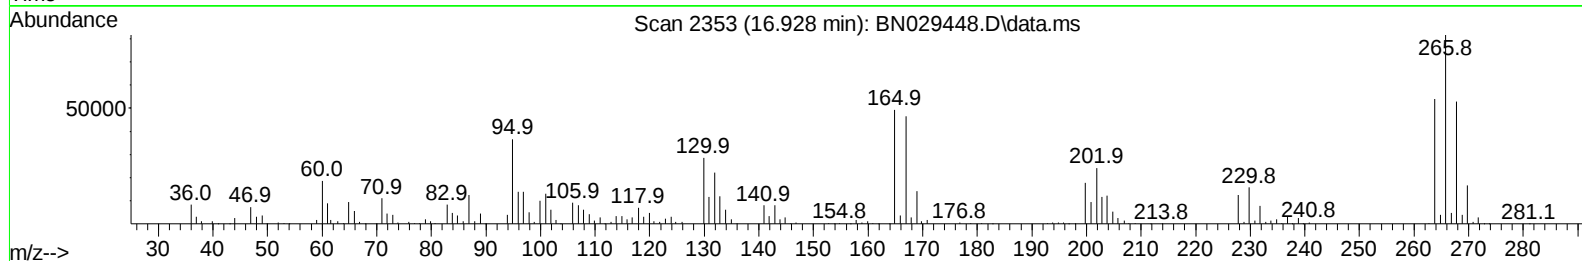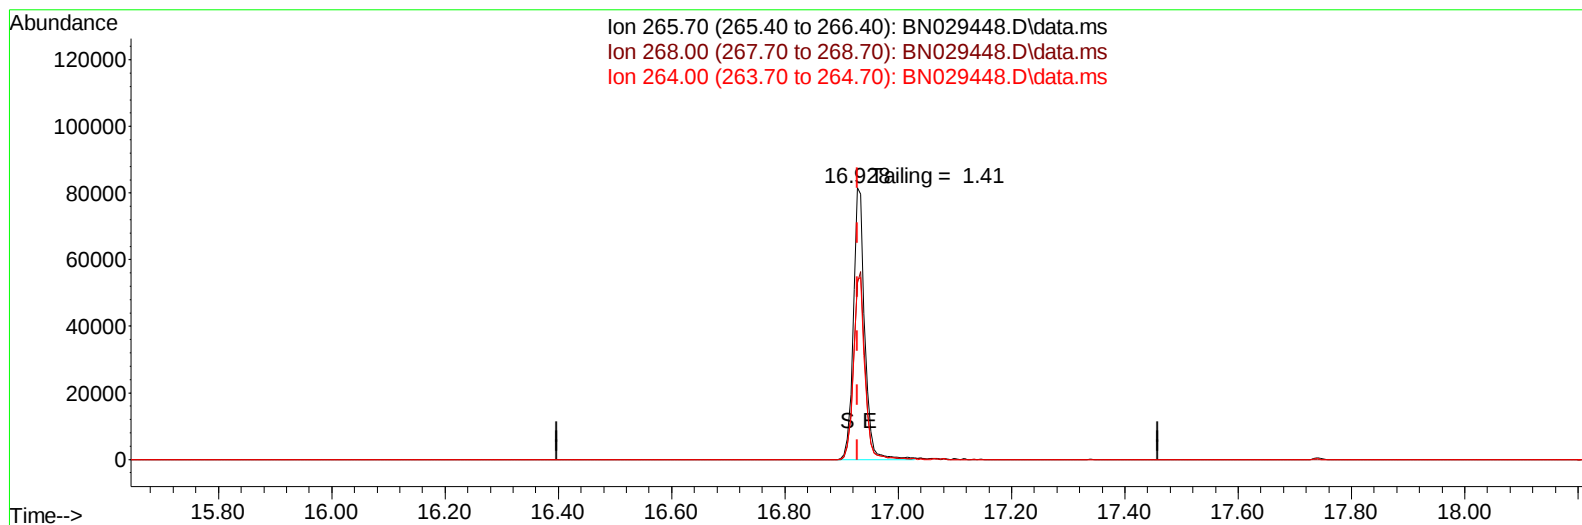

TIC: BN029448.D\data.ms

(70) Pentachlorophenol (C)

16.928min (0.000) 12358.50 ng




response 114153

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.97
264.00	61.60	66.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013124\
Data File : BN029448.D
Acq On : 31 Jan 2024 13:47
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 01 03:24:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 03:24:38 2024
Response via : Initial Calibration

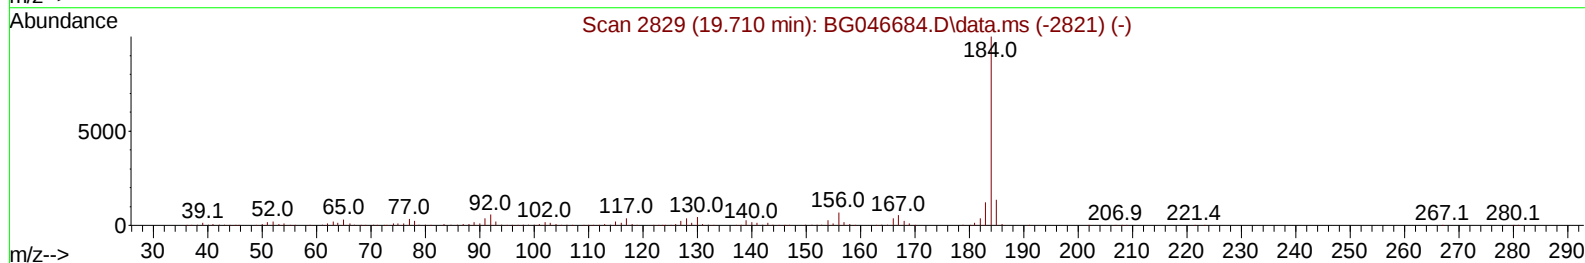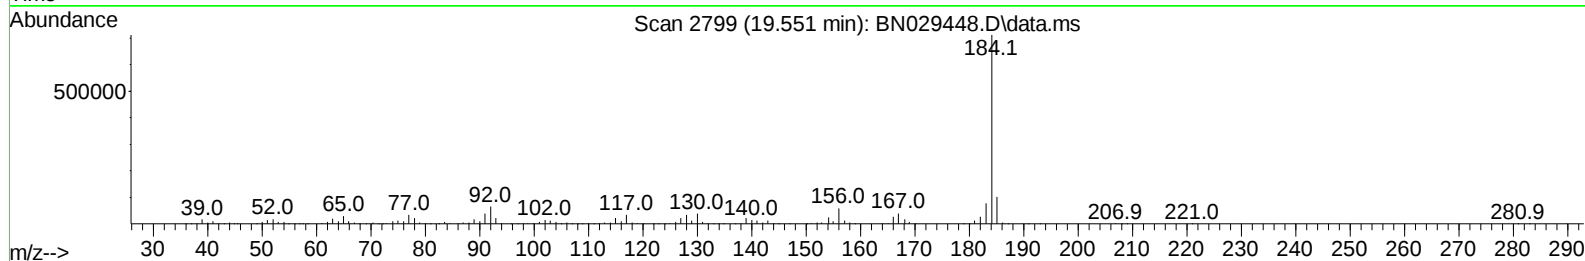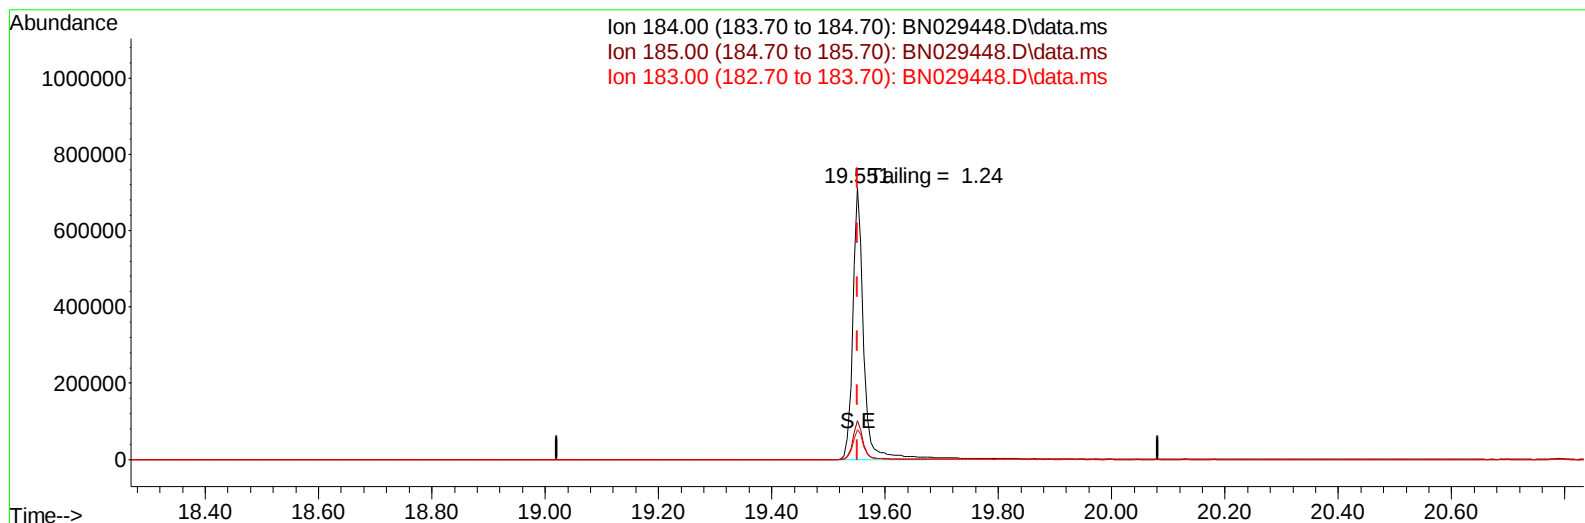

TIC: BN029448.D\data.ms

(77) Benzidine

19.551min (0.000) 0.00 ng

response 938301

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.39
183.00	13.20	10.93
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/31/2024	BNA_N	<u>BN029448.D</u>
Compound Name	Response	Retention Time
DDT	464436	20.792
DDD	4707	20.398
DDE	0	20.004
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4707	469143	1.00

Instrument :
BNA_N
ClientSampleId :
DFTPP