
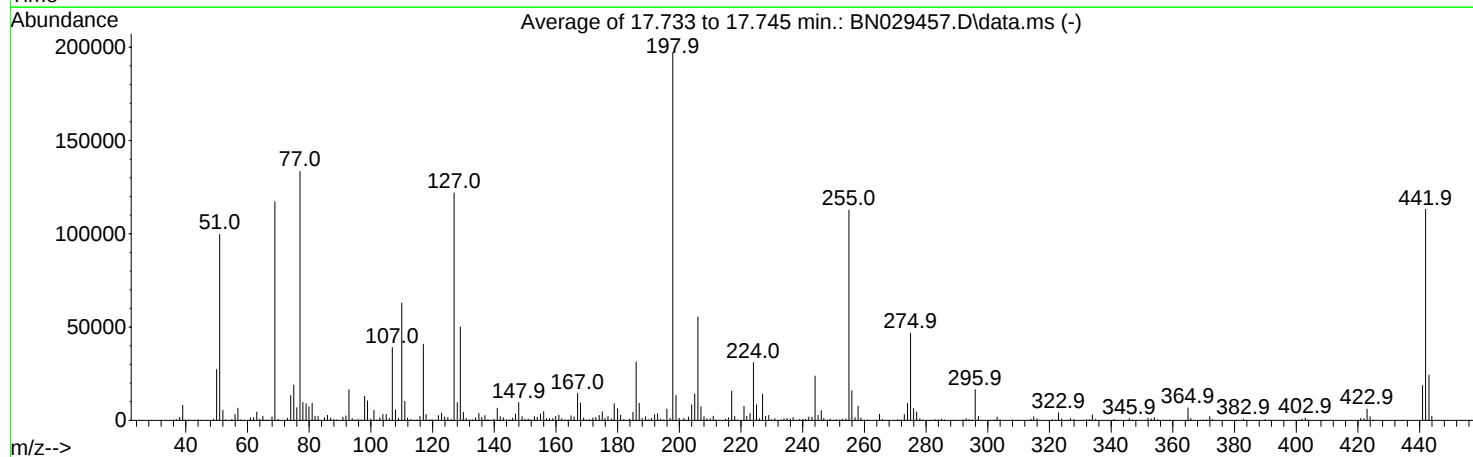


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013124\
Data File : BN029457.D
Acq On : 31 Jan 2024 20:35
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN012924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 01 01:51:59 2024

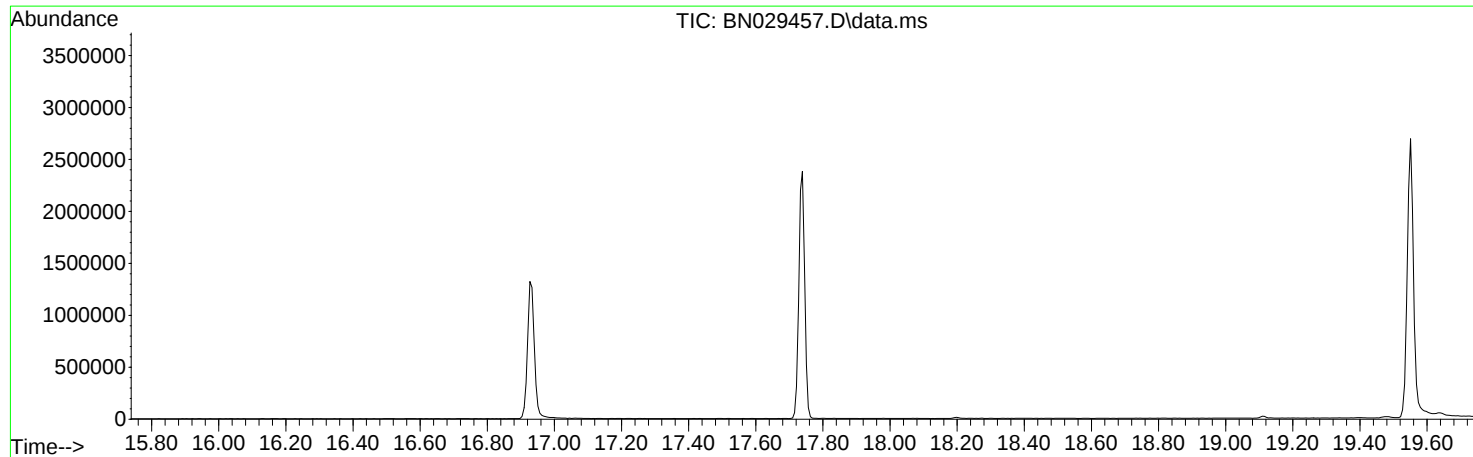




AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.6	99691	PASS
68	69	0.00	2	1.6	1882	PASS
69	198	0.00	100	59.4	117160	PASS
70	69	0.00	2	0.5	604	PASS
127	198	10	80	61.8	121936	PASS
197	198	0.00	2	0.6	1095	PASS
198	198	100	100	100.0	197163	PASS
199	198	5	9	6.8	13398	PASS
275	198	10	60	23.7	46725	PASS
365	198	1	100	3.4	6725	PASS
441	198	0.01	100	9.5	18737	PASS
442	442	50	100	100.0	113099	PASS
443	442	15	24	21.4	24237	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013124\
Data File : BN029457.D
Acq On : 31 Jan 2024 20:35
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 01 03:26:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 03:26:31 2024
Response via : Initial Calibration

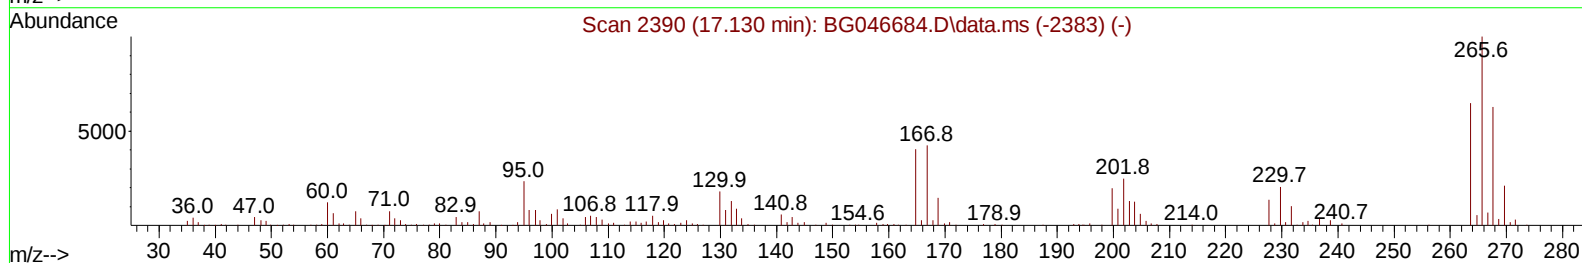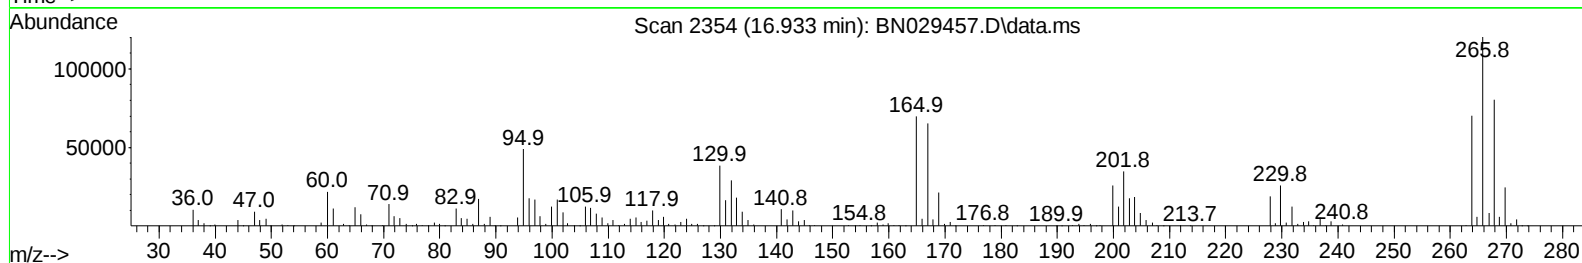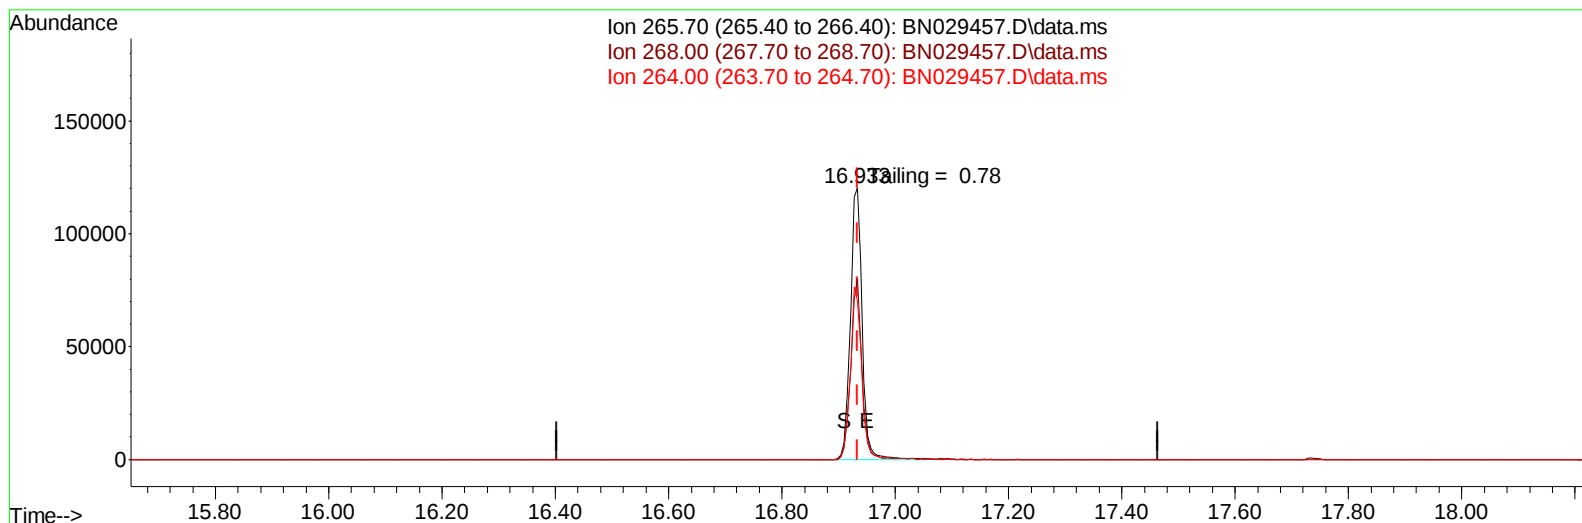

TIC: BN029457.D\data.ms

(70) Pentachlorophenol (C)

16.933min (0.000) 16134.63 ng




response 173850

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.70
264.00	61.60	58.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013124\
Data File : BN029457.D
Acq On : 31 Jan 2024 20:35
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 01 03:26:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 03:26:31 2024
Response via : Initial Calibration

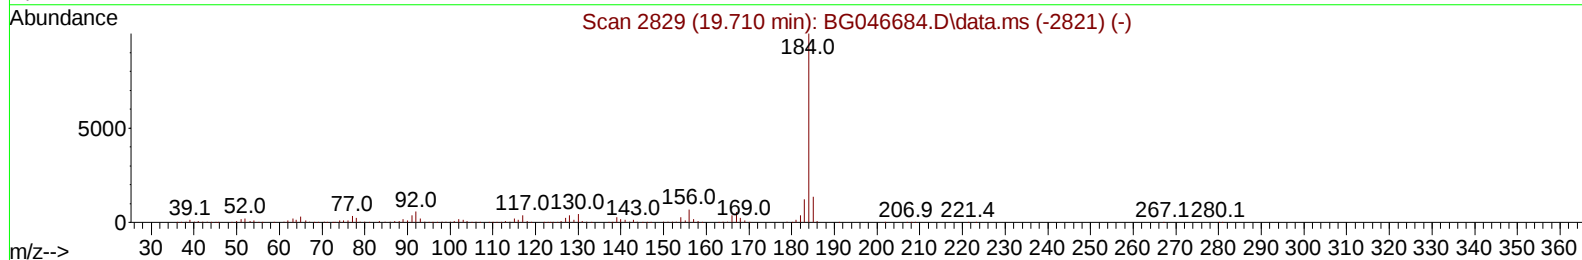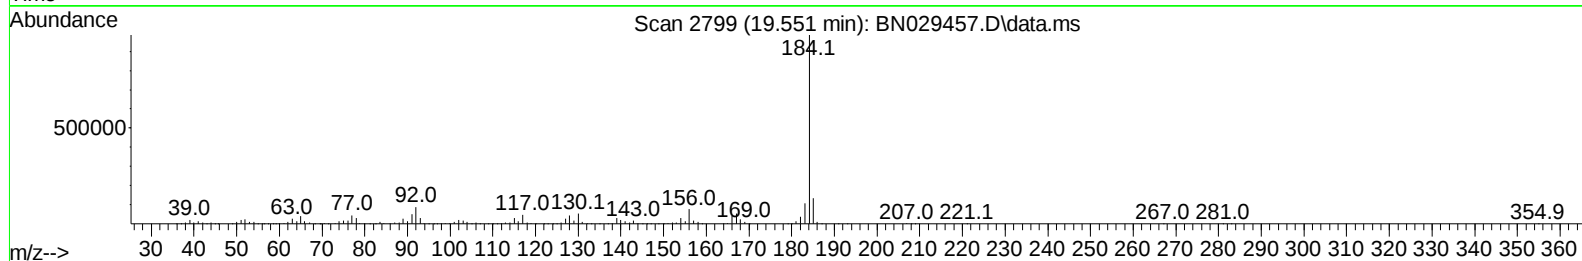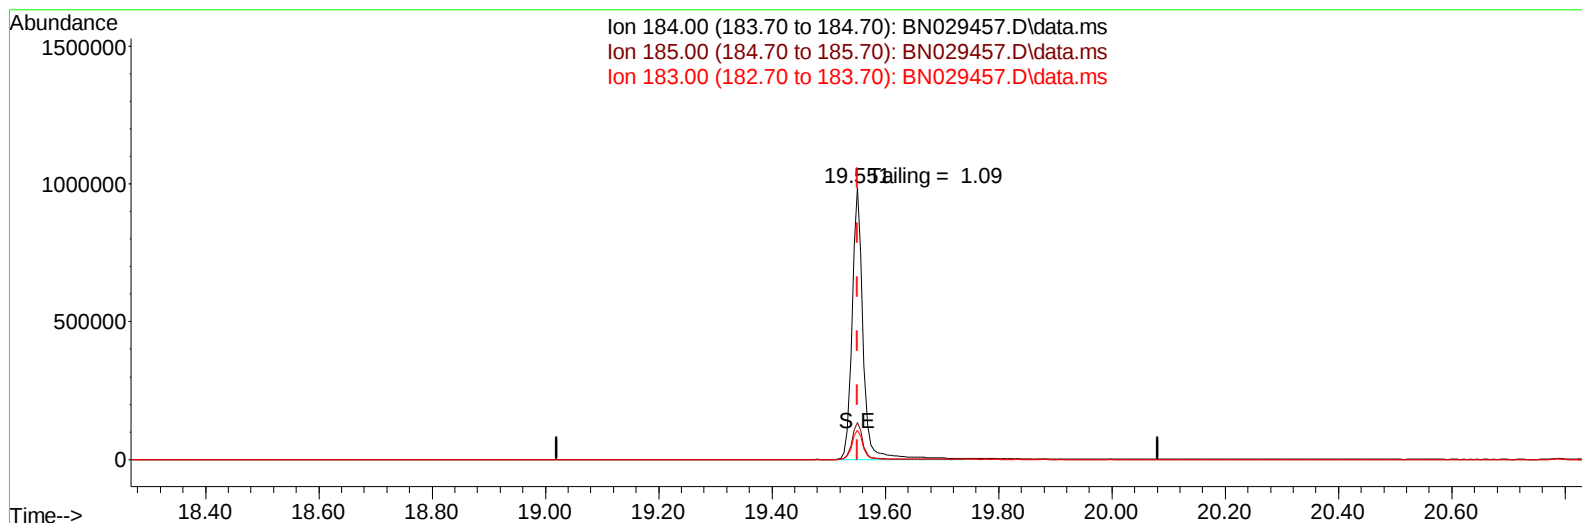

TIC: BN029457.D\data.ms

(77) Benzidine

19.551min (0.000) 0.00 ng

response 1347292

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.47
183.00	13.20	10.83
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/31/2024	BNA_N	<u>BN029457.D</u>
Compound Name	Response	Retention Time
DDT	659728	20.786
DDD	6664	20.392
DDE	0	20.004
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6664	666392	1.00

Instrument :
BNA_N
ClientSampleId :
DFTPP