




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013125\
Data File : BN036184.D
Acq On : 01 Feb 2025 00:52
Operator : RC/JU
Sample : Q1224-16
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A6323

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/03/2025
Supervised By :mohammad ahmed 02/04/2025

Quant Time: Feb 03 08:53:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 21 23:52:22 2025
Response via : Initial Calibration

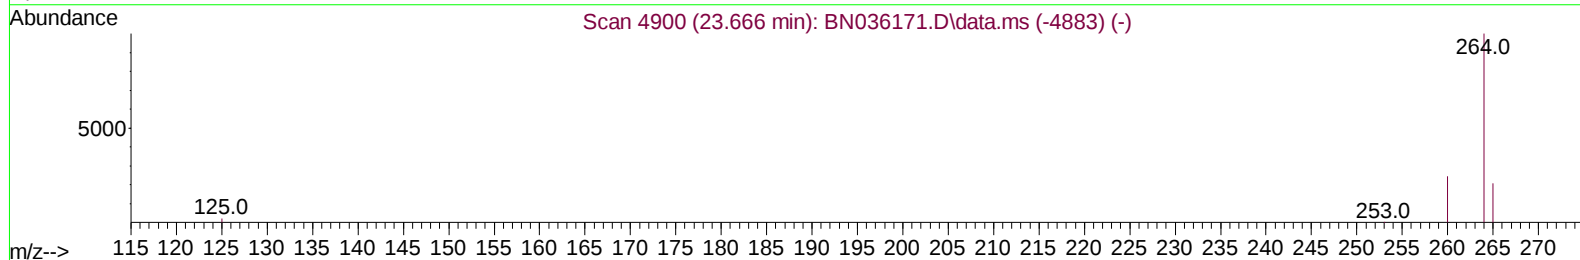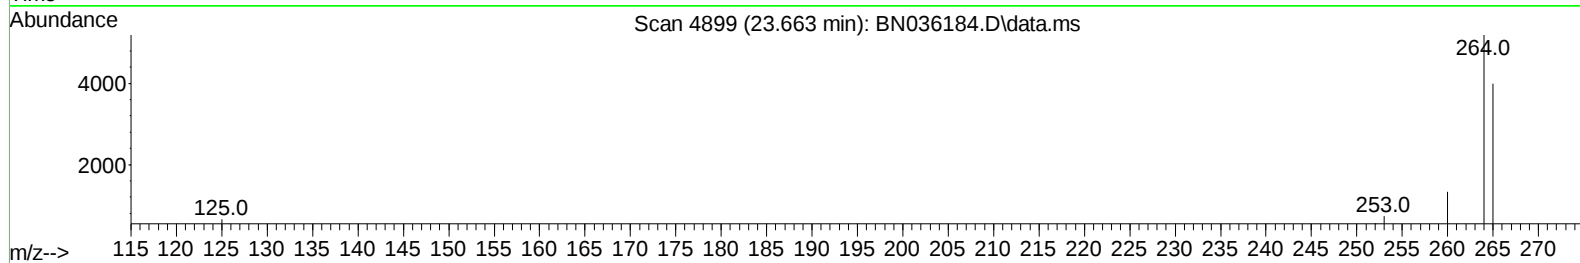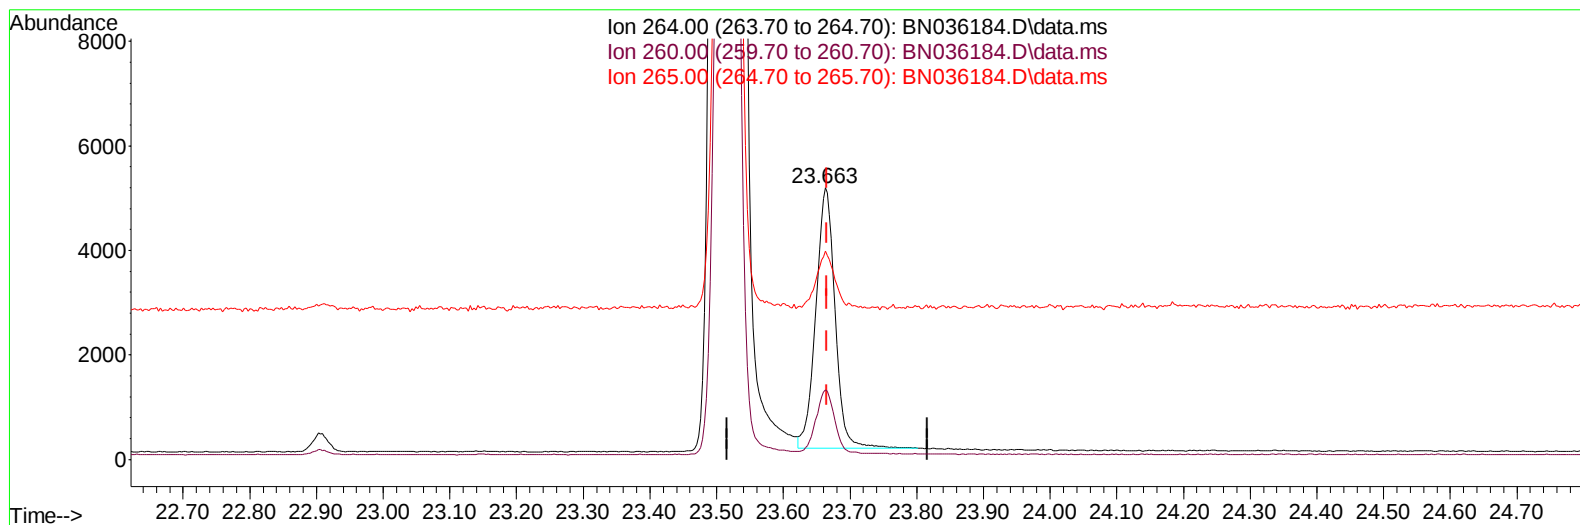

TIC: BN036184.D\data.ms

(23) Perylene-d12 (I)

23.663min (-0.003) 0.40 ng/u1

response 9921

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	25.64
265.00	53.20	76.82#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013125\
Data File : BN036184.D
Acq On : 01 Feb 2025 00:52
Operator : RC/JU
Sample : Q1224-16
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A6323

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/03/2025
Supervised By :mohammad ahmed 02/04/2025

Quant Time: Feb 03 08:53:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 21 23:52:22 2025
Response via : Initial Calibration

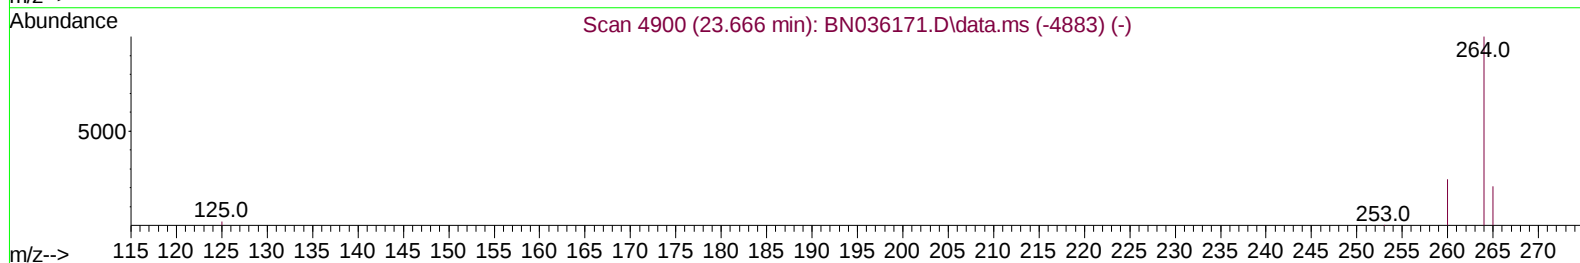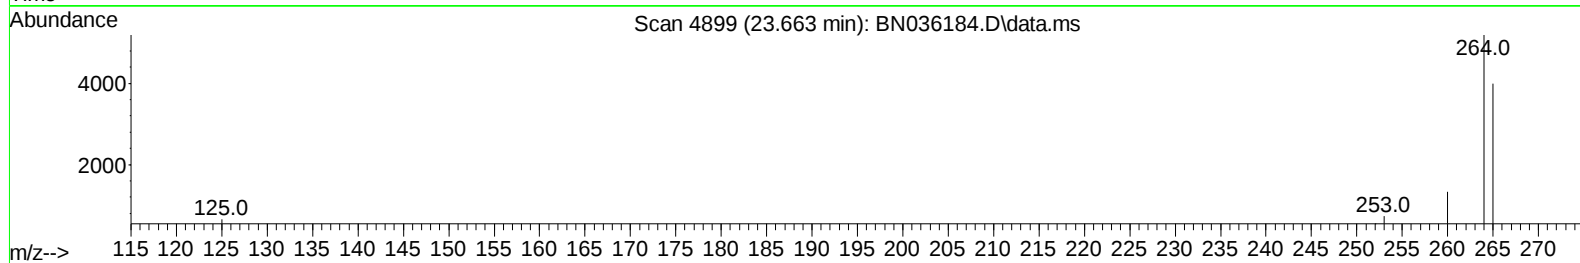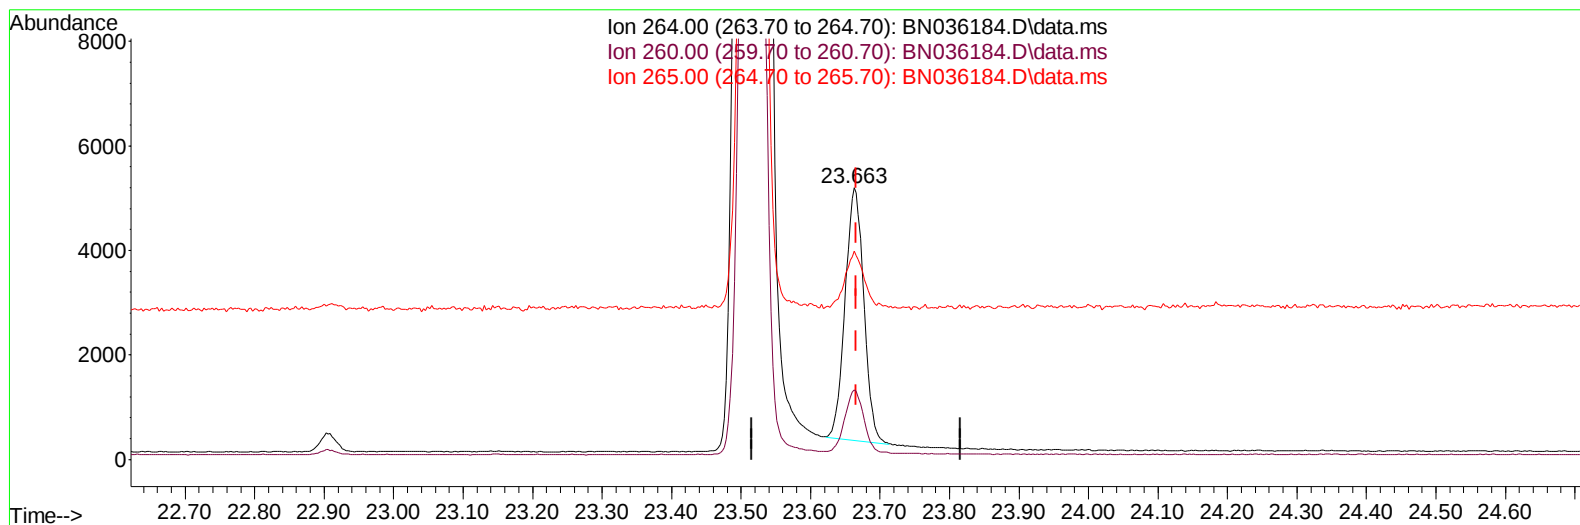

TIC: BN036184.D\data.ms

(23) Perylene-d12 (I)

23.663min (-0.003) 0.40 ng/u1 m

response 9013

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	25.64
265.00	53.20	76.82#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013125\
 Data File : BN036184.D
 Acq On : 01 Feb 2025 00:52
 Operator : RC/JU
 Sample : Q1224-16
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A6323

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/03/2025
 Supervised By :mohammad ahmed 02/04/2025

Quant Time: Feb 03 08:53:07 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 21 23:52:22 2025
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.795	152		2342	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.583	136		6212	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.436	164		3968	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.183	188		8763	0.400	ng/ul	0.00
17) Chrysene-d12	21.368	240		9089	0.400	ng/ul	0.00
23) Perylene-d12	23.663	264		9013m	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.259	96		9811	3.826	ng/ul	-0.02
6) 2-Methylnaphthalene-d10	12.178	152		1815	0.231	ng/ul	-0.02
18) Fluoranthene-d10	19.210	212		3778	0.151	ng/ul	0.00
Target Compounds							
15) Phenanthrene	17.221	178		989	0.039	ng/ul#	Qvalue 72

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013125\
Data File : BN036184.D
Acq On : 01 Feb 2025 00:52
Operator : RC/JU
Sample : Q1224-16
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A6323

Manual IntegrationsAPPROVED

Quant Time: Feb 03 08:53:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 21 23:52:22 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/03/2025
Supervised By :mohammad ahmed 02/04/2025

