




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013125\
Data File : BN036217.D
Acq On : 01 Feb 2025 21:16
Operator : RC/JU
Sample : Q1248-15
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A6346

Manual IntegrationsAPPROVED

Quant Time: Feb 03 12:06:08 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 21 23:52:22 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/03/2025
Supervised By :mohammad ahmed 02/04/2025

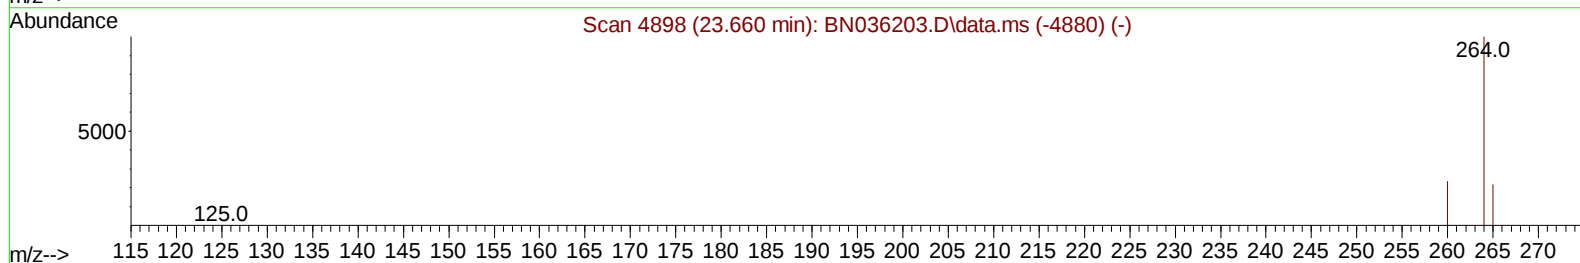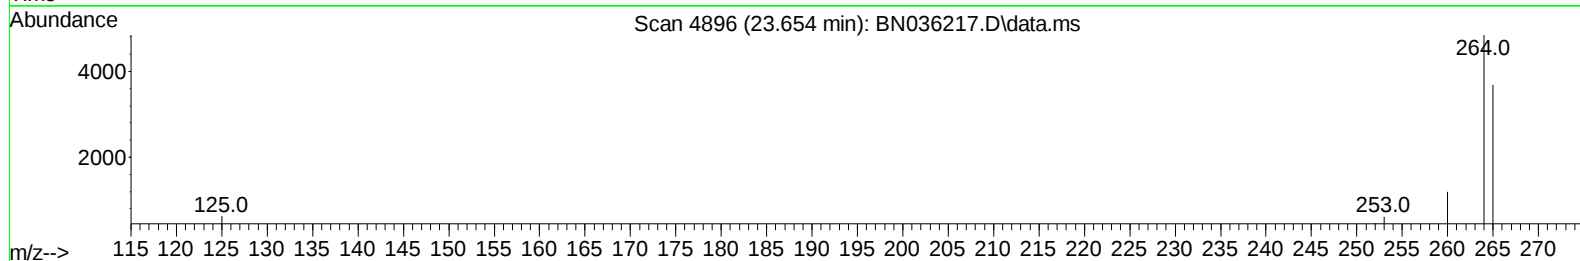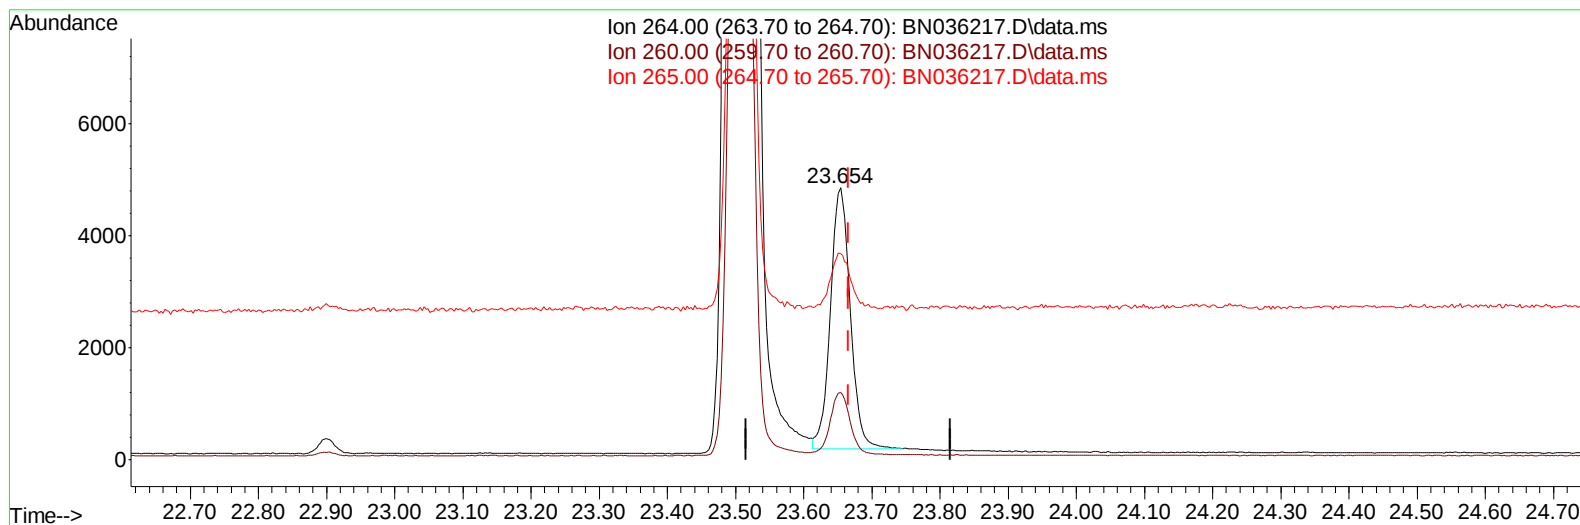

TIC: BN036217.D\data.ms

(23) Perylene-d12 (I)

23.654min (-0.012) 0.40 ng/u1

response 9463

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	24.72
265.00	53.20	75.88#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013125\
Data File : BN036217.D
Acq On : 01 Feb 2025 21:16
Operator : RC/JU
Sample : Q1248-15
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A6346

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/03/2025
Supervised By :mohammad ahmed 02/04/2025

Quant Time: Feb 03 12:06:08 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 21 23:52:22 2025
Response via : Initial Calibration

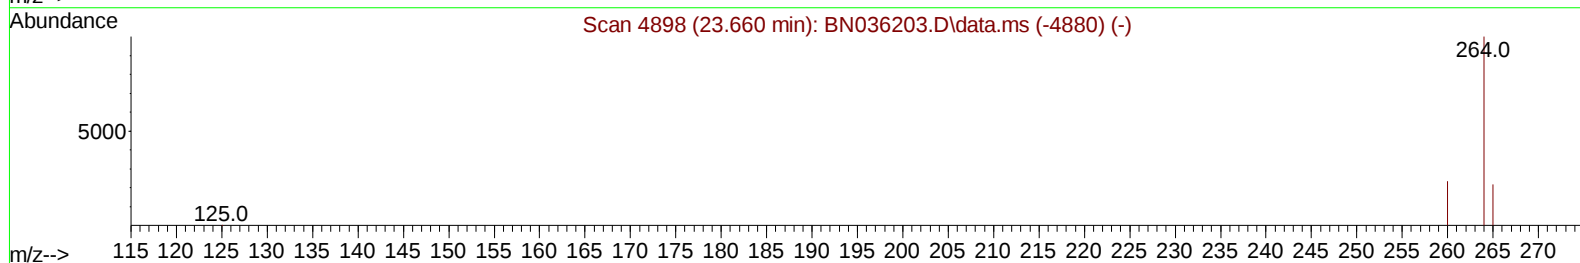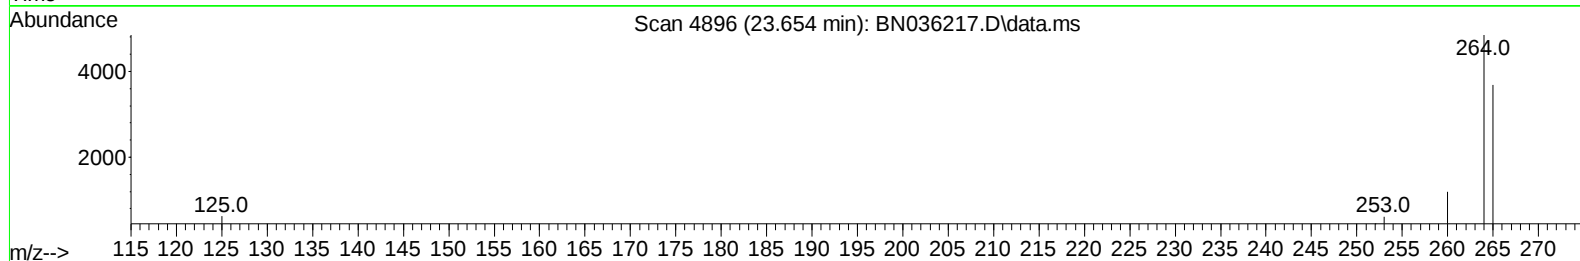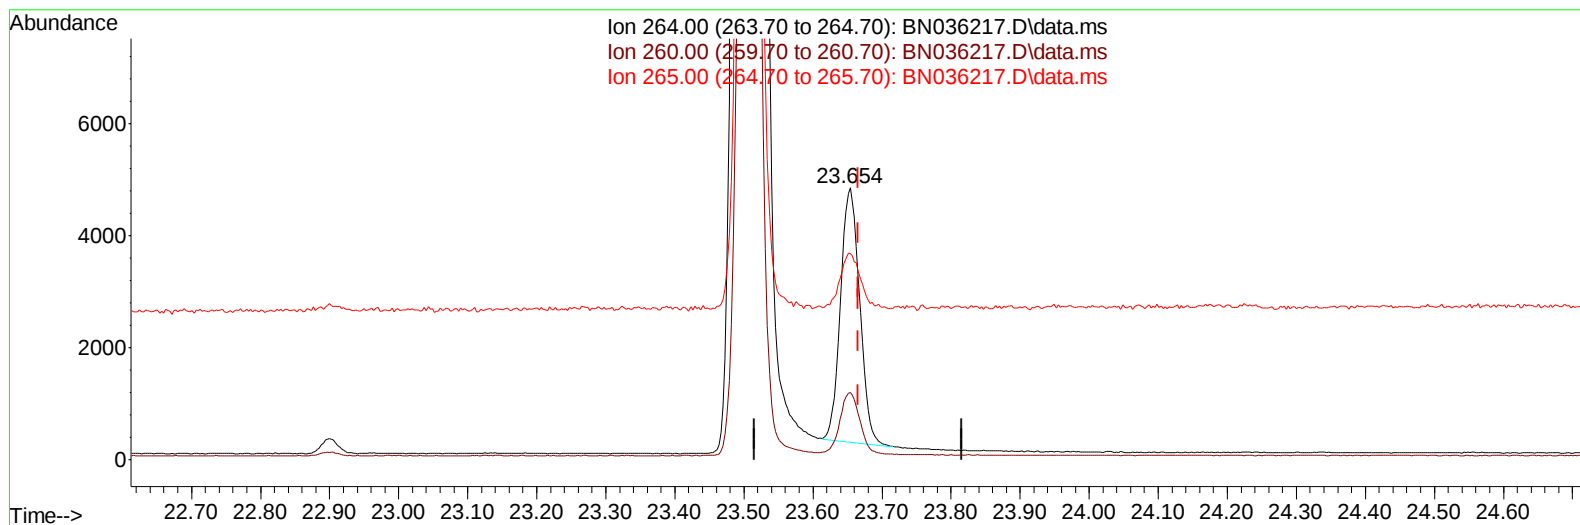

TIC: BN036217.D\data.ms

(23) Perylene-d12 (I)

23.654min (-0.012) 0.40 ng/ul m

response 8757

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	24.72
265.00	53.20	75.88#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013125\
 Data File : BN036217.D
 Acq On : 01 Feb 2025 21:16
 Operator : RC/JU
 Sample : Q1248-15
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A6346

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/03/2025
 Supervised By :mohammad ahmed 02/04/2025

Quant Time: Feb 03 12:06:08 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 21 23:52:22 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.786	152	2909	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.578	136	7625	0.400	ng/ul	-0.03
9) Acenaphthene-d10	14.431	164	4795	0.400	ng/ul	-0.02
13) Phenanthrene-d10	17.174	188	10287	0.400	ng/ul	-0.02
17) Chrysene-d12	21.365	240	10205	0.400	ng/ul	0.00
23) Perylene-d12	23.654	264	8757m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.255	96	9436	2.963	ng/ul	-0.02
6) 2-Methylnaphthalene-d10	12.172	152	1761	0.183	ng/ul	-0.03
18) Fluoranthene-d10	19.205	212	3340	0.119	ng/ul	-0.01

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013125\
Data File : BN036217.D
Acq On : 01 Feb 2025 21:16
Operator : RC/JU
Sample : Q1248-15
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A6346

Manual IntegrationsAPPROVED

Quant Time: Feb 03 12:06:08 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 21 23:52:22 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/03/2025
Supervised By :mohammad ahmed 02/04/2025

